


Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:41:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

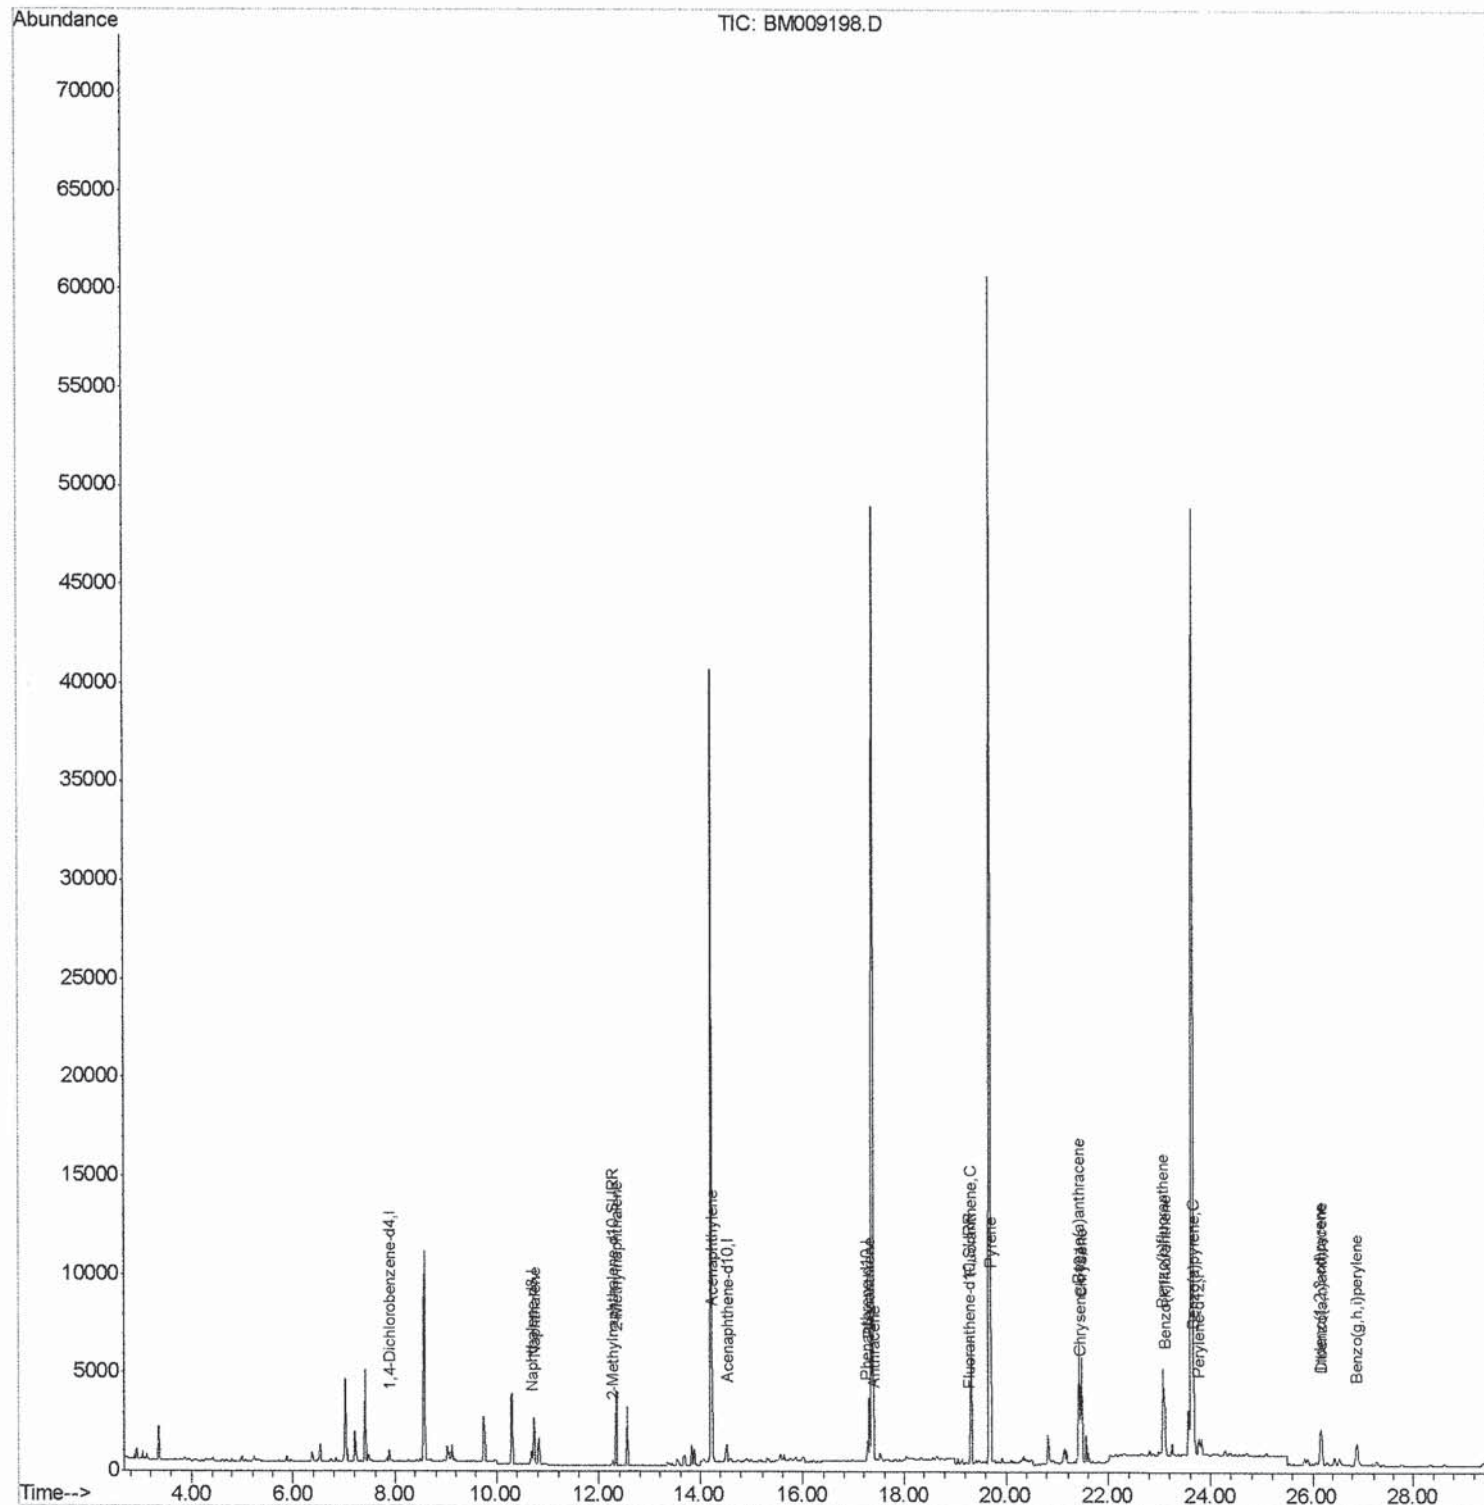




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:31:40 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

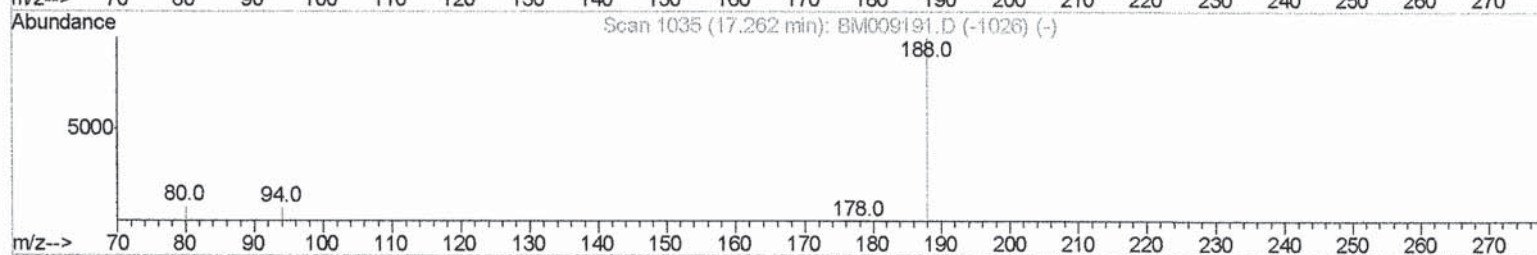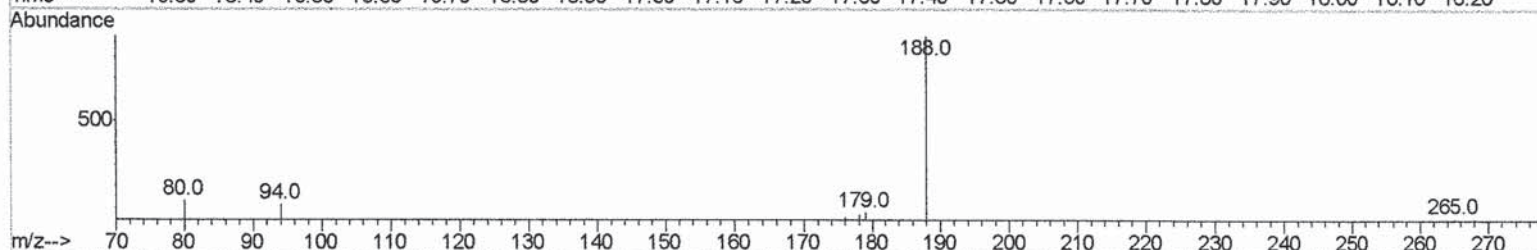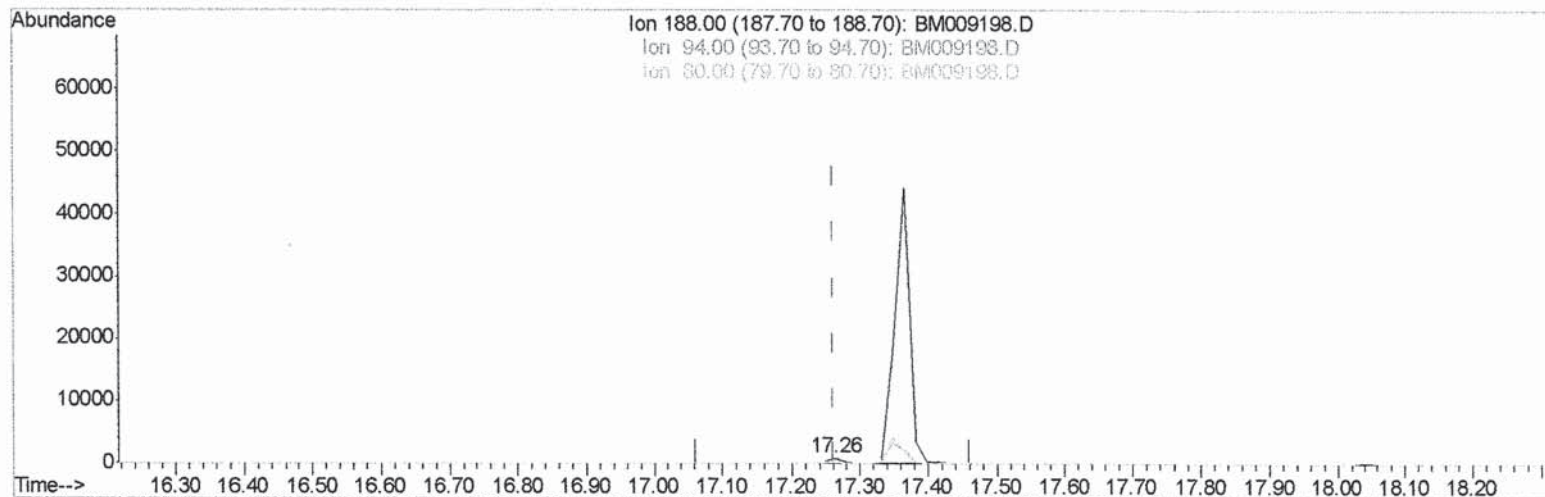

TIC: BM009198.D

(10) Phenanthrene-d10 (I)

17.262min (-0.000) 0.40ng/ul m

response 1276

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.92
80.00	11.80	14.70#
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:31:40 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

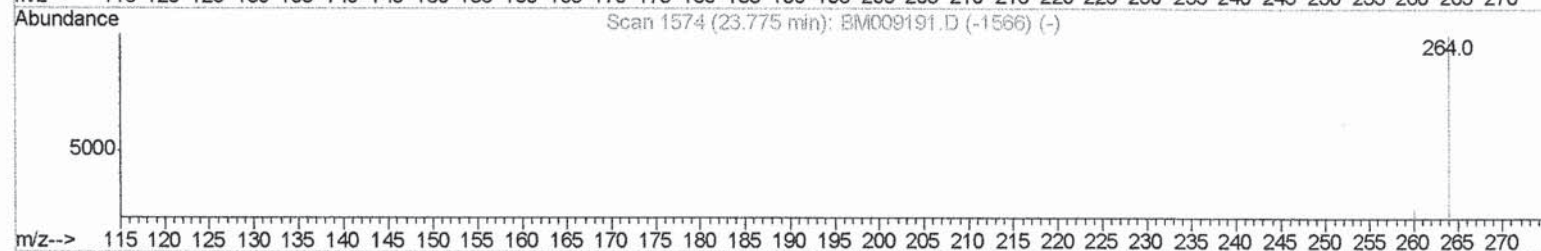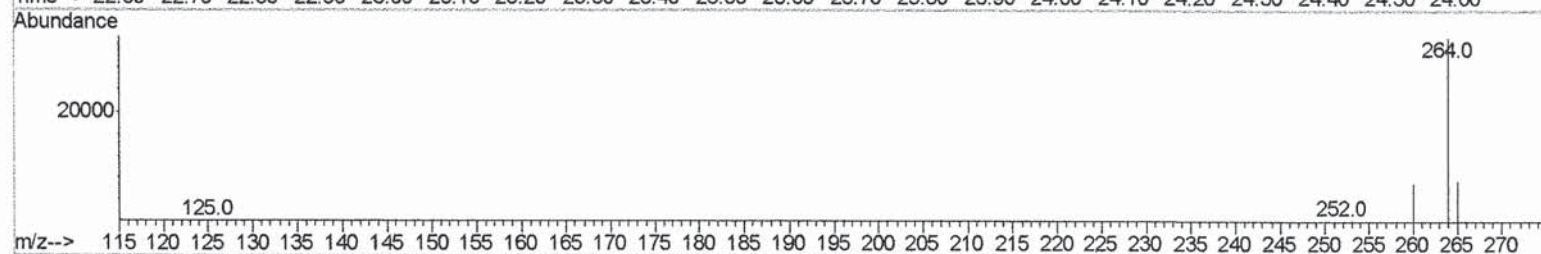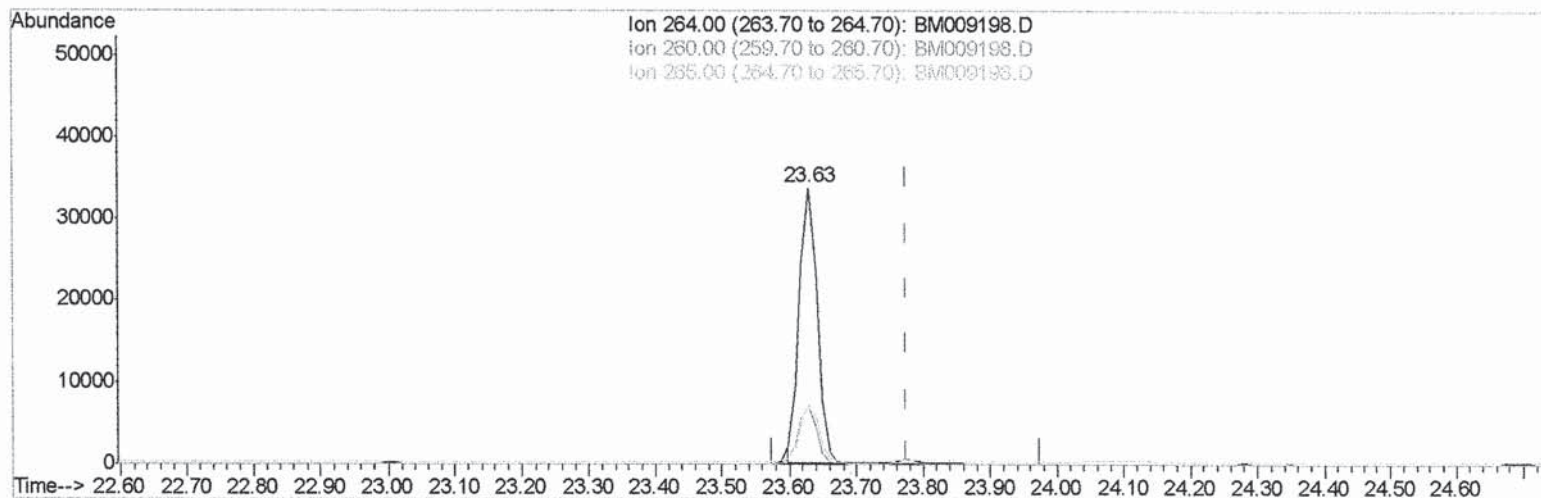

TIC: BM009198.D

(20) Perylene-d12 (I)

23.628min (-0.146) 0.40ng/ul

response 62492

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.03#
265.00	103.50	22.04#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:31:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

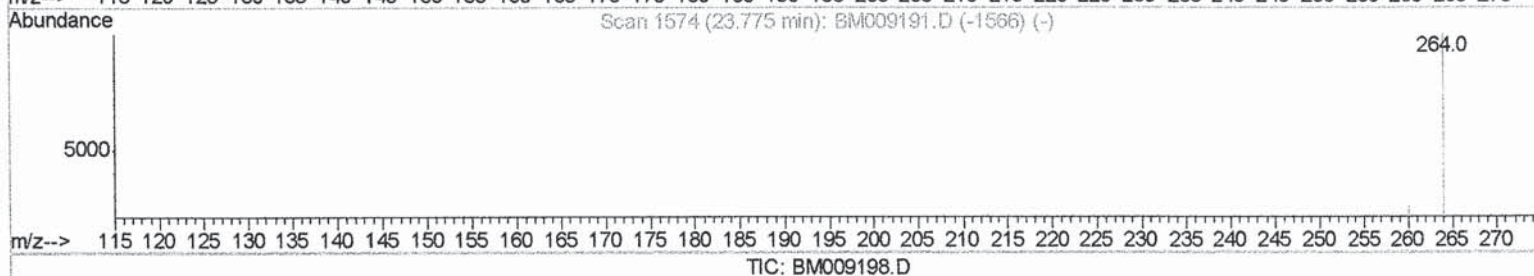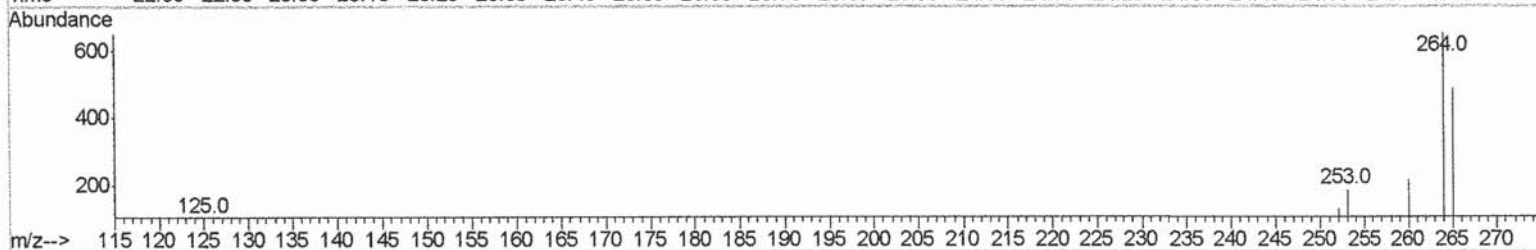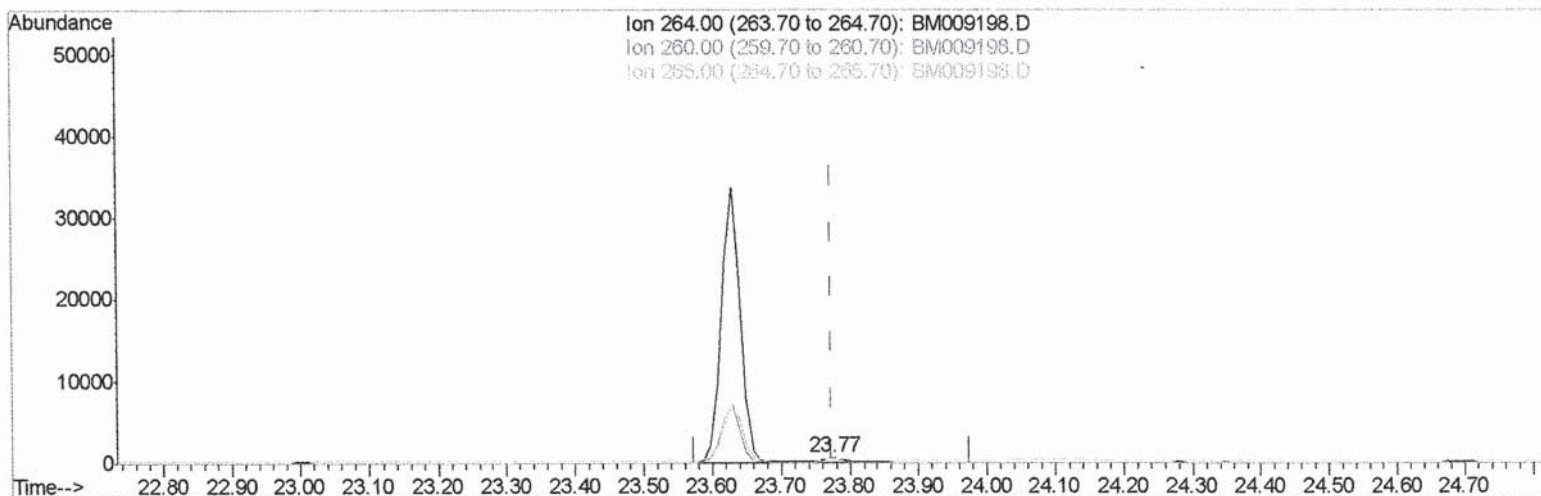

(20) Perylene-d12 (I)

23.774min (-0.000) 0.40ng/ul m

response 1195

Ion Exp% Act%

264.00 100 100

260.00 30.10 33.03

265.00 103.50 74.50#

0.00 0.00 0.00

SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

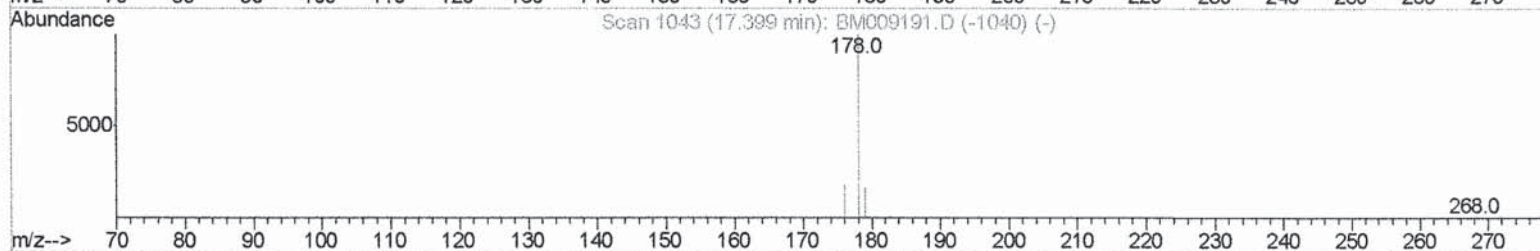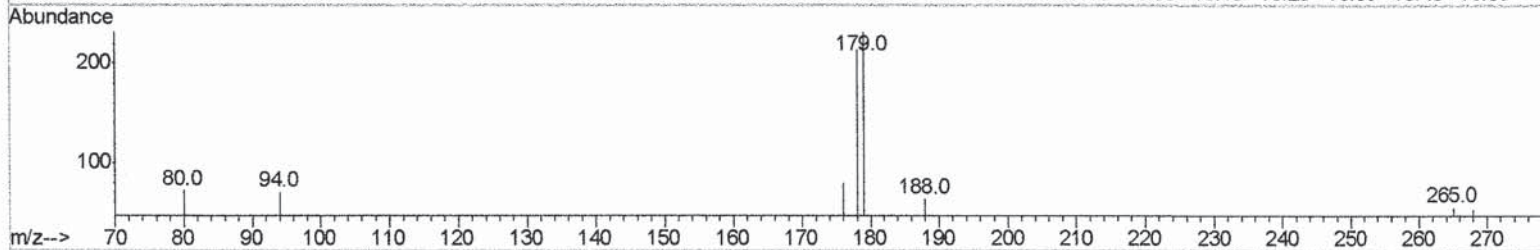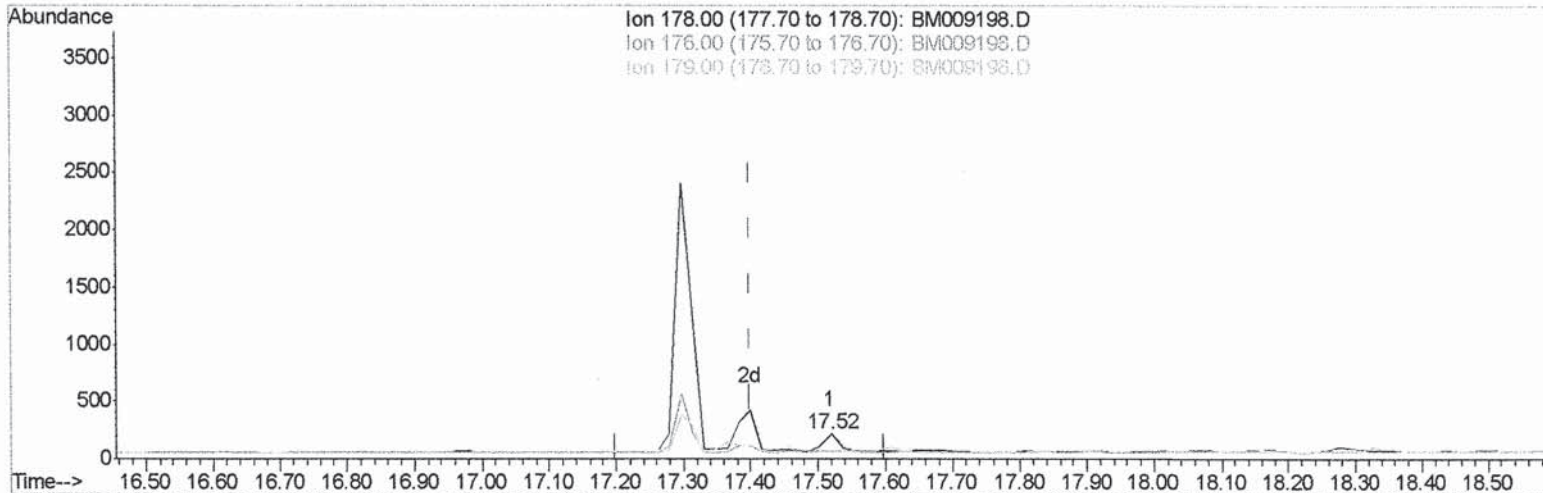

TIC: BM009198.D

(13) Anthracene

17.519min (+0.120) 0.06ng/ul

response 236

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	37.38#
179.00	18.40	108.41#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

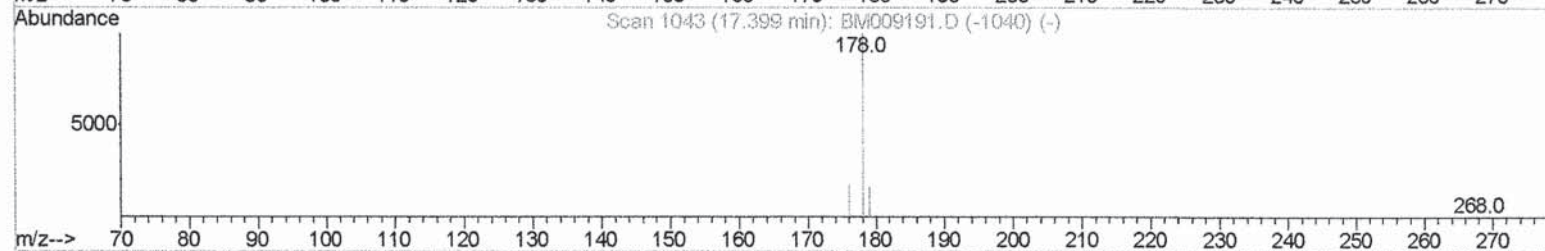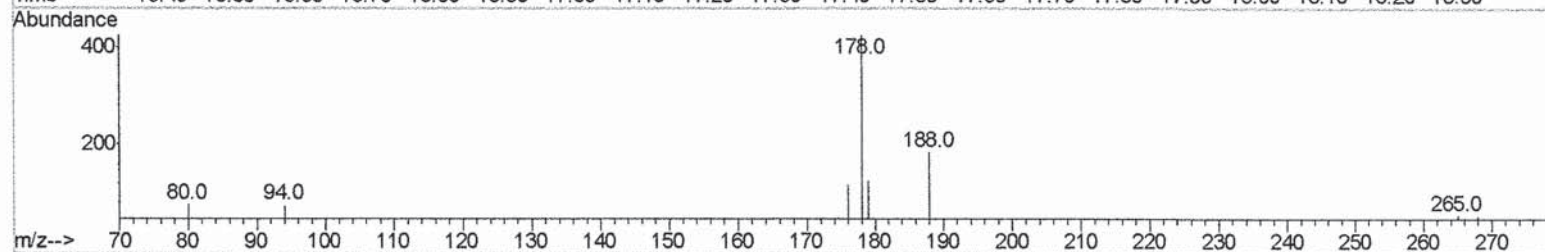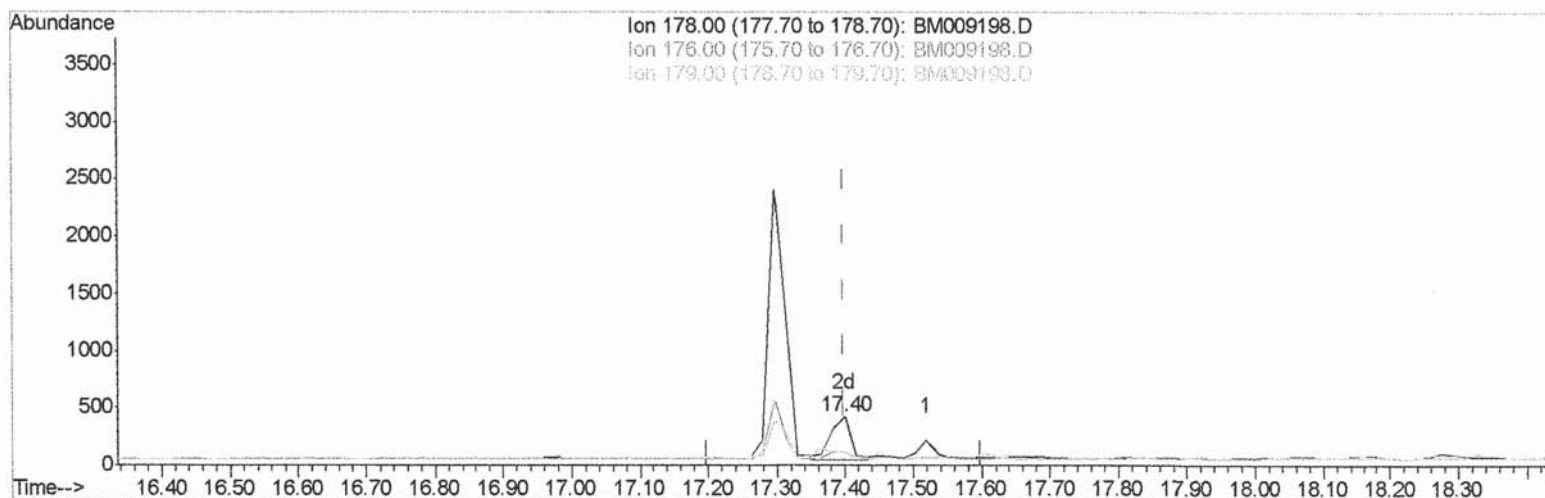

TIC: BM009198.D

(13) Anthracene

17.399min (-0.000) 0.21ng/ul m

response 815

Ion	Exp%	Act%
-----	------	------

178.00	100	100
--------	-----	-----

176.00	22.60	27.70#
--------	-------	--------

179.00	18.40	29.11#
--------	-------	--------

0.00	0.00	0.00
------	------	------

> SJ
 03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

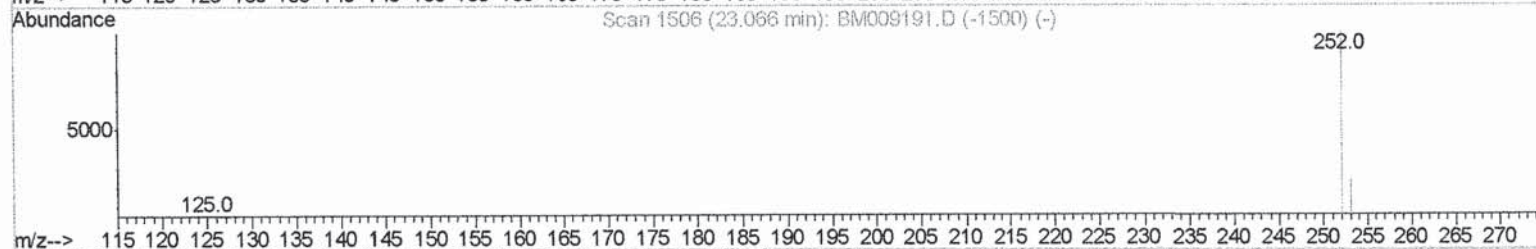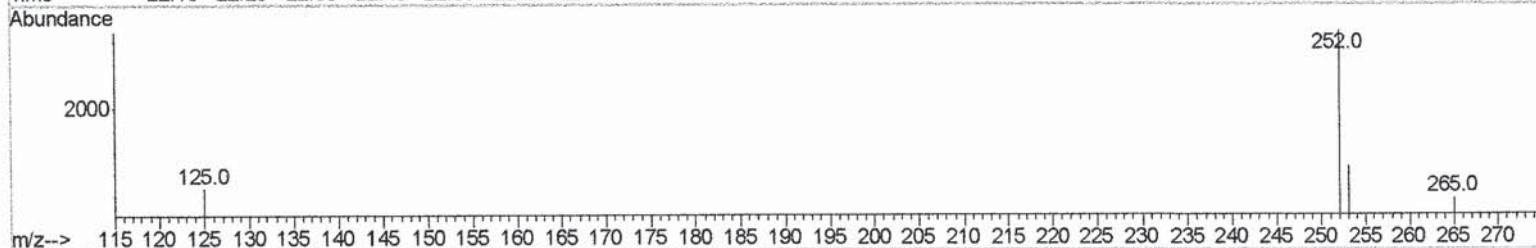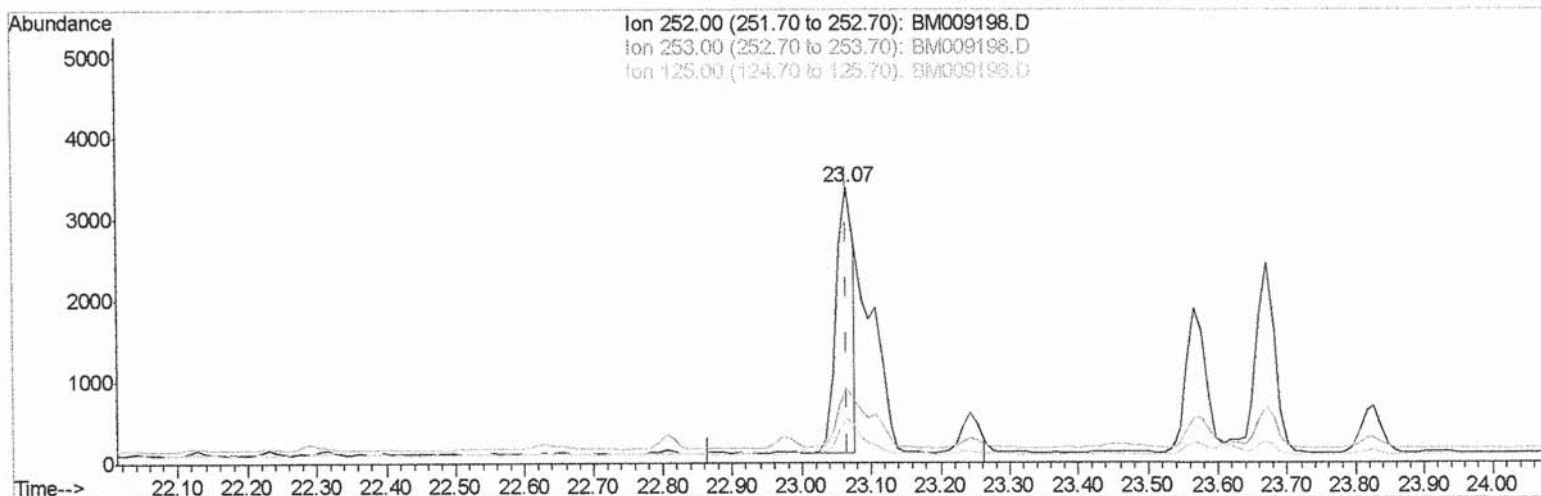

TIC: BM009198.D

(21) Benzo(b)fluoranthene
 23.066min (-0.000) 1.27ng/ul
 response 5942

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.23
125.00	17.50	16.52
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

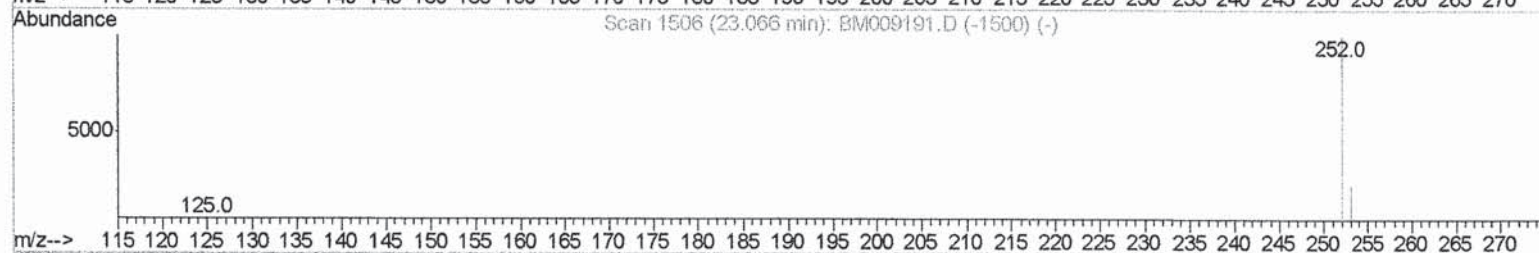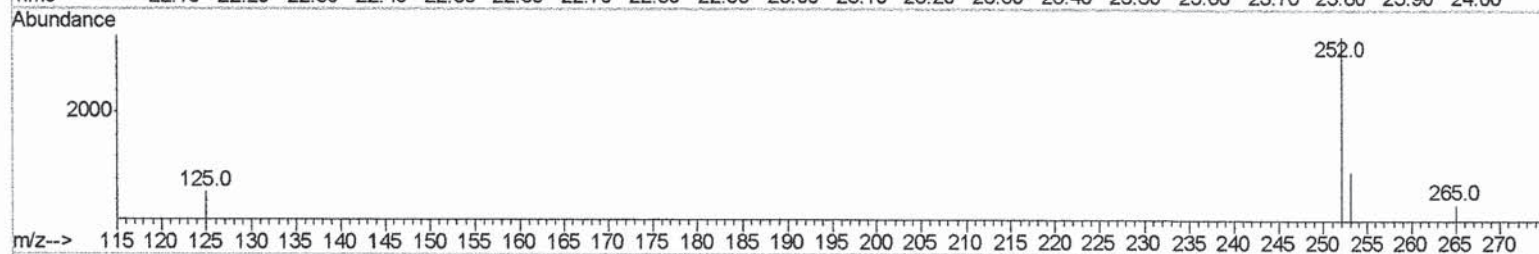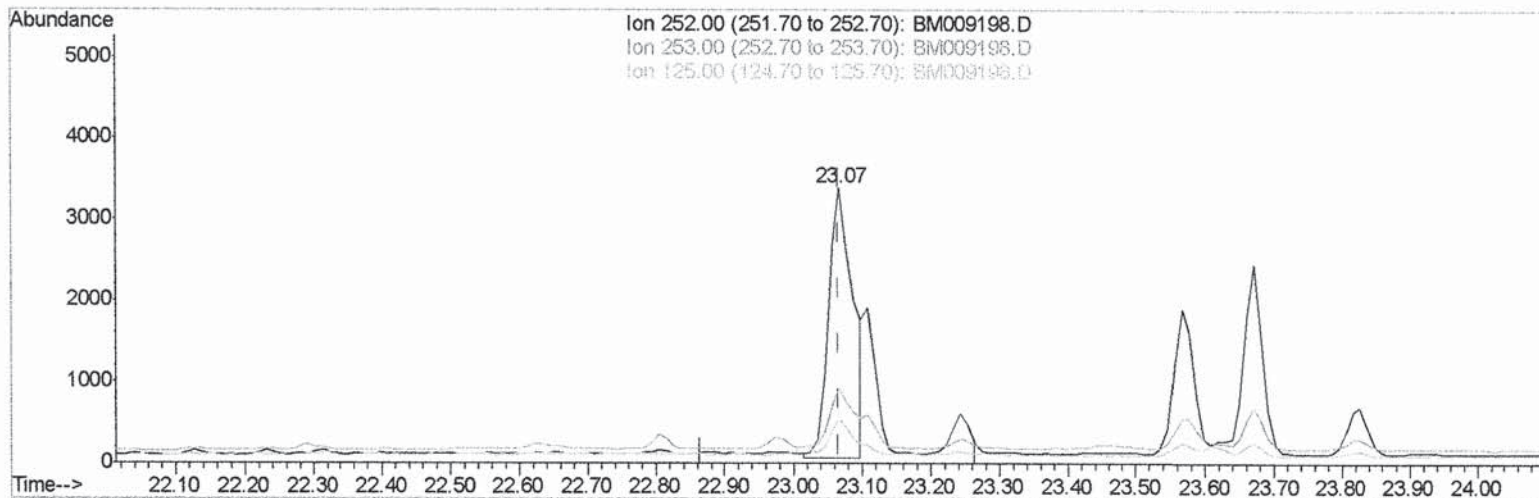

TIC: BM009198.D

(21) Benzo(b)fluoranthene

23.066min (-0.000) 1.81ng/ul m>

response 8481

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.23
125.00	17.50	16.52
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

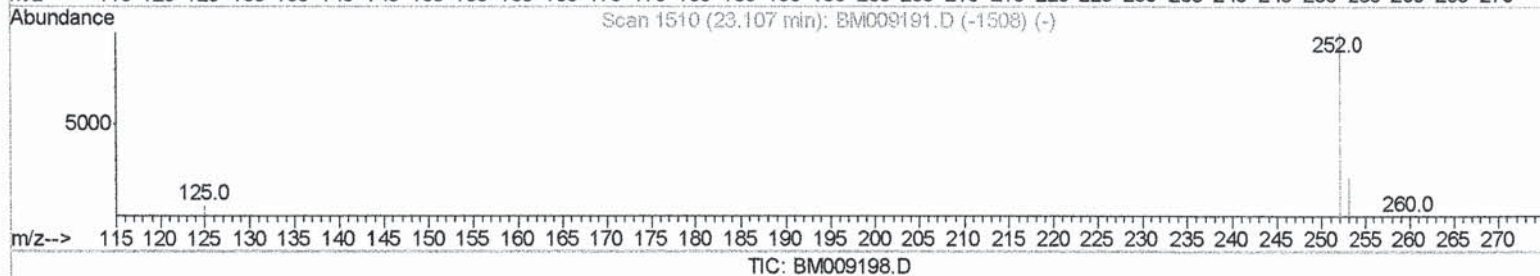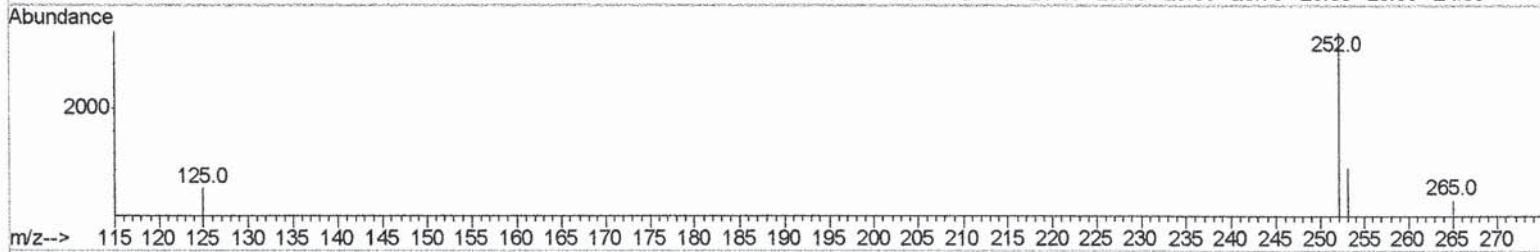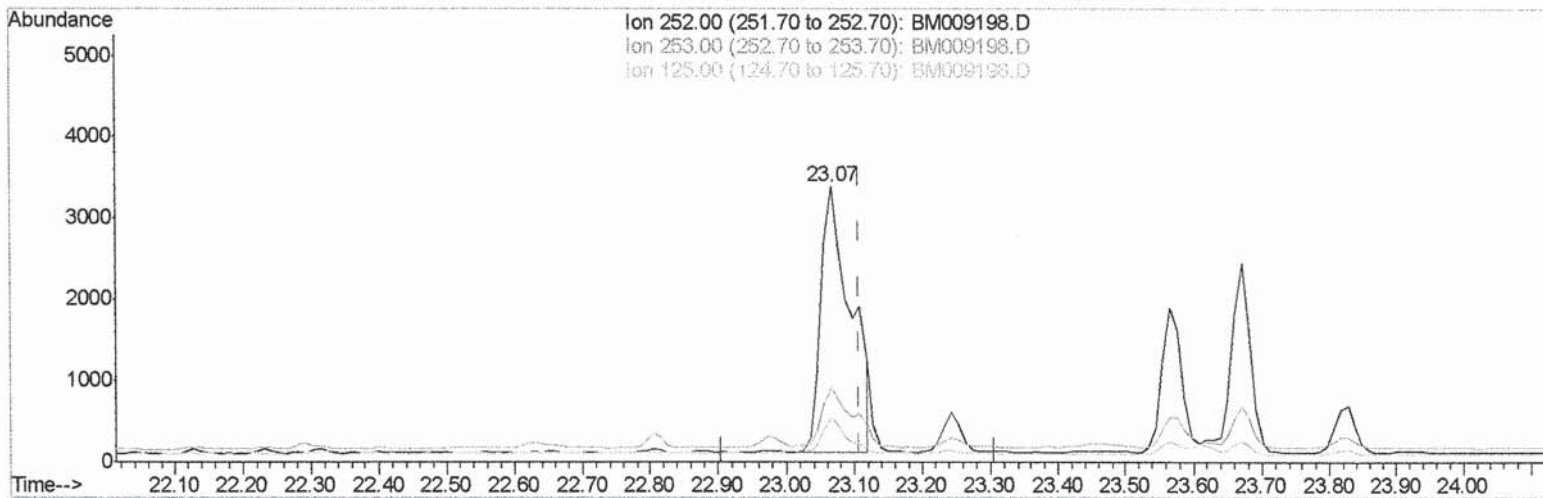

(22) Benzo(k)fluoranthene

23.066min (-0.042) 2.40ng/ul

response 9949

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	27.23
125.00	17.10	16.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

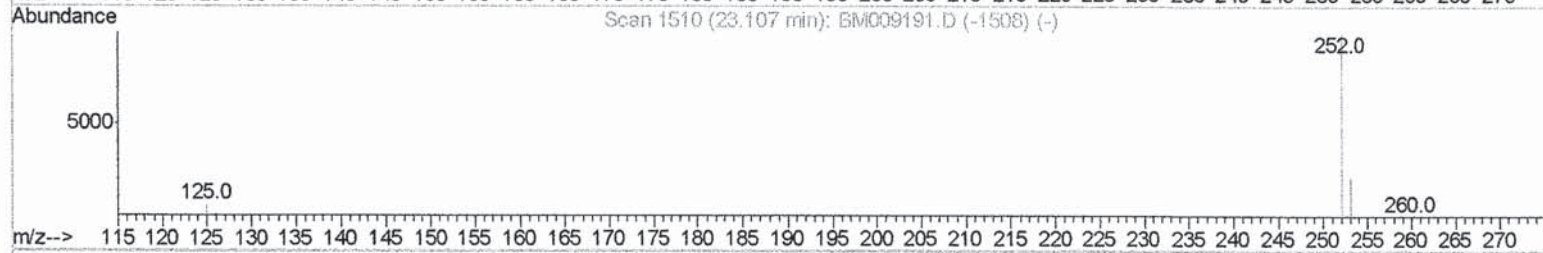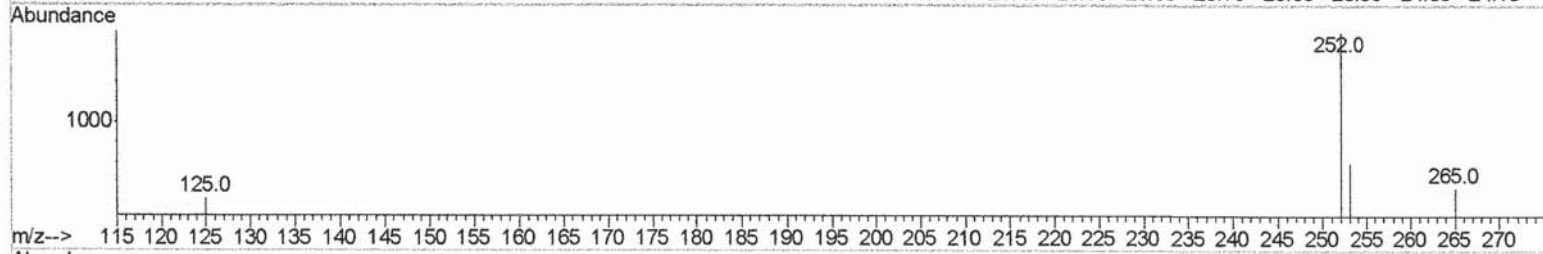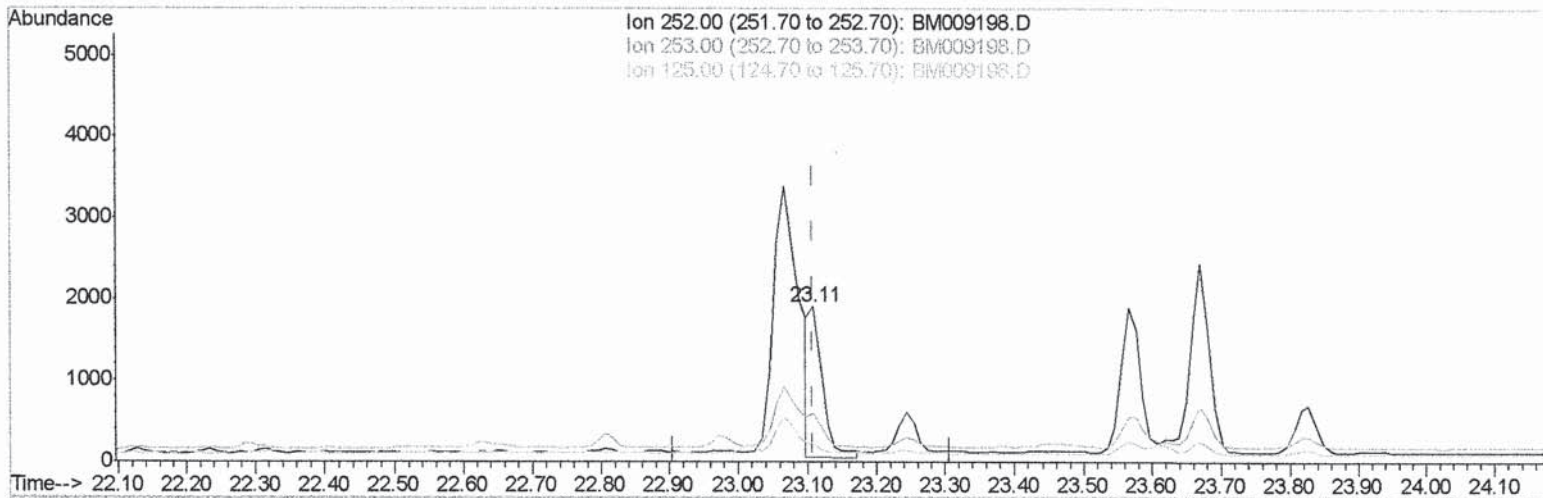

TIC: BM009198.D

(22) Benzo(k)fluoranthene

23.107min (-0.000) 0.58ng/ul m

response 2399

Ion Exp% Act%

252.00 100 100

253.00 30.60 31.38

125.00 17.10 11.94#

0.00 0.00 0.00

53
 03/13/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

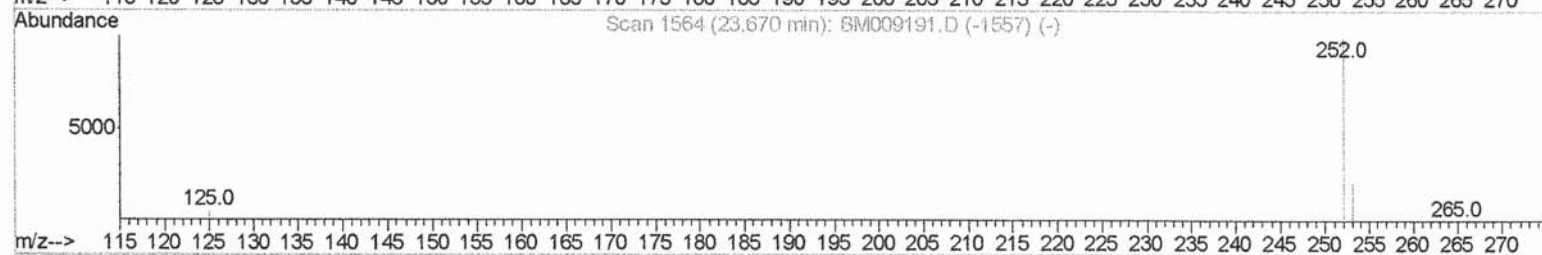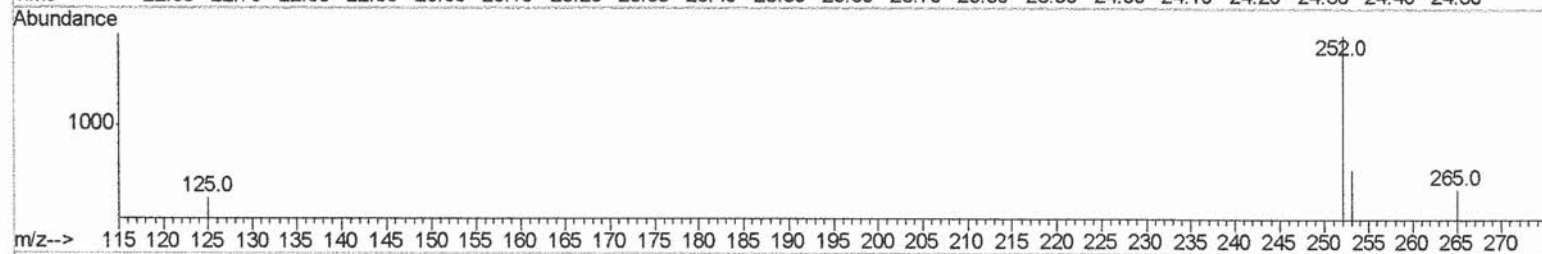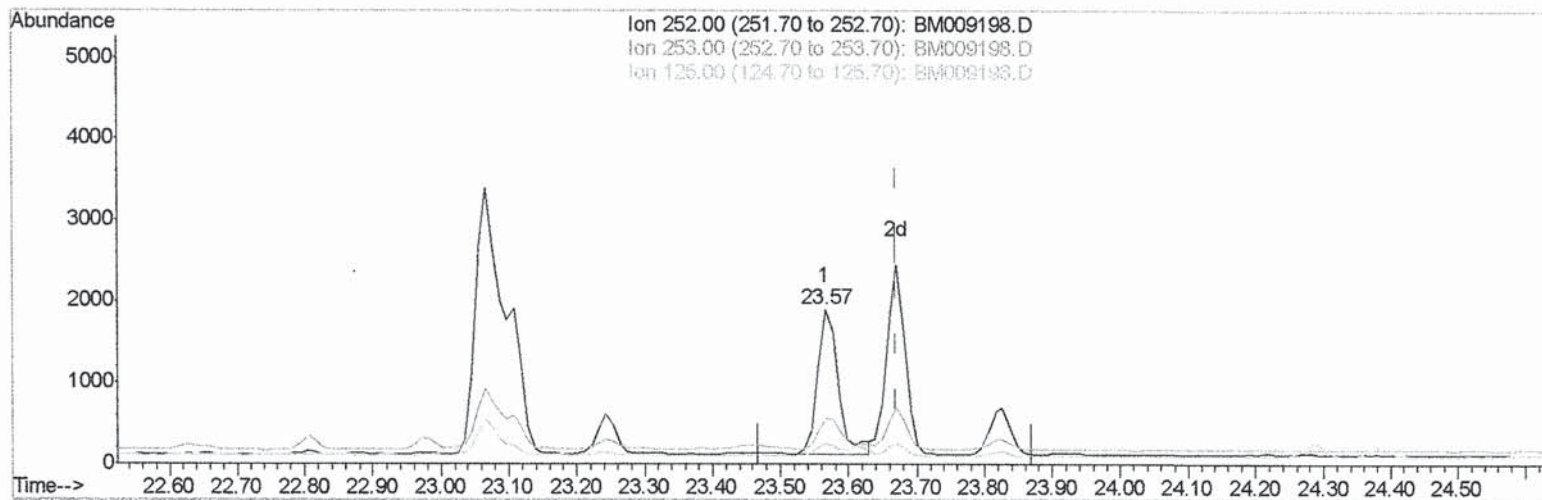

TIC: BM009198.D

(23) Benzo(a)pyrene (C)

23.566min (-0.104) 0.88ng/ul

response 3737

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	29.26
125.00	22.60	13.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

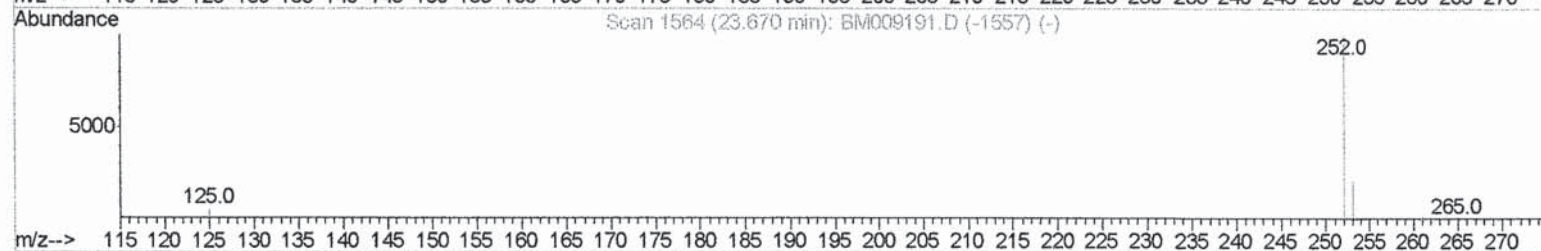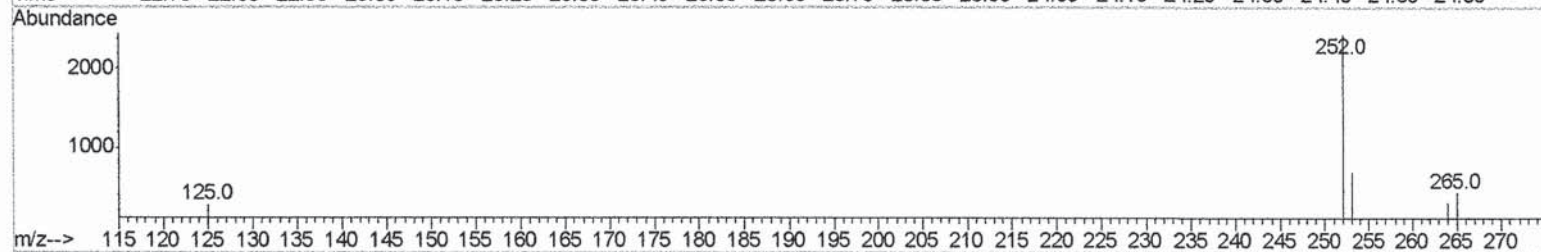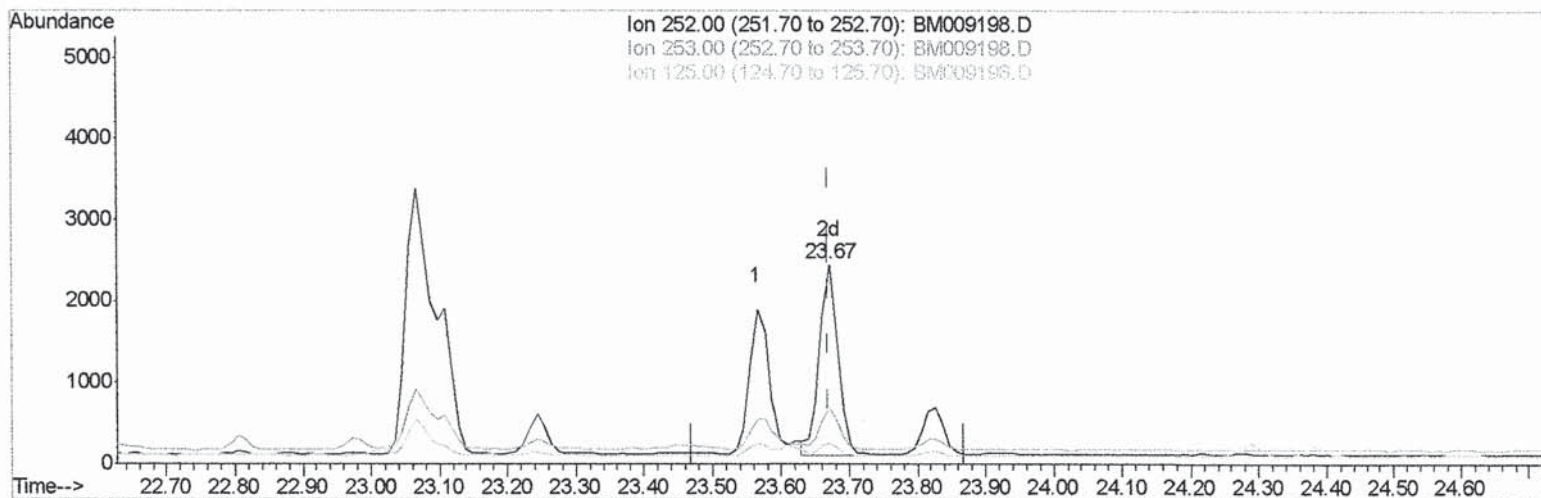

TIC: BM009198.D

(23) Benzo(a)pyrene (C)

23.670min (-0.000) 1.07ng/ul m

response 4510

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	28.16#
125.00	22.60	10.66#
0.00	0.00	0.00

Handwritten signature: SJ
 03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

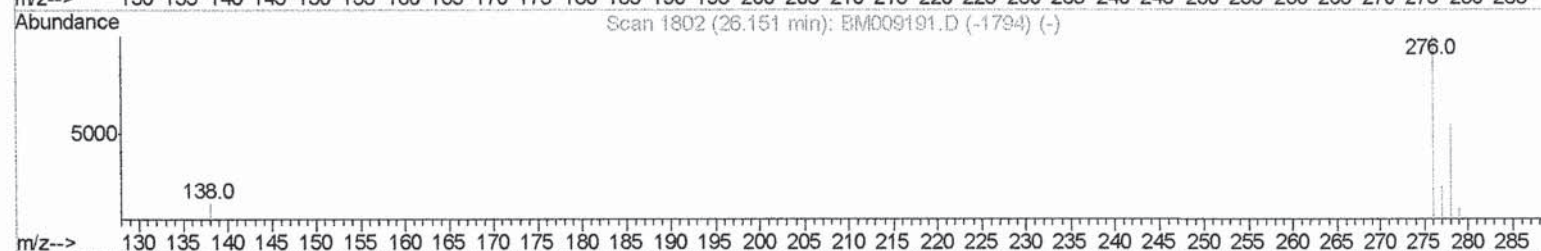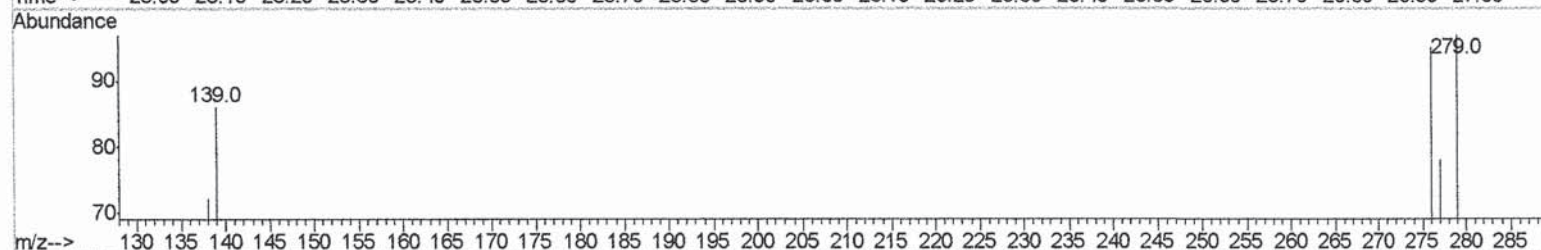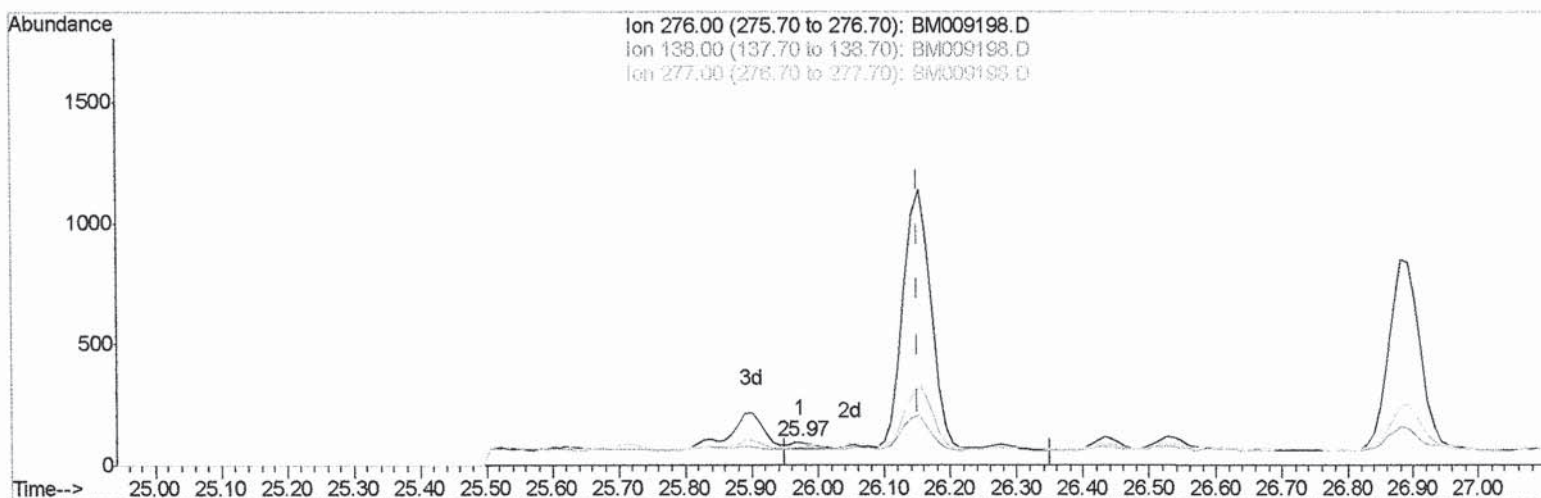

TIC: BM009198.D

(24) Indeno(1,2,3-cd)pyrene

25.974min (-0.177) 0.01ng/ul

response 72

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

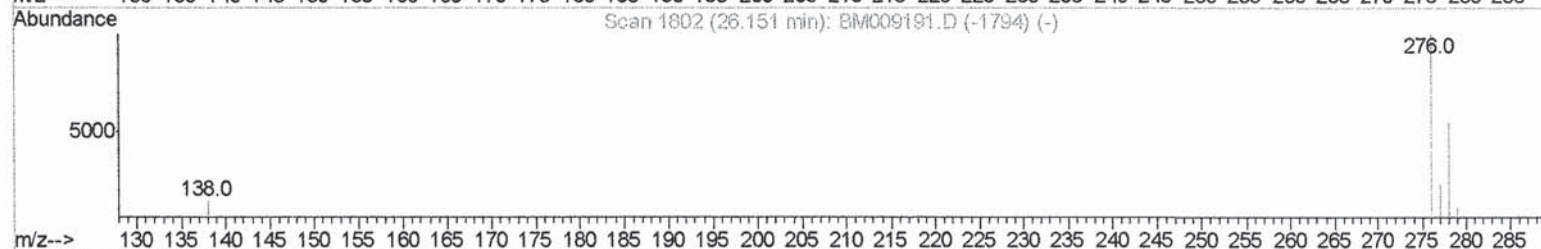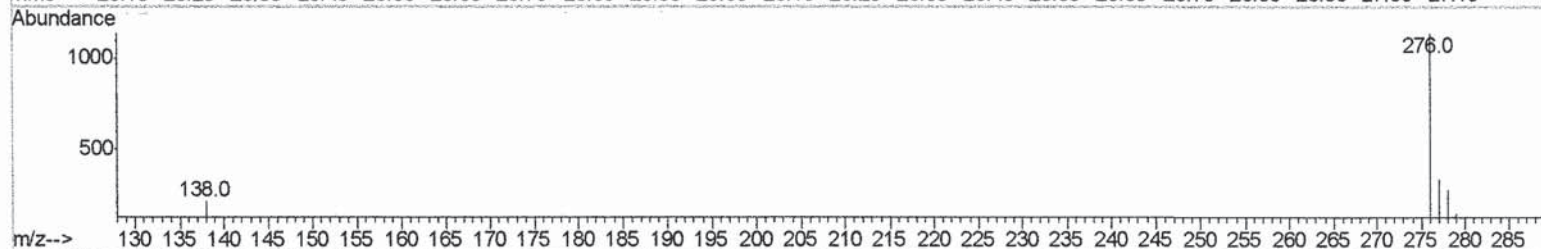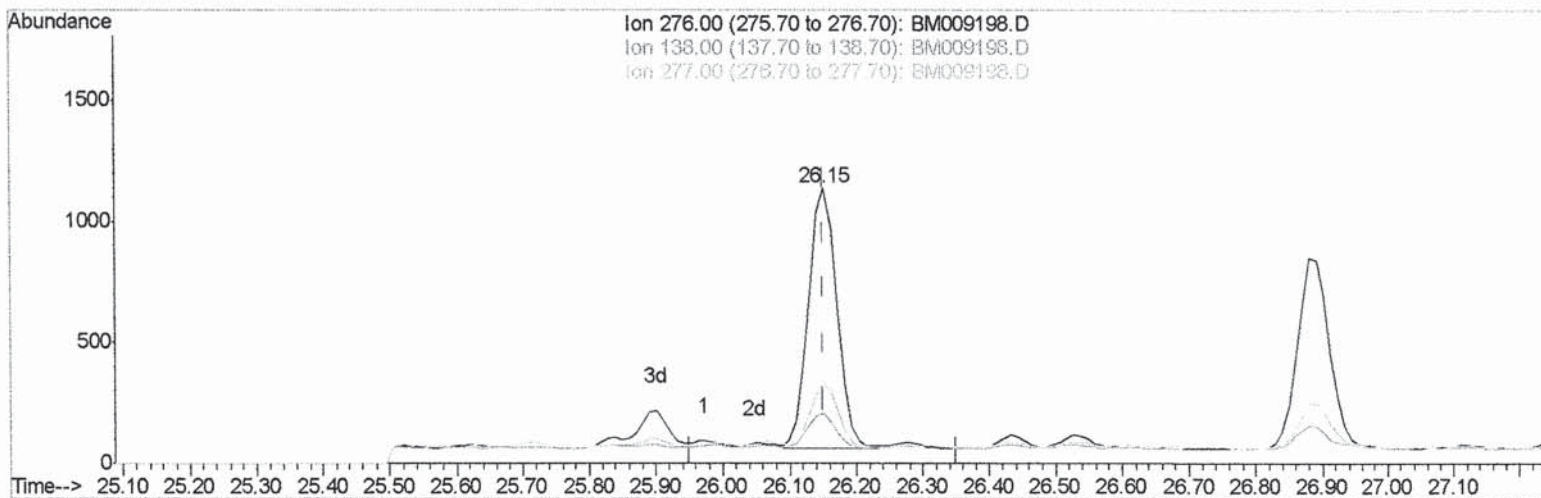

TIC: BM009198.D

(24) Indeno(1,2,3-cd)pyrene

26.151min (-0.000) 0.59ng/ul m

response 3165

Ion Exp% Act%

276.00 100 100

138.00 23.90 0.00#

277.00 24.50 0.00#

0.00 0.00 0.00

> $\frac{55}{03/13/17}$

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

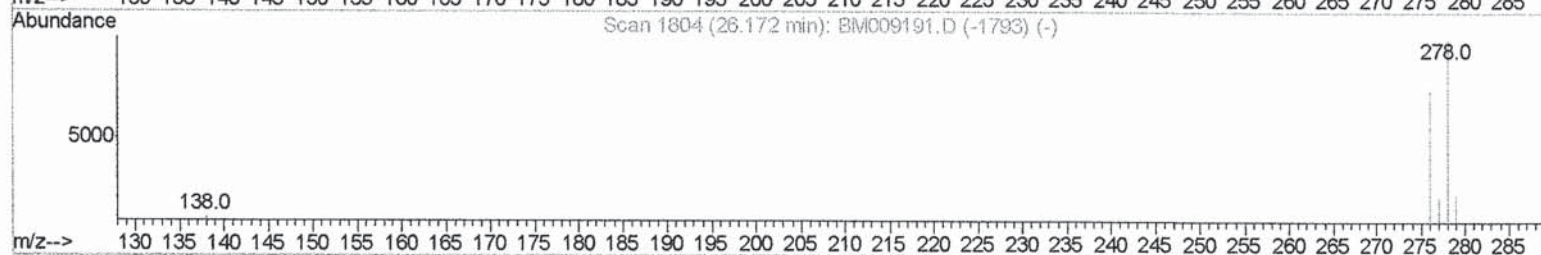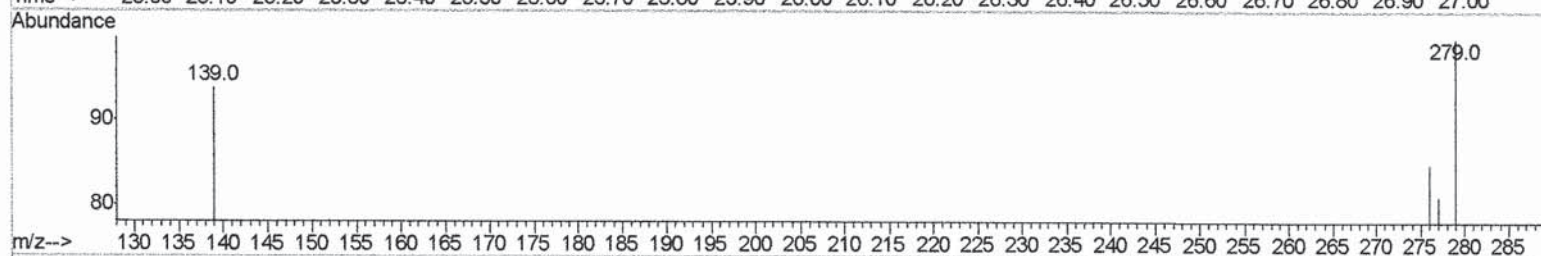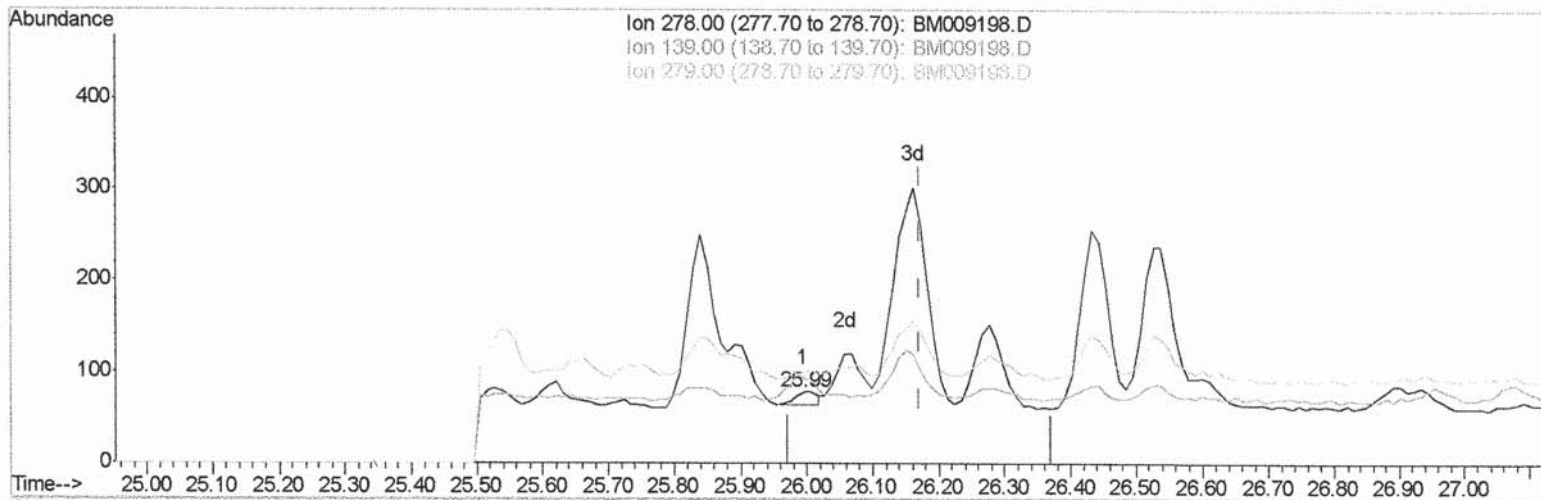

TIC: BM009198.D

(25) Dibenzo(a,h)anthracene

25.995min (-0.177) 0.01ng/ul

response 34

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	120.51#
279.00	32.40	128.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

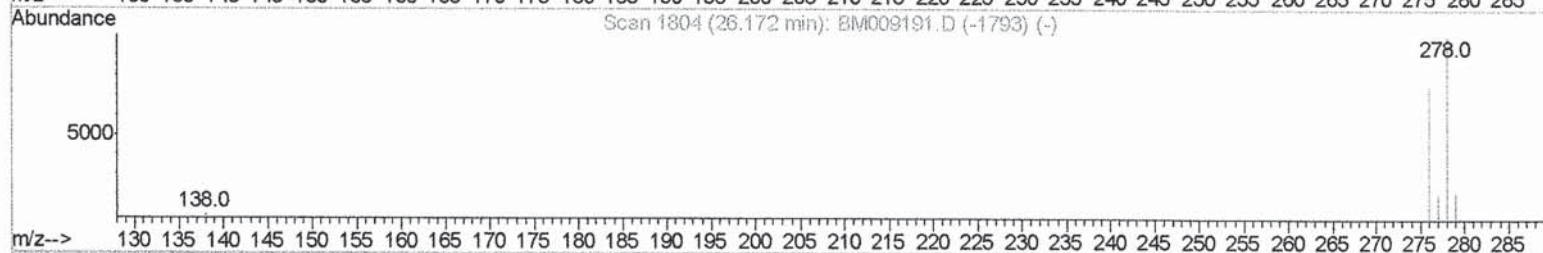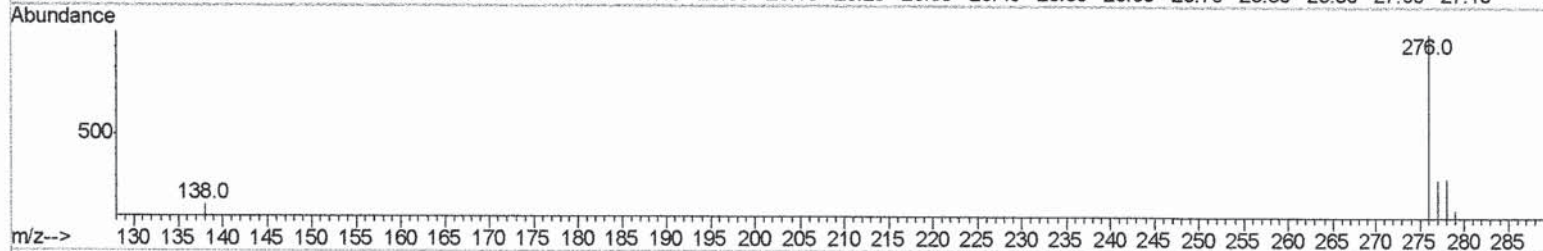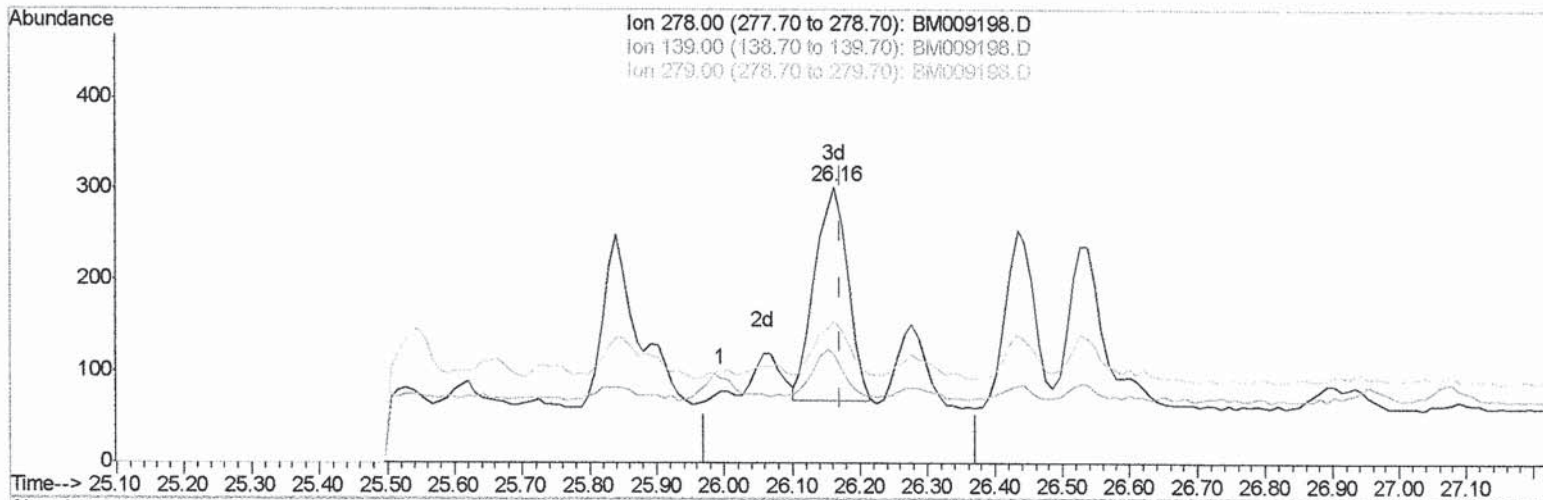

TIC: BM009198.D

(25) Dibenzo(a,h)anthracene

26.162min (-0.011) 0.18ng/ul m

response 798

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	39.40#
279.00	32.40	51.66#
0.00	0.00	0.00

SJ
 03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

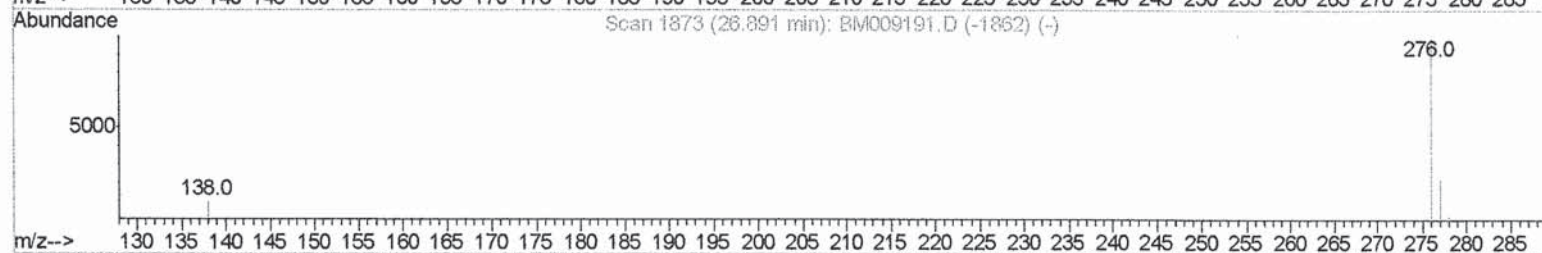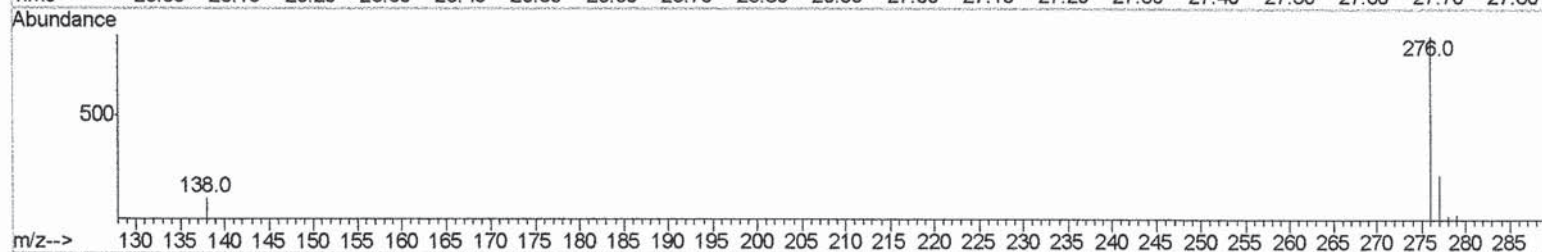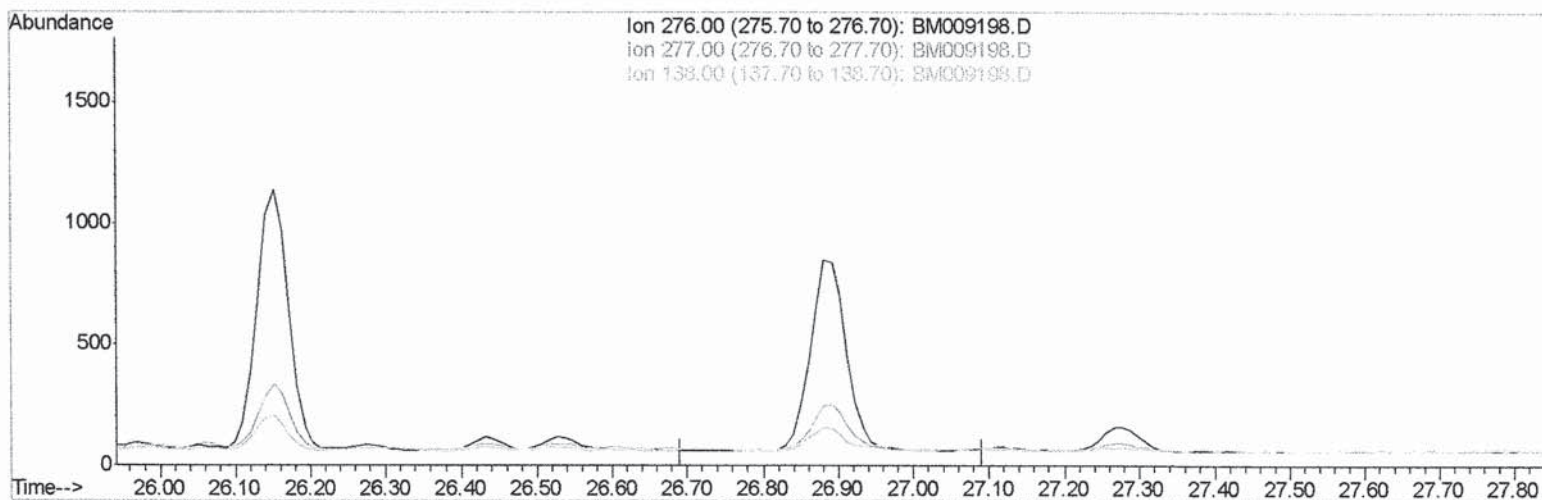

TIC: BM009198.D

(26) Benzo(g,h,i)perylene
 26.891min (-26.891) 0.00ng/ul
 response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:38:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

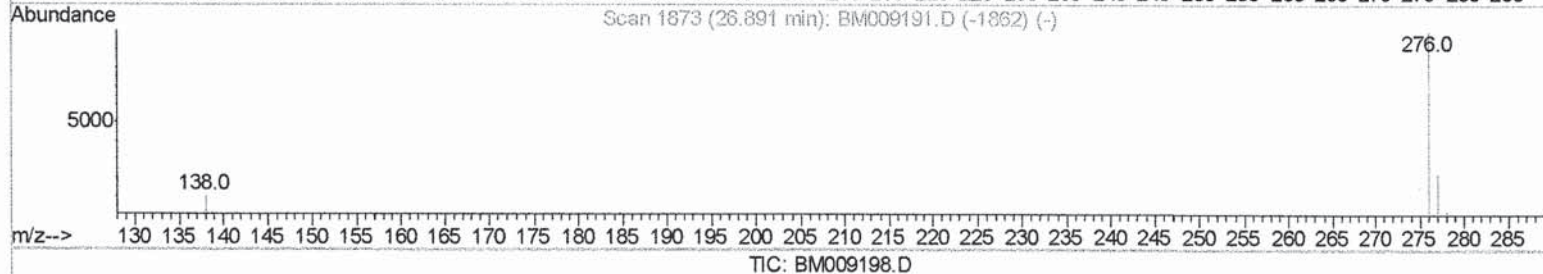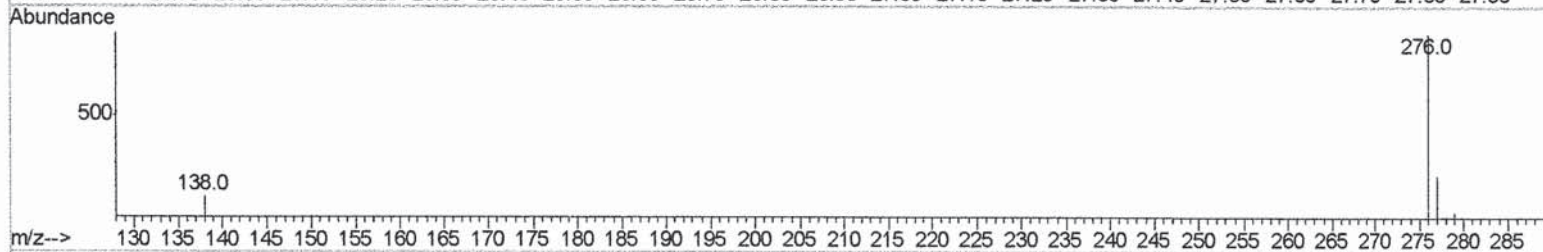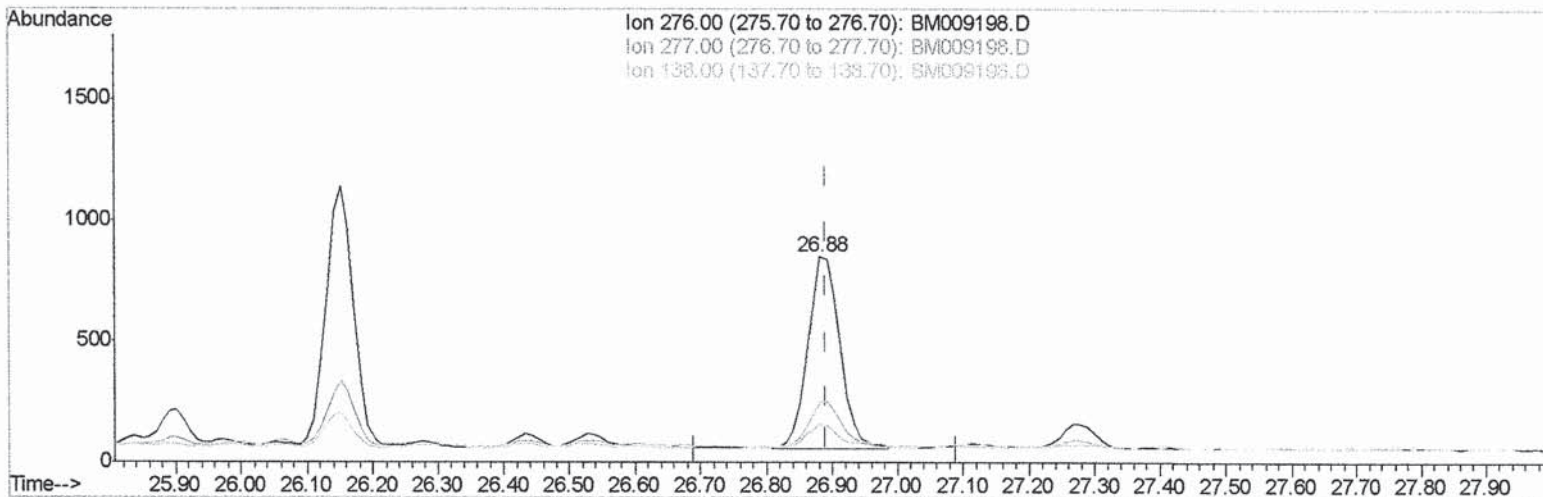

(26) Benzo(g,h,i)perylene

26.881min (-0.011) 0.59ng/ul m

response 2694

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	29.20
138.00	25.60	18.79#
0.00	0.00	0.00

57
03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009198.D
 Acq On : 11 Mar 2017 04:54
 Operator : SJ/MA
 Sample : I2072-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK3

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:31:40 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

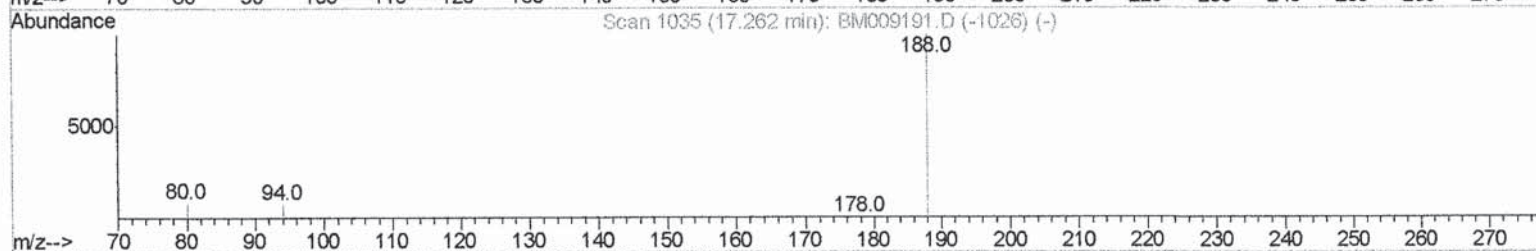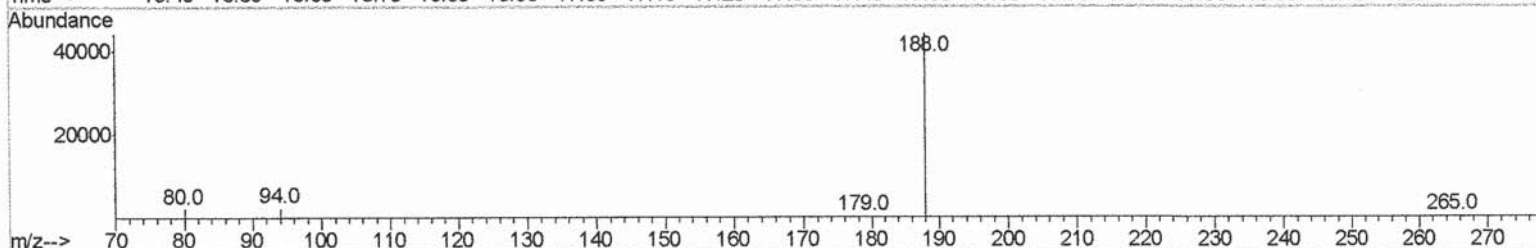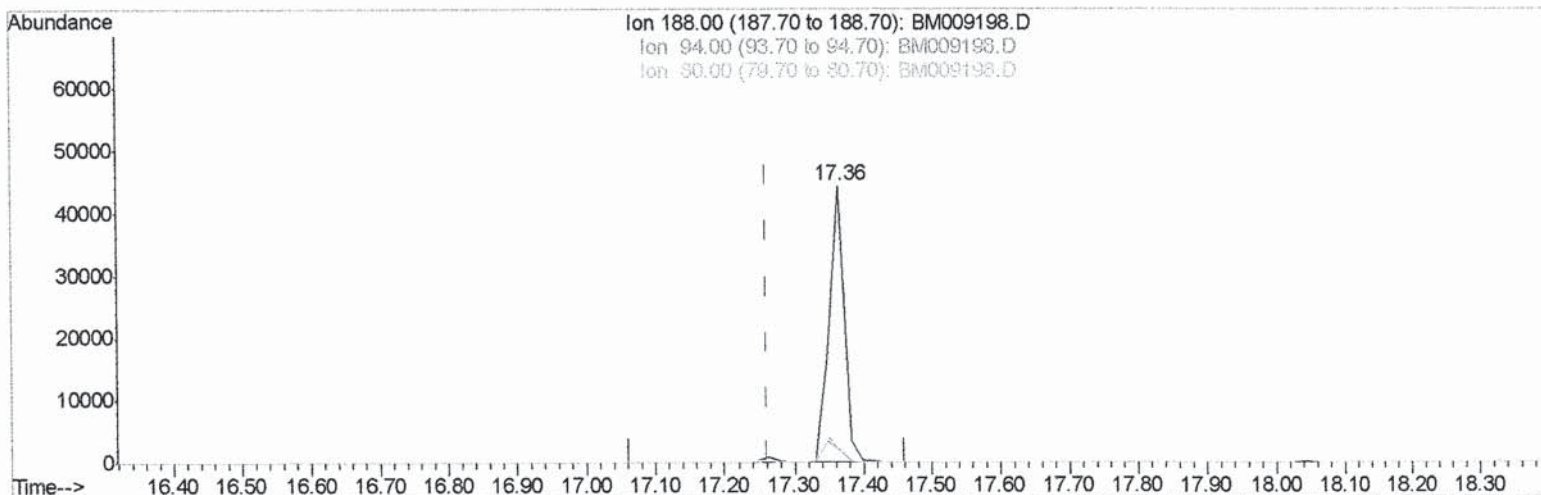

TIC: BM009198.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 66997

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.07#
80.00	11.80	4.59#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009198.D
Acq On : 11 Mar 2017 04:54
Operator : SJ/MA
Sample : I2072-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK3

Manual Integrations
APPROVED

mohammad
3/13/2017 2:15:22 PM

Quant Time: Mar 11 05:41:20 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	266	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	875	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	547	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1276m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1299	0.40	ng/ul	0.00
20) Perylene-d12	23.77	264	1195m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	322	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	850	0.21	ng/ul	0.00
Target Compounds						
					Ovalue	
3) Naphthalene	10.73	128	3315	1.31	ng/ul	98
5) 2-Methylnaphthalene	12.34	142	2665	1.47	ng/ul	99
7) Acenaphthylene	14.23	152	368	0.13	ng/ul#	54
12) Phenanthrene	17.30	178	3887	0.97	ng/ul	99
13) Anthracene	17.40	178	815m	0.21	ng/ul	
15) Fluoranthene	19.31	202	6833	1.31	ng/ul	96
17) Pyrene	19.69	202	7662	1.71	ng/ul	96
18) Benzo(a)anthracene	21.42	228	5330	1.23	ng/ul	98
19) Chrysene	21.47	228	5352	1.31	ng/ul	95
21) Benzo(b)fluoranthene	23.07	252	8481m	1.81	ng/ul	
22) Benzo(k)fluoranthene	23.11	252	2399m	0.58	ng/ul	
23) Benzo(a)pyrene	23.67	252	4510m	1.07	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.15	276	3165m	0.59	ng/ul	
25) Dibenzo(a,h)anthracene	26.16	278	798m	0.18	ng/ul	
26) Benzo(a,h,i)perylene	26.88	276	2694m	0.59	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed