
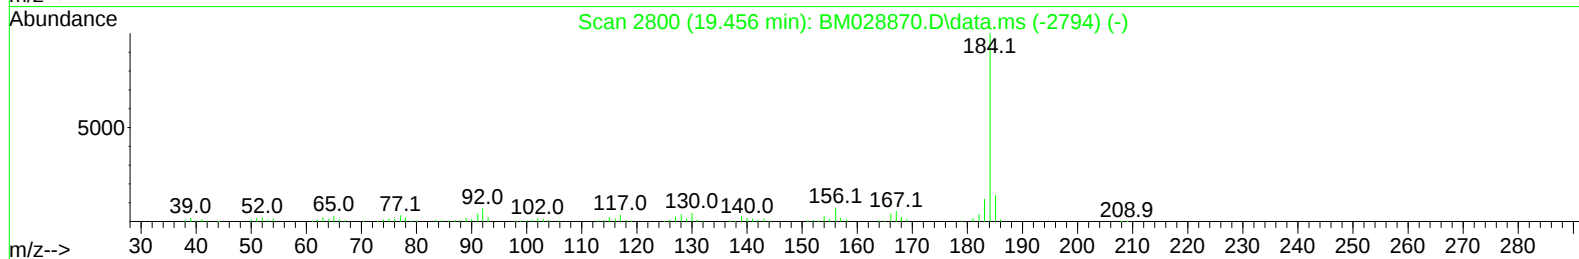
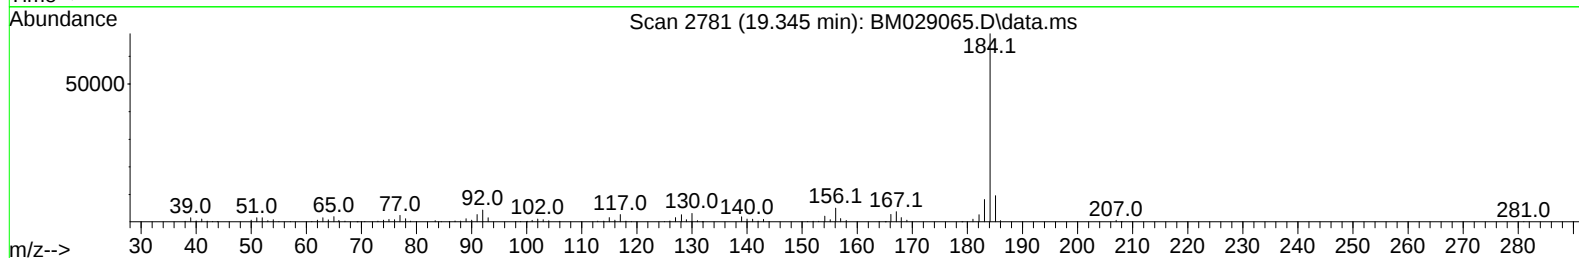


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031021\  
 Data File : BM029065.D  
 Acq On : 10 Mar 2021 12:05  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 12:43:33 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Mar 09 10:08:02 2021  
 Response via : Initial Calibration

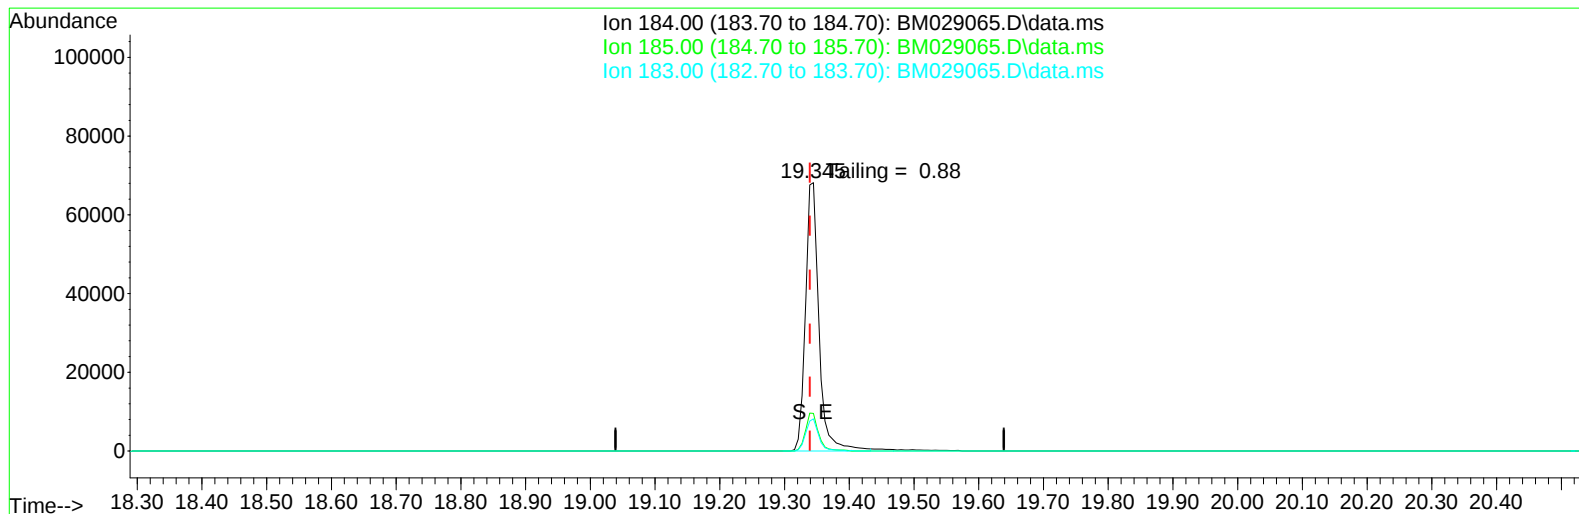




TIC: BM029065.D\data.ms

**(77) Benzidine****19.345min (+ 0.006) 0.00 ng****response 100523**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.04  |
| 183.00 | 12.10  | 12.01  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031021\  
Data File : BM029065.D  
Acq On : 10 Mar 2021 12:05  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 12:43:33 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 09 10:08:02 2021  
Response via : Initial Calibration

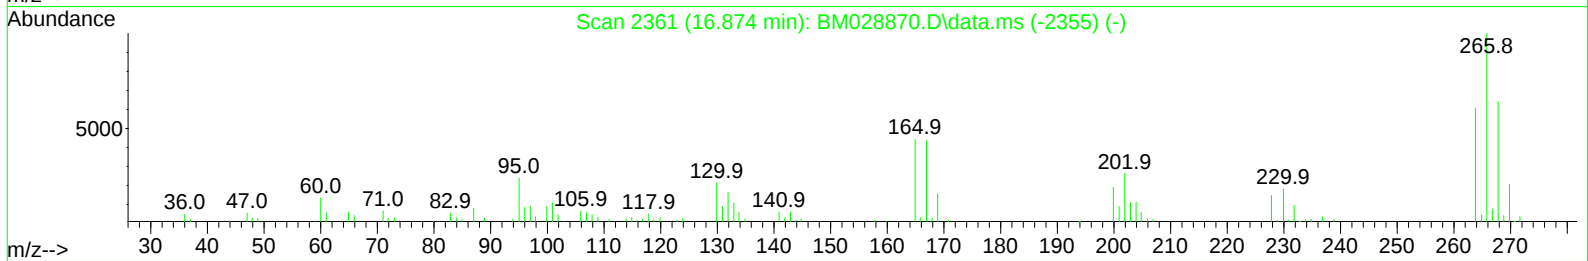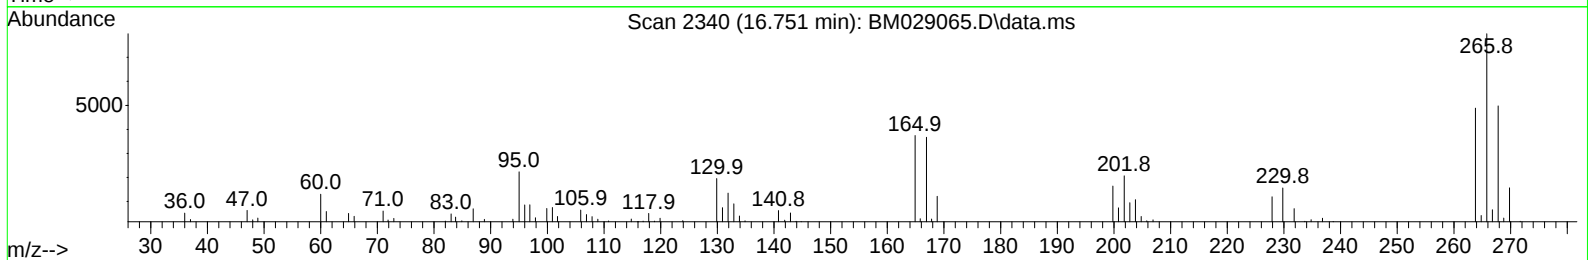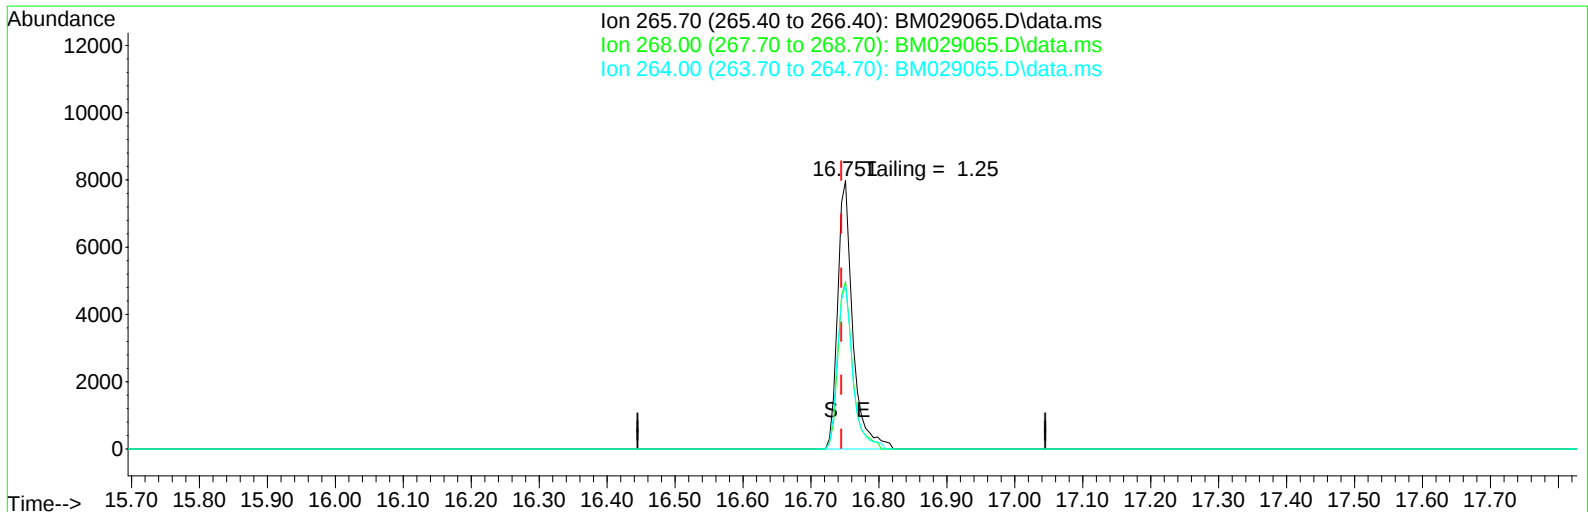

TIC: BM029065.D\data.ms

**(70) Pentachlorophenol (C)**

**16.751min (+ 0.006) 0.00 ng**

**response 12337**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 62.39  |
| 264.00 | 63.30  | 61.18  |
| 0.00   | 0.00   | 0.00   |