

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
 Data File : BM029067.D
 Acq On : 10 Mar 2021 13:19
 Operator : CG/JU
 Sample : PB135082BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135082BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.240	378	383	400	rBB	225895	321826	52.78%	11.925%
2	6.869	654	660	675	rBV	198530	312998	51.33%	11.598%
3	7.669	791	796	802	rBB	38924	56319	9.24%	2.087%
4	8.846	989	996	1004	rBV	123446	202821	33.26%	7.515%
5	10.463	1264	1271	1278	rBV	46002	72789	11.94%	2.697%
6	12.951	1687	1694	1708	rBV	282476	406641	66.68%	15.067%
7	14.339	1924	1930	1936	rBB2	60650	87589	14.36%	3.245%
8	15.839	2179	2185	2197	rBV	203203	292749	48.01%	10.847%
9	17.086	2391	2397	2405	rBB	74808	99974	16.39%	3.704%
10	19.710	2838	2843	2848	rBV	518662	609797	100.00%	22.595%
11	21.256	3102	3106	3112	rBV	94457	116034	19.03%	4.299%
12	23.415	3468	3473	3482	rVB2	65862	119269	19.56%	4.419%




Sum of corrected areas: 2698806

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
Data File : BM029067.D
Acq On : 10 Mar 2021 13:19
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

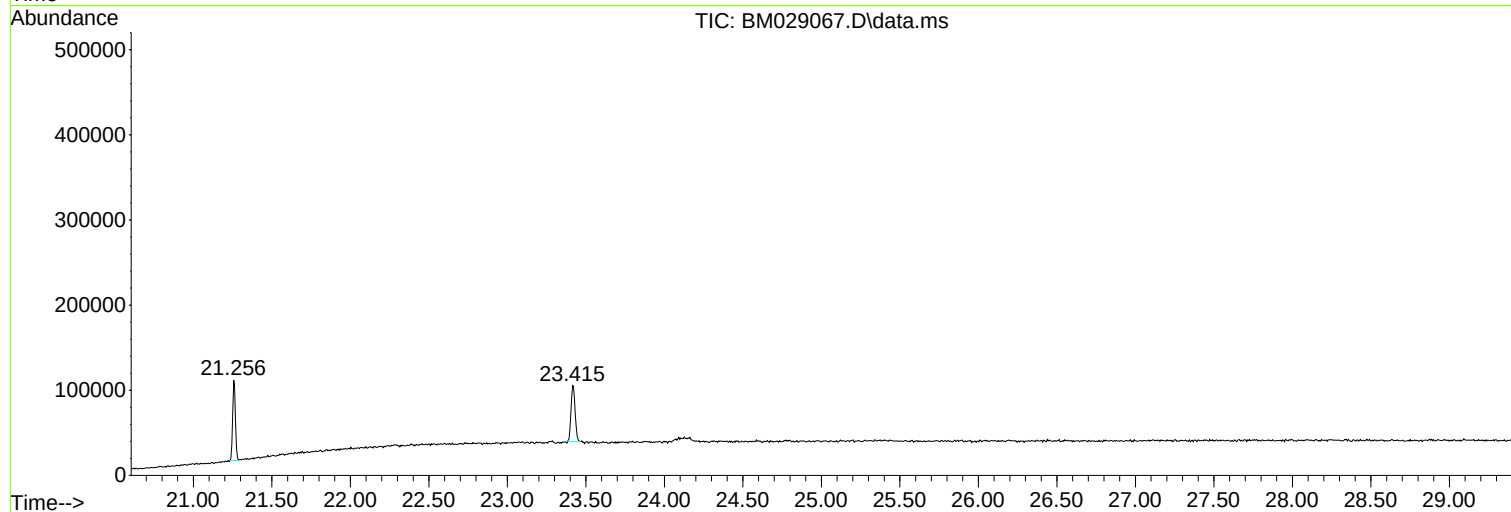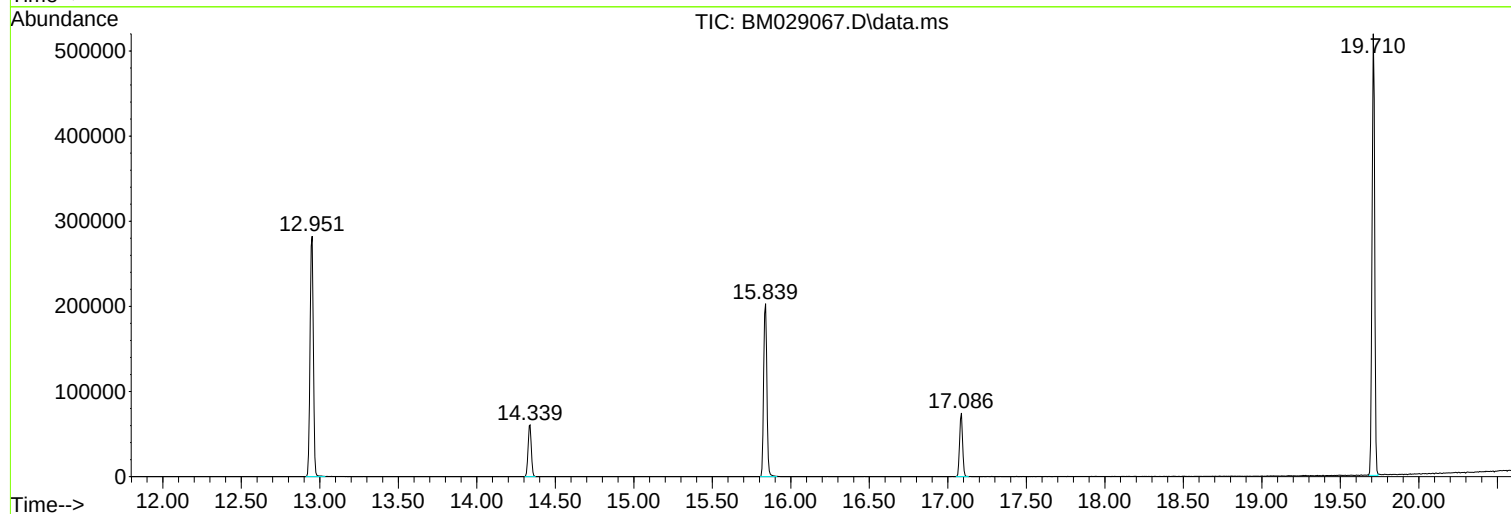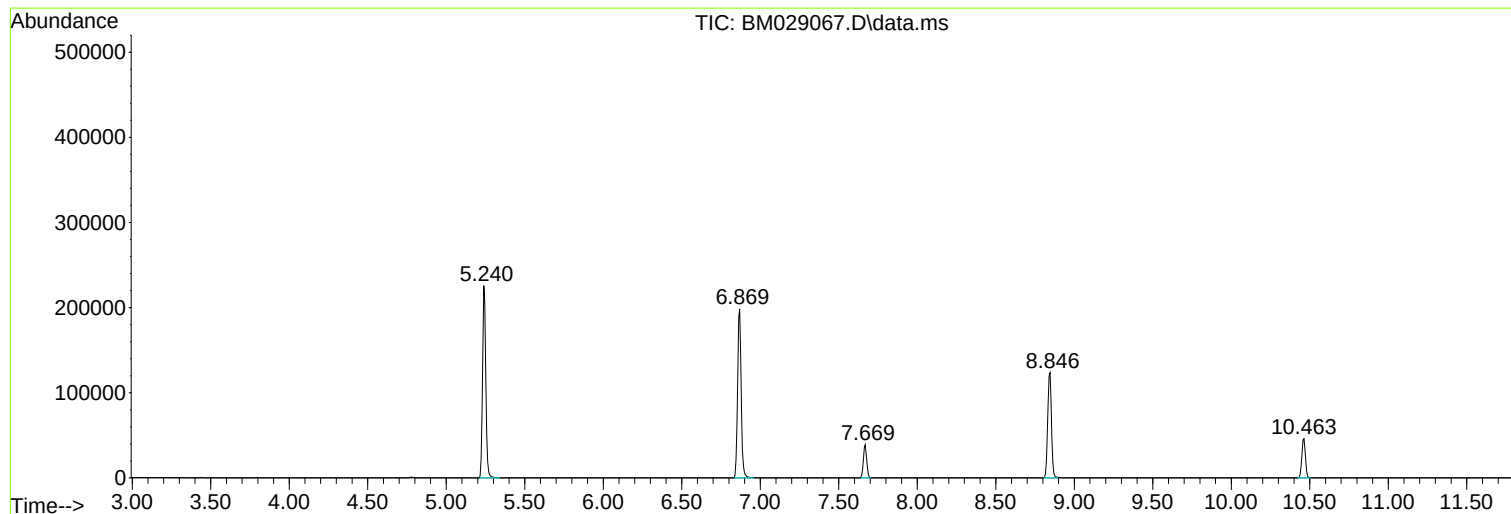

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
Data File : BM029067.D
Acq On : 10 Mar 2021 13:19
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
Data File : BM029067.D
Acq On : 10 Mar 2021 13:19
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------