
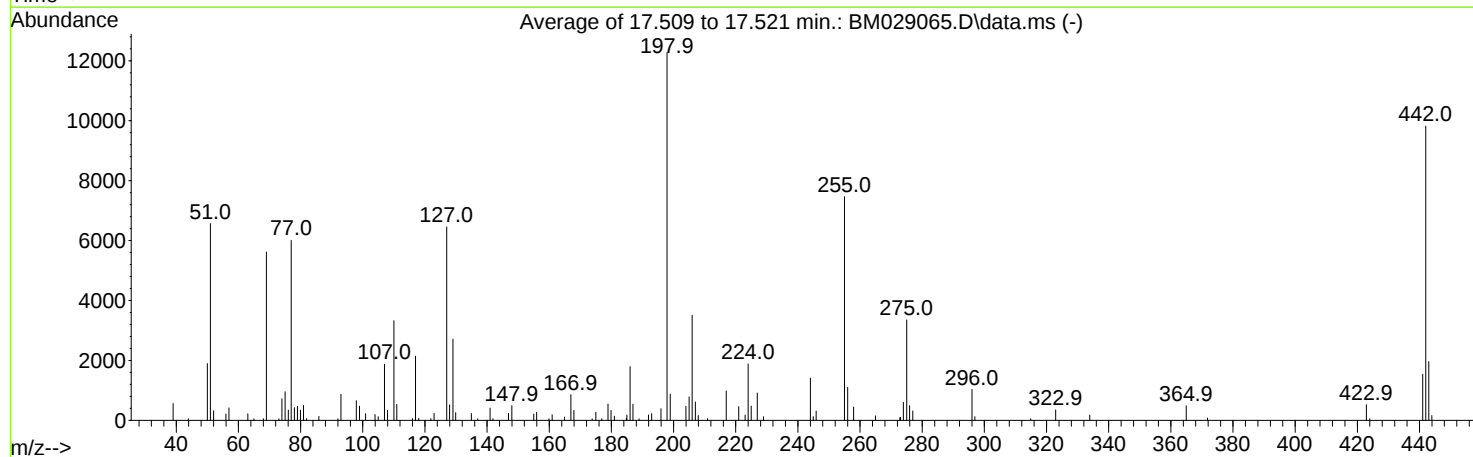


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
 Data File : BM029065.D
 Acq On : 10 Mar 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 09 10:08:02 2021

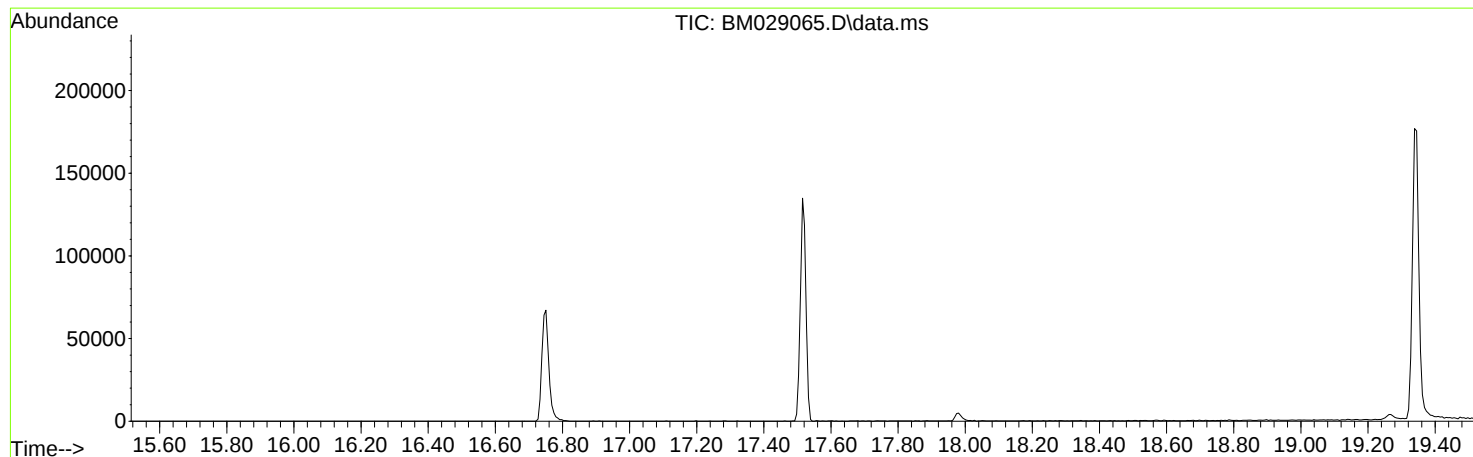

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2464




Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	6566	PASS
68	69	0.00	2	0.9	53	PASS
69	198	0.00	100	45.8	5618	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	6454	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12277	PASS
199	198	5	9	7.1	877	PASS
275	198	10	60	27.3	3356	PASS
365	198	1	100	4.0	487	PASS
441	198	0.01	100	12.5	1537	PASS
442	442	50	100	100.0	9821	PASS
443	442	15	24	20.0	1962	PASS

	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
3/10/2021	BNA_M	<u>BM029065.D</u>
Compound Name	Response	Retention Time
DDT	46579	20.55
DDD	703	20.12
DDE	0	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
703	47282	1.49

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
Data File : BM029065.D
Acq On : 10 Mar 2021 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 10 12:43:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

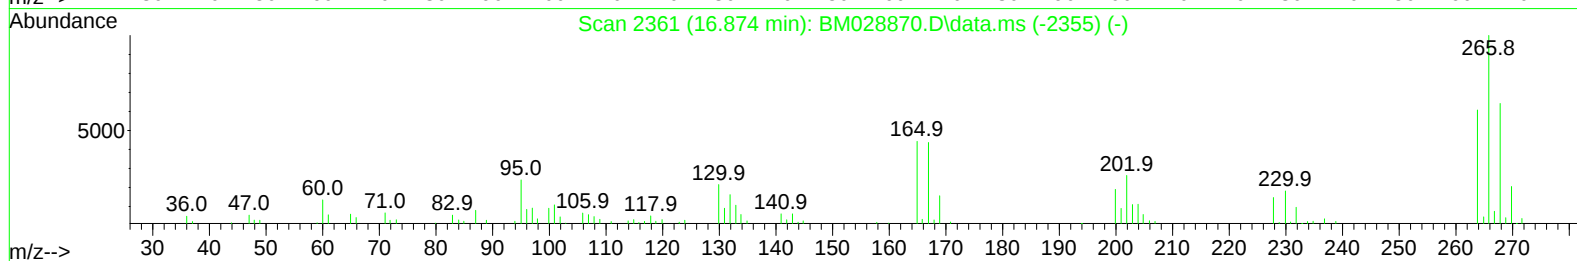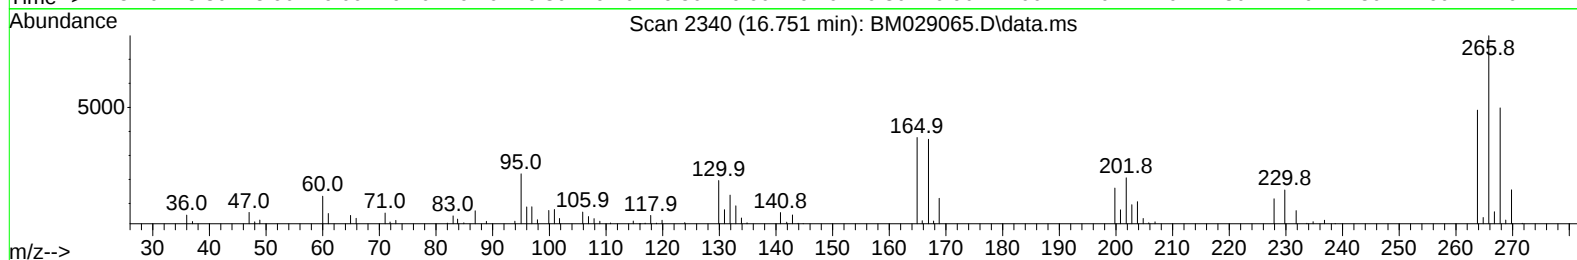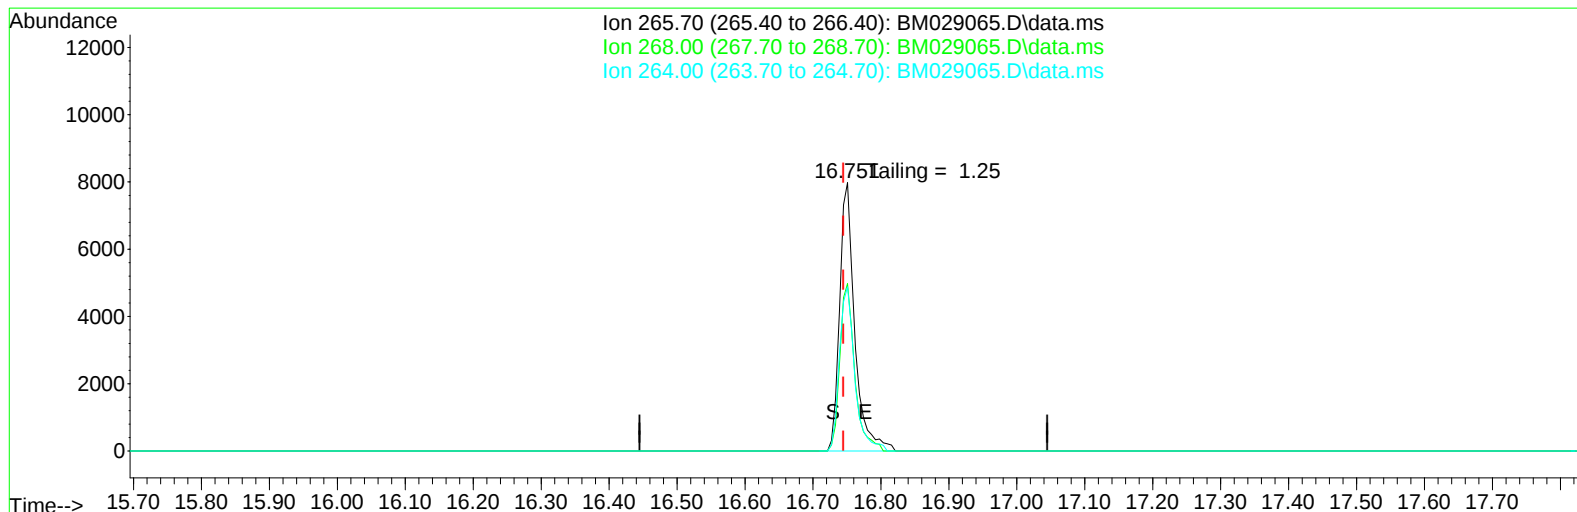

TIC: BM029065.D\data.ms

(70) Pentachlorophenol (C)

16.751min (+ 0.006) 0.00 ng




response 12337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.39
264.00	63.30	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031021\
 Data File : BM029065.D
 Acq On : 10 Mar 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 12:43:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 09 10:08:02 2021
 Response via : Initial Calibration

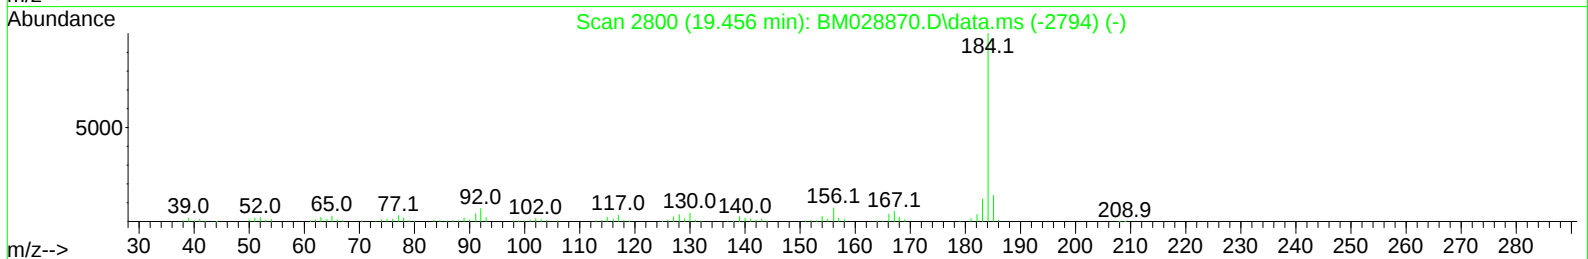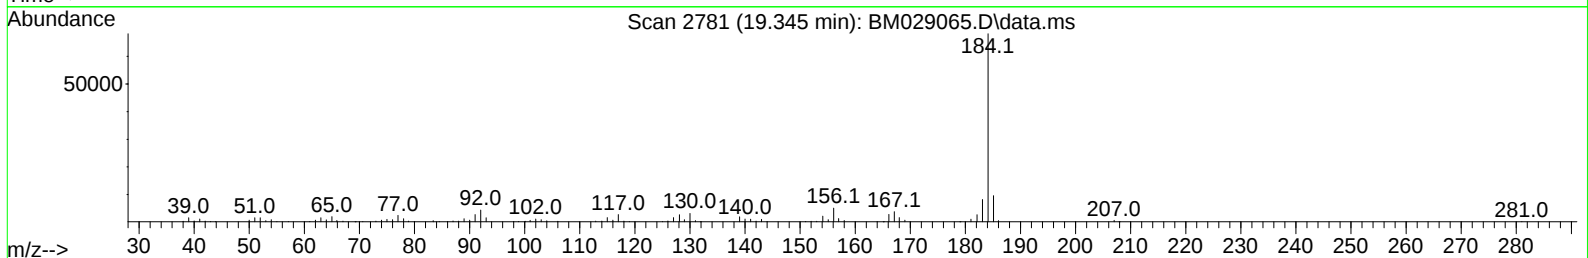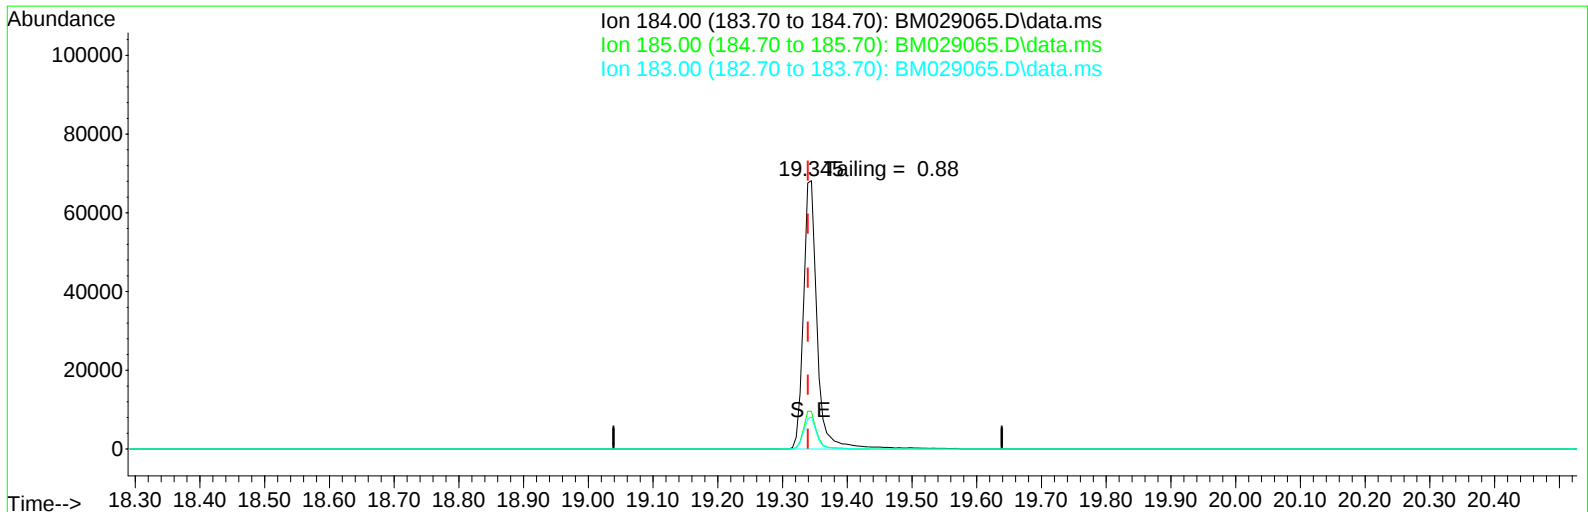

TIC: BM029065.D\data.ms

(77) Benzidine

19.345min (+ 0.006) 0.00 ng

response 100523

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.04
183.00	12.10	12.01
0.00	0.00	0.00