

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031022\
 Data File : BM034205.D
 Acq On : 10 Mar 2022 18:09
 Operator : CG/JU
 Sample : SSTD00546
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046

Quant Time: Mar 11 00:26:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 00:23:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	127742	20.000	ng/u1	0.00
20) Naphthalene-d8	10.766	136	498188	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.595	164	329290	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.330	188	655999	20.000	ng/u1	0.00
79) Chrysene-d12	21.500	240	628436	20.000	ng/u1	0.00
88) Perylene-d12	23.924	264	670904	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.325	96	5987	2.156	ng/uL	0.00
4) Pyridine-d5	3.749	84	30624	3.788	ng/u1	0.00
7) Phenol-d5	7.101	99	33092	3.306	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.272	67	23599	4.380	ng/u1	0.00
11) 2-Chlorophenol-d4	7.478	132	31519	3.799	ng/u1	0.00
15) 4-Methylphenol-d8	8.654	113	28072	3.347	ng/u1	0.00
21) Nitrobenzene-d5	9.113	128	15345	3.975	ng/u1	0.00
24) 2-Nitrophenol-d4	9.842	143	15669	3.737	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.383	165	33978	3.930	ng/u1	0.00
31) 4-Chloroaniline-d4	10.895	131	37310	3.159	ng/u1	0.00
46) Dimethylphthalate-d6	14.001	166	113151	4.528	ng/u1	0.00
49) Acenaphthylene-d8	14.283	160	137295	4.394	ng/u1	0.00
54) 4-Nitrophenol-d4	14.771	143	8519	1.832	ng/u1	0.00
60) Fluorene-d10	15.583	176	100824	4.534	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.689	200	13432	3.173	ng/u1	0.00
73) Anthracene-d10	17.430	188	142505	4.410	ng/u1	0.00
81) Pyrene-d10	19.718	212	155086	4.490	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.765	264	139303	3.914	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.360	88	6138	2.041	ng/uL	90
5) Pyridine	3.772	79	32994	4.036	ng/u1#	93
6) Benzaldehyde	7.084	77	25698	5.003	ng/u1	98
8) Phenol	7.131	94	32543	3.214	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.366	93	32390	4.122	ng/u1	97
12) 2-Chlorophenol	7.513	128	32225	3.760	ng/u1	97
13) 2-Methylphenol	8.395	108	25920	3.283	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.489	45	32895	4.717	ng/u1	97
16) Acetophenone	8.778	105	50101	3.792	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.760	70	25524	4.228	ng/u1	97
18) 4-Methylphenol	8.725	108	29756	3.451	ng/u1	87
19) Hexachloroethane	9.048	117	16459	4.670	ng/u1	95
22) Nitrobenzene	9.154	77	33352	3.821	ng/u1	99
23) Isophorone	9.684	82	67695	4.301	ng/u1	99
25) 2-Nitrophenol	9.872	139	15975	3.497	ng/u1	96
26) 2,4-Dimethylphenol	9.931	107	37266	4.033	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.172	93	41669	4.223	ng/u1#	96
29) 2,4-Dichlorophenol	10.407	162	33828	3.959	ng/u1	100
30) Naphthalene	10.819	128	121195	4.544	ng/u1	99
32) 4-Chloroaniline	10.925	127	36458	3.031	ng/u1	99
33) Hexachlorobutadiene	11.113	225	31718	4.874	ng/u1	98
34) Caprolactam	11.666	113	3238	1.259	ng/u1	89
35) 4-Chloro-3-methylphenol	12.042	107	30410	3.642	ng/u1	98
36) 2-Methylnaphthalene	12.425	142	82081	4.291	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031022\
 Data File : BM034205.D
 Acq On : 10 Mar 2022 18:09
 Operator : CG/JU
 Sample : SSTD00546
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046

Quant Time: Mar 11 00:26:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 00:23:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.642	142	83838	4.277	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.795	216	54043	4.698	ng/ul	99
40) Hexachlorocyclopentadiene	12.777	237	33529	4.318	ng/ul	97
41) 2,4,6-Trichlorophenol	13.030	196	27709	3.946	ng/ul	94
42) 2,4,5-Trichlorophenol	13.095	196	27470	3.547	ng/ul	96
43) 1,1'-Biphenyl	13.430	154	113870	4.441	ng/ul	100
44) 2-Chloronaphthalene	13.472	162	91254	4.529	ng/ul	99
45) 2-Nitroaniline	13.666	65	13331	2.875	ng/ul	94
47) Dimethylphthalate	14.042	163	114107	4.515	ng/ul	99
48) 2,6-Dinitrotoluene	14.160	165	19149	3.812	ng/ul	98
50) Acenaphthylene	14.313	152	137755	4.373	ng/ul	99
51) 3-Nitroaniline	14.489	138	11768	2.561	ng/ul	95
52) Acenaphthene	14.660	153	93871	4.500	ng/ul	98
53) 2,4-Dinitrophenol	14.695	184	6824	2.147	ng/ul	98
55) 4-Nitrophenol	14.783	109	8338	2.068	ng/ul	90
56) Dibenzofuran	14.989	168	136063	4.429	ng/ul	98
57) 2,4-Dinitrotoluene	14.942	165	24203	3.295	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.213	232	26657	3.971	ng/ul	96
59) Diethylphthalate	15.407	149	103622	4.177	ng/ul	99
61) Fluorene	15.636	166	109847	4.346	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.630	204	60529	4.448	ng/ul	99
63) 4-Nitroaniline	15.765	138	71	0.017	ng/ul	91
66) 4,6-Dinitro-2-methylph...	15.707	198	13533	3.166	ng/ul#	94
67) N-Nitrosodiphenylamine	15.842	169	88089	4.503	ng/ul	100
68) 4-Bromophenyl-phenylether	16.524	248	34751	4.845	ng/ul	98
69) Hexachlorobenzene	16.642	284	44742	4.795	ng/ul	98
70) Atrazine	16.789	200	30539	3.856	ng/ul	96
71) Pentachlorophenol	16.983	266	20506	3.463	ng/ul	96
72) Phenanthrene	17.371	178	168509	4.540	ng/ul	100
74) Anthracene	17.465	178	159156	4.244	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.395	216	55093	4.901	ng/uL	97
76) Pentachlorobenzene	14.913	250	53120	5.047	ng/uL	99
77) Carbazole	17.730	167	98982	2.960	ng/ul	100
78) Di-n-butylphthalate	18.301	149	142149	3.900	ng/ul	99
80) Fluoranthene	19.383	202	177232	4.371	ng/ul	98
82) Pyrene	19.748	202	197796	4.716	ng/ul	99
83) Butylbenzylphthalate	20.642	149	57635	4.016	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.424	252	38093	3.117	ng/ul#	94
85) Benzo(a)anthracene	21.489	228	166472	4.018	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.418	149	83953	3.996	ng/ul	99
87) Chrysene	21.542	228	198519	4.905	ng/ul	99
89) Di-n-octyl phthalate	22.347	149	141632	3.398	ng/ul	100
90) Benzo(b)fluoranthene	23.189	252	172677	3.718	ng/ul	100
91) Benzo(k)fluoranthene	23.236	252	177077	4.058	ng/ul	98
93) Benzo(a)pyrene	23.818	252	169440	3.886	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.453	276	158534	3.483	ng/ul	95
95) Dibenzo(a,h)anthracene	26.465	278	126836	3.229	ng/ul	95
96) Benzo(g,h,i)perylene	27.218	276	159406	4.190	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


BNA M

ClientSampleId :

SSTD005046

Quant Time: Mar 11 00:26:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 00:23:33 2022
Response via : Initial Calibration




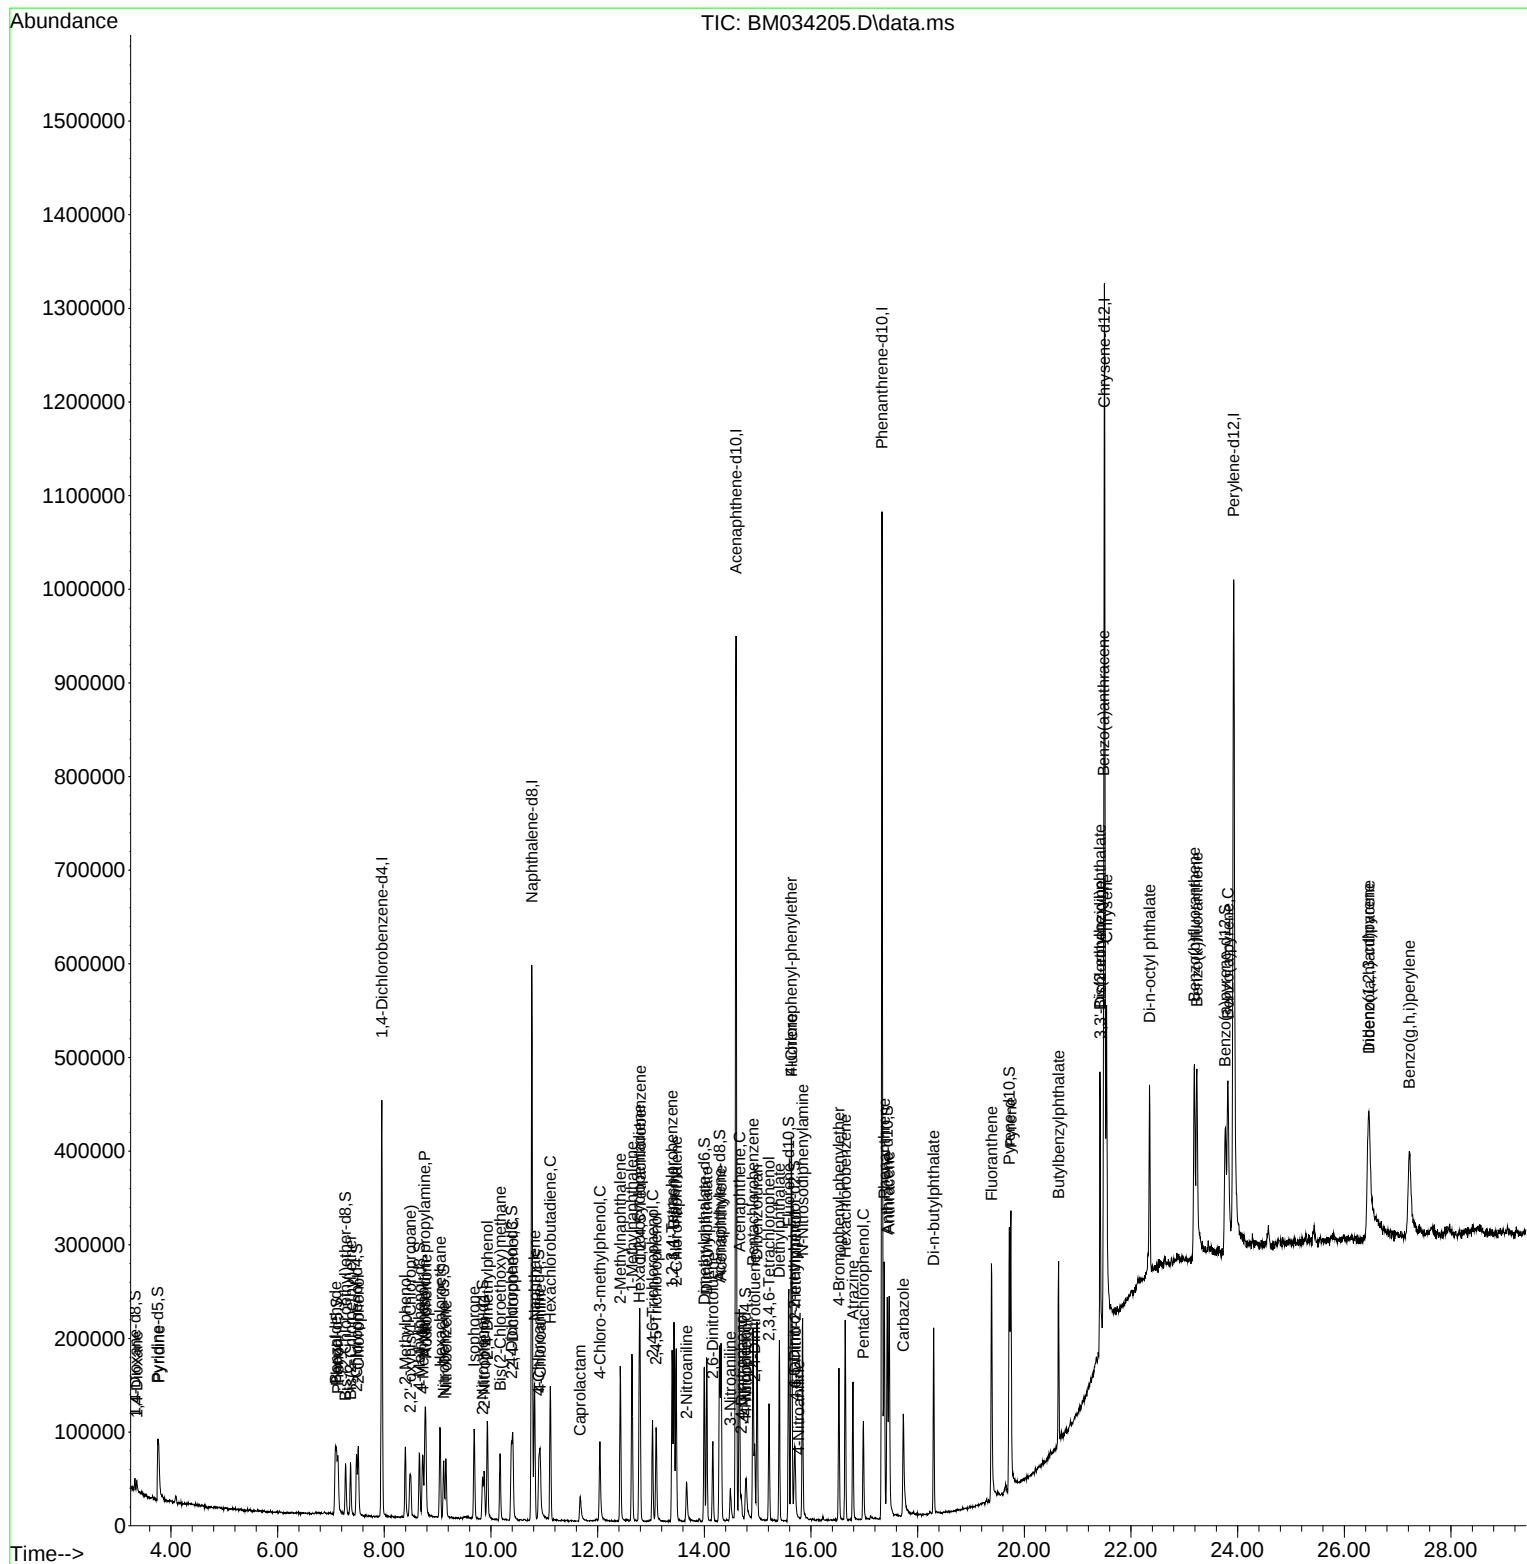




#2
1,4-Dioxane
Concen: 2.041 ng/uL
RT: 3.360 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion: 88 Resp: 6138
Ion Ratio Lower Upper
88 100
43 22.7 21.0 31.6
58 51.0 47.8 71.8

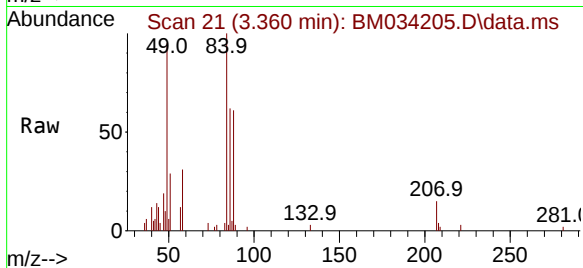

#5
Pyridine
Concen: 4.036 ng/uL
RT: 3.772 min Scan# 91
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion: 79 Resp: 32994
Ion Ratio Lower Upper
79 100
52 62.6 47.7 71.5
51 39.3 25.6 38.4




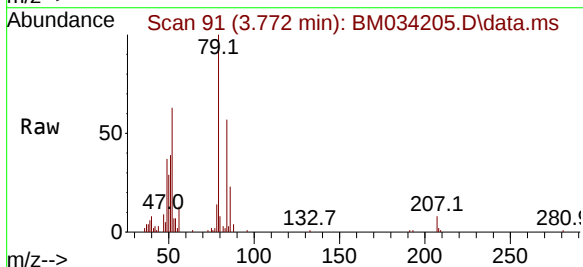




#6
Benzaldehyde
Concen: 5.003 ng/ul
RT: 7.084 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion: 77 Resp: 25698
Ion Ratio Lower Upper
77 100
105 101.9 80.8 121.2
106 98.7 76.6 115.0

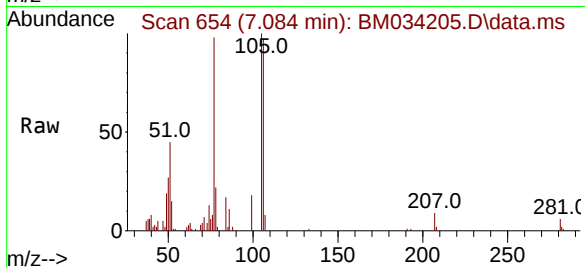

#8
Phenol
Concen: 3.214 ng/ul
RT: 7.131 min Scan# 662
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion: 94 Resp: 32543
Ion Ratio Lower Upper
94 100
65 30.8 22.9 34.3
66 44.9 33.7 50.5




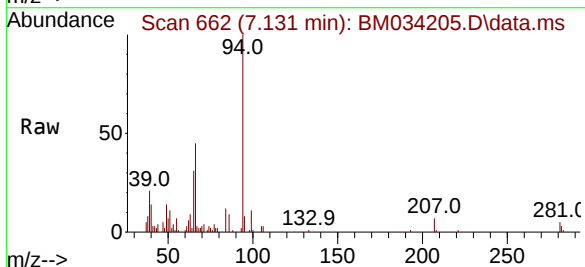




#10
 Bis(2-Chloroethyl)ether
 Concen: 4.122 ng/ul
 RT: 7.366 min Scan# 702
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046


Tgt Ion: 93	Resp:	32390	
Ion	Ratio	Lower	Upper
93	100		
63	71.4	54.7	82.1
95	32.4	26.6	39.8

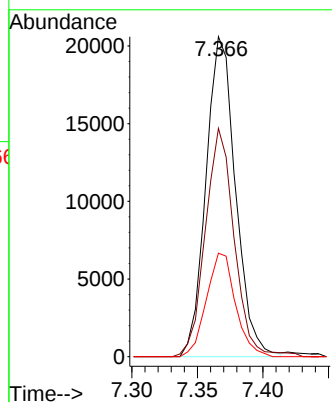

#12
 2-Chlorophenol
 Concen: 3.760 ng/ul
 RT: 7.513 min Scan# 727
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:128	Resp:	32225	
Ion	Ratio	Lower	Upper
128	100		
64	37.3	30.6	46.0
130	34.2	25.8	38.6



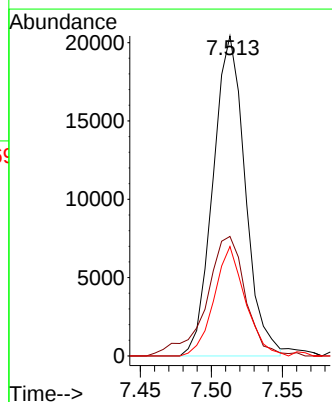



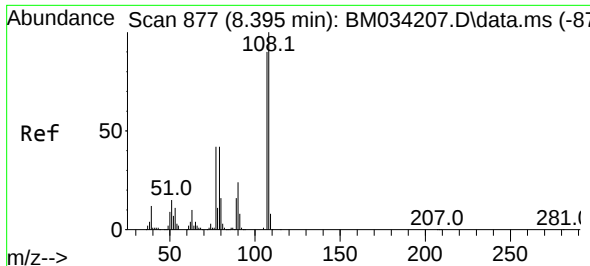

#13
2-Methylphenol
Concen: 3.283 ng/ul
RT: 8.395 min Scan# 877
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:108 Resp: 25920
Ion Ratio Lower Upper
108 100
107 90.6 71.9 107.9

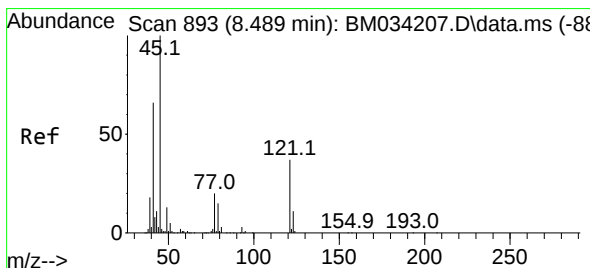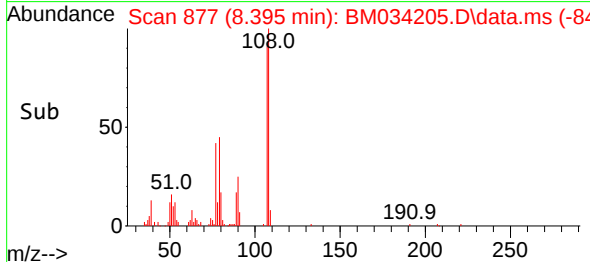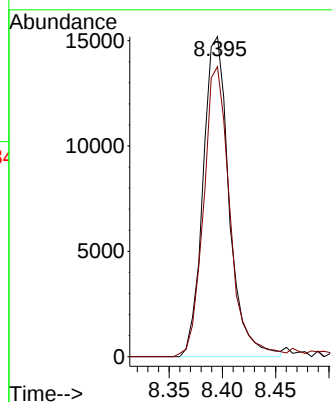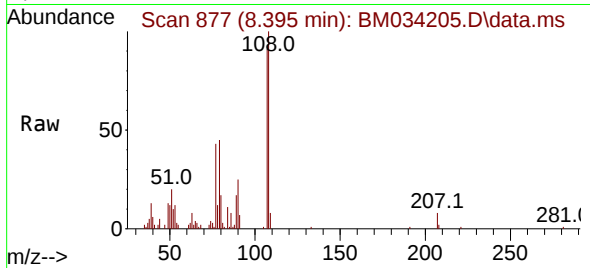

#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.717 ng/ul
RT: 8.489 min Scan# 893
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion: 45 Resp: 32895
Ion Ratio Lower Upper
45 100
77 23.4 17.1 25.7
79 16.5 12.8 19.2


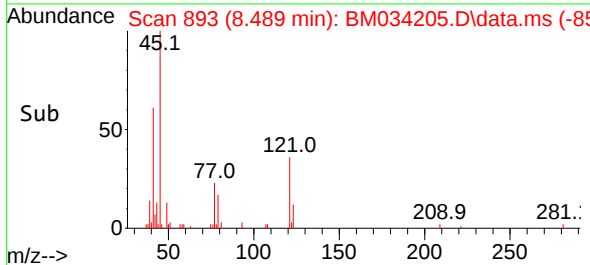

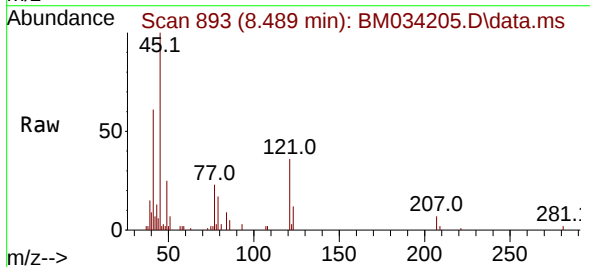




#16
Acetophenone
Concen: 3.792 ng/ul
RT: 8.778 min Scan# 942
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:105 Resp: 50101
Ion Ratio Lower Upper
105 100
77 76.2 59.4 89.2
51 25.0 19.3 28.9



#17
N-Nitroso-di-n-propylamine
Concen: 4.228 ng/ul
RT: 8.760 min Scan# 939
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion: 70 Resp: 25524
Ion Ratio Lower Upper
70 100
42 49.5 40.6 60.8
101 8.7 8.2 12.2
130 22.6 19.9 29.9



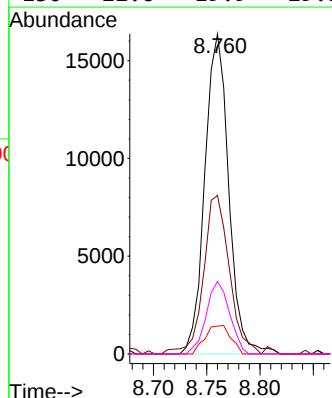





#18
4-Methylphenol
Concen: 3.451 ng/ul
RT: 8.725 min Scan# 91
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:108 Resp: 29756
Ion Ratio Lower Upper
108 100
107 97.2 89.0 133.4

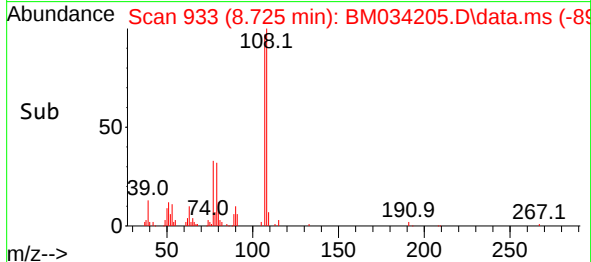

#19
Hexachloroethane
Concen: 4.670 ng/ul
RT: 9.048 min Scan# 988
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:117 Resp: 16459
Ion Ratio Lower Upper
117 100
201 116.2 89.9 134.9
199 77.6 57.2 85.8



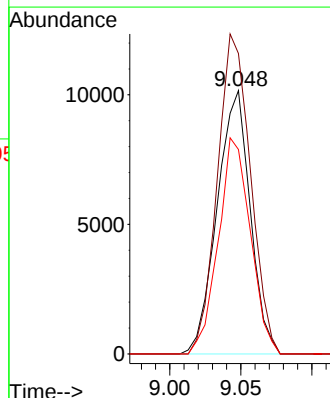





#22
Nitrobenzene
Concen: 3.821 ng/ul
RT: 9.154 min Scan# 1006
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion: 77 Resp: 33352
Ion Ratio Lower Upper
77 100
123 47.5 38.2 57.2
65 12.5 10.6 15.8

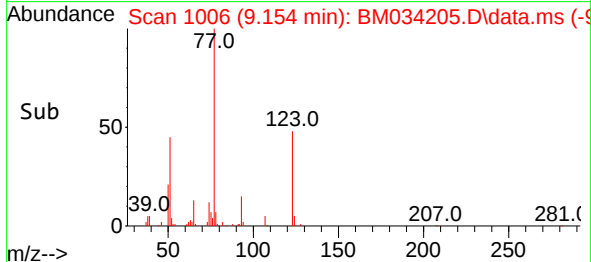

#23
Isophorone
Concen: 4.301 ng/ul
RT: 9.684 min Scan# 1096
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion: 82 Resp: 67695
Ion Ratio Lower Upper
82 100
95 8.5 6.8 10.2
138 20.1 16.5 24.7









#25
2-Nitrophenol
Concen: 3.497 ng/ul
RT: 9.872 min Scan# 1128
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:139 Resp: 15975
Ion Ratio Lower Upper
139 100
65 51.0 37.8 56.6
109 33.8 26.5 39.7

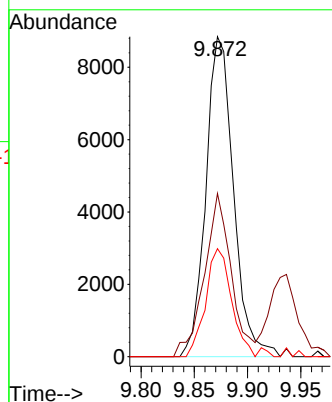

#26
2,4-Dimethylphenol
Concen: 4.033 ng/ul
RT: 9.931 min Scan# 1138
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:107 Resp: 37266
Ion Ratio Lower Upper
107 100
121 51.4 40.8 61.2
122 89.1 69.0 103.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.223 ng/ul
 RT: 10.172 min Scan# 1179
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SST005046


Tgt Ion: 93 Resp: 41669
 Ion Ratio Lower Upper
 93 100
 95 33.2 25.4 38.2
 123 15.1 9.5 14.3#



#29
 2,4-Dichlorophenol
 Concen: 3.959 ng/ul
 RT: 10.407 min Scan# 1219
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion: 162 Resp: 33828
 Ion Ratio Lower Upper
 162 100
 164 65.4 52.8 79.2
 98 32.5 26.0 39.0









#30
Naphthalene
Concen: 4.544 ng/ul
RT: 10.819 min Scan# 1289
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:128 Resp: 121195
Ion Ratio Lower Upper
128 100
129 11.4 8.7 13.1
127 12.5 9.9 14.9

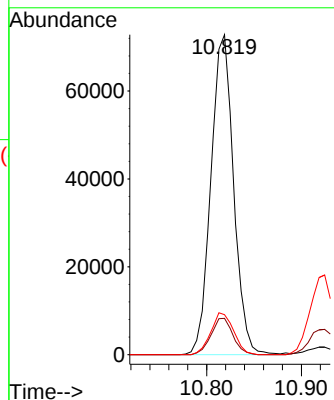

#32
4-Chloroaniline
Concen: 3.031 ng/ul
RT: 10.925 min Scan# 1307
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09


Tgt Ion:127 Resp: 36458
Ion Ratio Lower Upper
127 100
129 31.8 25.1 37.7

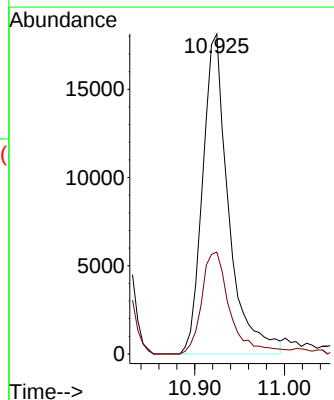






#33
Hexachlorobutadiene
Concen: 4.874 ng/ul
RT: 11.113 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Instrument :
BNA_M
ClientSampleId :
SSTD005046







Tgt Ion:225 Resp: 31718
Ion Ratio Lower Upper
225 100
223 64.3 50.6 75.8
227 61.6 50.3 75.5

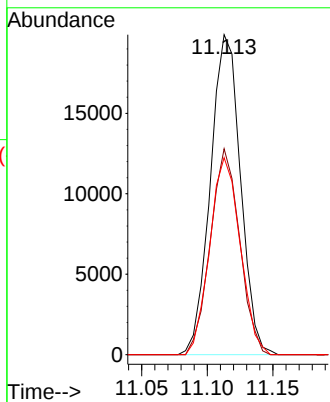

#34
Caprolactam
Concen: 1.259 ng/ul
RT: 11.666 min Scan# 1433
Delta R.T. -0.012 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:113 Resp: 3238
Ion Ratio Lower Upper
113 100
55 117.5 100.9 151.3
56 86.3 81.0 121.4









#35
4-Chloro-3-methylphenol
Concen: 3.642 ng/ul
RT: 12.042 min Scan# 1497
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:107 Resp: 30410
Ion Ratio Lower Upper
107 100
144 30.9 23.0 34.4
142 88.6 69.8 104.8

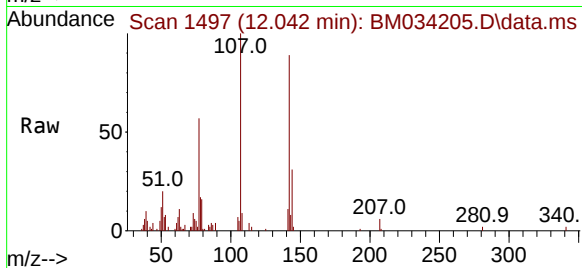

#36
2-Methylnaphthalene
Concen: 4.291 ng/ul
RT: 12.425 min Scan# 1562
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:142 Resp: 82081
Ion Ratio Lower Upper
142 100
141 85.0 71.4 107.0

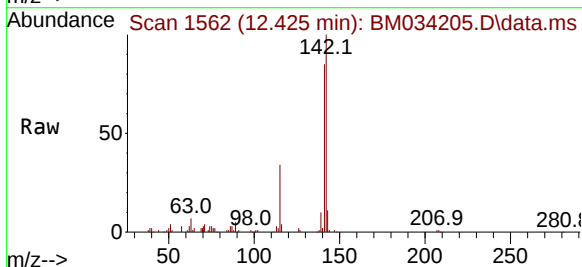



#37

1-Methylnaphthalene

Concen: 4.277 ng/ul

RT: 12.642 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09

Instrument :

BNA_M

ClientSampleId :

SSTD005046





Tgt Ion:142 Resp: 83838

Ion Ratio Lower Upper

142 100

141 93.7 74.5 111.7

116 3.8 3.0 4.6

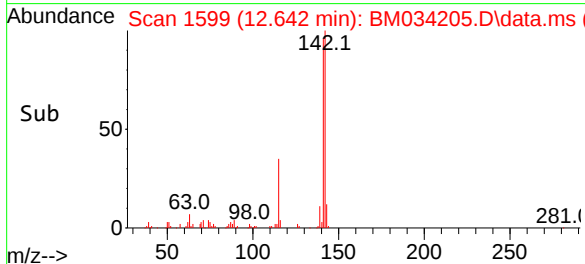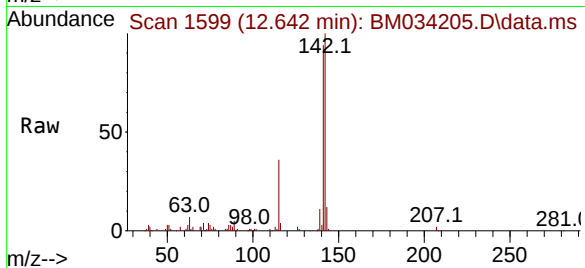

#39

1,2,4,5-Tetrachlorobenzene

Concen: 4.698 ng/ul

RT: 12.795 min Scan# 1625

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09

Tgt Ion:216 Resp: 54043




Ion Ratio Lower Upper


216 100

214 76.8 62.2 93.2

179 19.5 15.4 23.2

108 14.3 11.8 17.6


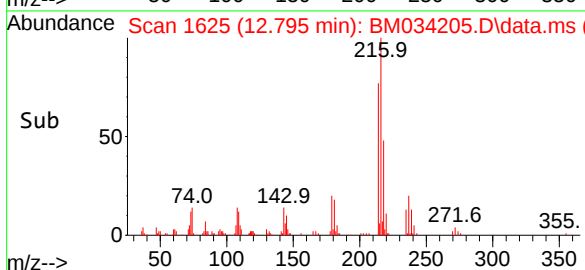
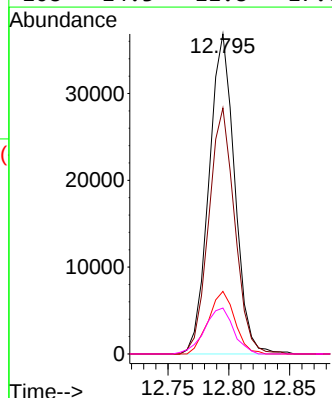
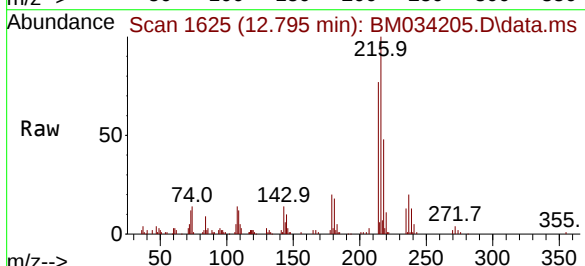




#40
Hexachlorocyclopentadiene
Concen: 4.318 ng/ul
RT: 12.777 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:237 Resp: 33529
Ion Ratio Lower Upper
237 100
235 63.7 52.9 79.3
272 13.6 11.8 17.8

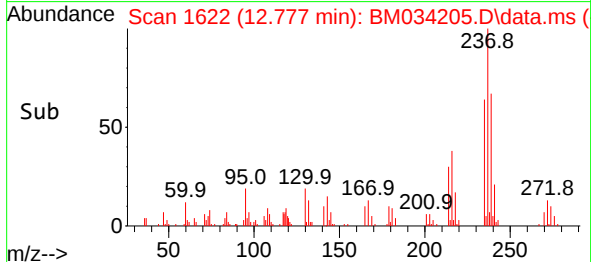

#41
2,4,6-Trichlorophenol
Concen: 3.946 ng/ul
RT: 13.030 min Scan# 1665
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:196 Resp: 27709
Ion Ratio Lower Upper
196 100
198 96.2 80.8 121.2
200 28.5 26.5 39.7









#42
2,4,5-Trichlorophenol
Concen: 3.547 ng/ul
RT: 13.095 min Scan# 1
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:196 Resp: 27470
Ion Ratio Lower Upper
196 100
198 93.6 78.0 117.0
200 33.4 24.5 36.7



#43
1,1'-Biphenyl
Concen: 4.441 ng/ul
RT: 13.430 min Scan# 1733
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:154 Resp: 113870
Ion Ratio Lower Upper
154 100
153 40.6 32.6 49.0
76 9.8 7.7 11.5





#44

2-Chloronaphthalene

Concen: 4.529 ng/ul

RT: 13.472 min Scan# 1740

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09

Instrument :

BNA_M

ClientSampleId :

SSTD005046





Tgt Ion:162 Resp: 91254

Ion Ratio Lower Upper

162 100

164 32.9 26.6 40.0

127 35.7 29.6 44.4

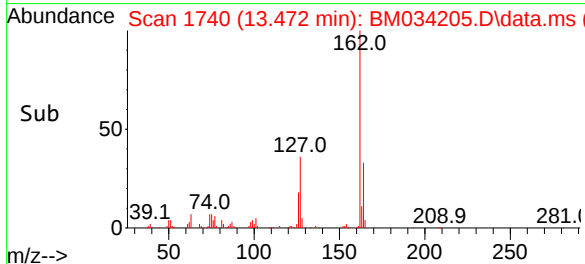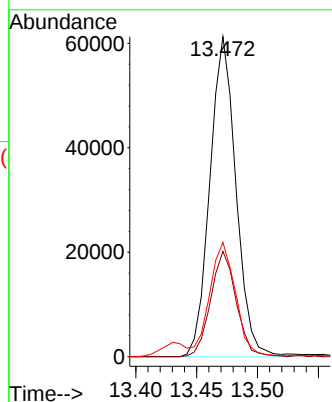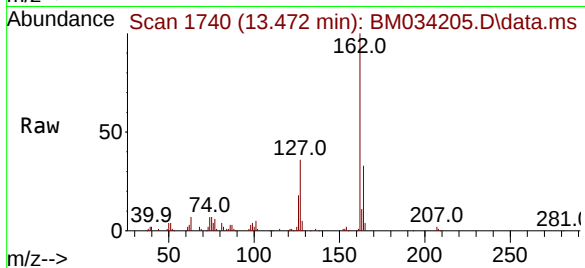

#45

2-Nitroaniline

Concen: 2.875 ng/ul

RT: 13.666 min Scan# 1773

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09




Tgt Ion: 65 Resp: 13331


Ion Ratio Lower Upper

65 100

92 73.7 57.4 86.2

138 128.0 94.8 142.2




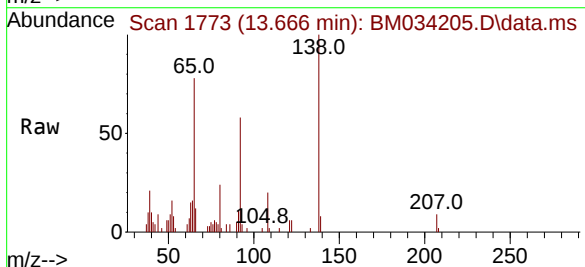




#47
Dimethylphthalate
Concen: 4.515 ng/ul
RT: 14.042 min Scan# 1837
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:163 Resp: 114107
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.2
164 9.6 7.8 11.8

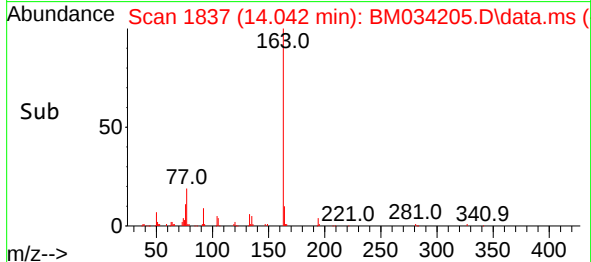

#48
2,6-Dinitrotoluene
Concen: 3.812 ng/ul
RT: 14.160 min Scan# 1857
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:165 Resp: 19149
Ion Ratio Lower Upper
165 100
89 53.0 44.2 66.4
121 20.9 16.7 25.1









#50
Acenaphthylene
Concen: 4.373 ng/ul
RT: 14.313 min Scan# 1884
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:152 Resp: 137755
Ion Ratio Lower Upper
152 100
151 19.2 15.8 23.8
153 13.3 10.2 15.2

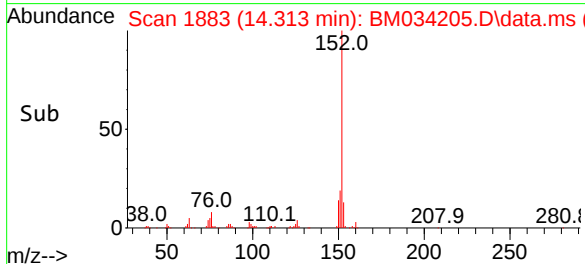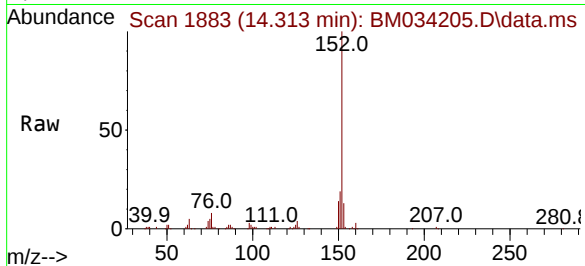

#51
3-Nitroaniline
Concen: 2.561 ng/ul
RT: 14.489 min Scan# 1913
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:138 Resp: 11768
Ion Ratio Lower Upper
138 100
108 9.7 8.3 12.5
92 103.6 87.0 130.4




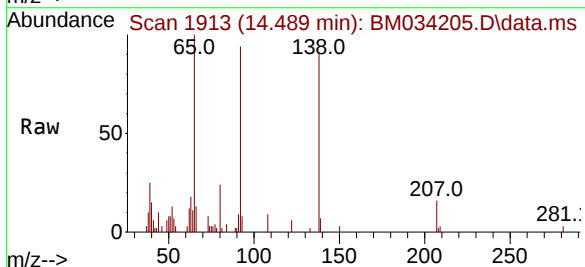




#52
Acenaphthene
Concen: 4.500 ng/ul
RT: 14.660 min Scan# 1942
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:153 Resp: 93871
Ion Ratio Lower Upper
153 100
152 46.0 37.4 56.0
154 86.0 71.0 106.4

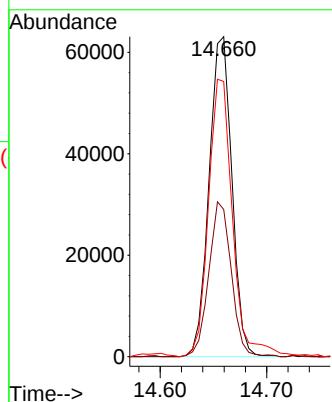

#53
2,4-Dinitrophenol
Concen: 2.147 ng/ul
RT: 14.695 min Scan# 1948
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:184 Resp: 6824
Ion Ratio Lower Upper
184 100
63 55.3 43.8 65.6
154 59.7 49.9 74.9









#55
4-Nitrophenol
Concen: 2.068 ng/ul
RT: 14.783 min Scan# 1963
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:109 Resp: 8338
Ion Ratio Lower Upper
109 100
139 99.5 94.6 142.0
65 106.6 83.5 125.3

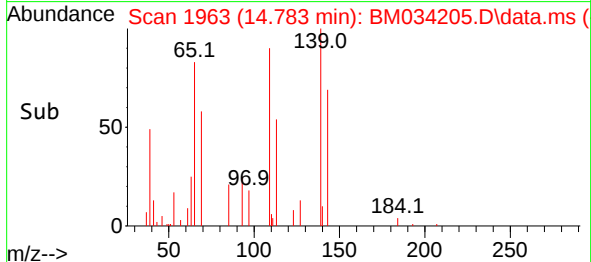

#56
Dibenzofuran
Concen: 4.429 ng/ul
RT: 14.989 min Scan# 1998
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:168 Resp: 136063
Ion Ratio Lower Upper
168 100
139 36.1 29.8 44.6









#57
2,4-Dinitrotoluene
Concen: 3.295 ng/ul
RT: 14.942 min Scan# 1991
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:165	Resp:	24203
Ion Ratio	Lower	Upper
165	100	
63	41.7	30.2 45.4
182	2.8	2.2 3.2

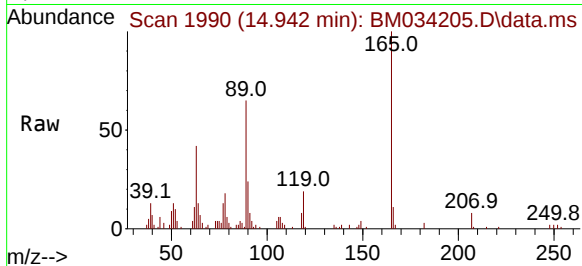

#58
2,3,4,6-Tetrachlorophenol
Concen: 3.971 ng/ul
RT: 15.213 min Scan# 2036
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:232	Resp:	26657
Ion Ratio	Lower	Upper
232	100	
131	37.4	32.2 48.4
130	2.6	1.9 2.9
166	27.2	23.0 34.4




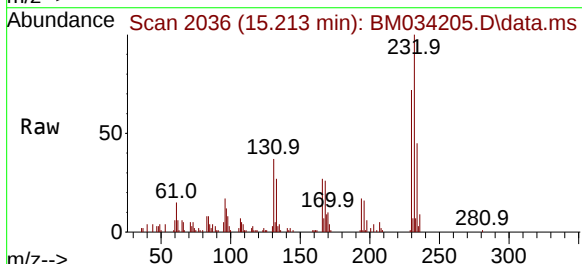




#59
Diethylphthalate
Concen: 4.177 ng/ul
RT: 15.407 min Scan# 2069
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:149 Resp: 103622
Ion Ratio Lower Upper
149 100
177 22.3 17.9 26.9
150 12.2 10.2 15.2

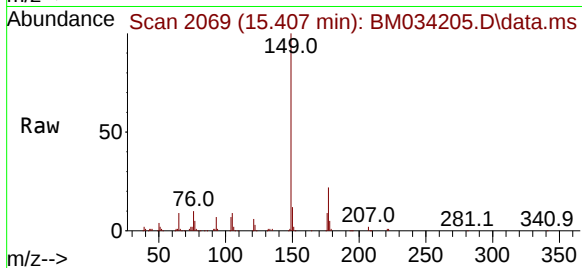

#61
Fluorene
Concen: 4.346 ng/ul
RT: 15.636 min Scan# 2108
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:166 Resp: 109847
Ion Ratio Lower Upper
166 100
165 94.6 76.9 115.3
167 12.8 10.8 16.2




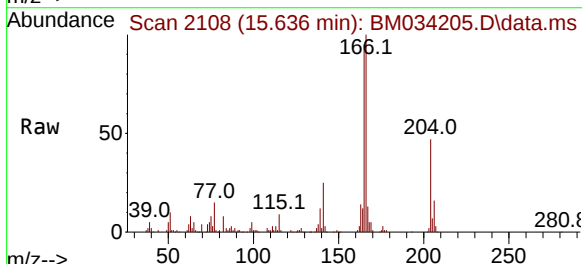




#62
4-Chlorophenyl-phenylether
Concen: 4.448 ng/ul
RT: 15.630 min Scan# 2107
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:204 Resp: 60529
Ion Ratio Lower Upper
204 100
206 30.4 25.5 38.3
141 55.3 44.2 66.2

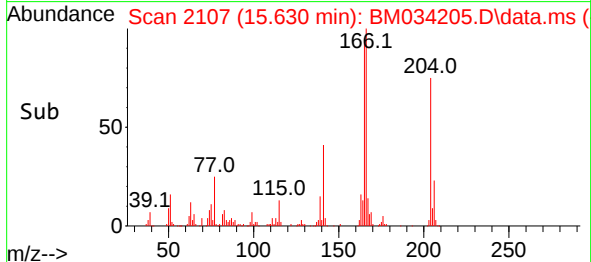

#63
4-Nitroaniline
Concen: 0.017 ng/ul
RT: 15.765 min Scan# 2130
Delta R.T. 0.118 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:138 Resp: 71
Ion Ratio Lower Upper
138 100
92 43.8 36.3 54.5
108 74.6 68.9 103.3









#66
 4,6-Dinitro-2-methylphenol
 Concen: 3.166 ng/ul
 RT: 15.707 min Scan# 2120
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SST005046


Tgt Ion:198 Resp: 13533
 Ion Ratio Lower Upper
 198 100
 182 7.8 3.8 5.6#
 77 20.2 18.5 27.7

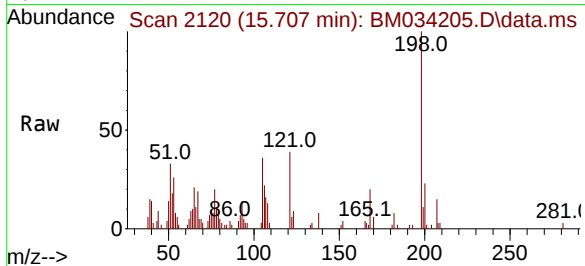

#67
 N-Nitrosodiphenylamine
 Concen: 4.503 ng/ul
 RT: 15.842 min Scan# 2143
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:169 Resp: 88089
 Ion Ratio Lower Upper
 169 100
 168 65.8 52.8 79.2
 167 35.5 28.1 42.1




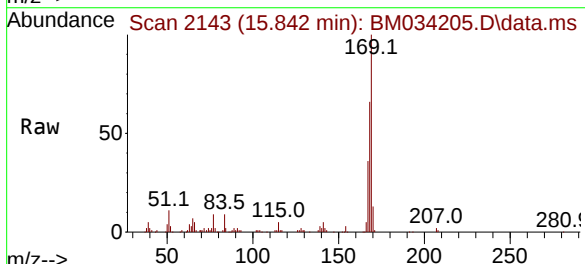




#68
4-Bromophenyl-phenylether
Concen: 4.845 ng/ul
RT: 16.524 min Scan# 2259
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:248 Resp: 34751
Ion Ratio Lower Upper
248 100
250 97.0 78.4 117.6
141 62.3 51.4 77.2

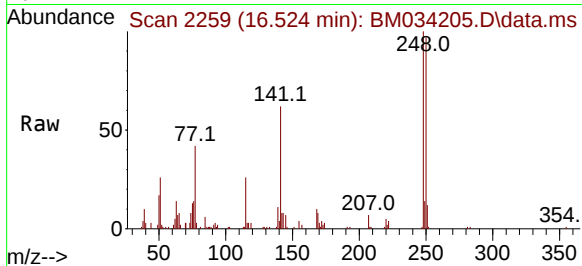

#69
Hexachlorobenzene
Concen: 4.795 ng/ul
RT: 16.642 min Scan# 2279
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:284 Resp: 44742
Ion Ratio Lower Upper
284 100
142 29.4 24.6 36.8
249 29.5 24.1 36.1

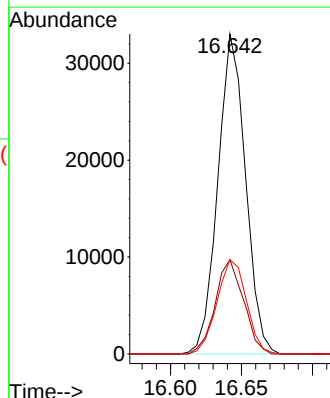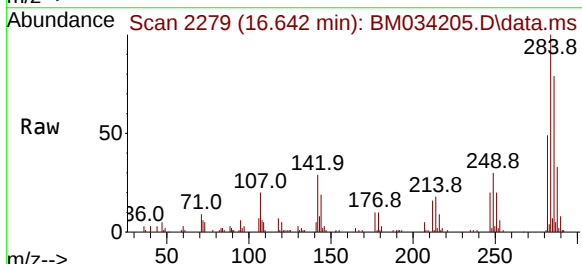



#70

Atrazine

Concen: 3.856 ng/ul

RT: 16.789 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09

Instrument :

BNA_M

ClientSampleId :

SSTD005046





Tgt Ion:200 Resp: 30539

Ion Ratio Lower Upper

200 100

173 24.3 20.2 30.4

215 51.3 38.4 57.6

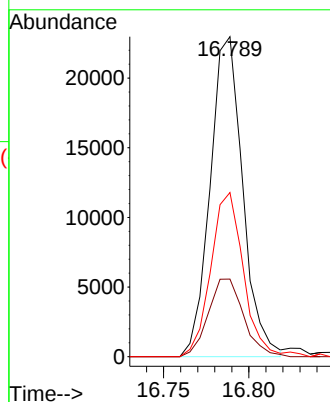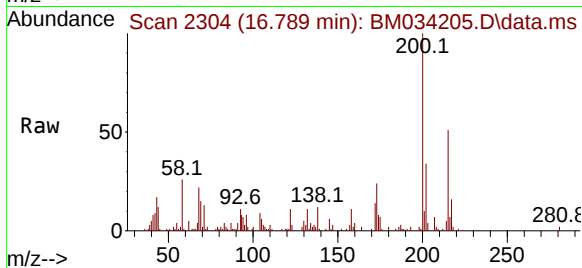

#71

Pentachlorophenol

Concen: 3.463 ng/ul

RT: 16.983 min Scan# 2337

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09




Tgt Ion:266 Resp: 20506


Ion Ratio Lower Upper

266 100

264 63.3 49.3 73.9

268 67.2 50.3 75.5




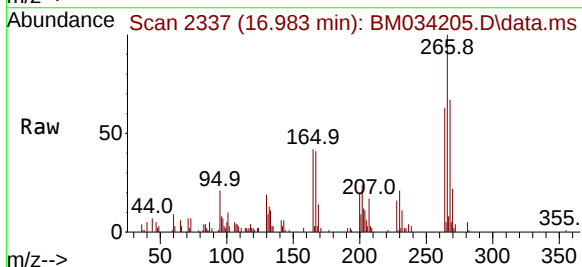




#72
Phenanthrene
Concen: 4.540 ng/ul
RT: 17.371 min Scan# 2403
Delta R.T. -0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:178 Resp: 168509
Ion Ratio Lower Upper
178 100
179 14.9 11.7 17.5
176 18.9 15.0 22.4

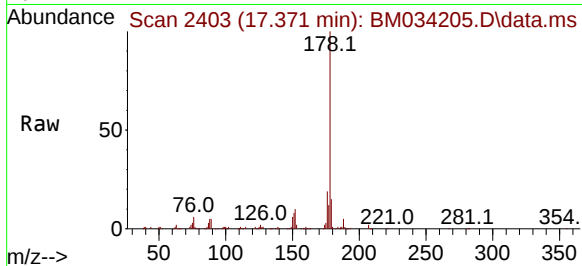

#74
Anthracene
Concen: 4.244 ng/ul
RT: 17.465 min Scan# 2419
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:178 Resp: 159156
Ion Ratio Lower Upper
178 100
179 15.5 11.9 17.9
176 18.7 14.4 21.6

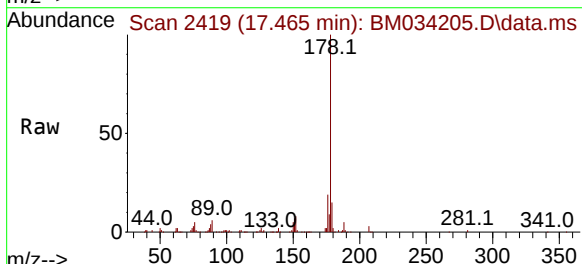



#75

1,2,3,4-Tetrachlorobenzene

Concen: 4.901 ng/uL

RT: 13.395 min Scan# 1727

Delta R.T. -0.006 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09

Instrument :

BNA_M

ClientSampleId :

SSTD005046





Tgt Ion:216 Resp: 55093

Ion Ratio Lower Upper

216 100

214 80.0 62.0 93.0

218 48.5 37.8 56.8

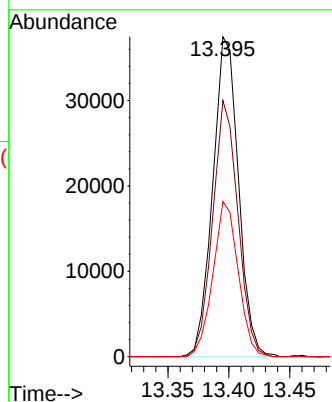

#76

Pentachlorobenzene

Concen: 5.047 ng/uL

RT: 14.913 min Scan# 1985

Delta R.T. 0.000 min

Lab File: BM034205.D

Acq: 10 Mar 2022 18:09




Tgt Ion:250 Resp: 53120


Ion Ratio Lower Upper

250 100

248 63.6 50.6 75.8

252 60.9 50.2 75.4



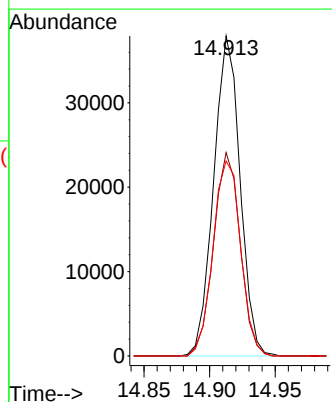





#77
 Carbazole
 Concen: 2.960 ng/ul
 RT: 17.730 min Scan# 2464
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046


Tgt Ion:167 Resp: 98982
 Ion Ratio Lower Upper
 167 100
 166 20.8 16.6 25.0
 139 12.6 9.9 14.9

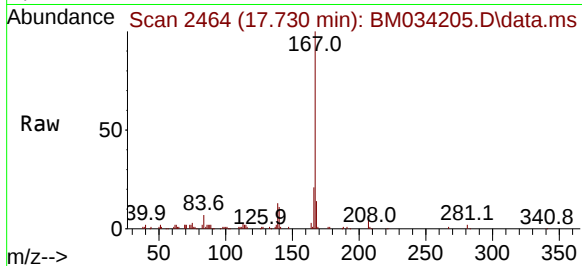

#78
 Di-n-butylphthalate
 Concen: 3.900 ng/ul
 RT: 18.301 min Scan# 2561
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:149 Resp: 142149
 Ion Ratio Lower Upper
 149 100
 150 8.8 7.4 11.0
 104 4.9 4.2 6.2




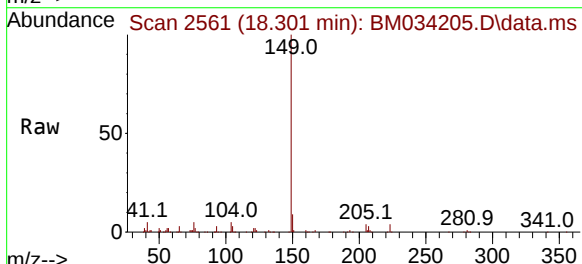




#80
 Fluoranthene
 Concen: 4.371 ng/ul
 RT: 19.383 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SST005046


Tgt Ion:202 Resp: 177232
 Ion Ratio Lower Upper
 202 100
 101 8.2 6.2 9.2
 100 6.5 4.7 7.1

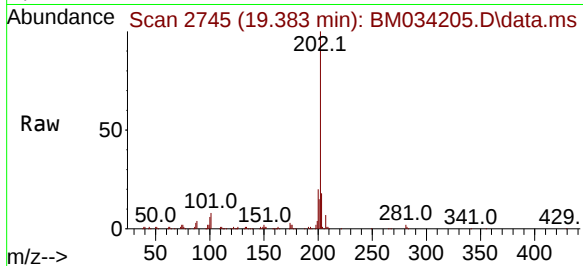

#82
 Pyrene
 Concen: 4.716 ng/ul
 RT: 19.748 min Scan# 2807
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:202 Resp: 197796
 Ion Ratio Lower Upper
 202 100
 101 8.3 7.0 10.4
 100 7.8 5.8 8.6




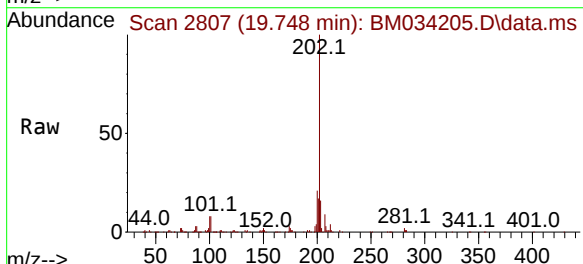




#83
Butylbenzylphthalate
Concen: 4.016 ng/ul
RT: 20.642 min Scan# 2959
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:149 Resp: 57635
Ion Ratio Lower Upper
149 100
91 62.1 50.9 76.3
206 26.9 19.3 28.9

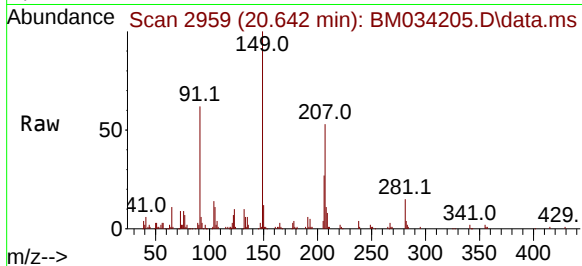

#84
3,3'-Dichlorobenzidine
Concen: 3.117 ng/ul
RT: 21.424 min Scan# 3092
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:252 Resp: 38093
Ion Ratio Lower Upper
252 100
254 58.7 50.7 76.1
126 10.0 6.6 9.8




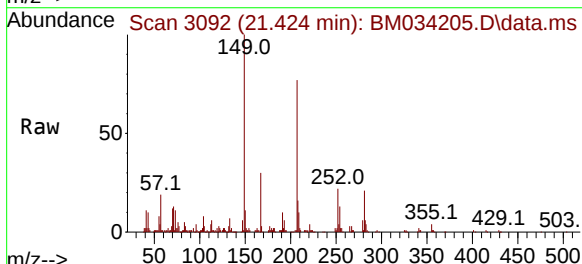




#85
 Benzo(a)anthracene
 Concen: 4.018 ng/ul
 RT: 21.489 min Scan# 3103
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09




Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046


Tgt Ion:228 Resp: 166472
 Ion Ratio Lower Upper
 228 100
 229 19.6 15.4 23.2
 226 25.1 21.0 31.4



#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.996 ng/ul
 RT: 21.418 min Scan# 3091
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:149 Resp: 83953
 Ion Ratio Lower Upper
 149 100
 167 28.4 22.1 33.1
 279 4.7 4.2 6.2



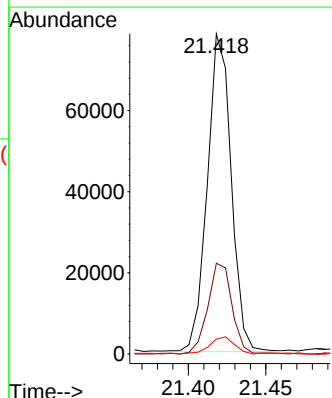





#87
Chrysene
Concen: 4.905 ng/ul
RT: 21.542 min Scan# 3112
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:228 Resp: 198519
Ion Ratio Lower Upper
228 100
226 30.0 23.4 35.2
229 19.4 15.4 23.0



#89
Di-n-octyl phthalate
Concen: 3.398 ng/ul
RT: 22.347 min Scan# 3249
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:149 Resp: 141632









#90
Benzo(b)fluoranthene
Concen: 3.718 ng/ul
RT: 23.189 min Scan# 31
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:252 Resp: 172677
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.0
125 7.1 5.8 8.6



#91
Benzo(k)fluoranthene
Concen: 4.058 ng/ul
RT: 23.236 min Scan# 3400
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:252 Resp: 177077
Ion Ratio Lower Upper
252 100
253 23.0 17.5 26.3
125 6.9 5.1 7.7









#93
Benzo(a)pyrene
Concen: 3.886 ng/ul
RT: 23.818 min Scan# 3499
Delta R.T. 0.000 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09




Instrument :
BNA_M
ClientSampleId :
SSTD005046


Tgt Ion:252 Resp: 169440
Ion Ratio Lower Upper
252 100
253 20.6 17.5 26.3
125 8.1 6.2 9.4

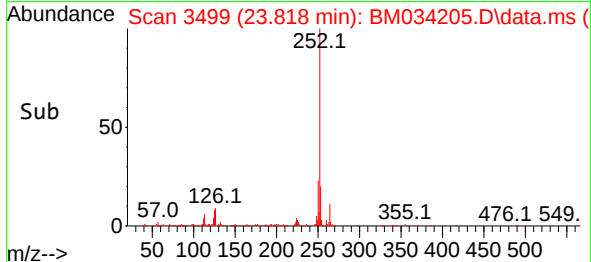

#94
Indeno(1,2,3-cd)pyrene
Concen: 3.483 ng/ul
RT: 26.453 min Scan# 3947
Delta R.T. 0.006 min
Lab File: BM034205.D
Acq: 10 Mar 2022 18:09

Tgt Ion:276 Resp: 158534
Ion Ratio Lower Upper
276 100
138 15.4 13.6 20.4
277 22.0 19.9 29.9









#95
 Dibenzo(a,h)anthracene
 Concen: 3.229 ng/ul
 RT: 26.465 min Scan# 3949
 Delta R.T. 0.000 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Instrument :
 BNA_M
 ClientSampleId :
 SSTD005046

Tgt Ion:278 Resp: 126836
 Ion Ratio Lower Upper
 278 100
 139 13.9 9.6 14.4
 279 26.9 19.3 28.9



#96
 Benzo(g,h,i)perylene
 Concen: 4.190 ng/ul
 RT: 27.218 min Scan# 4077
 Delta R.T. -0.006 min
 Lab File: BM034205.D
 Acq: 10 Mar 2022 18:09

Tgt Ion:276 Resp: 159406
 Ion Ratio Lower Upper
 276 100
 138 15.0 11.8 17.6
 277 22.7 18.8 28.2

