


Data Path : Z:\HPCHEM1\BNA_M\Data\BM031115\
 Data File : BM000682.D
 Acq On : 10 Mar 2015 20:56
 Operator : TP/IZ
 Sample : DFTPP34
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP34

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\Methods\SOM02.2-EPA-BM031115.M
 Title : SVOA CALIBRATION
 Last Update : Thu Mar 12 07:14:19 2015

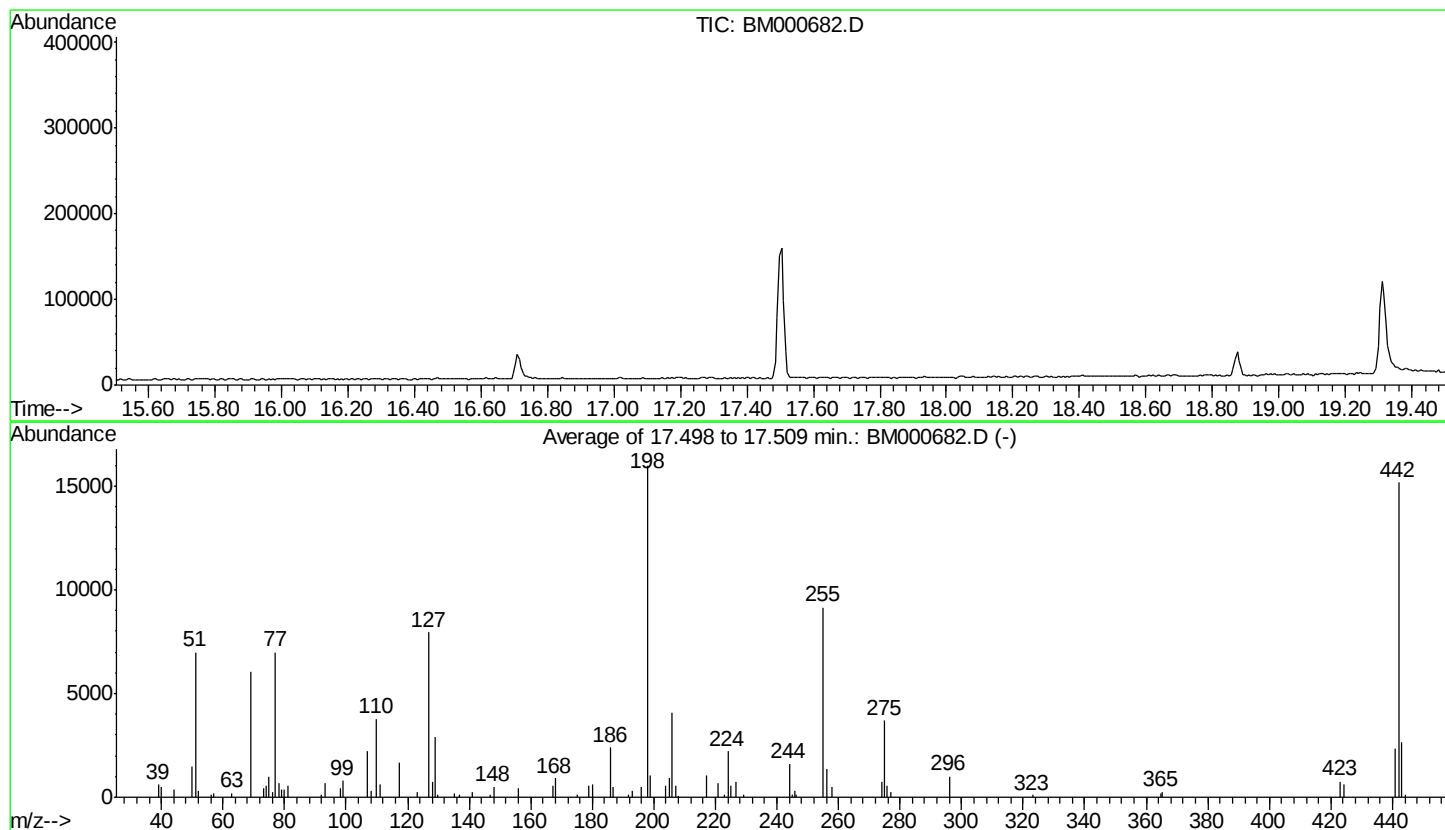

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	6984	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.8	6044	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	7945	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15991	PASS
199	198	5	9	6.7	1064	PASS
275	198	10	60	23.1	3690	PASS
365	198	1	100	1.7	266	PASS
441	443	0.01	100	87.6	2338	PASS
442	198	50	100	94.9	15169	PASS
443	442	15	24	17.6	2668	PASS

m/z	Abundance
39.00	691.0
40.00	3377.0
44.00	4088.0
50.00	1827.0
51.10	8243.0
52.00	514.0
56.00	341.0
57.00	582.0
63.00	303.0
69.00	7604.0
73.00	340.0
74.10	611.0
75.00	1329.0
76.10	428.0
77.00	8751.0
78.00	868.0
78.90	619.0
79.90	553.0
81.00	675.0
91.80	323.0
93.00	1100.0
98.00	659.0
99.00	822.0
107.00	2653.0
108.00	598.0
110.00	4634.0
111.10	734.0
117.10	2146.0
123.00	363.0
127.00	9469.0
128.00	903.0
129.00	3179.0
129.90	321.0
141.00	348.0
146.90	373.0
148.00	523.0
156.00	302.0
167.00	709.0
168.00	1154.0
178.90	720.0
180.00	731.0
186.00	2586.0
186.80	838.0
193.00	303.0
195.90	699.0
198.00	17968.0
199.00	1120.0
204.00	678.0
205.10	1160.0
206.10	4320.0
207.00	1989.0
207.90	438.0
217.00	961.0
221.10	788.0
224.10	2301.0
225.10	494.0
226.80	861.0
244.00	1708.0
245.90	522.0
255.00	9345.0
256.10	1423.0
258.00	493.0
274.10	709.0
275.00	3714.0
276.00	575.0
277.10	301.0
295.90	1003.0
323.00	310.0
365.10	429.0
423.00	575.0
424.00	644.0
441.00	2396.0
442.00	12998.0
443.10	2348.0

Instrument :
BNA_M
ClientSampleId :
DFTPP34

m/z	Abundance
39.00	649.0
40.00	3526.0
44.00	3580.0
50.10	1629.0
51.10	8049.0
52.10	373.0
63.00	309.0
69.00	6990.0
73.00	502.0
74.00	664.0
75.00	1182.0
75.90	385.0
77.10	8014.0
78.00	833.0
78.90	439.0
80.00	529.0
81.00	637.0
93.00	561.0
98.00	656.0
99.00	1048.0
107.10	2682.0
108.00	370.0
110.00	4192.0
111.00	703.0
117.10	1592.0
123.00	419.0
127.00	9298.0
127.90	925.0
129.00	3284.0
135.00	484.0
137.00	340.0
141.00	449.0
148.00	643.0
156.00	595.0
167.00	536.0
168.00	1100.0
174.90	445.0
178.90	602.0
180.00	671.0
186.00	2937.0
186.90	669.0
191.80	305.0
192.90	397.0
196.00	360.0
198.00	18488.0
199.00	1466.0
204.00	709.0
205.10	939.0
206.00	4493.0
207.10	1820.0
208.00	318.0
217.00	1224.0
220.90	810.0
222.80	321.0
224.10	2547.0
225.00	745.0
226.90	927.0
229.00	427.0
244.10	1951.0
245.90	384.0
255.00	11208.0
256.00	1630.0
257.90	502.0
274.00	907.0
275.00	4524.0
275.90	609.0
276.90	374.0
296.00	1217.0
365.00	369.0
423.00	878.0
424.10	790.0
441.10	2609.0
442.00	18912.0
443.00	3209.0
444.00	330.0

Instrument :
BNA_M
ClientSampleId :
DFTPP34

m/z	Abundance
38.90	501.0
40.00	3373.0
44.00	3678.0
50.00	928.0
51.00	4661.0
68.90	3538.0
73.10	408.0
74.00	382.0
75.00	531.0
77.10	4207.0
78.00	427.0
80.80	390.0
92.90	340.0
99.10	533.0
106.90	1342.0
110.00	2503.0
110.90	389.0
117.10	1197.0
127.00	5068.0
127.90	327.0
128.90	2201.0
148.10	331.0
155.90	377.0
167.00	514.0
167.80	497.0
178.90	391.0
180.00	507.0
186.00	1620.0
193.00	302.0
195.90	473.0
198.00	11518.0
199.00	607.0
204.10	372.0
205.00	730.0
206.10	3349.0
207.10	1591.0
208.00	402.0
216.90	888.0
221.00	378.0
224.00	1742.0
225.00	456.0
226.90	478.0
244.00	1187.0
245.10	338.0
246.10	304.0
255.00	6939.0
256.00	1065.0
258.00	465.0
274.00	527.0
275.00	2833.0
276.00	476.0
295.90	825.0
364.80	508.0
423.00	802.0
424.00	470.0
441.00	2010.0
442.10	13599.0
443.10	2449.0

Instrument :
BNA_M
ClientSampleId :
DFTPP34

Scan 2513 (17.468 min): BM000682.D
DFTPP34

m/z	Abundance
40.00	2935.0
44.00	3408.0
207.10	1264.0
208.10	303.0

Instrument :
BNA_M
ClientSampleId :
DFTPP34