

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
 Data File : BM029087.D
 Acq On : 11 Mar 2021 10:05
 Operator : CG/JU
 Sample : PB135092BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135092BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	377	382	398	rBV	204614	303534	53.66%	11.941%
2	6.863	653	659	673	rBV	184588	293806	51.94%	11.558%
3	7.663	790	795	802	rBB	36955	54260	9.59%	2.135%
4	8.839	989	995	1009	rBV	117548	189764	33.55%	7.465%
5	10.457	1264	1270	1279	rBB	42994	69375	12.26%	2.729%
6	12.945	1686	1693	1701	rBV	269244	380583	67.28%	14.972%
7	14.333	1923	1929	1937	rBB	56978	83087	14.69%	3.269%
8	15.833	2178	2184	2198	rBB	199380	278519	49.24%	10.957%
9	17.080	2390	2396	2407	rBB	69924	94388	16.69%	3.713%
10	19.703	2837	2842	2847	rBV	467246	565679	100.00%	22.254%
11	21.250	3101	3105	3111	rBV	90771	111634	19.73%	4.392%
12	23.409	3466	3472	3482	rBV	64042	117307	20.74%	4.615%




Sum of corrected areas: 2541936

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
Data File : BM029087.D
Acq On : 11 Mar 2021 10:05
Operator : CG/JU
Sample : PB135092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135092BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

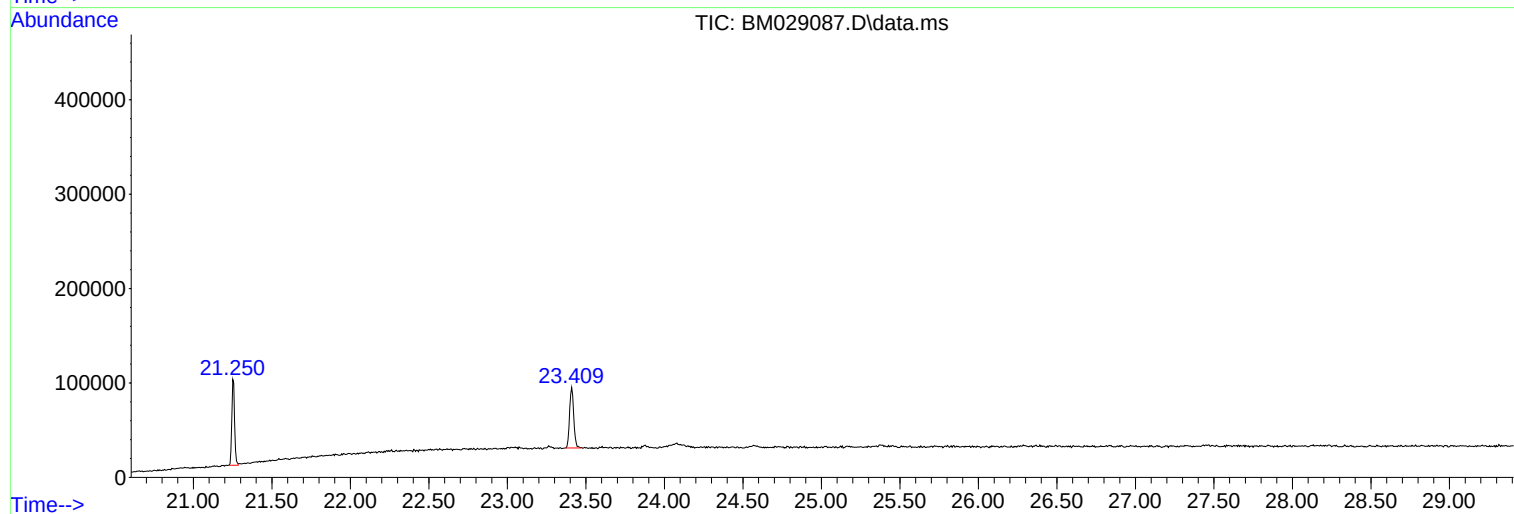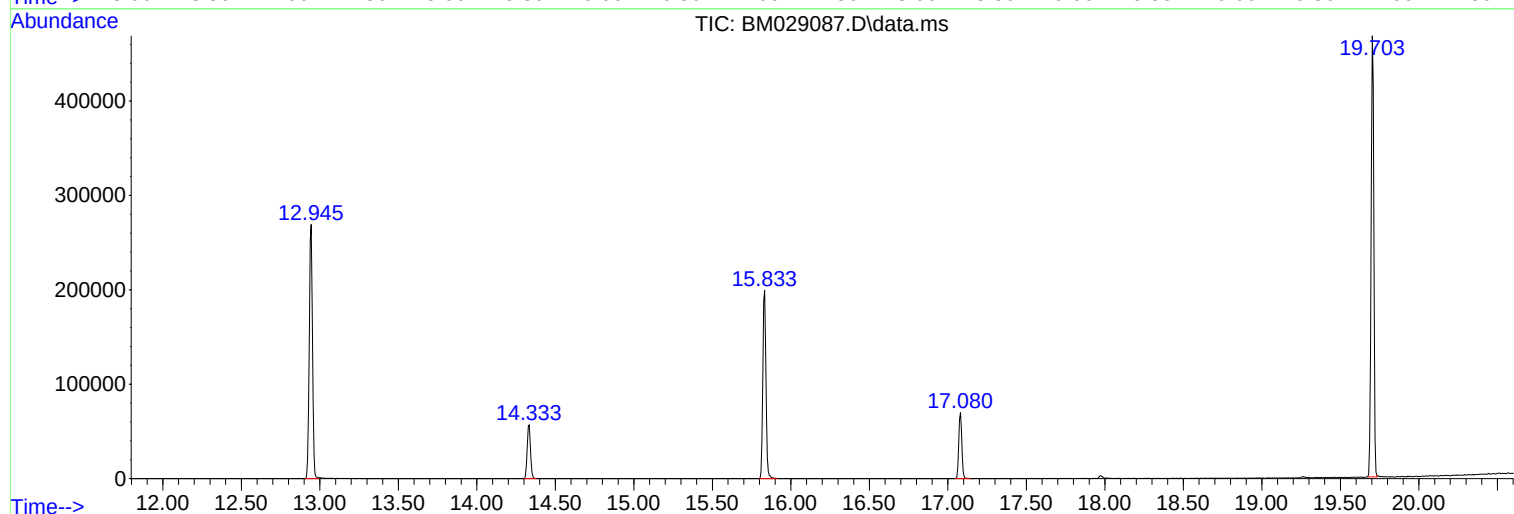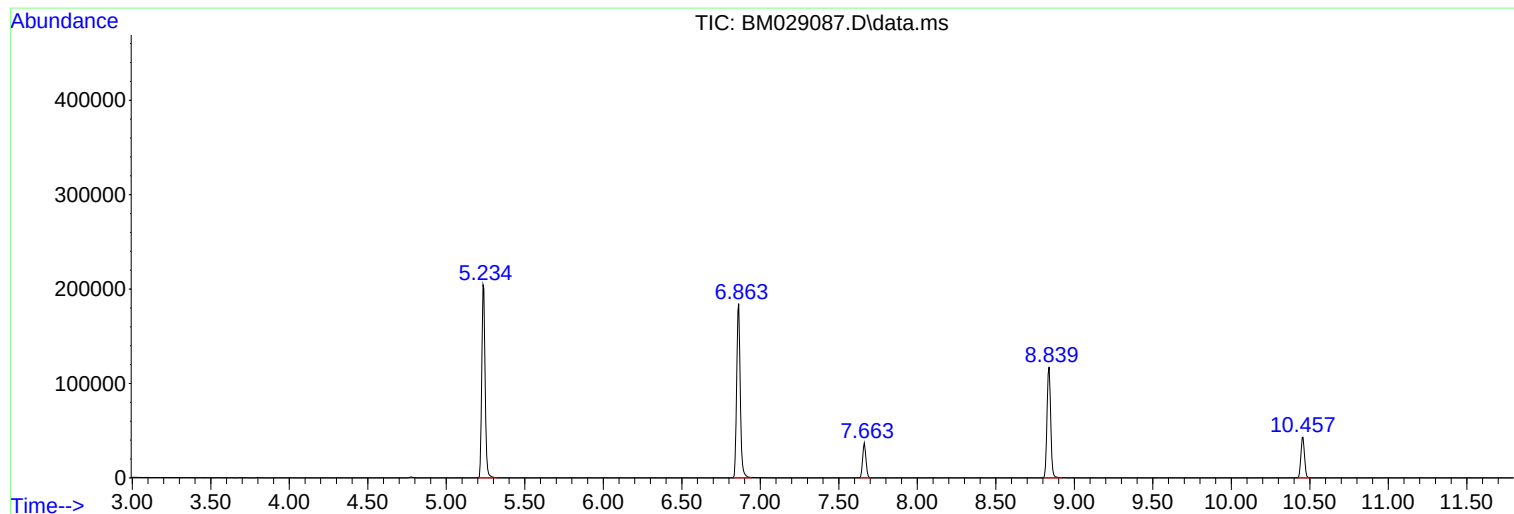

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
Data File : BM029087.D
Acq On : 11 Mar 2021 10:05
Operator : CG/JU
Sample : PB135092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135092BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
Data File : BM029087.D
Acq On : 11 Mar 2021 10:05
Operator : CG/JU
Sample : PB135092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135092BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------