

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031121\  
 Data File : BM029095.D  
 Acq On : 11 Mar 2021 15:15  
 Operator : CG/JU  
 Sample : M1624-07  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 FLOORS-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029095.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.757       | 297           | 301         | 311          | rBV      | 78189          | 107942        | 5.09%           | 1.574%        |
| 2         | 5.245       | 379           | 384         | 397          | rVB      | 42539          | 70123         | 3.30%           | 1.022%        |
| 3         | 6.763       | 634           | 642         | 654          | rBV      | 10336          | 23222         | 1.09%           | 0.339%        |
| 4         | 6.869       | 654           | 660         | 678          | rVB2     | 60434          | 106394        | 5.01%           | 1.551%        |
| 5         | 7.663       | 789           | 795         | 802          | rVB      | 28840          | 44405         | 2.09%           | 0.647%        |
| 6         | 8.322       | 895           | 907         | 912          | rBV4     | 10326          | 28732         | 1.35%           | 0.419%        |
| 7         | 8.833       | 988           | 994         | 1004         | rBV      | 53097          | 91850         | 4.33%           | 1.339%        |
| 8         | 9.004       | 1016          | 1023        | 1030         | rVB3     | 15650          | 29941         | 1.41%           | 0.436%        |
| 9         | 9.857       | 1159          | 1168        | 1175         | rBV2     | 26216          | 54443         | 2.57%           | 0.794%        |
| 10        | 10.451      | 1264          | 1269        | 1274         | rVB      | 38676          | 58726         | 2.77%           | 0.856%        |
| 11        | 11.310      | 1406          | 1415        | 1424         | rBV      | 30727          | 62416         | 2.94%           | 0.910%        |
| 12        | 12.286      | 1575          | 1581        | 1611         | rBV      | 53960          | 207019        | 9.75%           | 3.018%        |
| 13        | 12.939      | 1686          | 1692        | 1698         | rVB      | 129866         | 181347        | 8.54%           | 2.644%        |
| 14        | 14.327      | 1922          | 1928        | 1934         | rVB      | 53563          | 75298         | 3.55%           | 1.098%        |
| 15        | 15.827      | 2176          | 2183        | 2190         | rVB      | 43613          | 57450         | 2.71%           | 0.837%        |
| 16        | 16.492      | 2291          | 2296        | 2304         | rBV3     | 18376          | 32000         | 1.51%           | 0.466%        |
| 17        | 17.074      | 2385          | 2395        | 2399         | rBV      | 66004          | 89934         | 4.24%           | 1.311%        |
| 18        | 17.115      | 2399          | 2402        | 2408         | rVB      | 24554          | 34156         | 1.61%           | 0.498%        |
| 19        | 17.998      | 2540          | 2552        | 2556         | rBV      | 596763         | 990618        | 46.67%          | 14.441%       |
| 20        | 18.039      | 2556          | 2559        | 2564         | rVB      | 60478          | 78792         | 3.71%           | 1.149%        |
| 21        | 18.139      | 2572          | 2576        | 2580         | rVB2     | 20150          | 25210         | 1.19%           | 0.368%        |
| 22        | 18.645      | 2657          | 2662        | 2669         | rBV2     | 13867          | 21291         | 1.00%           | 0.310%        |
| 23        | 18.956      | 2710          | 2715        | 2718         | rBV      | 19632          | 38114         | 1.80%           | 0.556%        |
| 24        | 18.986      | 2718          | 2720        | 2724         | rVV2     | 21062          | 25511         | 1.20%           | 0.372%        |
| 25        | 19.027      | 2724          | 2727        | 2730         | rVB      | 24903          | 25943         | 1.22%           | 0.378%        |
| 26        | 19.139      | 2741          | 2746        | 2753         | rBV2     | 67601          | 128897        | 6.07%           | 1.879%        |
| 27        | 19.268      | 2758          | 2768        | 2777         | rBV      | 474573         | 703217        | 33.13%          | 10.251%       |
| 28        | 19.333      | 2777          | 2779        | 2786         | rVB5     | 16388          | 22336         | 1.05%           | 0.326%        |
| 29        | 19.533      | 2810          | 2813        | 2820         | rVV      | 33677          | 43301         | 2.04%           | 0.631%        |
| 30        | 19.609      | 2822          | 2826        | 2833         | rVV7     | 20118          | 32112         | 1.51%           | 0.468%        |
| 31        | 19.703      | 2837          | 2842        | 2849         | rVB      | 230157         | 318752        | 15.02%          | 4.647%        |
| 32        | 20.033      | 2895          | 2898        | 2903         | rVB3     | 31644          | 40377         | 1.90%           | 0.589%        |
| 33        | 20.192      | 2922          | 2925        | 2931         | rVB      | 21936          | 27331         | 1.29%           | 0.398%        |
| 34        | 20.256      | 2931          | 2936        | 2942         | rBV2     | 51297          | 69689         | 3.28%           | 1.016%        |
| 35        | 20.339      | 2947          | 2950        | 2953         | rBV2     | 48299          | 52730         | 2.48%           | 0.769%        |
| 36        | 20.503      | 2974          | 2978        | 2981         | rBV      | 20920          | 25998         | 1.22%           | 0.379%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031121\  
Data File : BM029095.D  
Acq On : 11 Mar 2021 15:15  
Operator : CG/JU  
Sample : M1624-07  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
FLOORS-4

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |         |         |
|----|--------|------|------|------|------|---------|---------|---------|---------|
| 37 | 20.574 | 2987 | 2990 | 2996 | rVB5 | 22453   | 28916   | 1.36%   | 0.422%  |
| 38 | 20.686 | 3006 | 3009 | 3013 | rVB2 | 19235   | 21485   | 1.01%   | 0.313%  |
| 39 | 20.968 | 3049 | 3057 | 3066 | rVB4 | 40690   | 119155  | 5.61%   | 1.737%  |
| 40 | 21.044 | 3067 | 3070 | 3073 | rBV3 | 16529   | 23351   | 1.10%   | 0.340%  |
| 41 | 21.168 | 3086 | 3091 | 3096 | rBV  | 1879727 | 2122402 | 100.00% | 30.940% |
| 42 | 21.256 | 3100 | 3106 | 3110 | rBV2 | 99407   | 159096  | 7.50%   | 2.319%  |
| 43 | 21.397 | 3127 | 3130 | 3137 | rVB3 | 21414   | 29766   | 1.40%   | 0.434%  |
| 44 | 21.562 | 3154 | 3158 | 3164 | rVB  | 51986   | 62740   | 2.96%   | 0.915%  |
| 45 | 21.815 | 3198 | 3201 | 3206 | rBV2 | 17138   | 23894   | 1.13%   | 0.348%  |
| 46 | 22.062 | 3240 | 3243 | 3248 | rVB  | 65459   | 80763   | 3.81%   | 1.177%  |
| 47 | 22.462 | 3307 | 3311 | 3316 | rVB4 | 38898   | 54299   | 2.56%   | 0.792%  |
| 48 | 23.409 | 3467 | 3472 | 3479 | rVB2 | 65991   | 108345  | 5.10%   | 1.579%  |




Sum of corrected areas: 6859829

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031121\  
Data File : BM029095.D  
Acq On : 11 Mar 2021 15:15  
Operator : CG/JU  
Sample : M1624-07  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
FLOORS-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

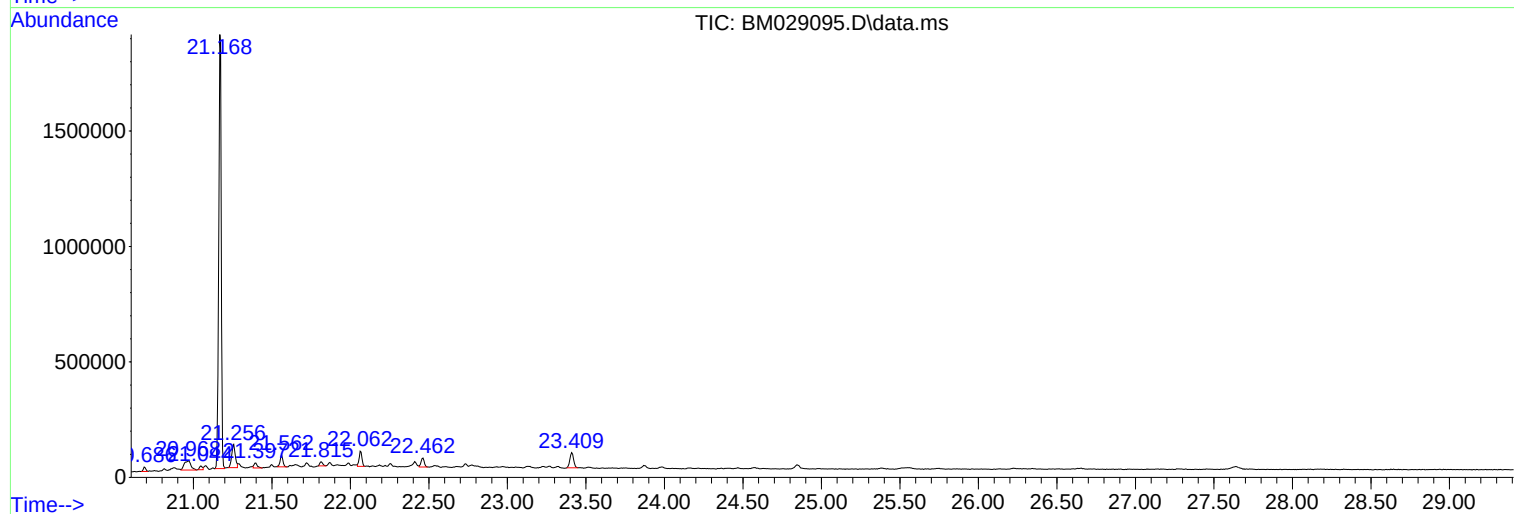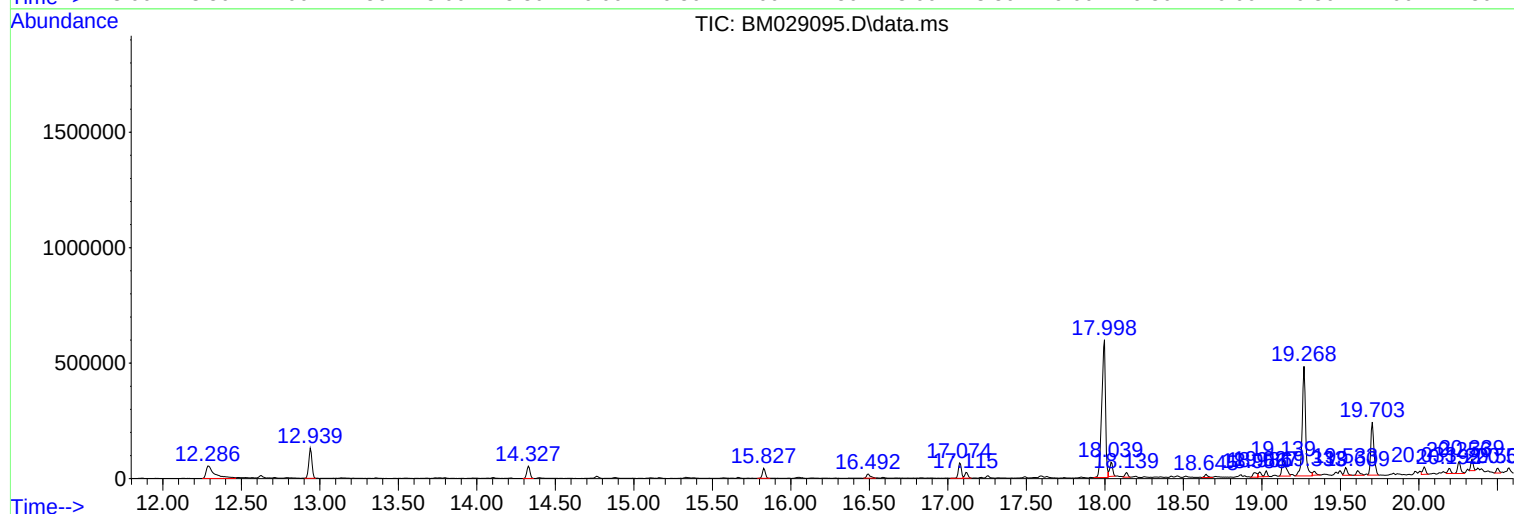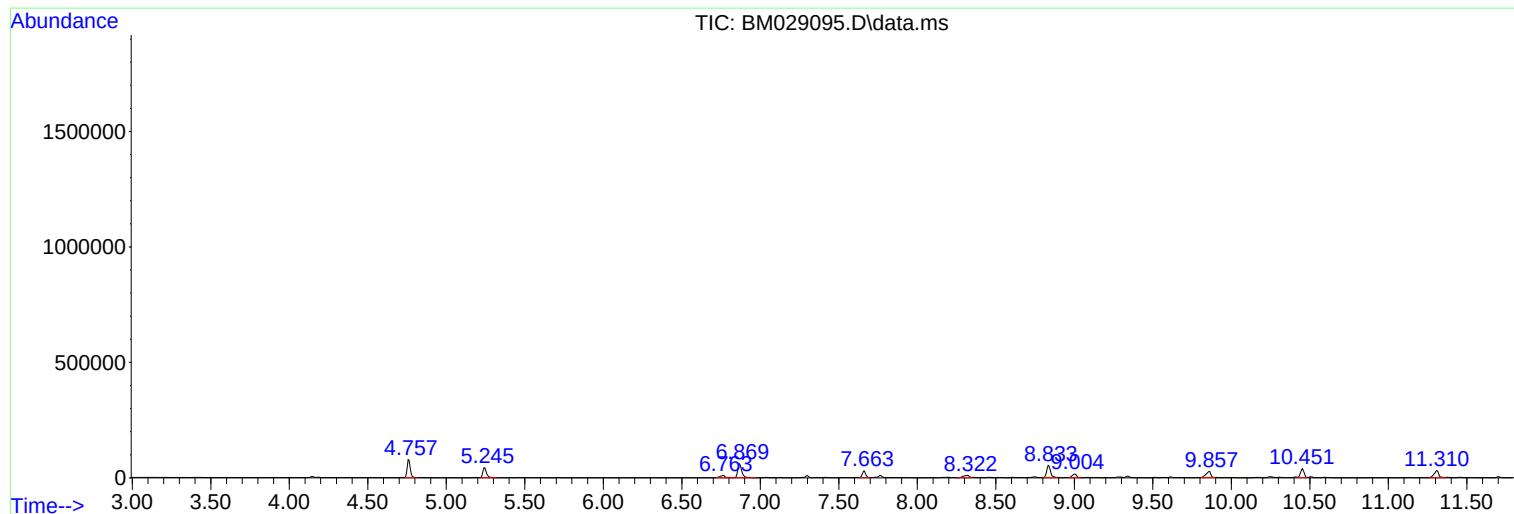

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031121\  
Data File : BM029095.D  
Acq On : 11 Mar 2021 15:15  
Operator : CG/JU  
Sample : M1624-07  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
FLOORS-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM031121\  
Data File : BM029095.D  
Acq On : 11 Mar 2021 15:15  
Operator : CG/JU  
Sample : M1624-07  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
FLOORS-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|