


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
 Data File : BM029085.D
 Acq On : 11 Mar 2021 08:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 12 12:30:15 2021

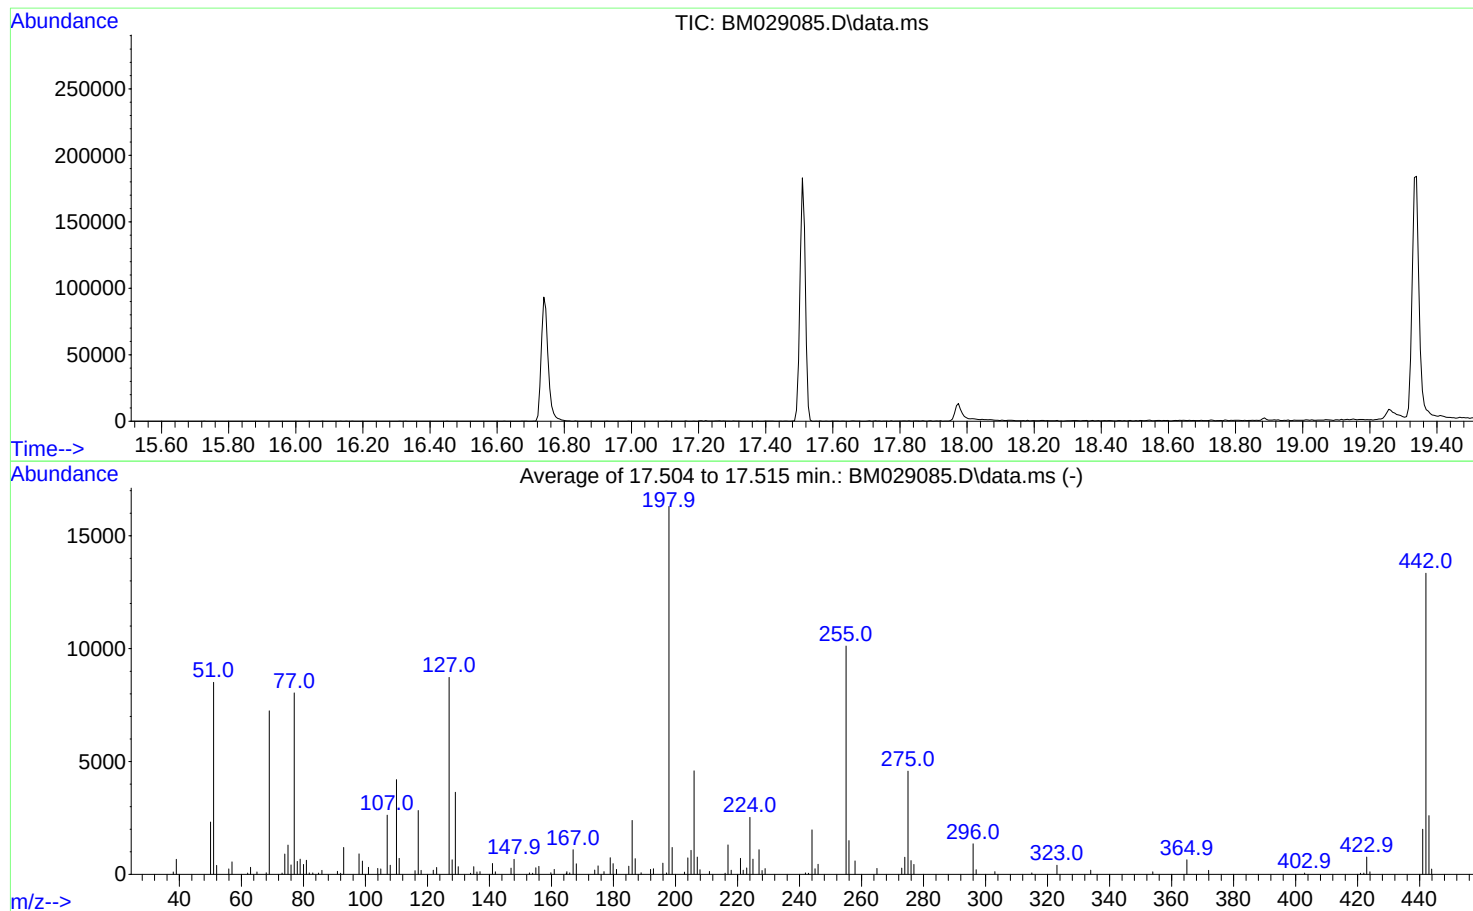




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	8510	PASS
68	69	0.00	2	1.0	70	PASS
69	198	0.00	100	44.5	7246	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	8728	PASS
197	198	0.00	2	0.4	62	PASS
198	198	100	100	100.0	16299	PASS
199	198	5	9	7.3	1193	PASS
275	198	10	60	28.1	4572	PASS
365	198	1	100	4.0	646	PASS
441	198	0.01	100	12.3	1998	PASS
442	442	50	100	100.0	13346	PASS
443	442	15	24	19.5	2604	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
Data File : BM029085.D
Acq On : 11 Mar 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 11 09:49:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

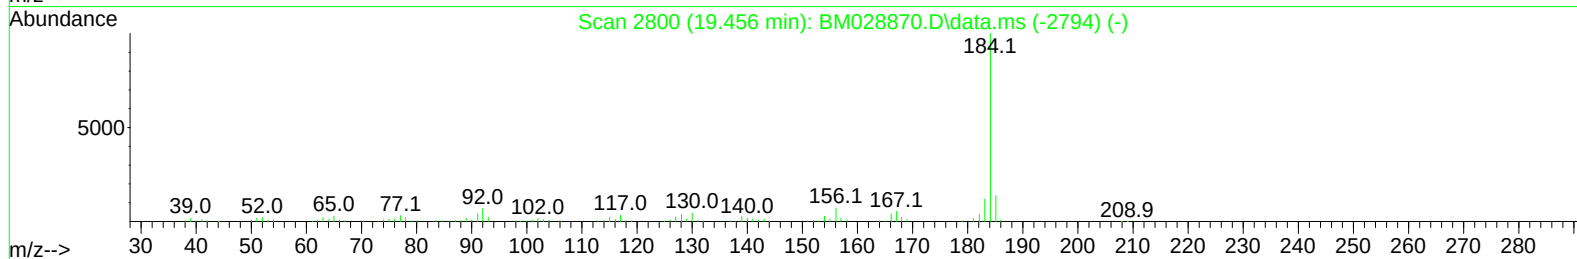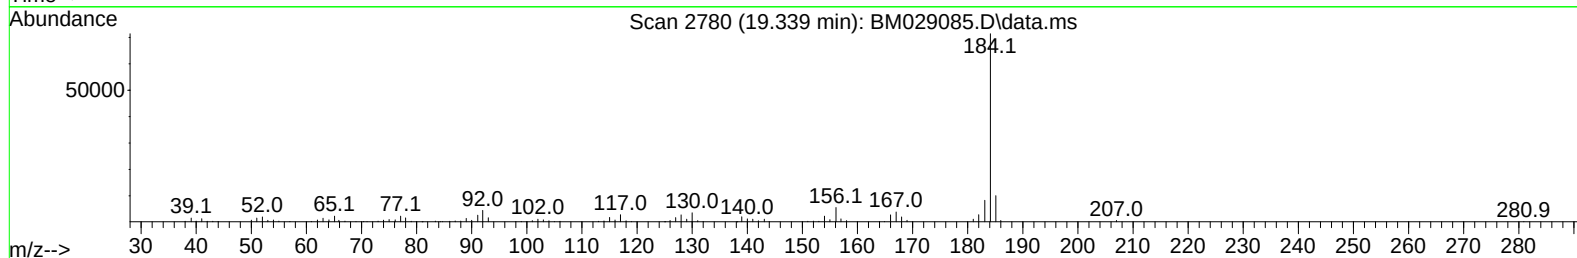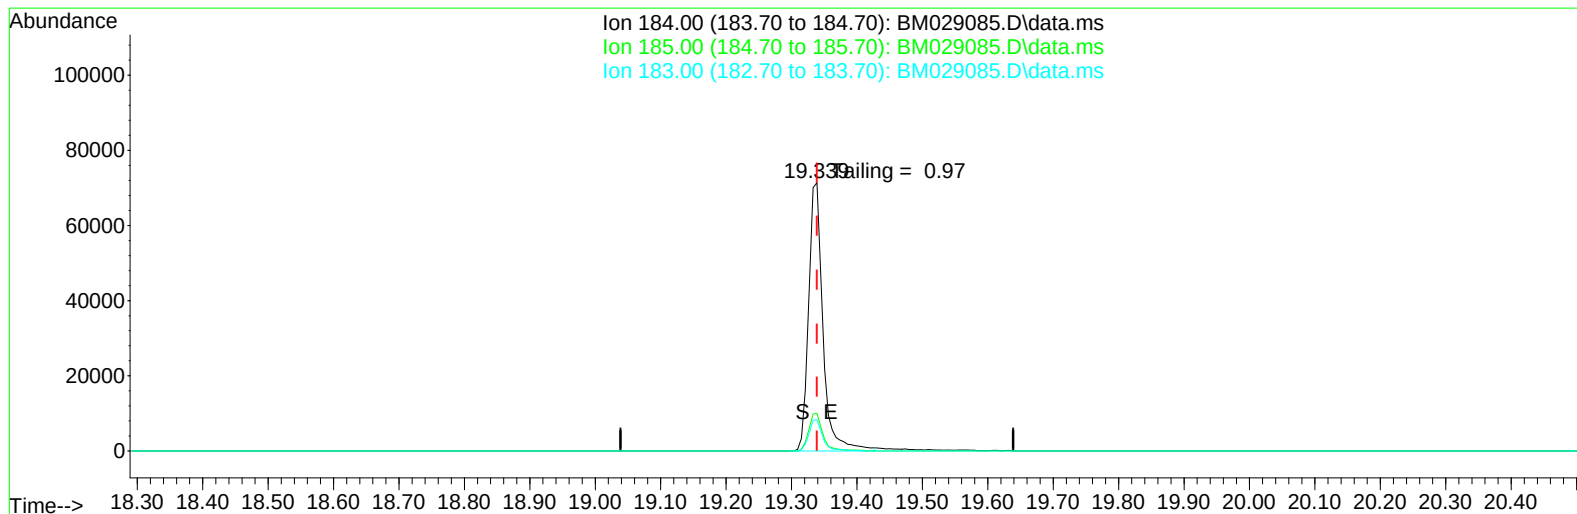

TIC: BM029085.D\data.ms

(77) Benzidine

19.339min (-0.000) 0.00 ng




response 110290

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.05
183.00	12.10	11.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031121\
Data File : BM029085.D
Acq On : 11 Mar 2021 08:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 11 09:49:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

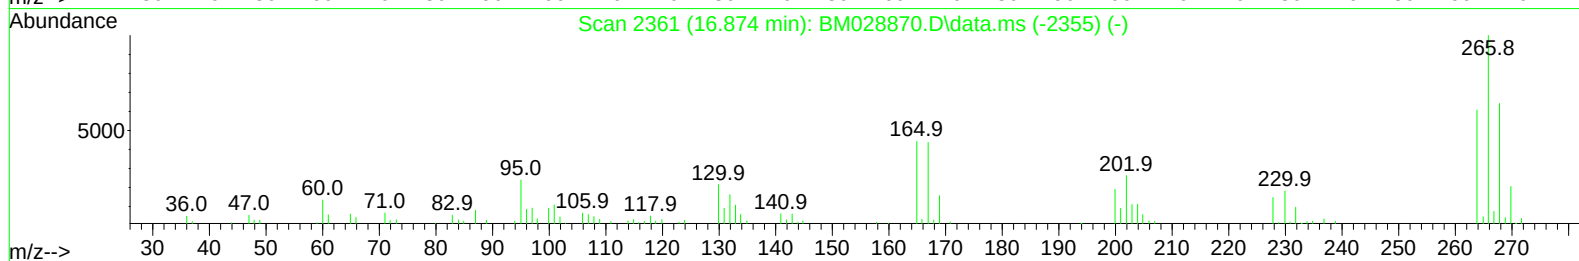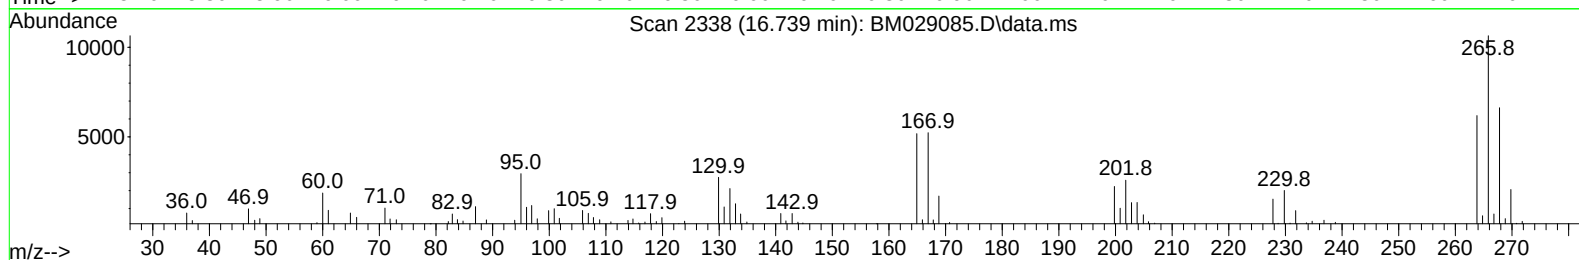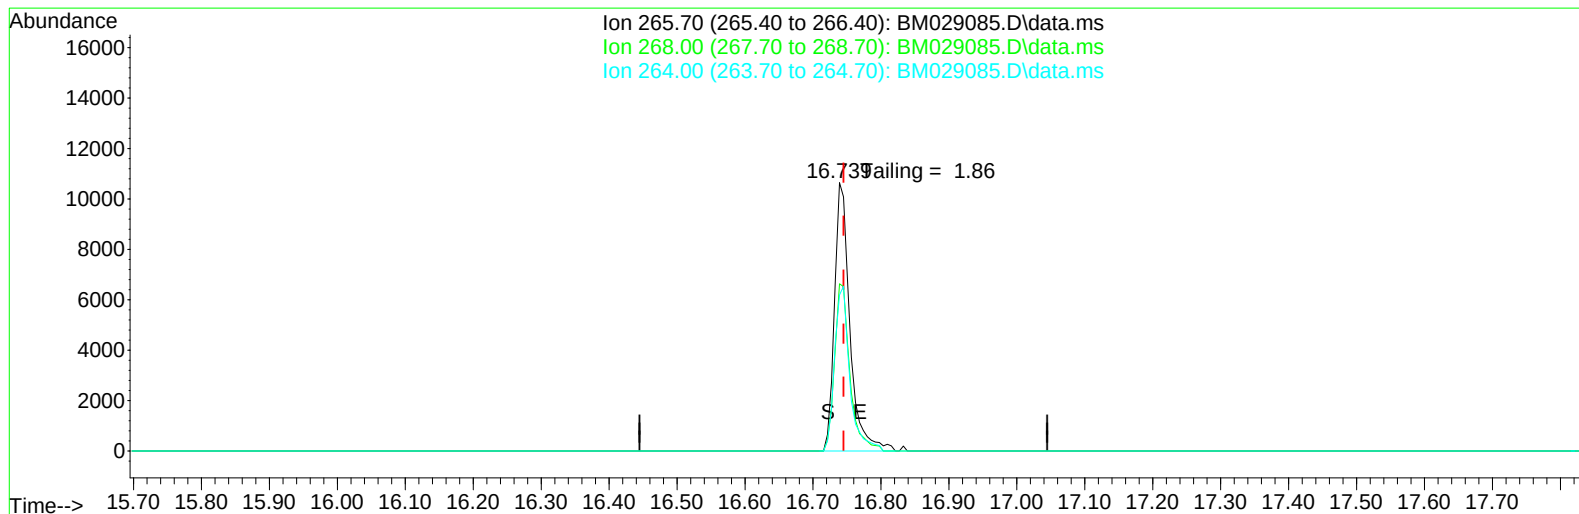

TIC: BM029085.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.006) 0.00 ng

response 16817

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.29
264.00	63.30	58.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/11/2021	BNA_M	<u>BM029085.D</u>
Compound Name	Response	Retention Time
DDT	54887	20.55
DDD	2028	20.12
DDE	0	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2028	56915	3.56

Instrument :
BNA_M
ClientSampleId :
DFTPP