




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:42:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

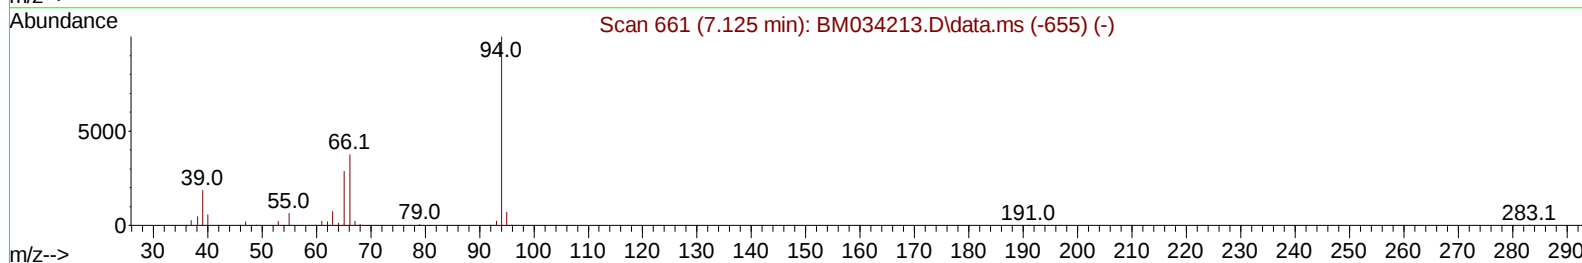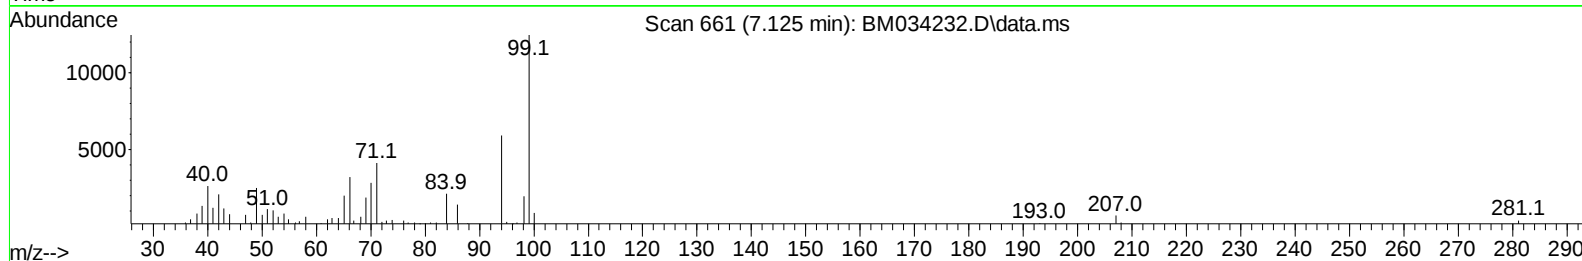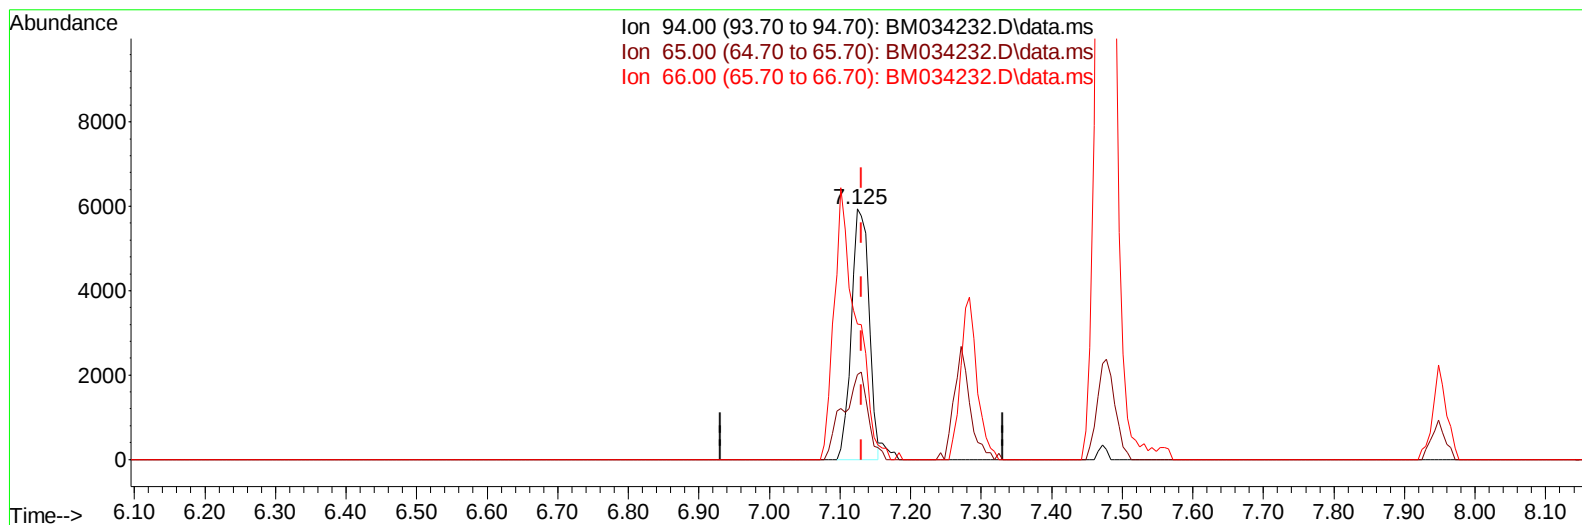

TIC: BM034232.D\data.ms

(8) Phenol

7.125min (-0.006) 1.01 ng/u1

response 10297

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	33.86
66.00	42.10	54.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:42:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

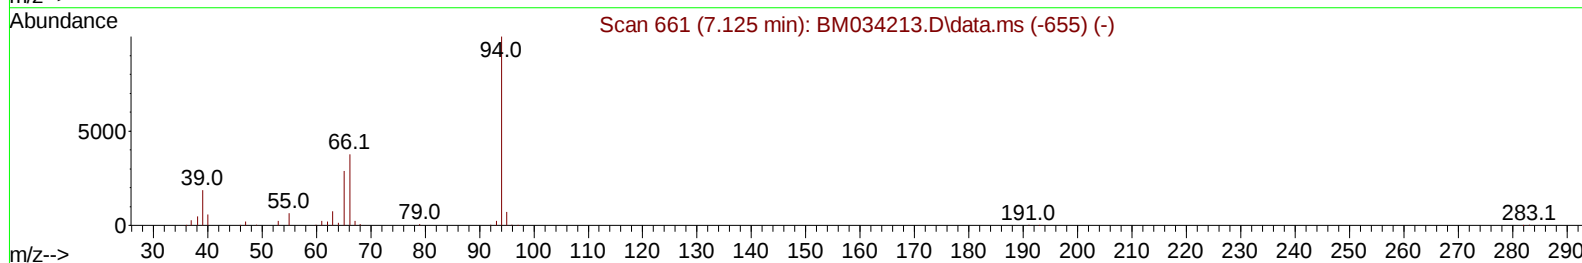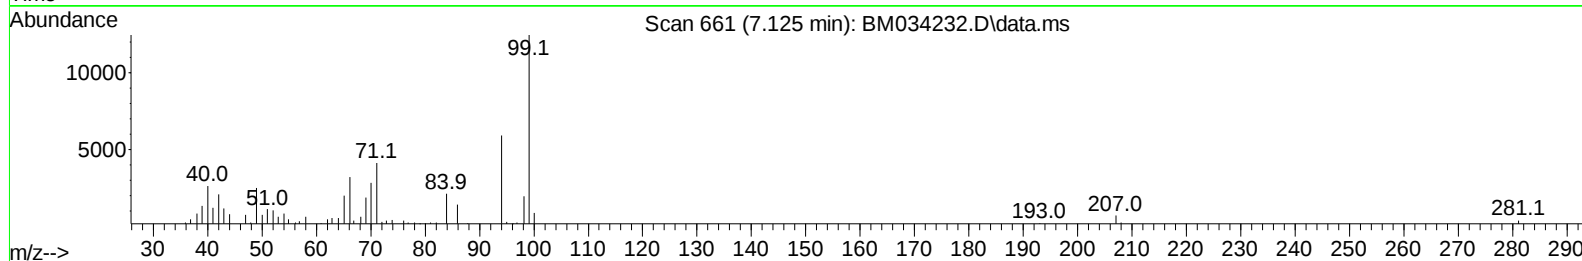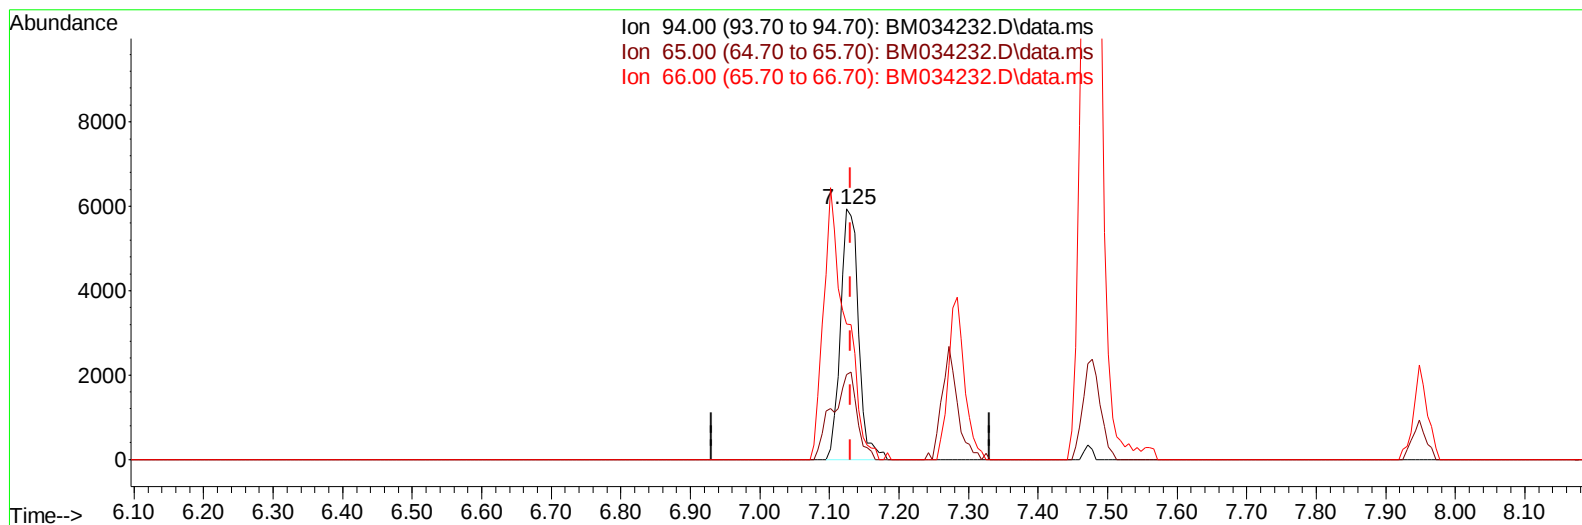

TIC: BM034232.D\data.ms

(8) Phenol

7.125min (-0.006) 1.04 ng/ul m

response 10652

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	33.86
66.00	42.10	54.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:42:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

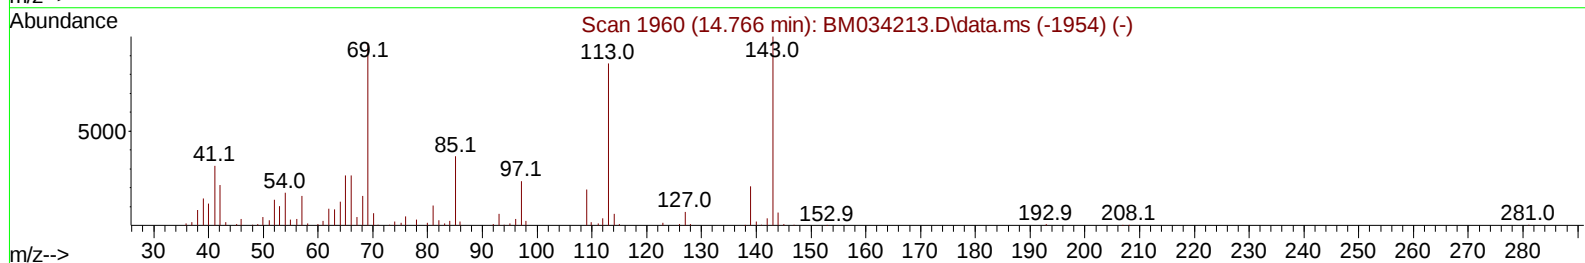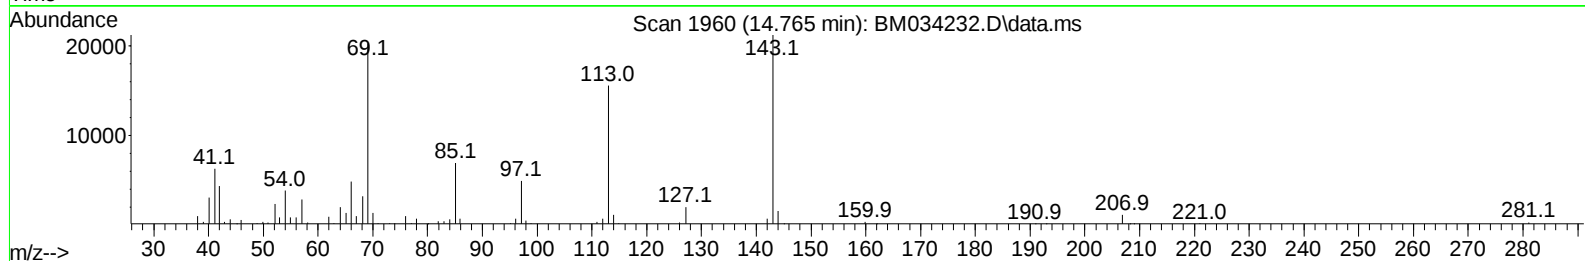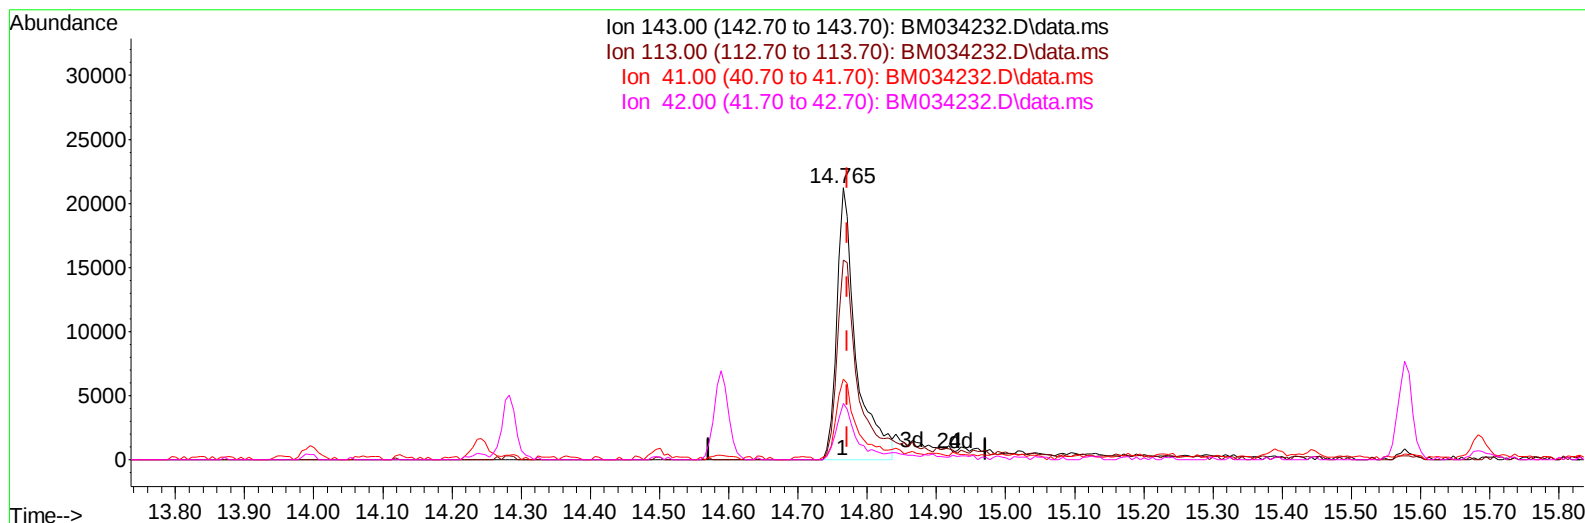

TIC: BM034232.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.765min (-0.006) 9.25 ng/u1

response 40756

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	73.41
41.00	31.90	29.71
42.00	19.10	20.77




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:42:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

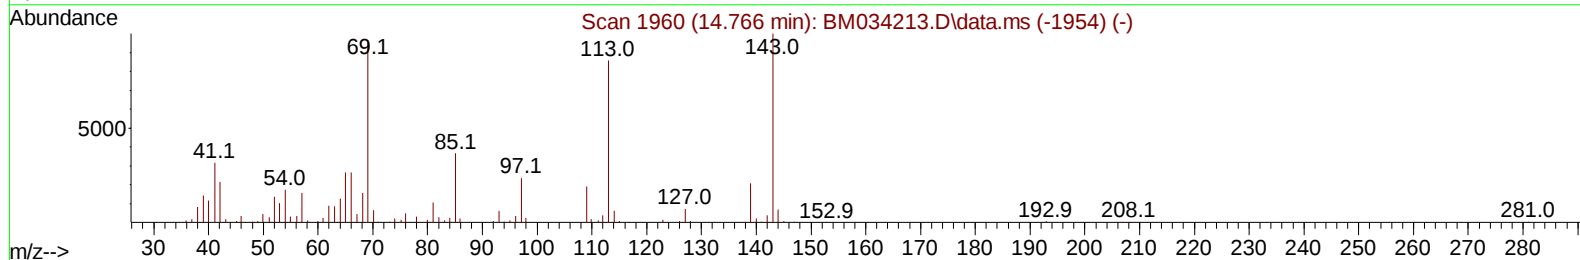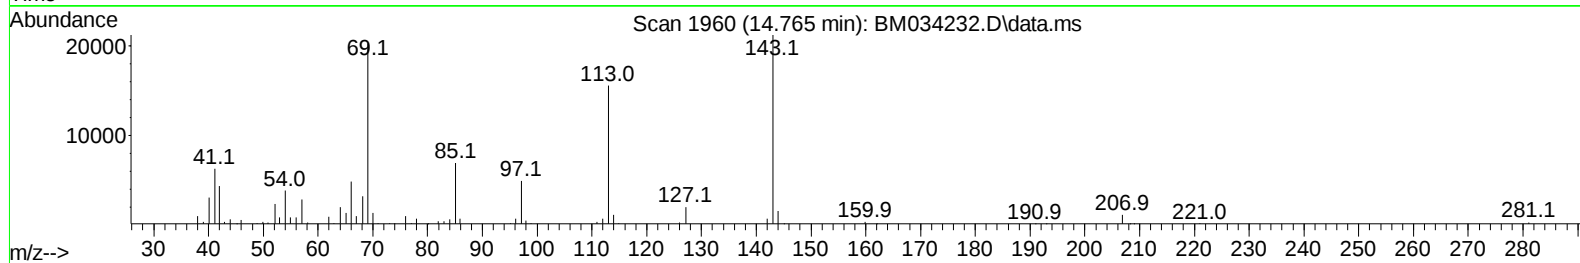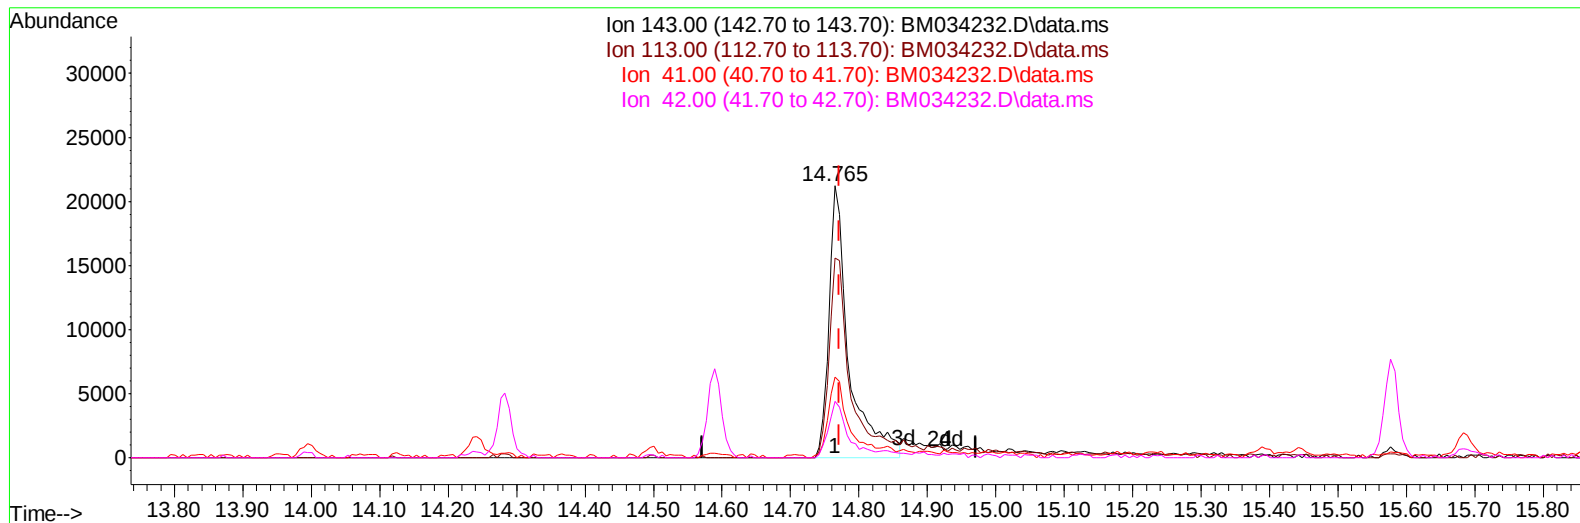

TIC: BM034232.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.765min (-0.006) 9.72 ng/ul m

response 42830

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	73.41
41.00	31.90	29.71
42.00	19.10	20.77

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:42:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	154592	20.000	ng/ul	0.00
20) Naphthalene-d8	10.766	136	595787	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.589	164	388635	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.330	188	770052	20.000	ng/ul	0.00
79) Chrysene-d12	21.500	240	717577	20.000	ng/ul	0.00
88) Perylene-d12	23.918	264	764604	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	13115	3.703	ng/uL	0.00
4) Pyridine-d5	3.748	84	60193	7.139	ng/ul	0.00
7) Phenol-d5	7.101	99	181649	17.559	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.272	67	121417	20.006	ng/ul	0.00
11) 2-Chlorophenol-d4	7.478	132	177910	19.899	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	159785	18.059	ng/ul	0.00
21) Nitrobenzene-d5	9.113	128	84874	19.860	ng/ul	0.00
24) 2-Nitrophenol-d4	9.836	143	77821	16.422	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.377	165	174457	18.364	ng/ul	0.00
31) 4-Chloroaniline-d4	10.895	131	213714	18.089	ng/ul	0.00
46) Dimethylphthalate-d6	13.995	166	510902	18.067	ng/ul	0.00
49) Acenaphthylene-d8	14.283	160	718467	20.004	ng/ul	0.00
54) 4-Nitrophenol-d4	14.765	143	42830m	9.724	ng/ul	0.00
60) Fluorene-d10	15.577	176	504608	20.385	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.689	200	45566	9.352	ng/ul	0.00
73) Anthracene-d10	17.430	188	735889	20.233	ng/ul	0.00
81) Pyrene-d10	19.712	212	849801	21.753	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.759	264	777721	20.617	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.125	94	10652m	1.044	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:42:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

