




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034234.D
 Acq On : 11 Mar 2022 22:49
 Operator : CG/JU
 Sample : N1816-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:43:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

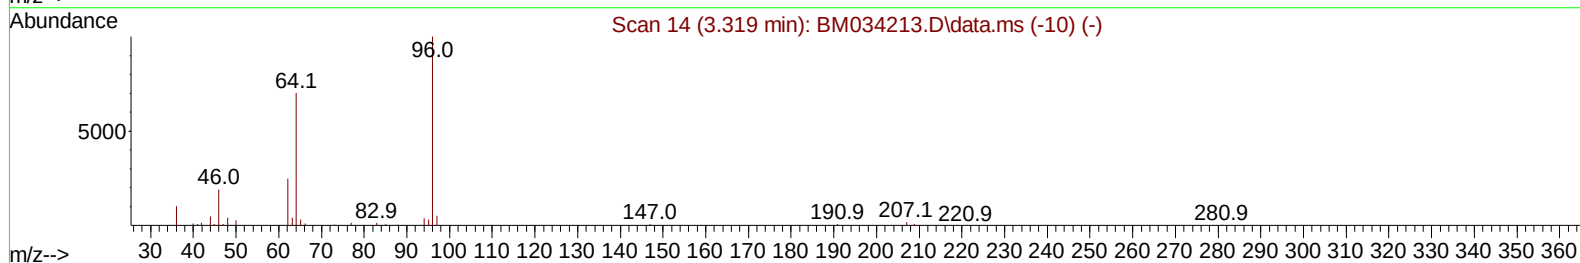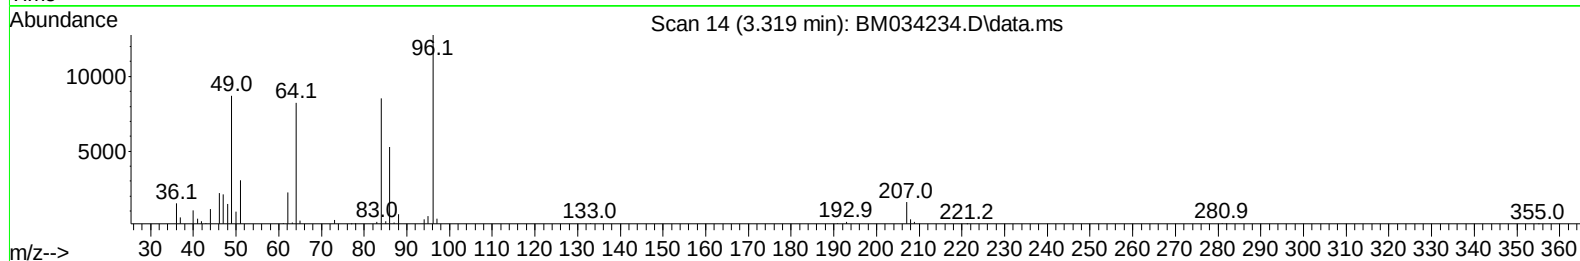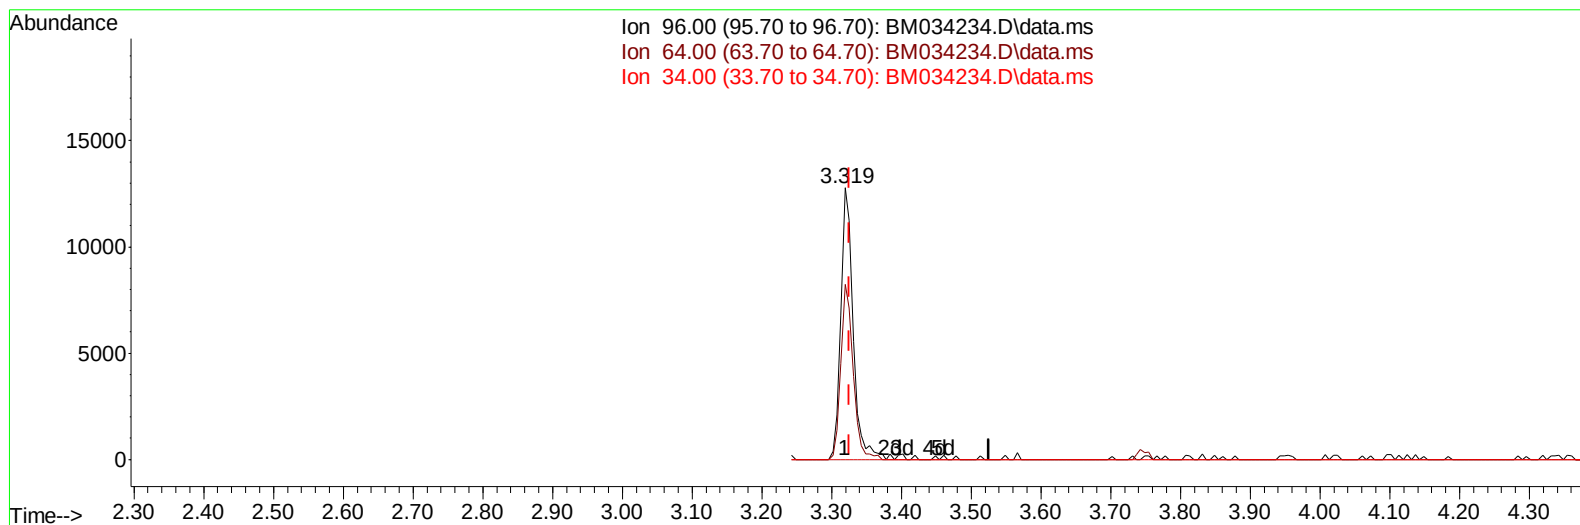

TIC: BM034234.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.006) 4.85 ng/uL

response 15616

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	64.60
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034234.D
Acq On : 11 Mar 2022 22:49
Operator : CG/JU
Sample : N1816-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:43:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

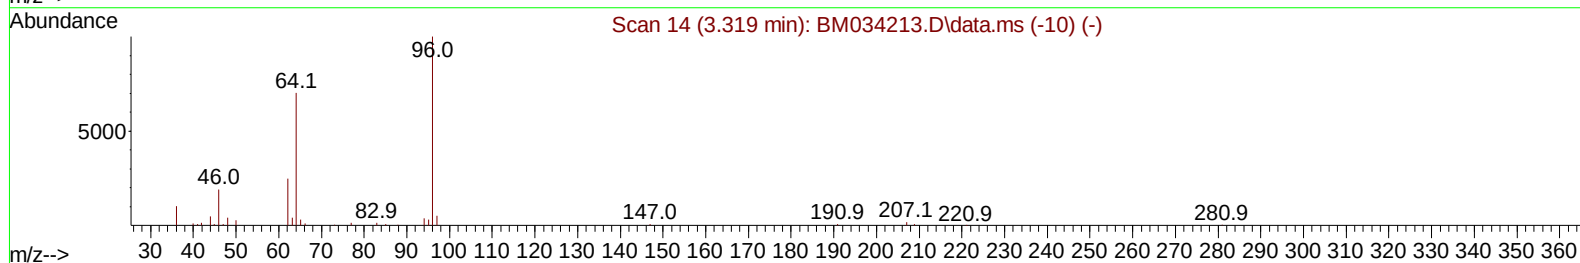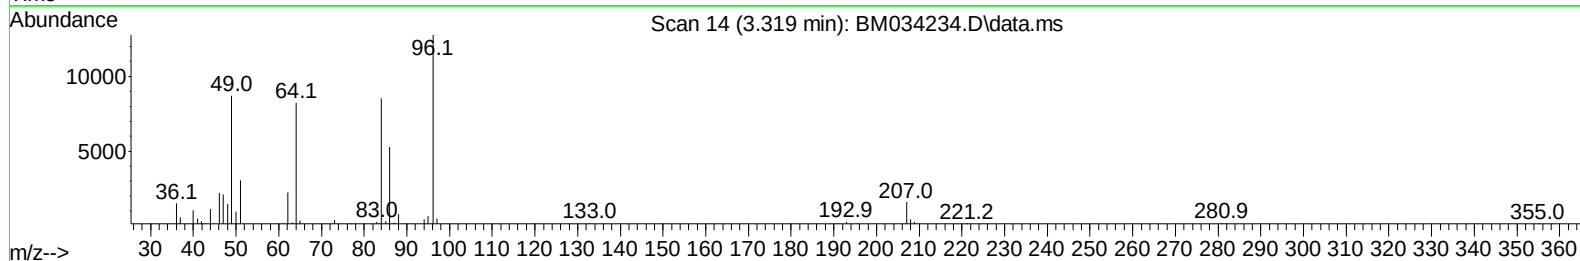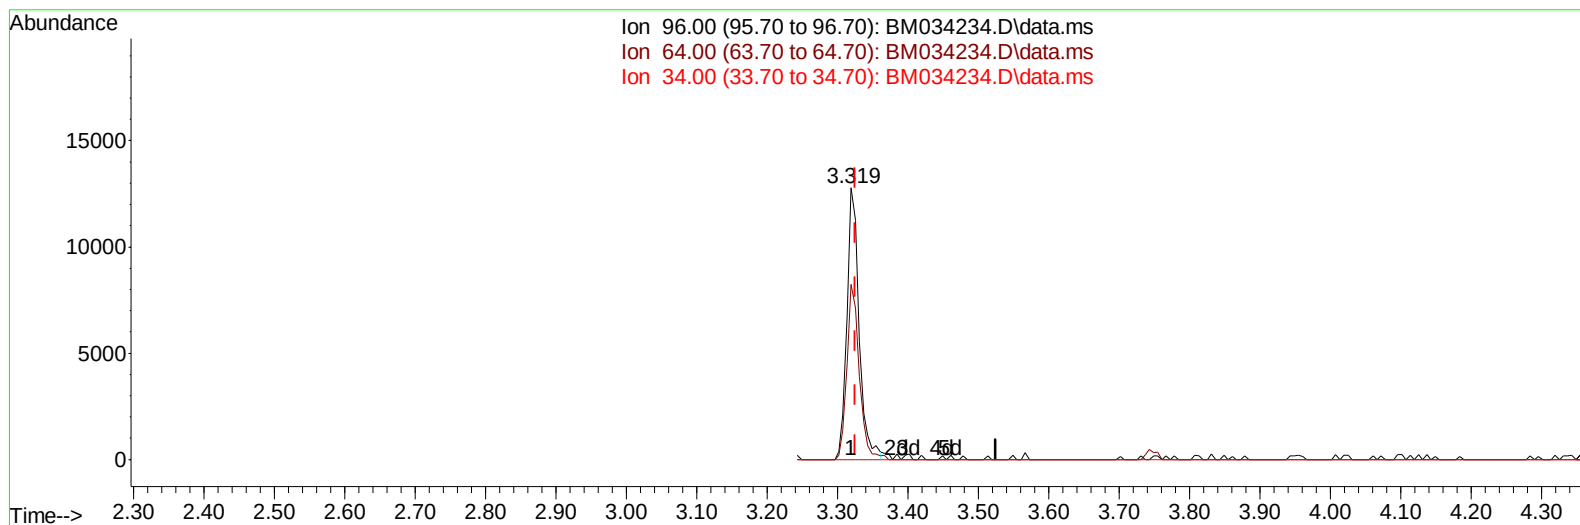

TIC: BM034234.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.006) 4.79 ng/uL m

response 15418

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	64.60
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034234.D
 Acq On : 11 Mar 2022 22:49
 Operator : CG/JU
 Sample : N1816-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:43:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

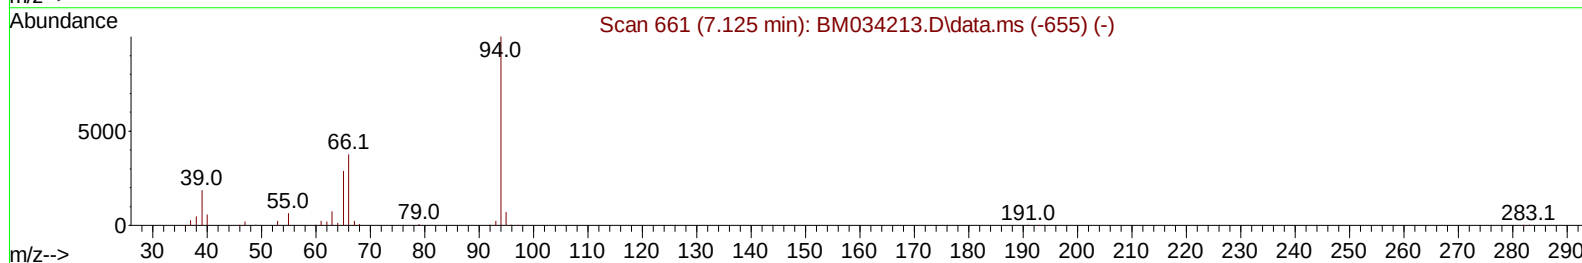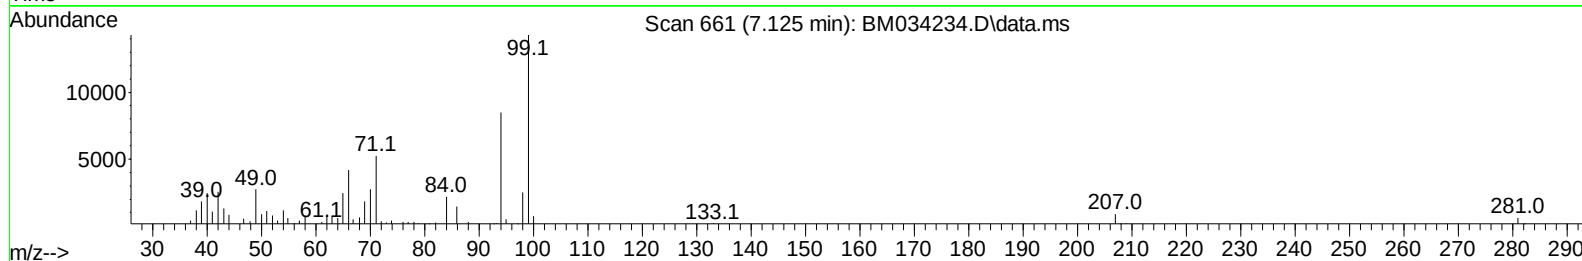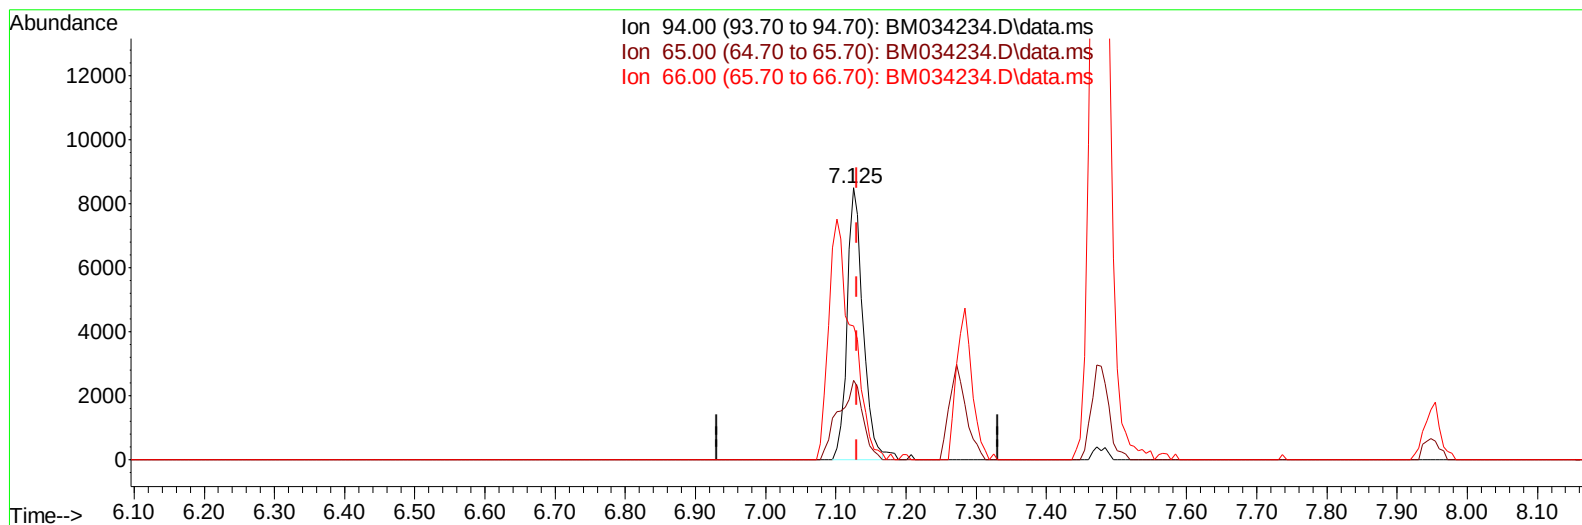

TIC: BM034234.D\data.ms

(8) Phenol

7.125min (-0.006) 1.43 ng/u1

response 13303

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	29.09
66.00	42.10	49.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034234.D
 Acq On : 11 Mar 2022 22:49
 Operator : CG/JU
 Sample : N1816-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:43:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

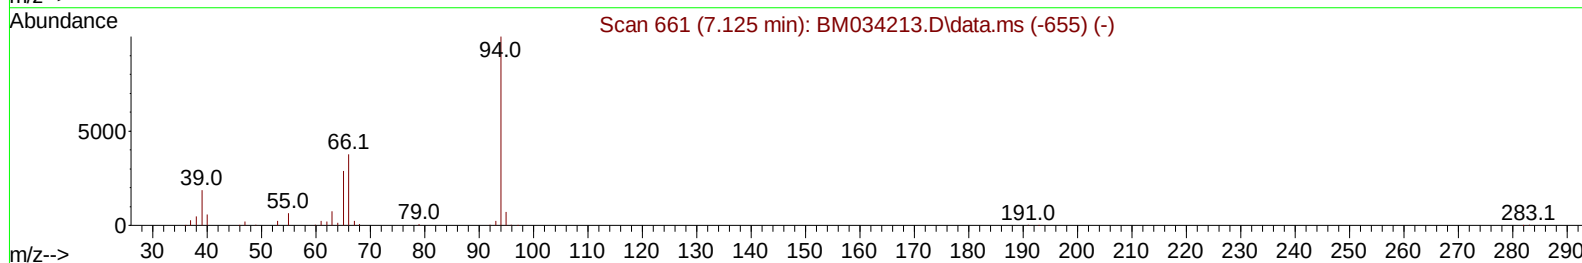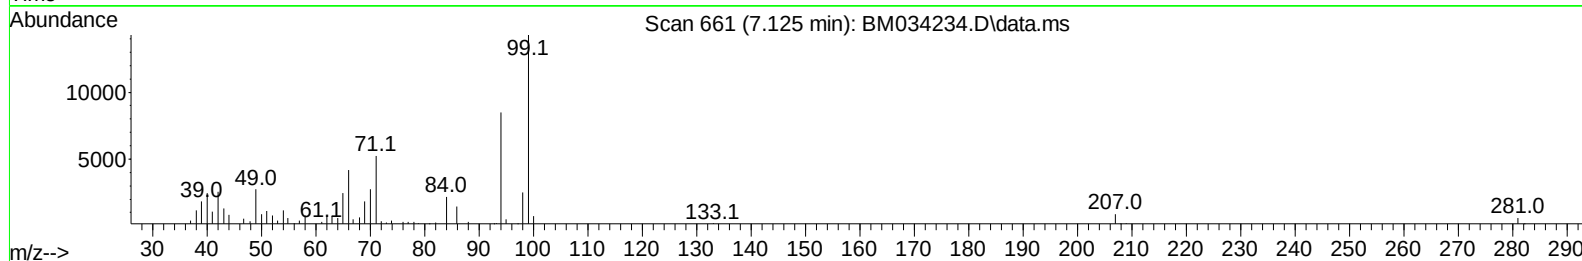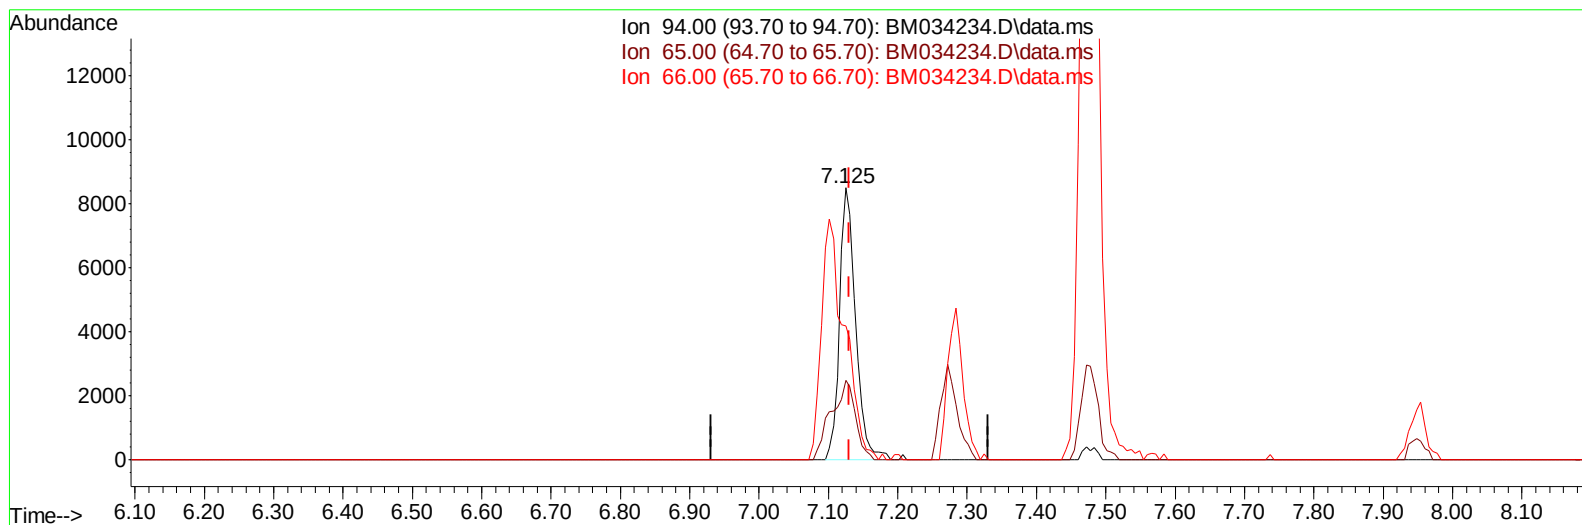

TIC: BM034234.D\data.ms

(8) Phenol

7.125min (-0.006) 1.46 ng/ul m

response 13531

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	29.09
66.00	42.10	49.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034234.D
Acq On : 11 Mar 2022 22:49
Operator : CG/JU
Sample : N1816-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:43:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

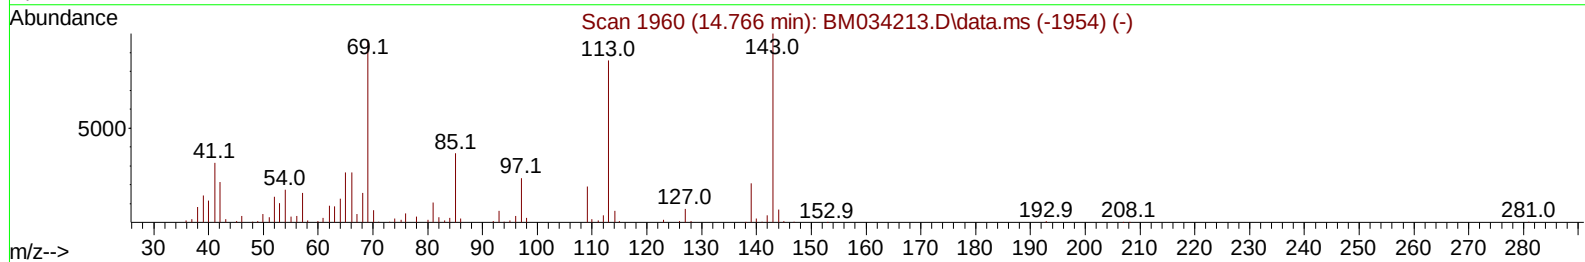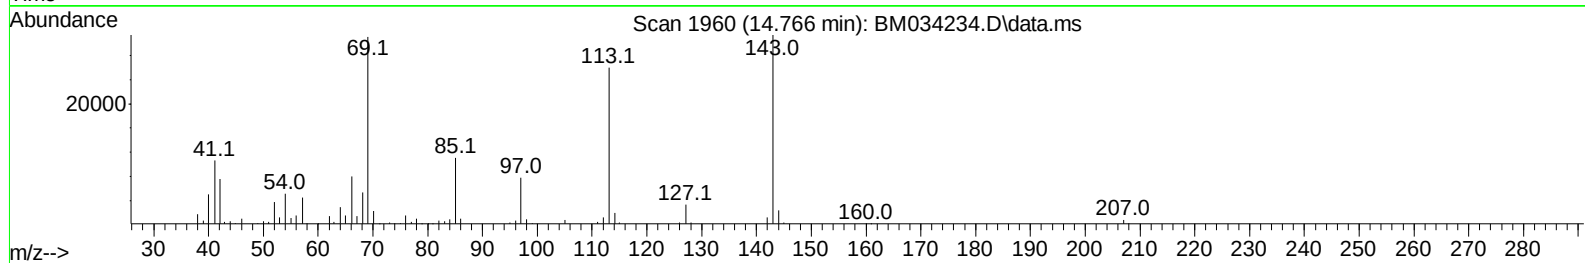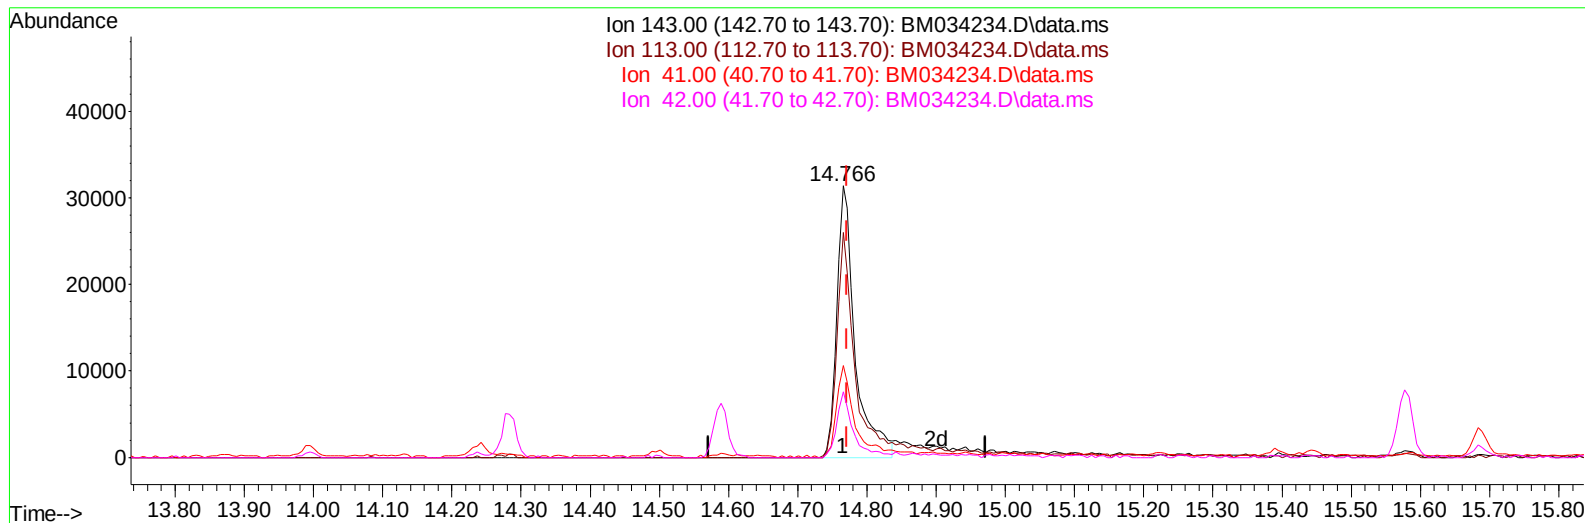

TIC: BM034234.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (-0.006) 14.67 ng/ul

response 57595

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	82.89
41.00	31.90	33.79
42.00	19.10	24.24#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034234.D
Acq On : 11 Mar 2022 22:49
Operator : CG/JU
Sample : N1816-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD6

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:43:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

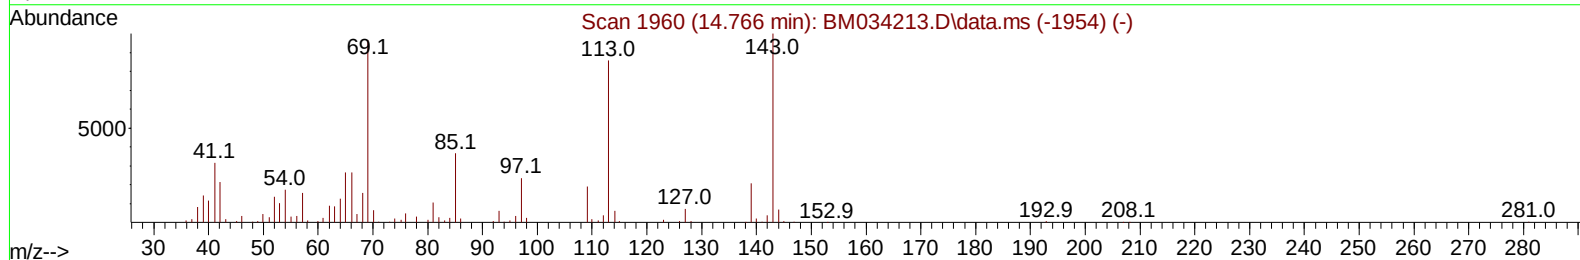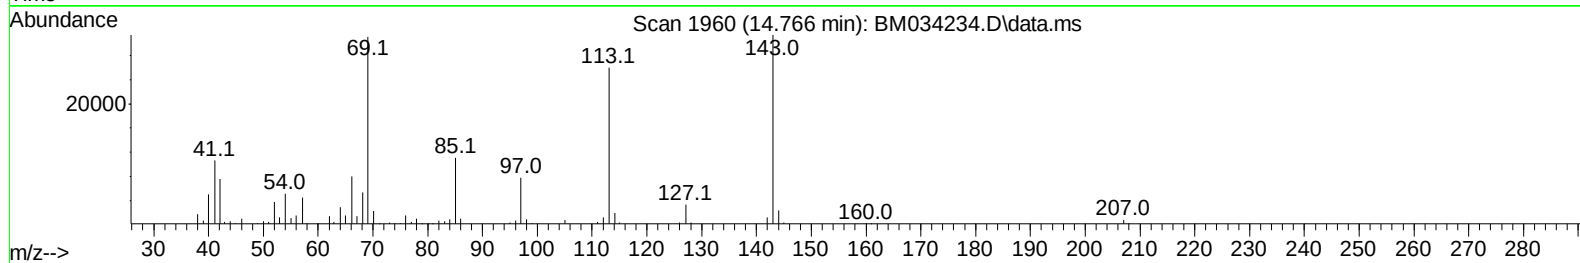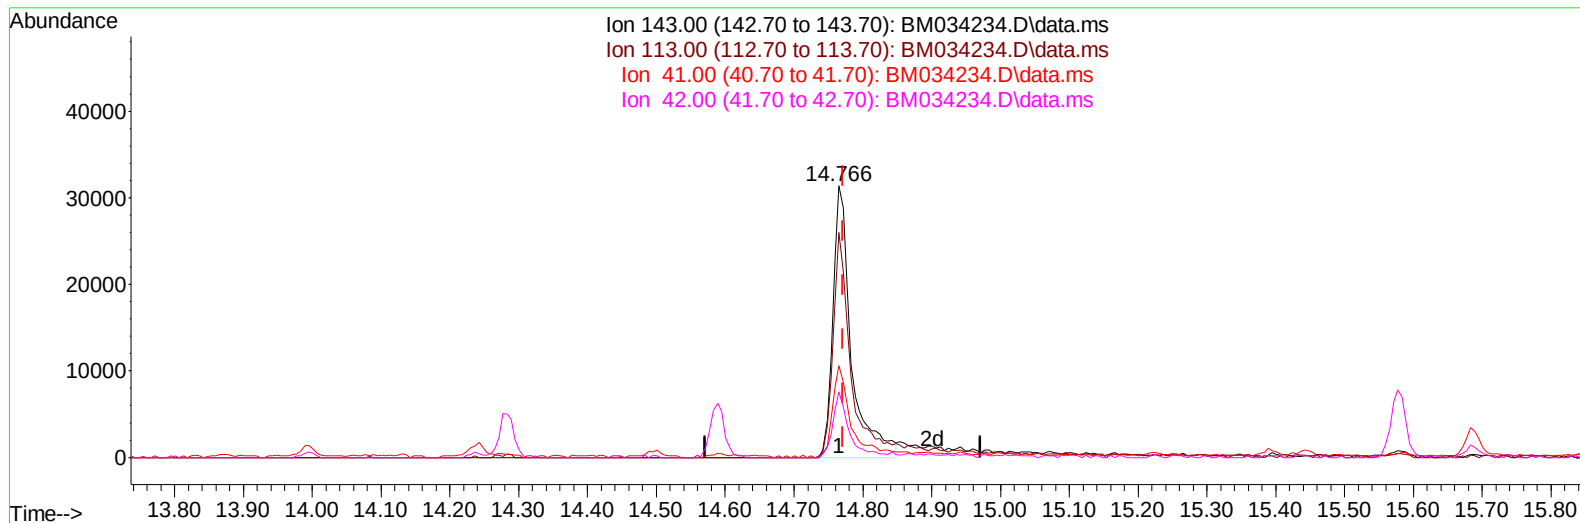

TIC: BM034234.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (-0.006) 15.00 ng/ul m

response 58879

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	82.89
41.00	31.90	33.79
42.00	19.10	24.24#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034234.D
 Acq On : 11 Mar 2022 22:49
 Operator : CG/JU
 Sample : N1816-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:43:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	140475	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	541734	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.589	164	346329	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.330	188	686092	20.000	ng/ul	0.00
79) Chrysene-d12	21.500	240	642686	20.000	ng/ul	0.00
88) Perylene-d12	23.918	264	665842	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	15418m	4.791	ng/uL	0.00
4) Pyridine-d5	3.743	84	173311	22.620	ng/ul	0.00
7) Phenol-d5	7.101	99	212368	22.591	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.272	67	139905	25.368	ng/ul	0.00
11) 2-Chlorophenol-d4	7.478	132	205511	25.296	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	185865	23.118	ng/ul	0.00
21) Nitrobenzene-d5	9.113	128	96218	24.761	ng/ul	0.00
24) 2-Nitrophenol-d4	9.836	143	104822	24.327	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.378	165	206148	23.865	ng/ul	0.00
31) 4-Chloroaniline-d4	10.895	131	245043	22.810	ng/ul	0.00
46) Dimethylphthalate-d6	13.995	166	656315	26.045	ng/ul	0.00
49) Acenaphthylene-d8	14.283	160	809003	25.277	ng/ul	0.00
54) 4-Nitrophenol-d4	14.766	143	58879m	15.000	ng/ul	0.00
60) Fluorene-d10	15.577	176	569250	25.806	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.689	200	78792	18.151	ng/ul	0.00
73) Anthracene-d10	17.430	188	822927	25.395	ng/ul	0.00
81) Pyrene-d10	19.712	212	984875	28.149	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.759	264	900467	27.412	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.125	94	13531m	1.459	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034234.D
Acq On : 11 Mar 2022 22:49
Operator : CG/JU
Sample : N1816-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 11 23:43:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

