




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034235.D
 Acq On : 11 Mar 2022 23:26
 Operator : CG/JU
 Sample : N1816-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 01:52:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

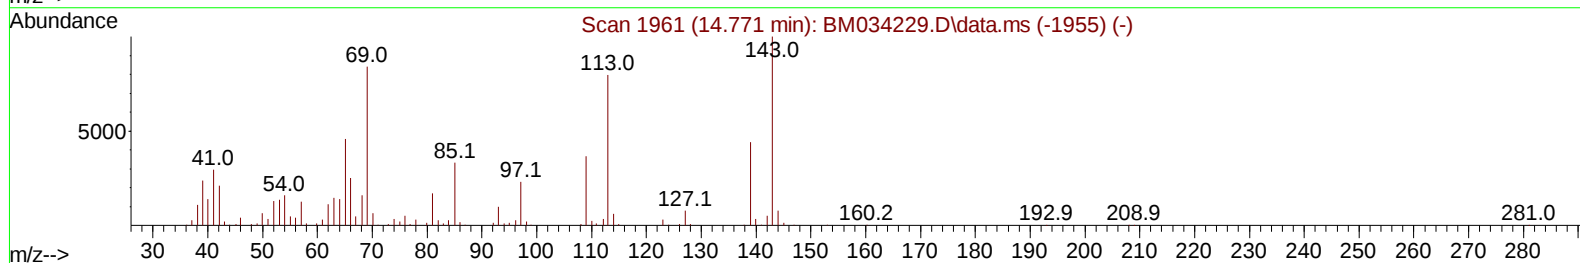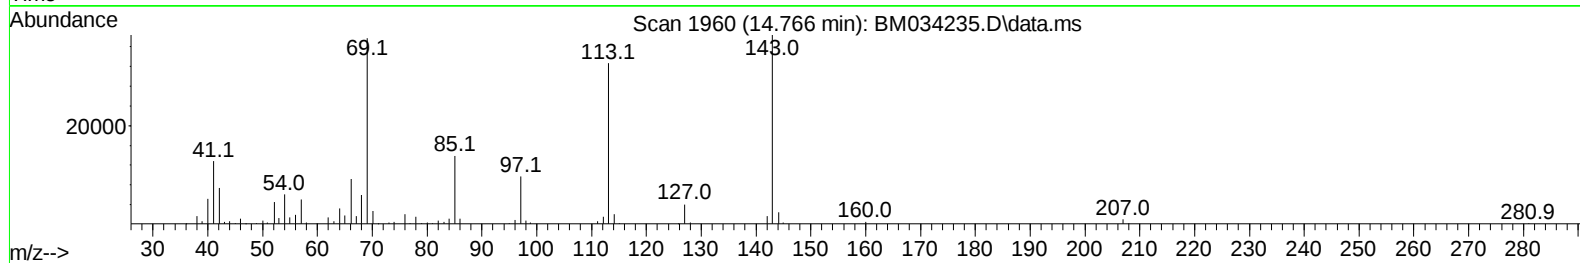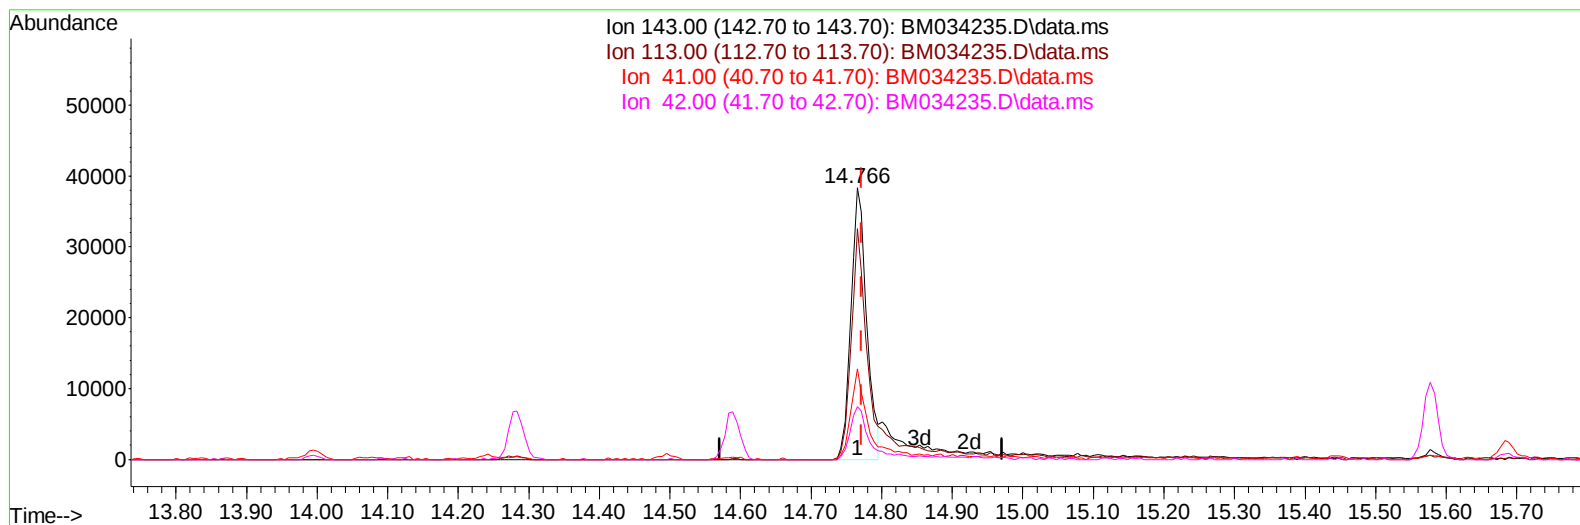

TIC: BM034235.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (-0.006) 13.59 ng/u1

response 59793

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	85.03
41.00	31.90	33.48
42.00	19.10	19.46




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034235.D
 Acq On : 11 Mar 2022 23:26
 Operator : CG/JU
 Sample : N1816-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 01:52:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

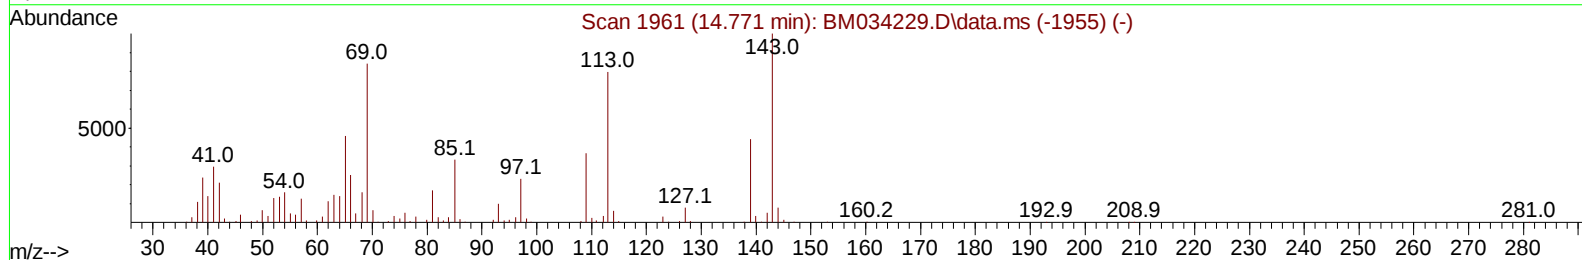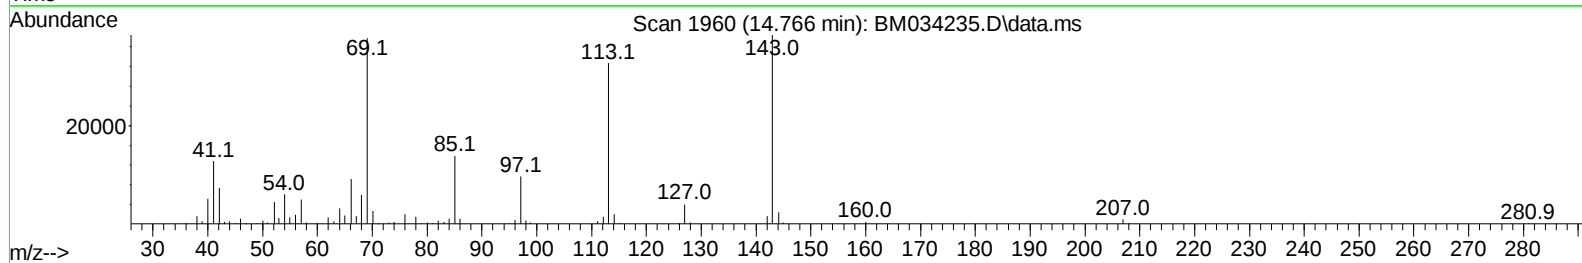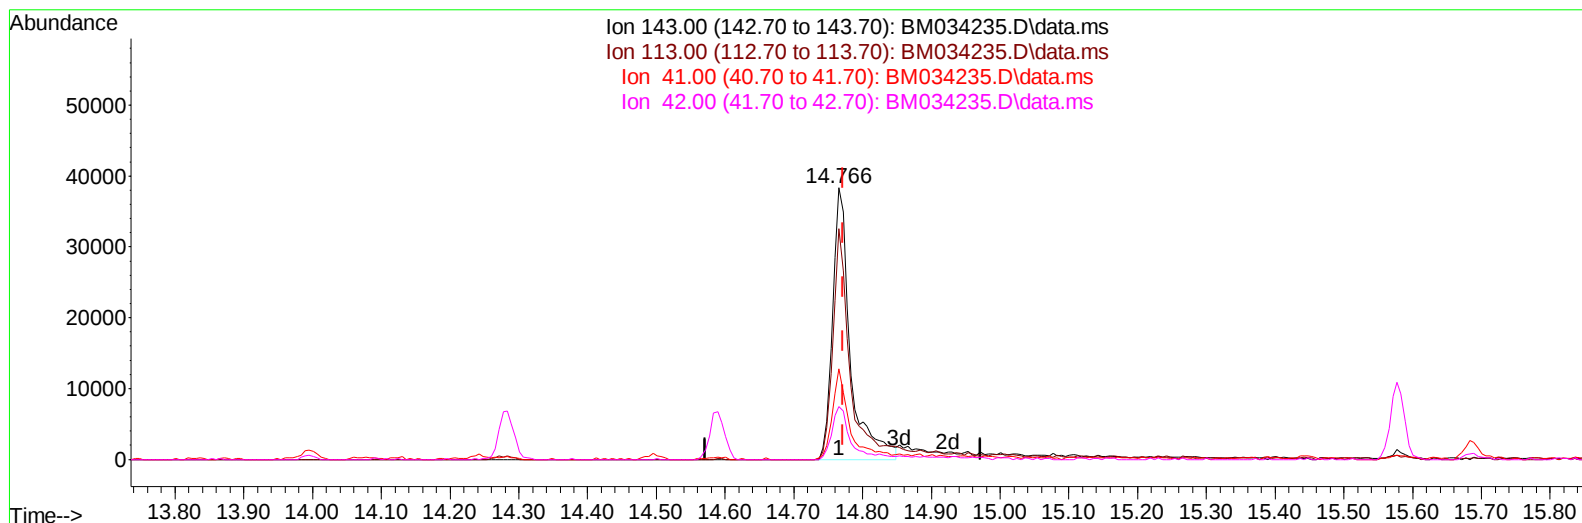

TIC: BM034235.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.766min (-0.006) 15.73 ng/ul m

response 69190

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	85.03
41.00	31.90	33.48
42.00	19.10	19.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034235.D
 Acq On : 11 Mar 2022 23:26
 Operator : CG/JU
 Sample : N1816-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 12 01:52:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.948	152	152819	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	596340	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.589	164	388065	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.330	188	751840	20.000	ng/ul	0.00
79) Chrysene-d12	21.500	240	672552	20.000	ng/ul	0.00
88) Perylene-d12	23.918	264	761300	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	18422	5.262	ng/uL	0.00
4) Pyridine-d5	3.749	84	62967	7.554	ng/ul	0.00
7) Phenol-d5	7.101	99	286359	28.001	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.272	67	185172	30.864	ng/ul	0.00
11) 2-Chlorophenol-d4	7.478	132	270296	30.583	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	249974	28.580	ng/ul	0.00
21) Nitrobenzene-d5	9.107	128	132165	30.898	ng/ul	0.00
24) 2-Nitrophenol-d4	9.836	143	127754	26.934	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.378	165	271897	28.594	ng/ul	0.00
31) 4-Chloroaniline-d4	10.889	131	325588	27.533	ng/ul	0.00
46) Dimethylphthalate-d6	13.995	166	755435	26.754	ng/ul	0.00
49) Acenaphthylene-d8	14.283	160	1080713	30.135	ng/ul	0.00
54) 4-Nitrophenol-d4	14.766	143	69190m	15.731	ng/ul	0.00
60) Fluorene-d10	15.577	176	756359	30.600	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.689	200	64559	13.572	ng/ul	0.00
73) Anthracene-d10	17.430	188	1111700	31.306	ng/ul	0.00
81) Pyrene-d10	19.712	212	1258139	34.362	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.759	264	1169481	31.137	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034235.D
Acq On : 11 Mar 2022 23:26
Operator : CG/JU
Sample : N1816-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 12 01:52:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

