




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034237.D
 Acq On : 12 Mar 2022 00:38
 Operator : CG/JU
 Sample : N1816-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

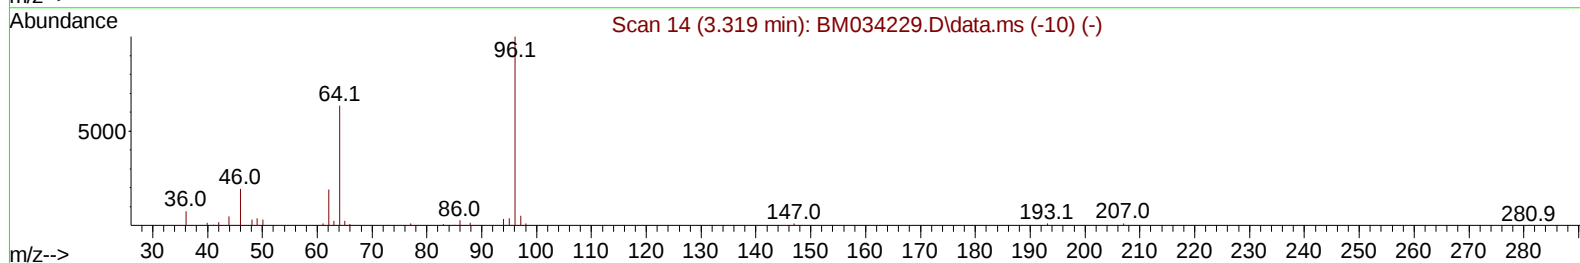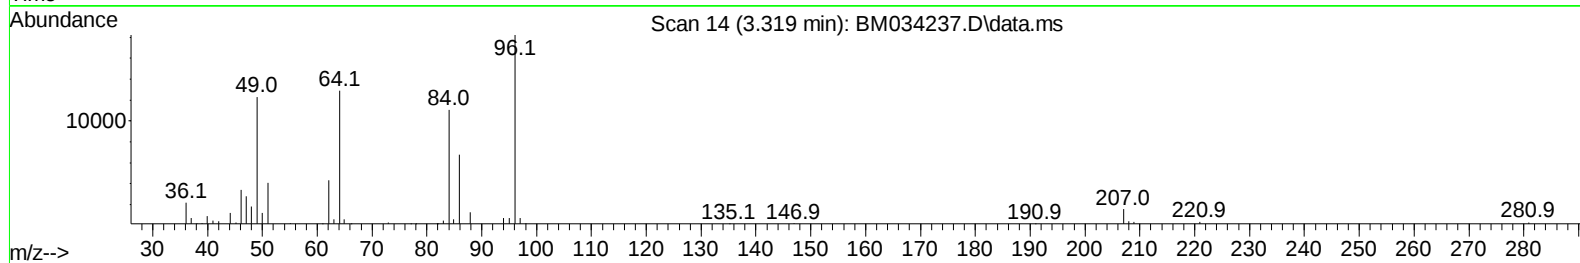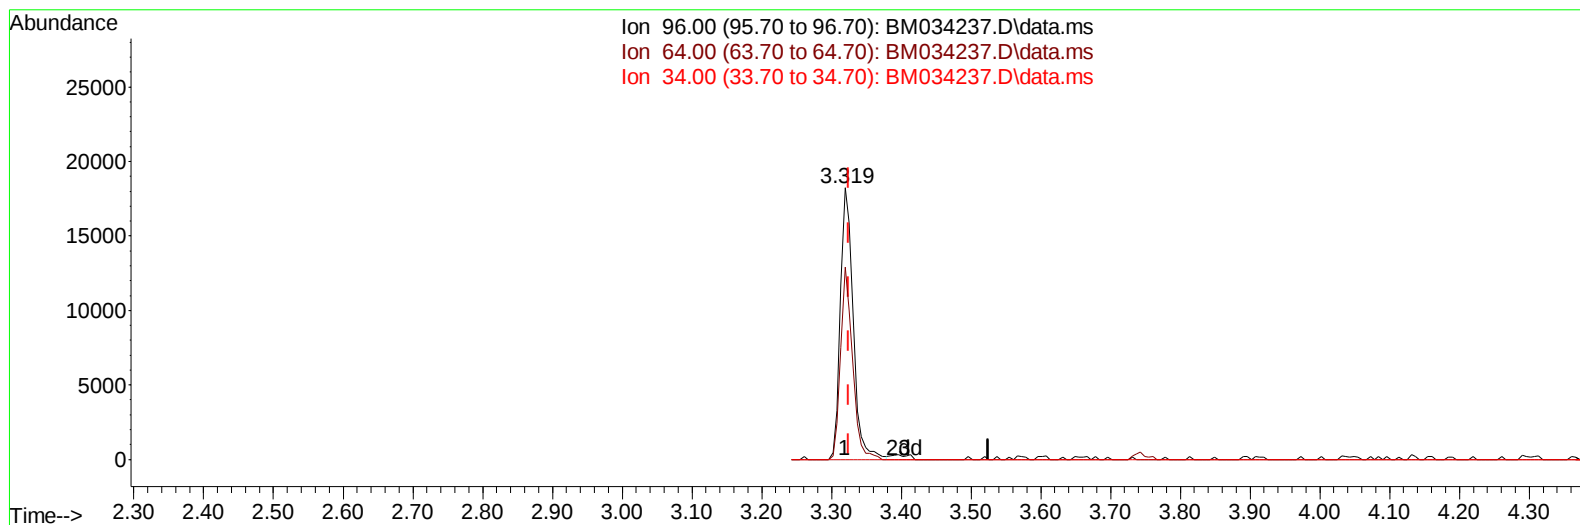

TIC: BM034237.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.006) 6.91 ng/uL

response 23249

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	70.88
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034237.D
 Acq On : 12 Mar 2022 00:38
 Operator : CG/JU
 Sample : N1816-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

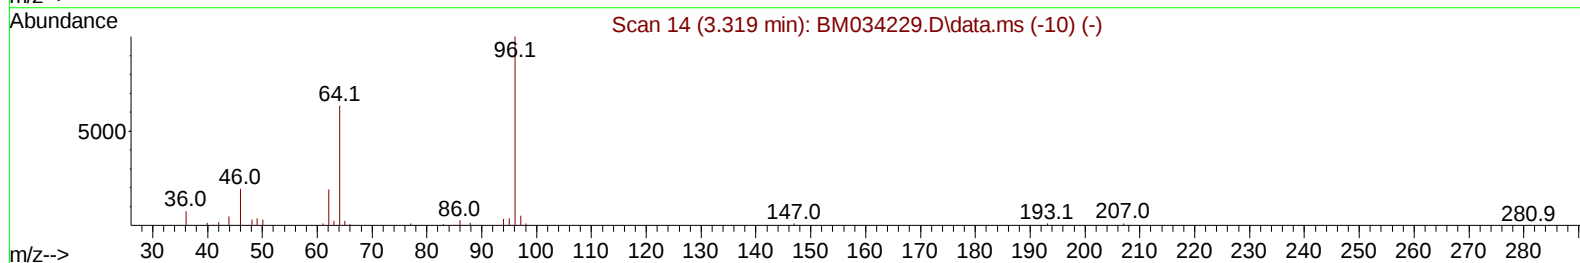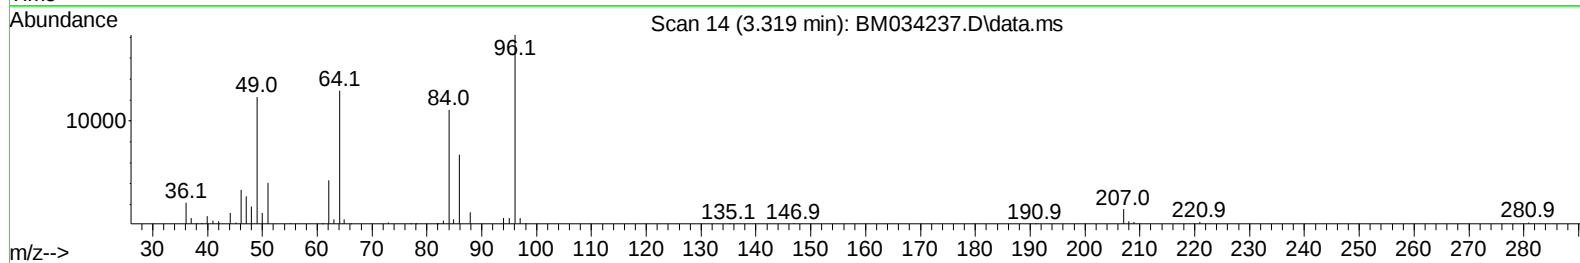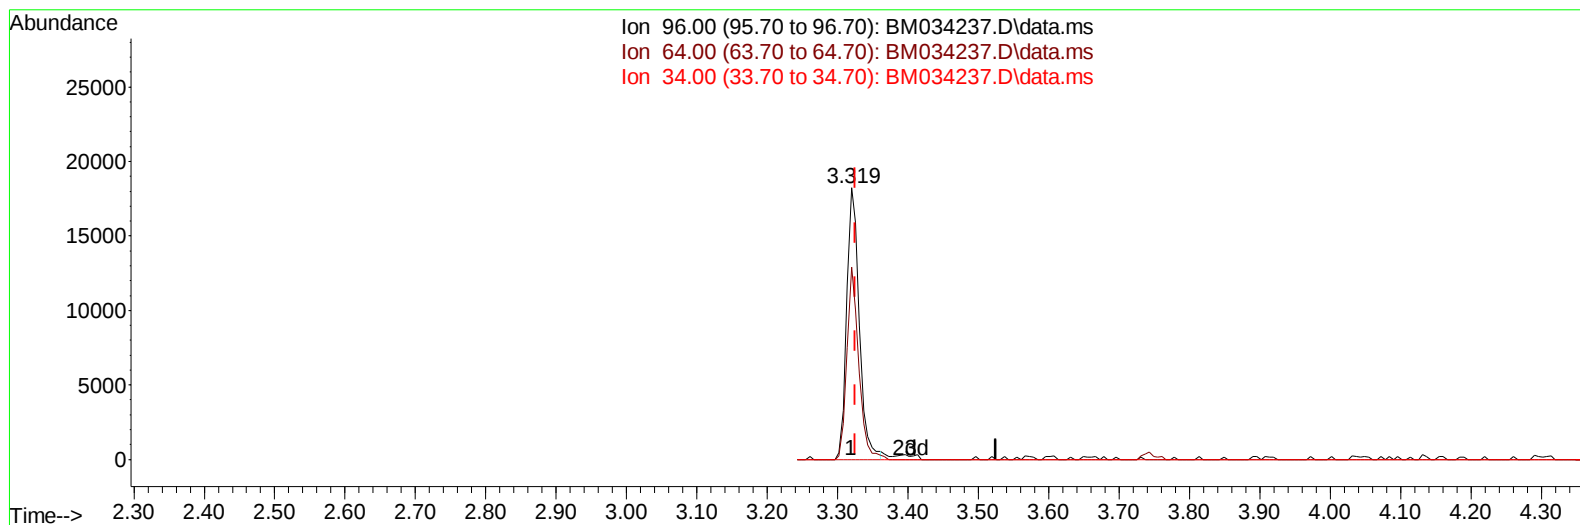

TIC: BM034237.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.319min (-0.006) 6.83 ng/uL m

response 22979

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	68.90	70.88
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034237.D
Acq On : 12 Mar 2022 00:38
Operator : CG/JU
Sample : N1816-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

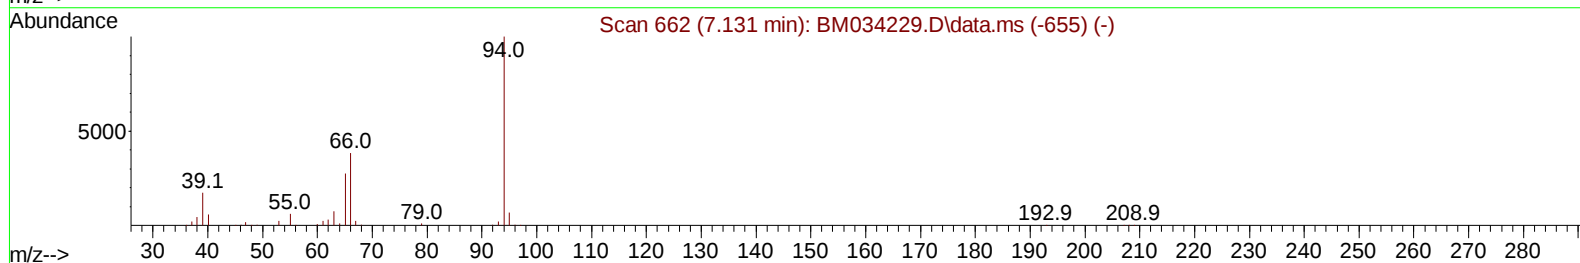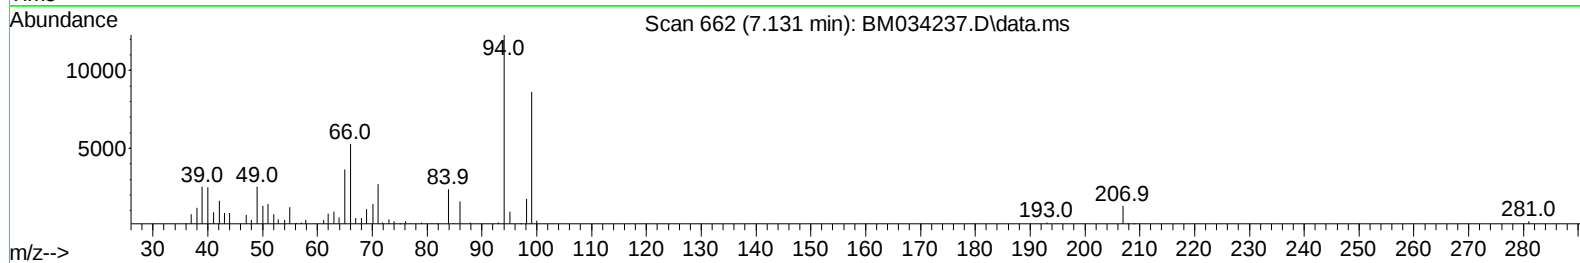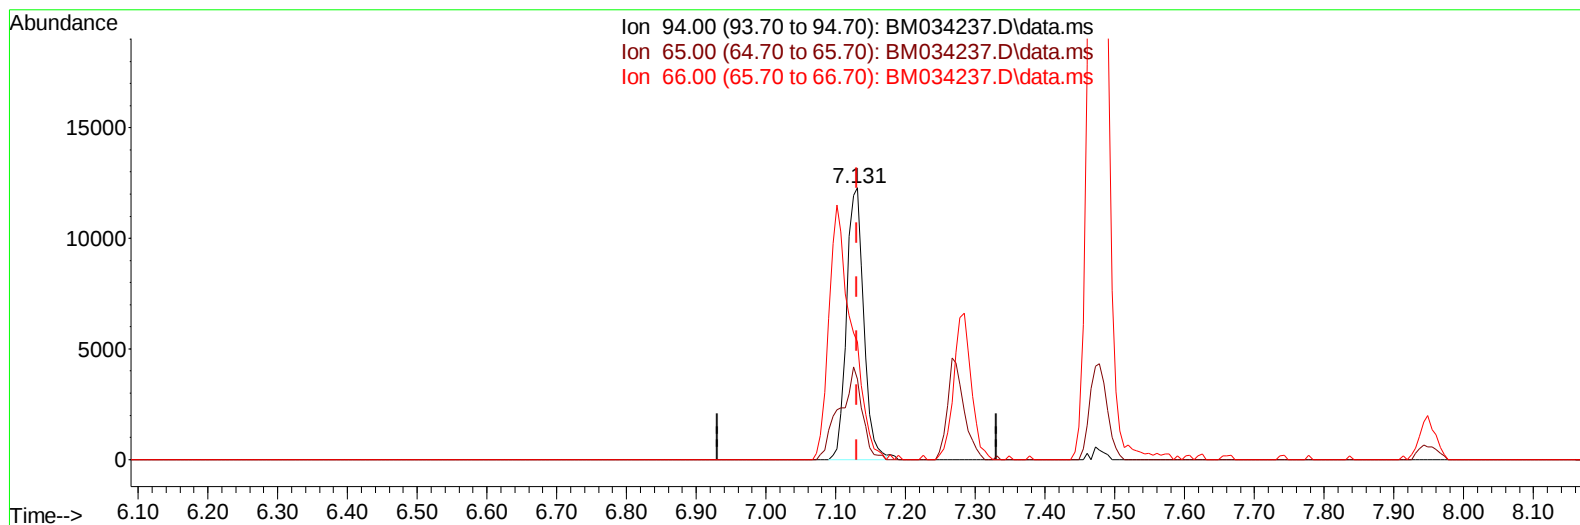

TIC: BM034237.D\data.ms

(8) Phenol

7.131min (+ 0.000) 2.16 ng/u1

response 20961

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	29.64
66.00	42.10	43.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034237.D
Acq On : 12 Mar 2022 00:38
Operator : CG/JU
Sample : N1816-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

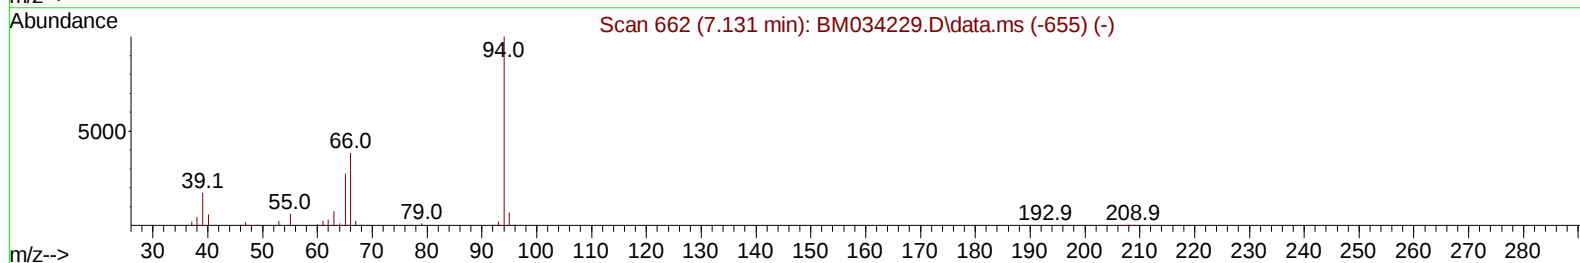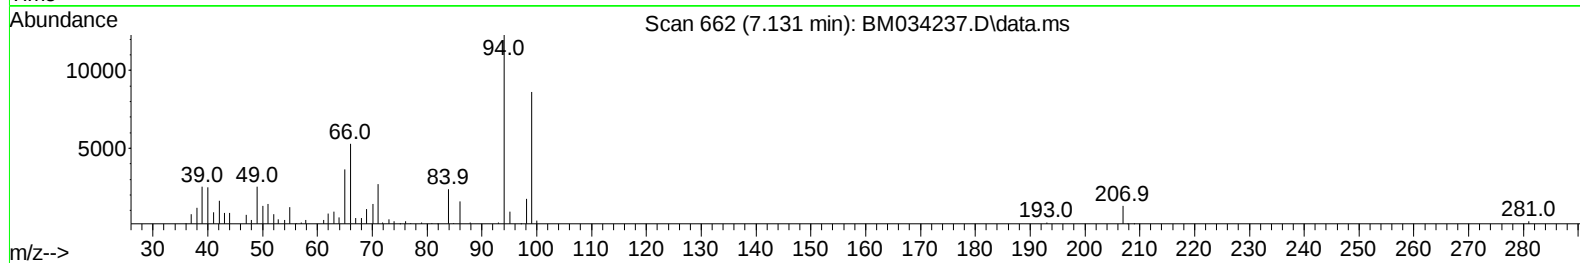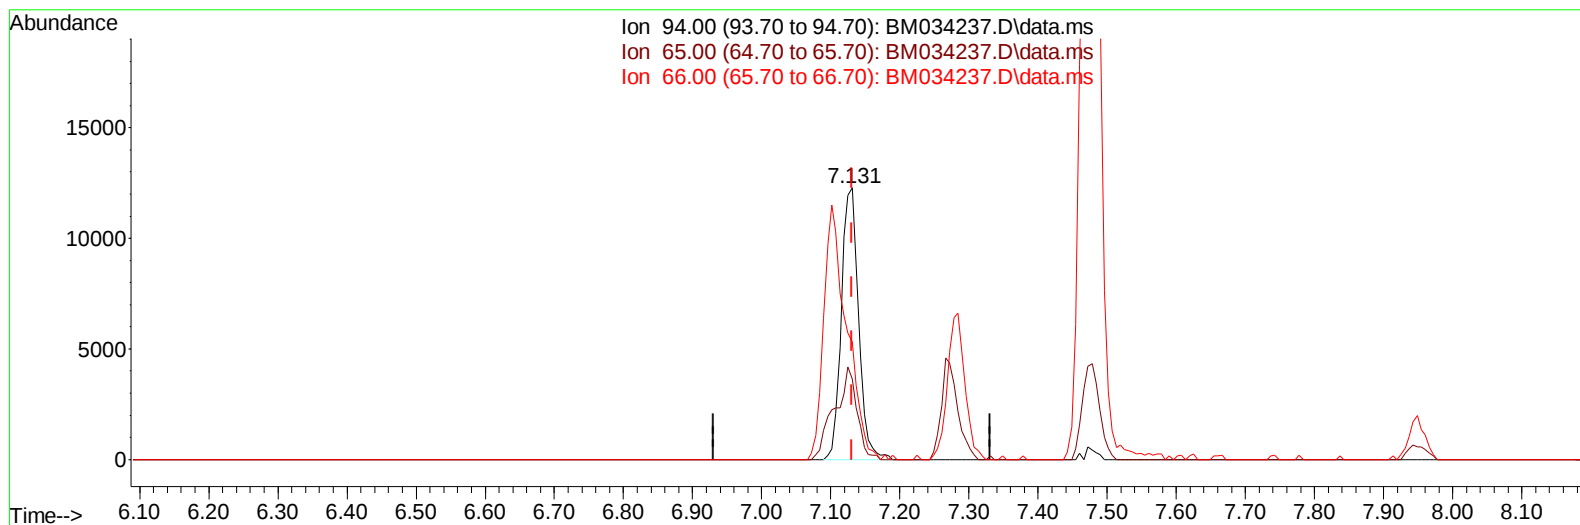

TIC: BM034237.D\data.ms

(8) Phenol

7.131min (+ 0.000) 2.17 ng/u1 m

response 21092

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	28.60	29.64
66.00	42.10	43.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034237.D
Acq On : 12 Mar 2022 00:38
Operator : CG/JU
Sample : N1816-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

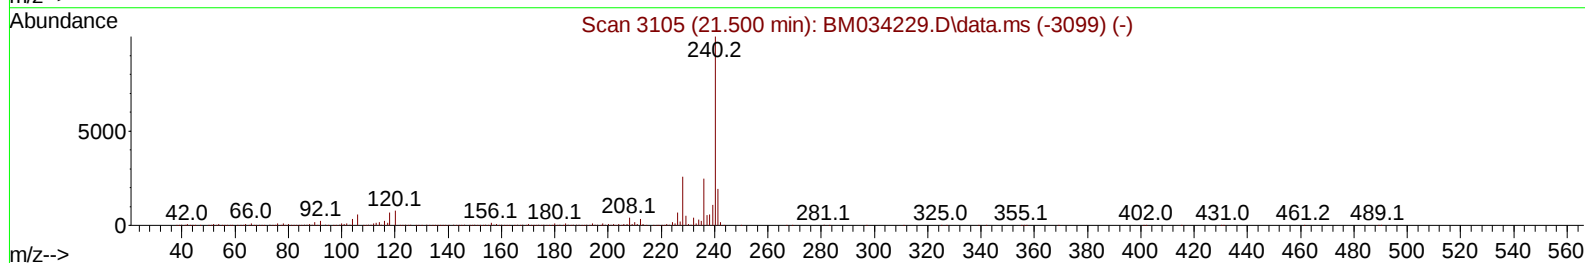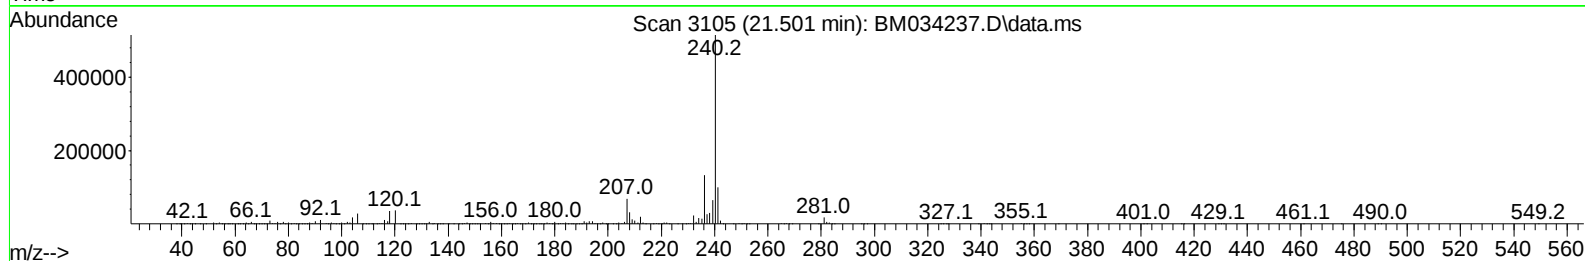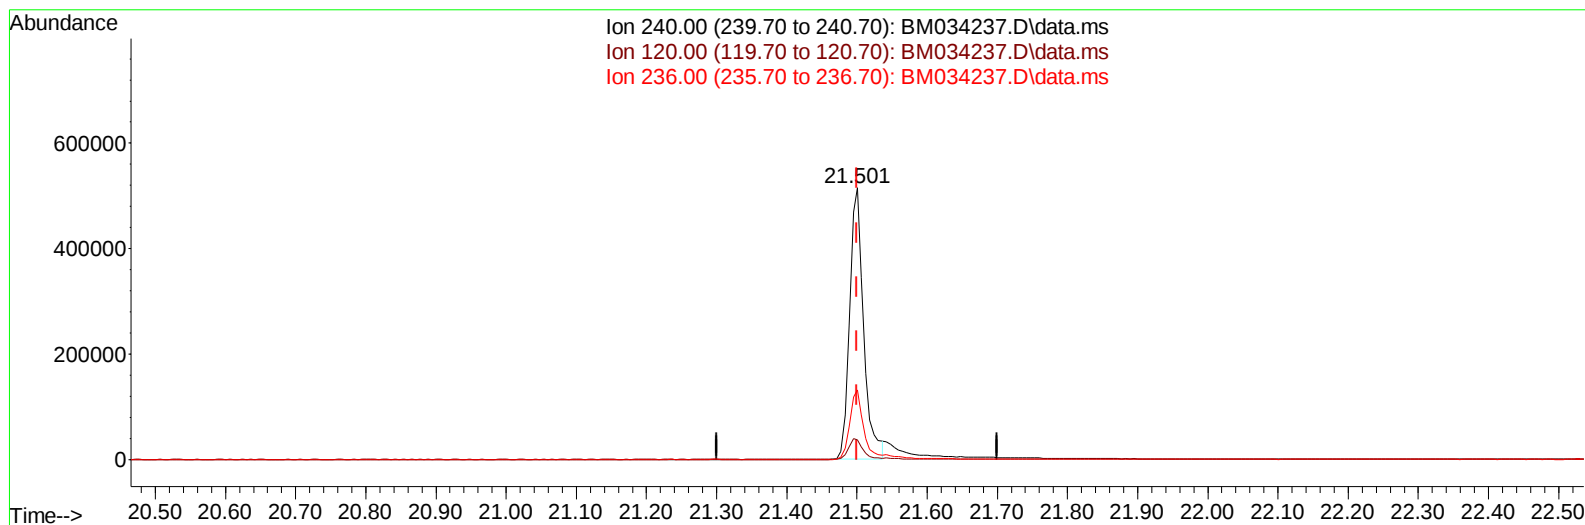

TIC: BM034237.D\data.ms

(79) Chrysene-d12 (I)

21.501min (+ 0.000) 20.00 ng/u1

response 718404

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	7.12
236.00	24.80	25.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034237.D
 Acq On : 12 Mar 2022 00:38
 Operator : CG/JU
 Sample : N1816-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

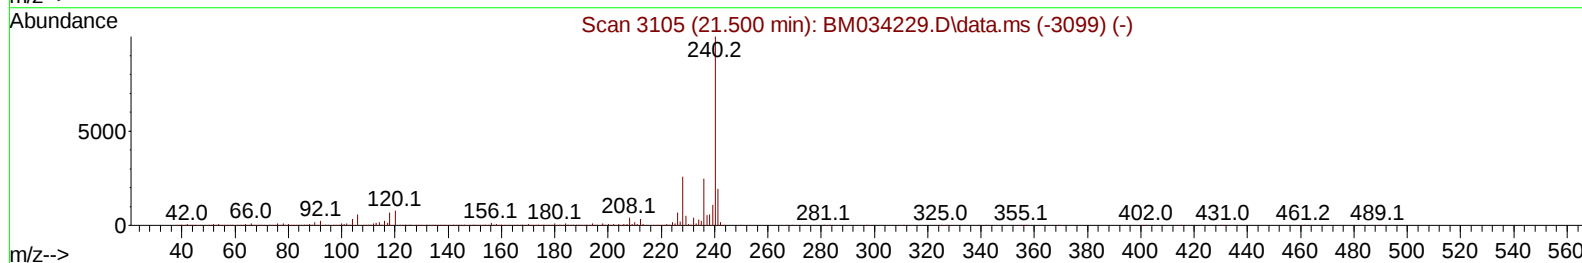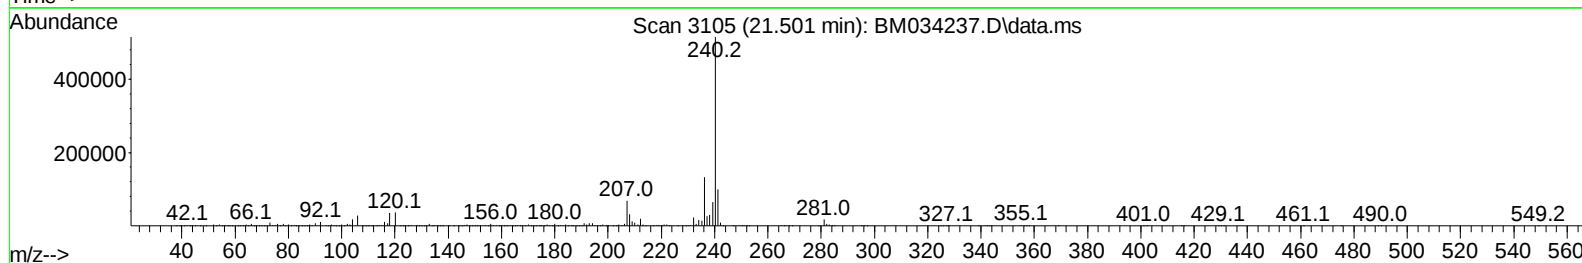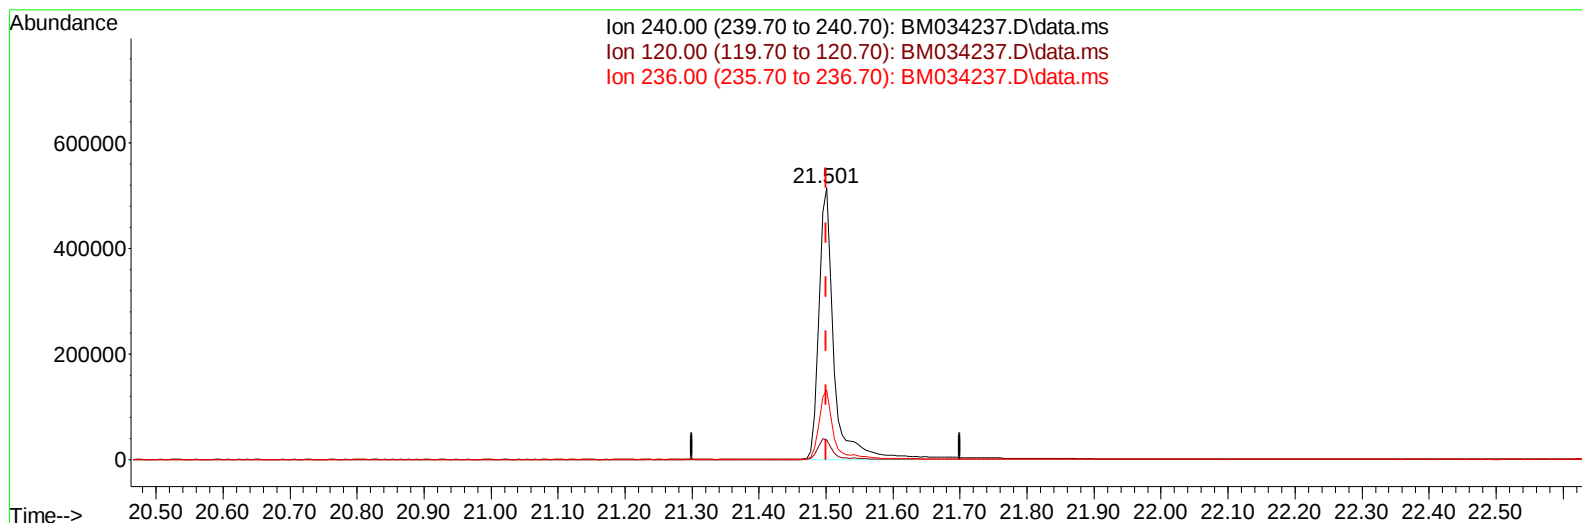

TIC: BM034237.D\data.ms

(79) Chrysene-d12 (I)

21.501min (+ 0.000) 20.00 ng/ul m

response 792449

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.90	7.12
236.00	24.80	25.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034237.D
 Acq On : 12 Mar 2022 00:38
 Operator : CG/JU
 Sample : N1816-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE1

Manual IntegrationsAPPROVED

Quant Time: Mar 12 02:25:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 11 02:00:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/14/2022
 Supervised By :mohammad ahmed 03/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.949	152	146893	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	573829	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.589	164	362670	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.330	188	746770	20.000	ng/ul	0.00
79) Chrysene-d12	21.501	240	792449m	20.000	ng/ul	0.00
88) Perylene-d12	23.918	264	900535	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.319	96	22979m	6.828	ng/uL	0.00
4) Pyridine-d5	3.743	84	273081	34.085	ng/ul	0.00
7) Phenol-d5	7.102	99	336006	34.181	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.272	67	208550	36.163	ng/ul	0.00
11) 2-Chlorophenol-d4	7.478	132	308717	36.339	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	284568	33.848	ng/ul	0.00
21) Nitrobenzene-d5	9.107	128	148884	36.172	ng/ul	0.00
24) 2-Nitrophenol-d4	9.837	143	164368	36.013	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.378	165	313178	34.227	ng/ul	0.00
31) 4-Chloroaniline-d4	10.890	131	381872	33.559	ng/ul	0.00
46) Dimethylphthalate-d6	13.995	166	987859	37.435	ng/ul	0.00
49) Acenaphthylene-d8	14.283	160	1239663	36.987	ng/ul	0.00
54) 4-Nitrophenol-d4	14.766	143	115155	28.016	ng/ul	0.00
60) Fluorene-d10	15.577	176	867394	37.550	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.689	200	135902	28.764	ng/ul	0.00
73) Anthracene-d10	17.424	188	1333267	37.800	ng/ul	0.00
81) Pyrene-d10	19.712	212	1649041	38.224	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.765	264	1694536	38.141	ng/ul	0.00
Target Compounds						
						Qvalue
8) Phenol	7.131	94	21092m	2.175	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034237.D
Acq On : 12 Mar 2022 00:38
Operator : CG/JU
Sample : N1816-16
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/14/2022
Supervised By :mohammad ahmed 03/14/2022

Quant Time: Mar 12 02:25:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 11 02:00:05 2022
Response via : Initial Calibration

