

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034214.D
 Acq On : 11 Mar 2022 10:09
 Operator : CG/JU
 Sample : PB143172BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	19	rVB	26296	32388	1.64%	0.148%
2	3.743	83	86	104	rBV	265435	387843	19.64%	1.767%
3	4.090	142	145	151	rVB	14968	21588	1.09%	0.098%
4	6.607	572	573	576	rBV3	2174	2331	0.12%	0.011%
5	7.101	651	657	666	rBV	270040	433407	21.95%	1.975%
6	7.272	680	686	698	rVB	249346	398834	20.20%	1.817%
7	7.478	714	721	730	rBV	322372	517109	26.19%	2.356%
8	7.572	735	737	740	rVV3	2522	2243	0.11%	0.010%
9	7.884	788	790	792	rBV3	2009	2317	0.12%	0.011%
10	7.948	795	801	810	rVV	418905	664323	33.64%	3.027%
11	8.654	914	921	934	rBV	351935	586616	29.71%	2.673%
12	9.113	991	999	1009	rBV	286220	496608	25.15%	2.263%
13	9.837	1116	1122	1131	rBV	227824	396622	20.09%	1.807%
14	10.378	1208	1214	1225	rBV	392519	663534	33.60%	3.024%
15	10.513	1232	1237	1239	rVB6	1671	2605	0.13%	0.012%
16	10.766	1272	1280	1289	rVB	551338	928833	47.04%	4.232%
17	10.895	1294	1302	1321	rBV	307132	605445	30.66%	2.759%
18	11.131	1338	1342	1345	rBV4	1539	2116	0.11%	0.010%
19	11.325	1372	1375	1377	rBV3	1846	2177	0.11%	0.010%
20	12.354	1546	1550	1551	rBV3	4384	4845	0.25%	0.022%
21	12.772	1619	1621	1628	rBV4	1349	2520	0.13%	0.011%
22	12.983	1653	1657	1662	rVB4	2067	2867	0.15%	0.013%
23	13.995	1823	1829	1842	rBV	798956	1124824	56.97%	5.126%
24	14.101	1845	1847	1851	rVB4	2142	2808	0.14%	0.013%
25	14.283	1871	1878	1888	rBV	902405	1309349	66.31%	5.966%
26	14.395	1896	1897	1901	rVB3	2286	2218	0.11%	0.010%
27	14.589	1923	1930	1941	rBV	890960	1316395	66.67%	5.999%
28	14.766	1954	1960	1976	rBV	134141	287563	14.56%	1.310%
29	15.401	2067	2068	2072	rVB3	2231	2005	0.10%	0.009%
30	15.577	2092	2098	2111	rBV	1121121	1662241	84.18%	7.574%
31	15.689	2111	2117	2131	rVB	253945	390917	19.80%	1.781%
32	15.818	2137	2139	2143	rVB4	6049	6237	0.32%	0.028%
33	15.930	2157	2158	2163	rVB4	2188	2088	0.11%	0.010%
34	17.001	2338	2340	2346	rBV5	1507	2548	0.13%	0.012%
35	17.118	2356	2360	2365	rVB4	3603	5432	0.28%	0.025%
36	17.330	2389	2396	2404	rBV	1018841	1449532	73.41%	6.605%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034214.D
 Acq On : 11 Mar 2022 10:09
 Operator : CG/JU
 Sample : PB143172BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

37	17.430	2407	2413	2428	rVV	1143420	1675379	84.85%	7.634%
38	17.677	2452	2455	2457	rBV4	2676	2823	0.14%	0.013%
39	18.118	2527	2530	2534	rBV6	3110	3812	0.19%	0.017%
40	18.171	2537	2539	2544	rVB5	1889	2380	0.12%	0.011%
41	18.348	2565	2569	2573	rBV5	2724	3993	0.20%	0.018%
42	19.283	2725	2728	2733	rBV4	13652	19796	1.00%	0.090%
43	19.354	2737	2740	2745	rVV2	8801	14991	0.76%	0.068%
44	19.712	2796	2801	2819	rBV	1325346	1974547	100.00%	8.998%
45	21.500	3100	3105	3120	rBV	823350	1408166	71.32%	6.417%
46	23.759	3483	3489	3507	rBV2	728092	1706984	86.45%	7.778%
47	23.918	3510	3516	3530	rVB2	628351	1411131	71.47%	6.430%




Sum of corrected areas: 21945330

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034214.D
Acq On : 11 Mar 2022 10:09
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

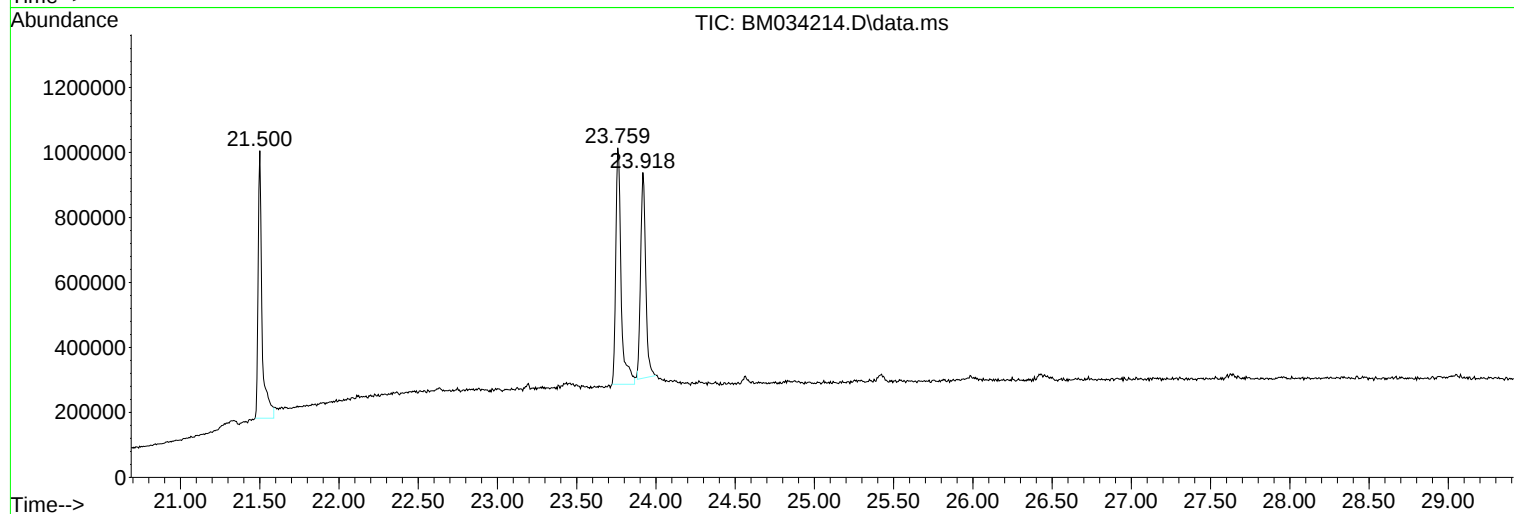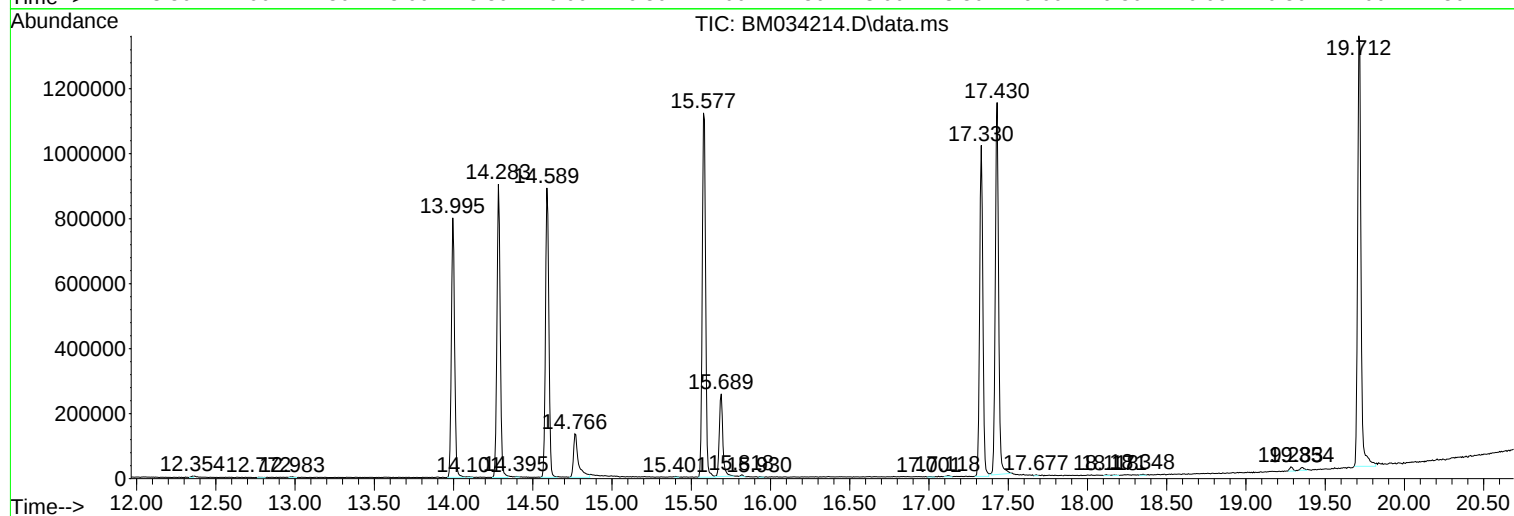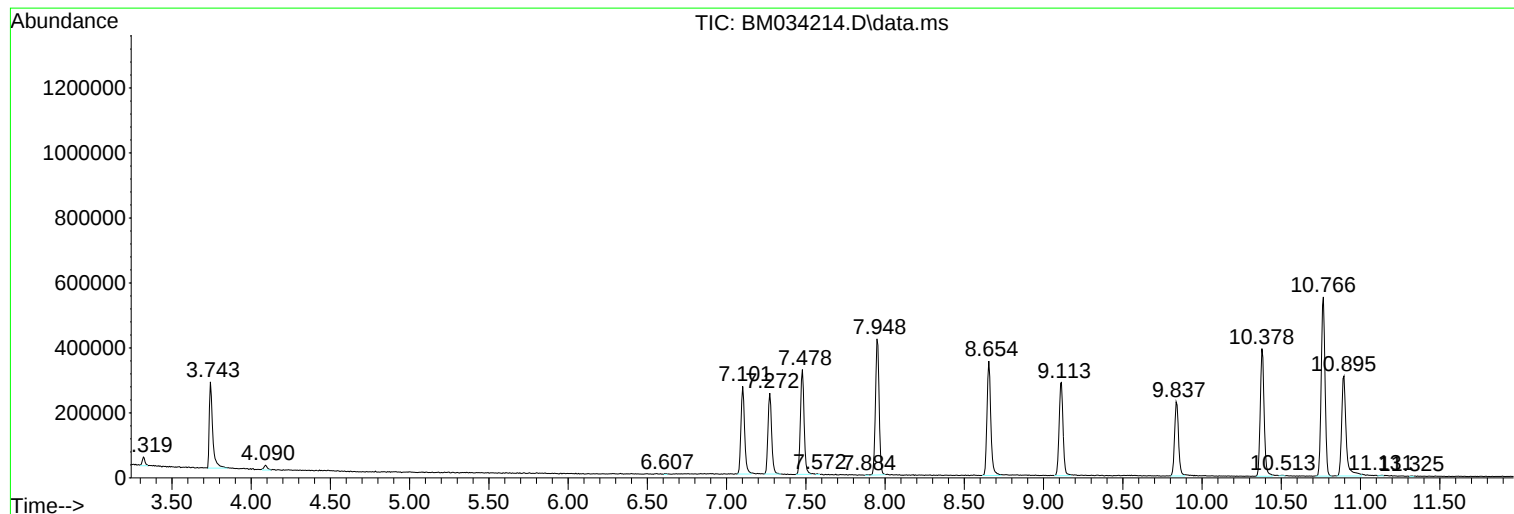

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034214.D
Acq On : 11 Mar 2022 10:09
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034214.D
Acq On : 11 Mar 2022 10:09
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------