

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034225.D
 Acq On : 11 Mar 2022 16:47
 Operator : CG/JU
 Sample : N1816-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	21	rVB	42218	53234	1.50%	0.146%
2	3.743	82	86	100	rBV	471535	649480	18.29%	1.780%
3	4.090	142	145	151	rVB2	12054	15435	0.43%	0.042%
4	5.025	301	304	310	rVB4	8073	11973	0.34%	0.033%
5	7.101	650	657	666	rBV	544985	863656	24.32%	2.367%
6	7.272	680	686	698	rVB	464391	738887	20.81%	2.025%
7	7.478	714	721	735	rBV	638135	997651	28.10%	2.734%
8	7.954	794	802	810	rBV	469221	765760	21.57%	2.099%
9	8.013	810	812	819	rVB5	5753	9389	0.26%	0.026%
10	8.654	914	921	933	rBV	722506	1183055	33.32%	3.242%
11	8.860	951	956	960	rBV7	2415	4877	0.14%	0.013%
12	9.113	991	999	1010	rBV	573171	945510	26.63%	2.591%
13	9.289	1027	1029	1032	rVB4	4217	4026	0.11%	0.011%
14	9.572	1069	1077	1083	rVB	32305	54464	1.53%	0.149%
15	9.842	1115	1123	1135	rBV	454248	792553	22.32%	2.172%
16	10.377	1207	1214	1230	rBV	768750	1316965	37.09%	3.609%
17	10.766	1272	1280	1289	rVB	636968	1056034	29.74%	2.894%
18	10.895	1295	1302	1314	rBV	654993	1161300	32.71%	3.183%
19	11.695	1433	1438	1443	rBV5	2806	4934	0.14%	0.014%
20	11.807	1452	1457	1463	rBV6	3792	7848	0.22%	0.022%
21	12.201	1518	1524	1531	rVB4	13258	22733	0.64%	0.062%
22	12.360	1544	1551	1555	rBV3	9647	20040	0.56%	0.055%
23	12.936	1646	1649	1652	rBV3	2780	3563	0.10%	0.010%
24	13.007	1659	1661	1666	rVB4	4429	5639	0.16%	0.015%
25	13.089	1672	1675	1681	rVB4	2765	5300	0.15%	0.015%
26	13.154	1681	1686	1689	rVV5	4182	7259	0.20%	0.020%
27	13.430	1728	1733	1743	rVB	19381	29487	0.83%	0.081%
28	14.001	1823	1830	1841	rBV	1371920	1967382	55.41%	5.392%
29	14.283	1870	1878	1890	rBV	1620690	2420654	68.17%	6.634%
30	14.501	1911	1915	1921	rVB6	5286	7383	0.21%	0.020%
31	14.595	1924	1931	1942	rBV	973771	1462517	41.19%	4.008%
32	14.765	1952	1960	1984	rBV	329369	636449	17.92%	1.744%
33	14.942	1988	1990	1997	rVV5	5367	10744	0.30%	0.029%
34	15.001	1997	2000	2005	rVB6	4914	8429	0.24%	0.023%
35	15.583	2090	2099	2111	rBV	2082069	2988315	84.16%	8.189%
36	15.689	2111	2117	2134	rVV	491764	720572	20.29%	1.975%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034225.D
 Acq On : 11 Mar 2022 16:47
 Operator : CG/JU
 Sample : N1816-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

37	15.818	2136	2139	2145	rVB	8619	13405	0.38%	0.037%
38	17.124	2354	2361	2365	rBV7	4799	9620	0.27%	0.026%
39	17.330	2390	2396	2407	rBV	1150452	1633709	46.01%	4.477%
40	17.430	2407	2413	2426	rBV	2121382	2997780	84.43%	8.215%
41	18.006	2508	2511	2514	rBV4	6557	8244	0.23%	0.023%
42	18.224	2544	2548	2554	rBV2	47555	66473	1.87%	0.182%
43	18.659	2619	2622	2625	rVB4	7736	8283	0.23%	0.023%
44	19.024	2681	2684	2689	rBV6	4227	7427	0.21%	0.020%
45	19.289	2724	2729	2735	rBV3	27144	45367	1.28%	0.124%
46	19.353	2735	2740	2743	rBV2	40288	56377	1.59%	0.155%
47	19.495	2761	2764	2768	rBV6	15911	23337	0.66%	0.064%
48	19.718	2796	2802	2809	rBV	2539777	3550813	100.00%	9.731%
49	21.212	3052	3056	3061	rBV2	126282	169103	4.76%	0.463%
50	21.500	3100	3105	3122	rBV	1047144	1736380	48.90%	4.759%
51	23.765	3483	3490	3498	rBV2	1582393	3255275	91.68%	8.921%
52	23.924	3510	3517	3537	rVB	856650	1954605	55.05%	5.357%




Sum of corrected areas: 36489695

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034225.D
Acq On : 11 Mar 2022 16:47
Operator : CG/JU
Sample : N1816-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

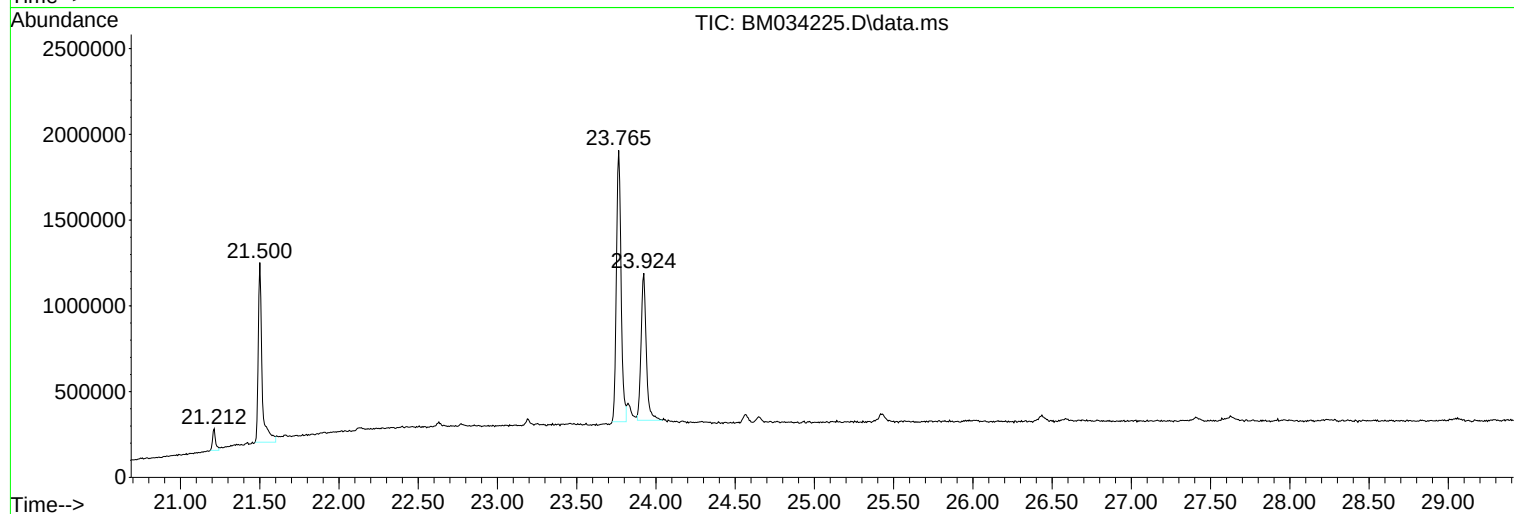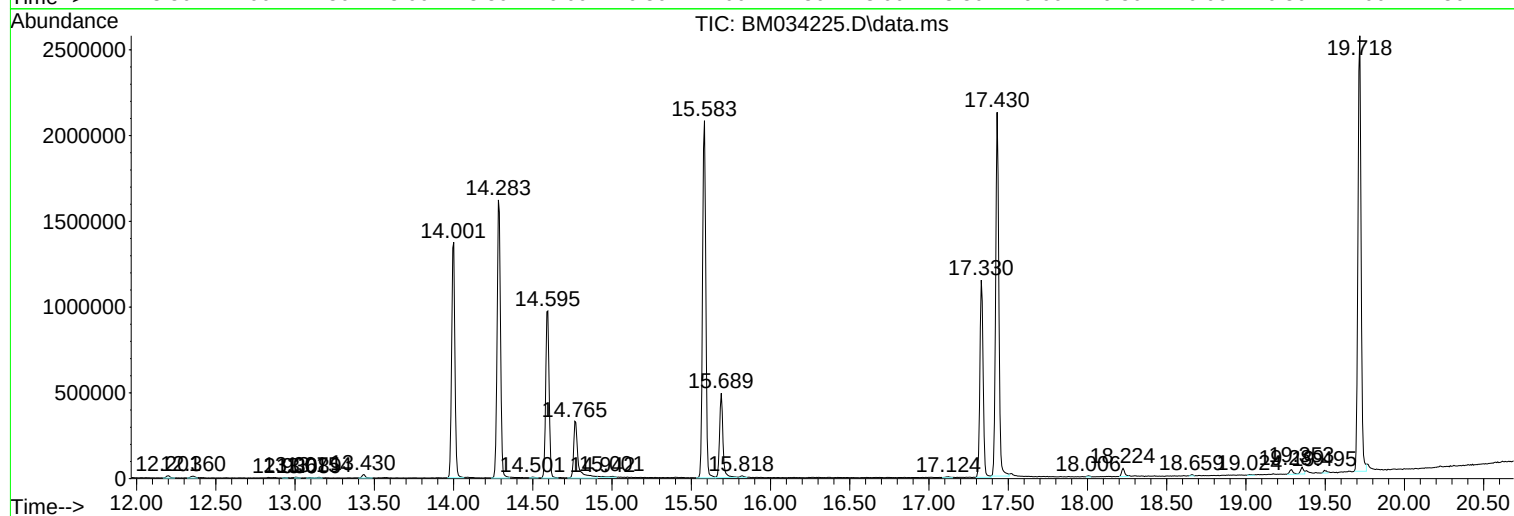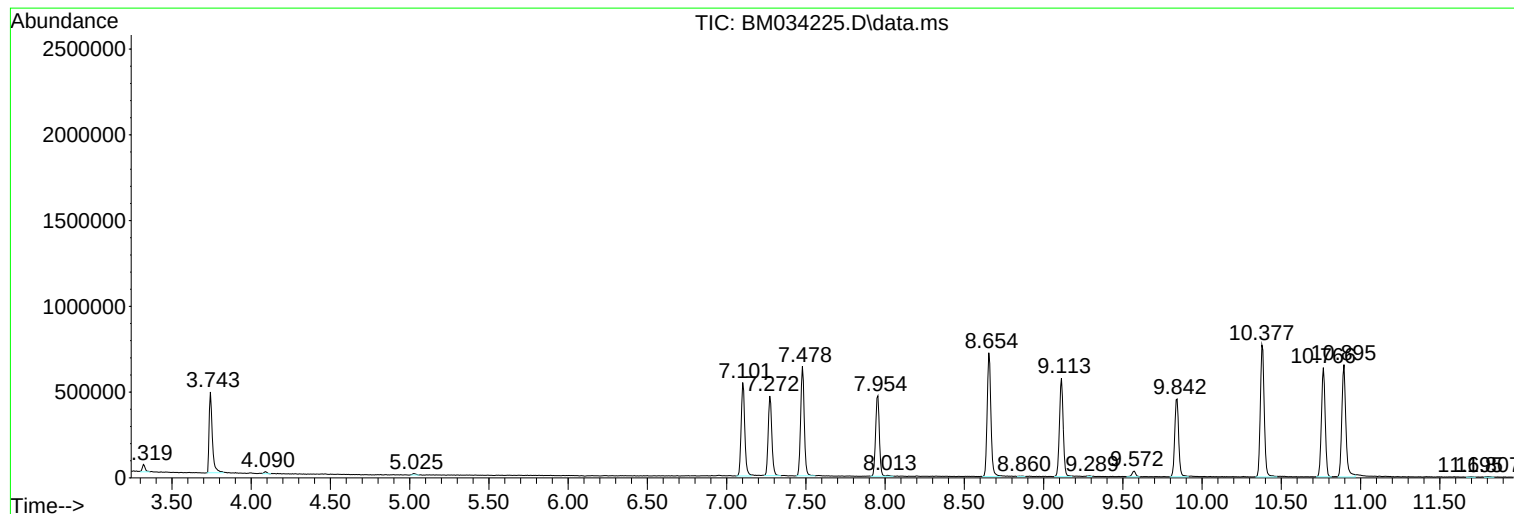

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034225.D
Acq On : 11 Mar 2022 16:47
Operator : CG/JU
Sample : N1816-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034225.D
Acq On : 11 Mar 2022 16:47
Operator : CG/JU
Sample : N1816-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------