

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034230.D
 Acq On : 11 Mar 2022 20:25
 Operator : CG/JU
 Sample : PB143172BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK172

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	22	rVB	33781	45018	1.98%	0.175%
2	3.743	83	86	103	rBV	323628	461517	20.26%	1.795%
3	4.090	142	145	152	rVB	18404	23595	1.04%	0.092%
4	7.101	650	657	665	rBV	348081	547636	24.03%	2.130%
5	7.272	680	686	697	rVB	313607	483496	21.22%	1.881%
6	7.478	714	721	731	rBV	407764	640837	28.13%	2.493%
7	7.948	794	801	815	rVB	511984	810864	35.59%	3.154%
8	8.654	914	921	933	rBV	445879	741695	32.55%	2.885%
9	9.107	991	998	1007	rBV	358600	600901	26.37%	2.338%
10	9.836	1115	1122	1132	rBV	287304	494582	21.71%	1.924%
11	9.948	1139	1141	1144	rVB4	2484	2628	0.12%	0.010%
12	10.378	1207	1214	1228	rBV	488201	826496	36.27%	3.215%
13	10.766	1272	1280	1288	rBV	653778	1115897	48.97%	4.341%
14	10.889	1294	1301	1313	rBV	388768	729927	32.04%	2.840%
15	11.072	1331	1332	1336	rVB4	2875	2407	0.11%	0.009%
16	11.983	1480	1487	1491	rBV7	1567	3437	0.15%	0.013%
17	12.360	1545	1551	1556	rBV4	5182	10132	0.44%	0.039%
18	12.966	1652	1654	1659	rBV5	1563	2300	0.10%	0.009%
19	13.995	1823	1829	1843	rBV	922811	1294477	56.81%	5.036%
20	14.089	1843	1845	1851	rVB4	2342	3792	0.17%	0.015%
21	14.283	1871	1878	1888	rBV	1072562	1542186	67.68%	6.000%
22	14.589	1923	1930	1941	rBV	1063609	1523515	66.86%	5.927%
23	14.766	1954	1960	1972	rBV	186422	352417	15.47%	1.371%
24	15.318	2051	2054	2057	rBV4	1846	2525	0.11%	0.010%
25	15.395	2064	2067	2073	rVB6	3838	7243	0.32%	0.028%
26	15.577	2091	2098	2111	rBV	1338563	1931685	84.78%	7.515%
27	15.689	2111	2117	2127	rBV	300267	459324	20.16%	1.787%
28	15.818	2136	2139	2145	rVB6	7472	11180	0.49%	0.043%
29	16.936	2326	2329	2335	rBV6	1273	2470	0.11%	0.010%
30	17.112	2358	2359	2366	rVB4	3618	4555	0.20%	0.018%
31	17.330	2389	2396	2406	rBV	1178019	1666145	73.12%	6.482%
32	17.430	2406	2413	2429	rVB	1275554	1926169	84.54%	7.493%
33	18.206	2542	2545	2547	rBV4	2024	2879	0.13%	0.011%
34	18.777	2640	2642	2645	rBV4	2233	2449	0.11%	0.010%
35	19.283	2724	2728	2732	rBV4	14268	19799	0.87%	0.077%
36	19.353	2736	2740	2747	rBV3	11842	22793	1.00%	0.089%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034230.D
Acq On : 11 Mar 2022 20:25
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Title : SVOA CALIBRATION

37	19.712	2795	2801	2820	rBV	1622400	2278515	100.00%	8.864%
38	21.500	3100	3105	3119	rBV	990392	1618413	71.03%	6.296%
39	23.759	3483	3489	3497	rBV2	887035	1867591	81.97%	7.265%
40	23.918	3510	3516	3527	rVB2	767013	1621633	71.17%	6.309%




Sum of corrected areas: 25705120

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034230.D
Acq On : 11 Mar 2022 20:25
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

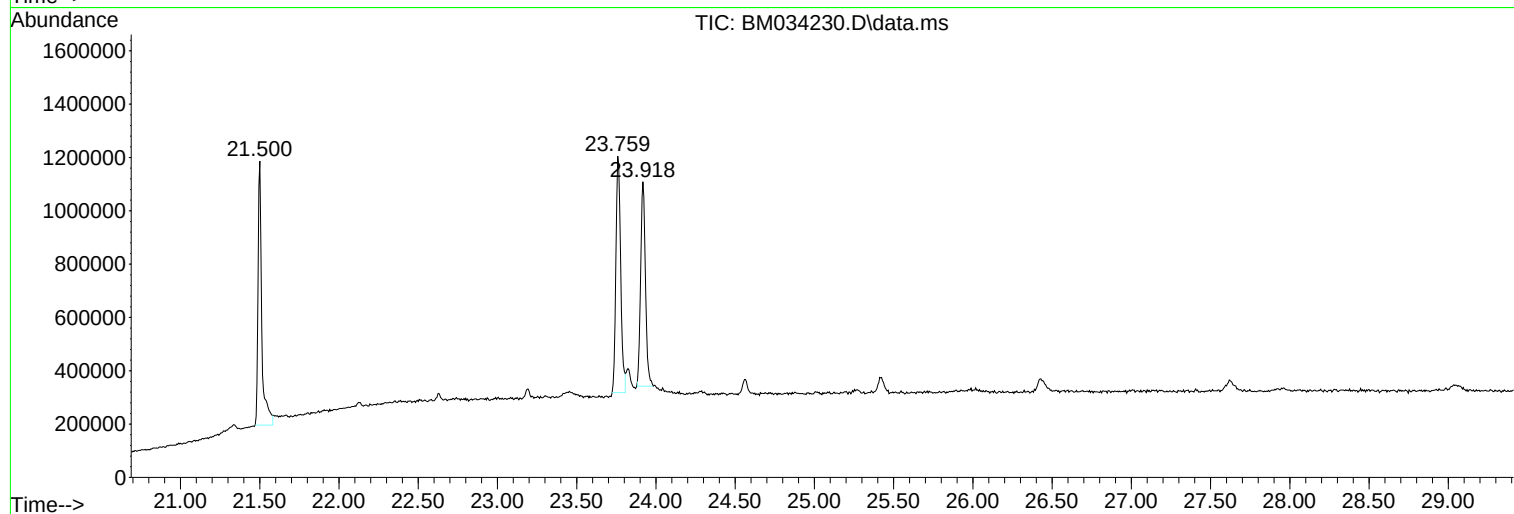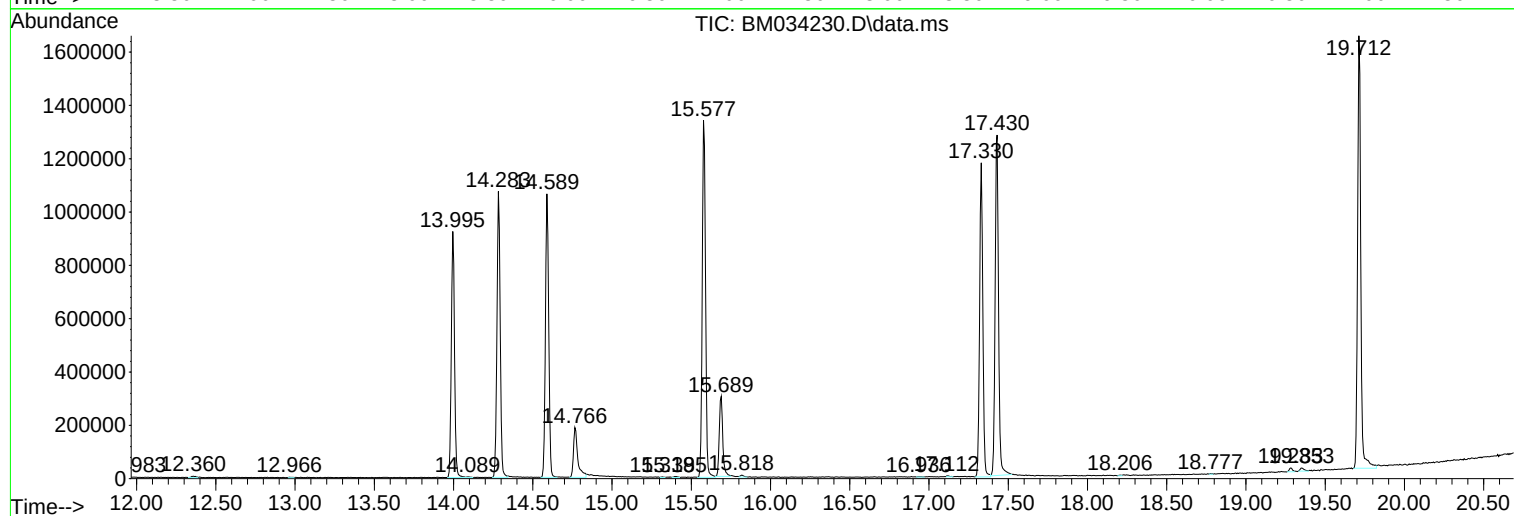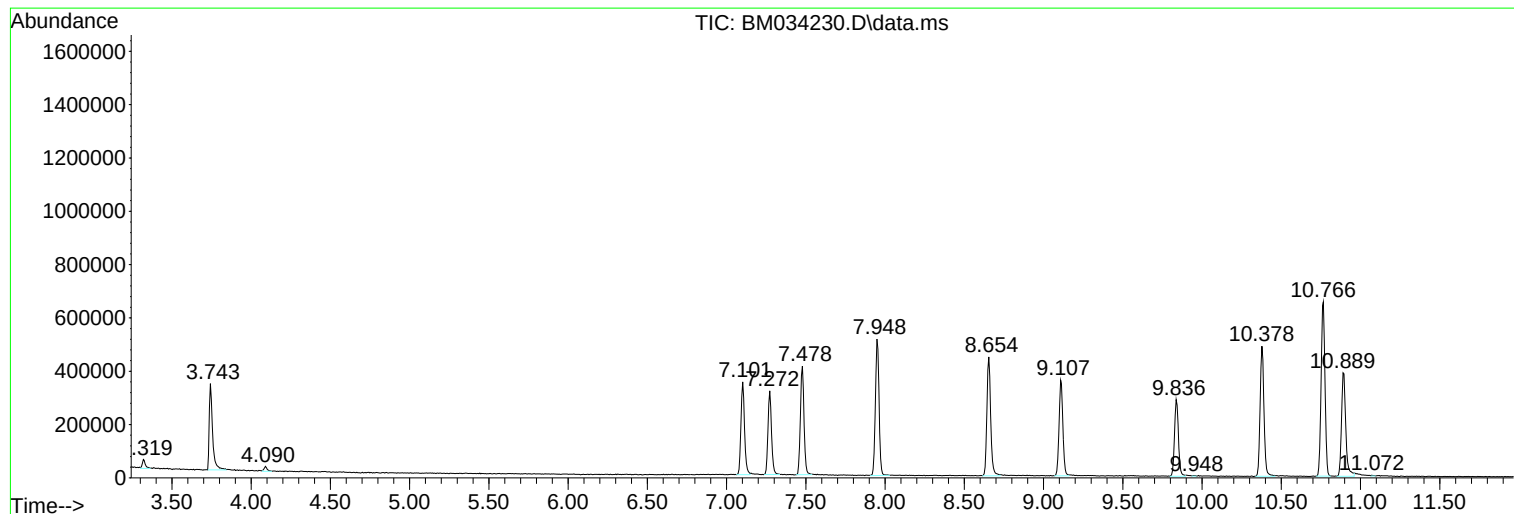

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034230.D
Acq On : 11 Mar 2022 20:25
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034230.D
Acq On : 11 Mar 2022 20:25
Operator : CG/JU
Sample : PB143172BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK172

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc