

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034231.D
 Acq On : 11 Mar 2022 21:01
 Operator : CG/JU
 Sample : N1816-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	22	rVB	49256	63206	1.81%	0.166%
2	3.743	82	86	107	rBV	519136	741642	21.24%	1.942%
3	4.090	141	145	150	rVB4	12692	16185	0.46%	0.042%
4	5.025	301	304	309	rVB3	8234	11340	0.32%	0.030%
5	5.172	327	329	333	rBV5	2480	3538	0.10%	0.009%
6	6.948	629	631	636	rVB4	4067	5448	0.16%	0.014%
7	7.101	650	657	671	rBV	625855	986121	28.25%	2.583%
8	7.272	680	686	695	rBV	512358	795766	22.79%	2.084%
9	7.478	714	721	735	rBV	696760	1096657	31.41%	2.872%
10	7.584	735	739	747	rVB8	3718	7974	0.23%	0.021%
11	7.948	795	801	809	rBV	556800	892446	25.56%	2.337%
12	8.019	810	813	820	rVB4	6412	10971	0.31%	0.029%
13	8.654	914	921	934	rBV	807582	1312711	37.60%	3.438%
14	9.107	990	998	1011	rBV	596116	1013820	29.04%	2.655%
15	9.289	1024	1029	1033	rVB6	4444	7517	0.22%	0.020%
16	9.566	1071	1076	1083	rVB	35815	56742	1.63%	0.149%
17	9.837	1114	1122	1140	rBV	511625	878638	25.17%	2.301%
18	10.378	1206	1214	1226	rBV	854980	1424940	40.82%	3.732%
19	10.766	1268	1280	1287	rBV	720752	1230334	35.24%	3.222%
20	10.895	1294	1302	1316	rBV	688248	1256068	35.98%	3.290%
21	11.795	1452	1455	1459	rBV3	2741	4197	0.12%	0.011%
22	12.195	1519	1523	1531	rBV	16246	25584	0.73%	0.067%
23	12.289	1535	1539	1544	rBV6	2216	4886	0.14%	0.013%
24	12.354	1544	1550	1557	rVB2	11173	19859	0.57%	0.052%
25	12.830	1626	1631	1634	rBV5	2981	5876	0.17%	0.015%
26	12.930	1643	1648	1653	rBV6	3228	4466	0.13%	0.012%
27	13.007	1656	1661	1664	rVB4	5234	7047	0.20%	0.018%
28	13.089	1669	1675	1680	rBV7	4075	6459	0.19%	0.017%
29	13.148	1680	1685	1689	rVB5	4803	6234	0.18%	0.016%
30	13.430	1726	1733	1739	rBV	26751	36097	1.03%	0.095%
31	13.995	1823	1829	1841	rBV	1430686	1999571	57.28%	5.237%
32	14.283	1871	1878	1889	rBV	1716321	2488025	71.27%	6.516%
33	14.501	1910	1915	1918	rBV5	5019	6097	0.17%	0.016%
34	14.589	1922	1930	1942	rBV	1145916	1641131	47.01%	4.298%
35	14.766	1954	1960	1974	rBV	362188	630381	18.06%	1.651%
36	14.995	1998	1999	2003	rVB4	4093	4535	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034231.D
 Acq On : 11 Mar 2022 21:01
 Operator : CG/JU
 Sample : N1816-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

37	15.577	2091	2098	2111	rBV	2067541	3014876	86.36%	7.896%
38	15.689	2111	2117	2126	rBV	485180	711316	20.38%	1.863%
39	15.818	2136	2139	2144	rVB2	10020	13444	0.39%	0.035%
40	16.260	2208	2214	2218	rBV7	2970	6530	0.19%	0.017%
41	17.118	2352	2360	2364	rBV5	4312	8651	0.25%	0.023%
42	17.330	2390	2396	2405	rBV	1284762	1782937	51.07%	4.670%
43	17.430	2406	2413	2424	rBV	2087204	2992123	85.71%	7.837%
44	18.007	2505	2511	2514	rBV6	6544	10065	0.29%	0.026%
45	18.224	2542	2548	2557	rBV2	53804	82098	2.35%	0.215%
46	19.283	2724	2728	2733	rBV4	25948	33880	0.97%	0.089%
47	19.354	2736	2740	2743	rBV	28801	42148	1.21%	0.110%
48	19.495	2761	2764	2769	rBV6	16967	25650	0.73%	0.067%
49	19.718	2795	2802	2808	rBV	2512111	3491013	100.00%	9.143%
50	21.206	3052	3055	3060	rBV	127189	171711	4.92%	0.450%
51	21.500	3100	3105	3118	rBV	1158617	1811874	51.90%	4.745%
52	23.765	3483	3490	3498	rBV	1550822	3200159	91.67%	8.381%
53	23.918	3510	3516	3533	rVB2	925124	2080815	59.60%	5.450%




Sum of corrected areas: 38181799

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034231.D
Acq On : 11 Mar 2022 21:01
Operator : CG/JU
Sample : N1816-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

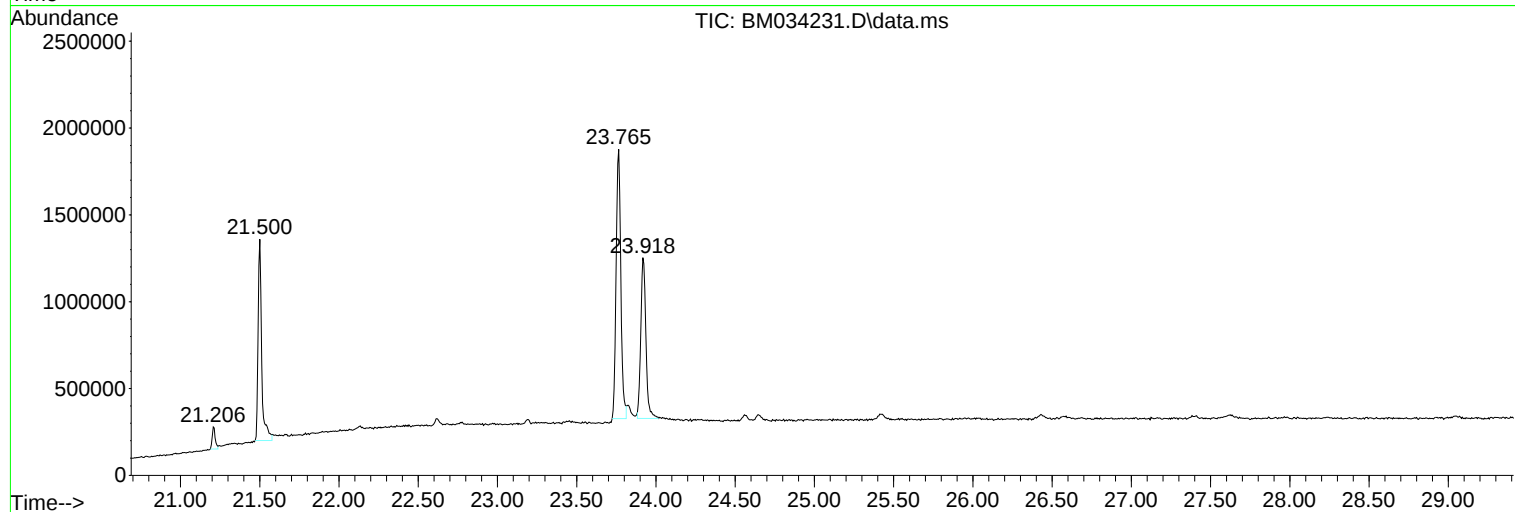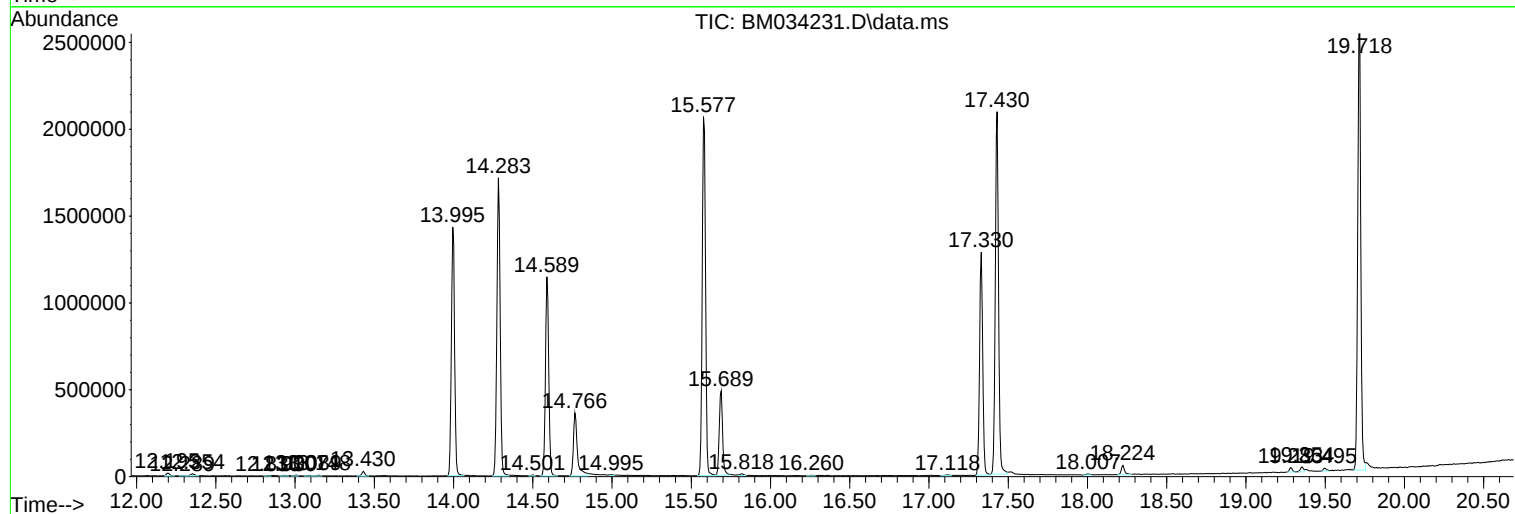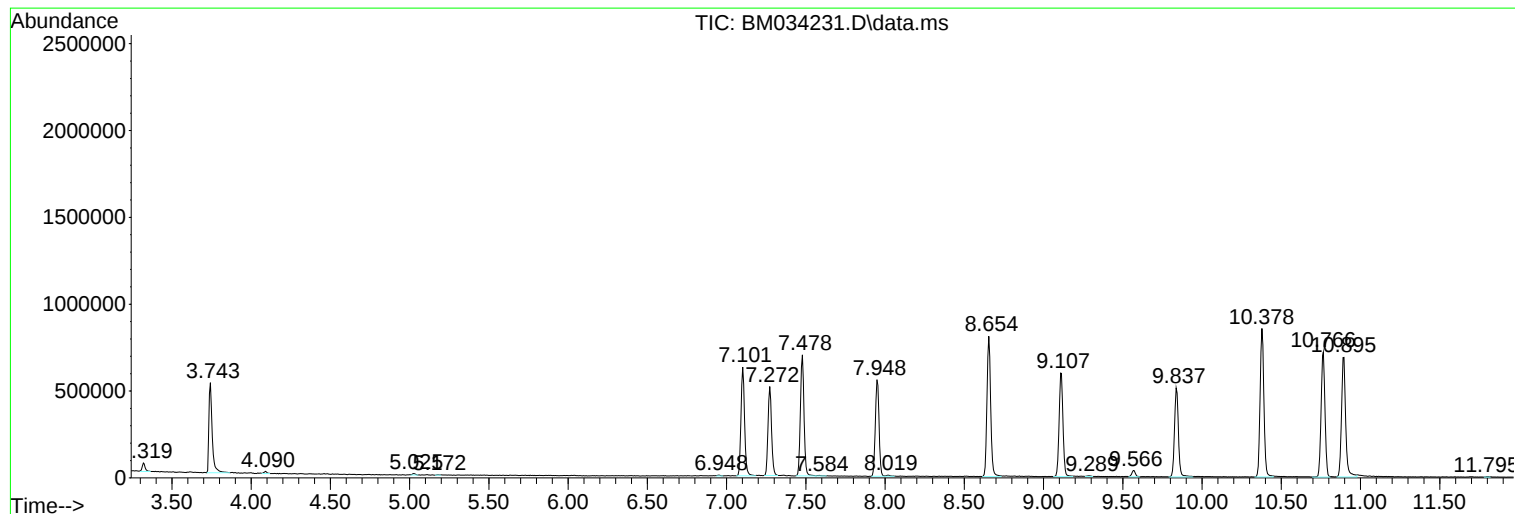

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034231.D
Acq On : 11 Mar 2022 21:01
Operator : CG/JU
Sample : N1816-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034231.D
Acq On : 11 Mar 2022 21:01
Operator : CG/JU
Sample : N1816-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------