

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	19	rVB	25090	32235	1.55%	0.126%
2	3.748	84	87	96	rBV	103852	154998	7.46%	0.606%
3	4.090	142	145	150	rVB3	11815	15483	0.75%	0.061%
4	5.560	390	395	397	rBV4	2324	3965	0.19%	0.016%
5	6.913	624	625	629	rBV3	2429	2455	0.12%	0.010%
6	6.948	629	631	633	rVV3	3316	3405	0.16%	0.013%
7	7.101	651	657	670	rBV	317982	540790	26.03%	2.116%
8	7.272	680	686	701	rVV	290885	463377	22.30%	1.813%
9	7.478	714	721	731	rBV	375965	606502	29.19%	2.373%
10	7.948	794	801	810	rBV	555413	875455	42.13%	3.425%
11	8.013	810	812	820	rVB6	5517	8988	0.43%	0.035%
12	8.195	839	843	846	rBV3	2063	2794	0.13%	0.011%
13	8.430	880	883	886	rVB4	1863	2309	0.11%	0.009%
14	8.654	914	921	936	rBV	418631	697262	33.56%	2.728%
15	8.777	940	942	947	rVB5	3865	4643	0.22%	0.018%
16	9.113	992	999	1010	rBV	334363	569303	27.40%	2.227%
17	9.289	1025	1029	1033	rVB8	3044	5098	0.25%	0.020%
18	9.566	1071	1076	1083	rVB2	17124	28044	1.35%	0.110%
19	9.836	1116	1122	1132	rBV	236501	400176	19.26%	1.566%
20	10.260	1190	1194	1198	rBV4	1729	2866	0.14%	0.011%
21	10.377	1206	1214	1227	rBV	455458	771292	37.12%	3.017%
22	10.554	1240	1244	1247	rBV5	2664	4096	0.20%	0.016%
23	10.766	1271	1280	1287	rVV	698808	1192505	57.39%	4.665%
24	10.895	1293	1302	1314	rBV	370946	681639	32.81%	2.667%
25	11.248	1359	1362	1366	rBV4	1989	2635	0.13%	0.010%
26	12.071	1498	1502	1507	rVB5	3089	5221	0.25%	0.020%
27	12.195	1518	1523	1526	rBV7	3143	4182	0.20%	0.016%
28	12.354	1545	1550	1557	rVB4	5408	9473	0.46%	0.037%
29	12.865	1634	1637	1640	rVB4	1763	2415	0.12%	0.009%
30	12.960	1650	1653	1657	rVB5	2404	2982	0.14%	0.012%
31	13.089	1669	1675	1676	rBV4	2299	3417	0.16%	0.013%
32	13.113	1676	1679	1682	rVV4	2604	3593	0.17%	0.014%
33	13.148	1682	1685	1689	rVV4	2170	3191	0.15%	0.012%
34	13.207	1692	1695	1702	rVB7	4203	7371	0.35%	0.029%
35	13.430	1728	1733	1739	rBV2	13438	17106	0.82%	0.067%
36	13.501	1739	1745	1750	rVV7	2536	5700	0.27%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

37	13.565	1752	1756	1759	rVV4	2411	4116	0.20%	0.016%
38	13.871	1804	1808	1810	rBV3	2376	2695	0.13%	0.011%
39	13.895	1810	1812	1815	rVV3	2122	2427	0.12%	0.009%
40	13.995	1823	1829	1841	rVV	771885	1072202	51.60%	4.195%
41	14.124	1847	1851	1854	rVB5	3168	4501	0.22%	0.018%
42	14.236	1866	1870	1872	rVV2	17154	22555	1.09%	0.088%
43	14.283	1872	1878	1890	rVB	1004957	1453727	69.96%	5.687%
44	14.401	1896	1898	1903	rVB5	2687	3466	0.17%	0.014%
45	14.501	1910	1915	1919	rVB3	8247	11316	0.54%	0.044%
46	14.589	1923	1930	1942	rBV	1121998	1627594	78.33%	6.368%
47	14.765	1955	1960	1972	rBV	124022	245804	11.83%	0.962%
48	14.954	1991	1992	1996	rVB4	3302	2485	0.12%	0.010%
49	14.995	1997	1999	2006	rVV7	3907	6164	0.30%	0.024%
50	15.054	2006	2009	2012	rVB5	2155	2634	0.13%	0.010%
51	15.177	2026	2030	2032	rBV5	2372	2449	0.12%	0.010%
52	15.224	2034	2038	2045	rVB2	11562	17885	0.86%	0.070%
53	15.289	2045	2049	2055	rBV7	1975	4365	0.21%	0.017%
54	15.395	2062	2067	2072	rBV2	14905	24477	1.18%	0.096%
55	15.442	2072	2075	2081	rVB3	7859	10135	0.49%	0.040%
56	15.577	2091	2098	2110	rBV	1274138	1810976	87.16%	7.085%
57	15.683	2111	2116	2132	rVV	170871	271321	13.06%	1.061%
58	15.818	2136	2139	2144	rBV5	4906	8430	0.41%	0.033%
59	15.942	2155	2160	2164	rVB7	6163	11148	0.54%	0.044%
60	15.995	2164	2169	2172	rBV6	6397	10187	0.49%	0.040%
61	16.130	2188	2192	2196	rBV7	2938	4314	0.21%	0.017%
62	16.218	2204	2207	2211	rVB6	4904	5780	0.28%	0.023%
63	16.265	2211	2215	2218	rBV3	7670	11414	0.55%	0.045%
64	16.306	2218	2222	2224	rVV3	7863	11032	0.53%	0.043%
65	16.330	2224	2226	2230	rVV5	5236	5269	0.25%	0.021%
66	16.371	2230	2233	2238	rVB7	4944	7162	0.34%	0.028%
67	16.471	2246	2250	2254	rBV4	7293	9063	0.44%	0.035%
68	16.653	2275	2281	2283	rBV5	3893	5468	0.26%	0.021%
69	16.677	2283	2285	2289	rVB4	2241	2494	0.12%	0.010%
70	16.706	2289	2290	2295	rBV5	2854	2734	0.13%	0.011%
71	16.806	2306	2307	2311	rVV4	5804	6565	0.32%	0.026%
72	16.859	2314	2316	2318	rVV3	2395	2379	0.11%	0.009%
73	16.889	2318	2321	2323	rVV4	2261	2866	0.14%	0.011%
74	16.948	2326	2331	2333	rBV3	2443	4376	0.21%	0.017%
75	17.048	2346	2348	2352	rVV4	2858	4274	0.21%	0.017%
76	17.095	2352	2356	2362	rVV8	11365	23732	1.14%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034232.D
 Acq On : 11 Mar 2022 21:37
 Operator : CG/JU
 Sample : N1816-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSE3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

77	17.153	2362	2366	2369	rVB6	5861	9689	0.47%	0.038%
78	17.253	2378	2383	2388	rVB5	15979	20655	0.99%	0.081%
79	17.330	2389	2396	2405	rBV	1252017	1795253	86.40%	7.023%
80	17.430	2406	2413	2426	rVV	1195290	1792842	86.29%	7.014%
81	17.636	2443	2448	2454	rVB8	6376	10974	0.53%	0.043%
82	17.706	2457	2460	2464	rBV6	2637	4667	0.22%	0.018%
83	17.836	2480	2482	2486	rVB4	4211	4700	0.23%	0.018%
84	17.912	2493	2495	2498	rVB4	2883	2476	0.12%	0.010%
85	17.942	2498	2500	2502	rBV3	2250	2436	0.12%	0.010%
86	18.006	2507	2511	2515	rVB3	17412	23071	1.11%	0.090%
87	18.224	2543	2548	2556	rBV3	21221	36730	1.77%	0.144%
88	18.342	2565	2568	2569	rBV3	3475	3248	0.16%	0.013%
89	18.524	2598	2599	2604	rBV4	3670	4524	0.22%	0.018%
90	18.653	2618	2621	2625	rBV6	9518	13875	0.67%	0.054%
91	18.777	2640	2642	2646	rBV5	4346	5672	0.27%	0.022%
92	19.083	2692	2694	2697	rBV4	5757	7222	0.35%	0.028%
93	19.289	2724	2729	2732	rBV4	16663	26601	1.28%	0.104%
94	19.353	2737	2740	2744	rVV	16031	20218	0.97%	0.079%
95	19.494	2762	2764	2767	rBV4	9040	10073	0.48%	0.039%
96	19.712	2796	2801	2808	rBV	1509182	2077792	100.00%	8.129%
97	21.206	3052	3055	3060	rBV2	140357	176506	8.49%	0.691%
98	21.500	3100	3105	3119	rBV	1111092	1808887	87.06%	7.077%
99	23.759	3483	3489	3498	rBV	861869	1800714	86.66%	7.045%
100	23.918	3510	3516	3533	rVB2	909465	2023051	97.37%	7.915%


Sum of corrected areas: 25560823

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

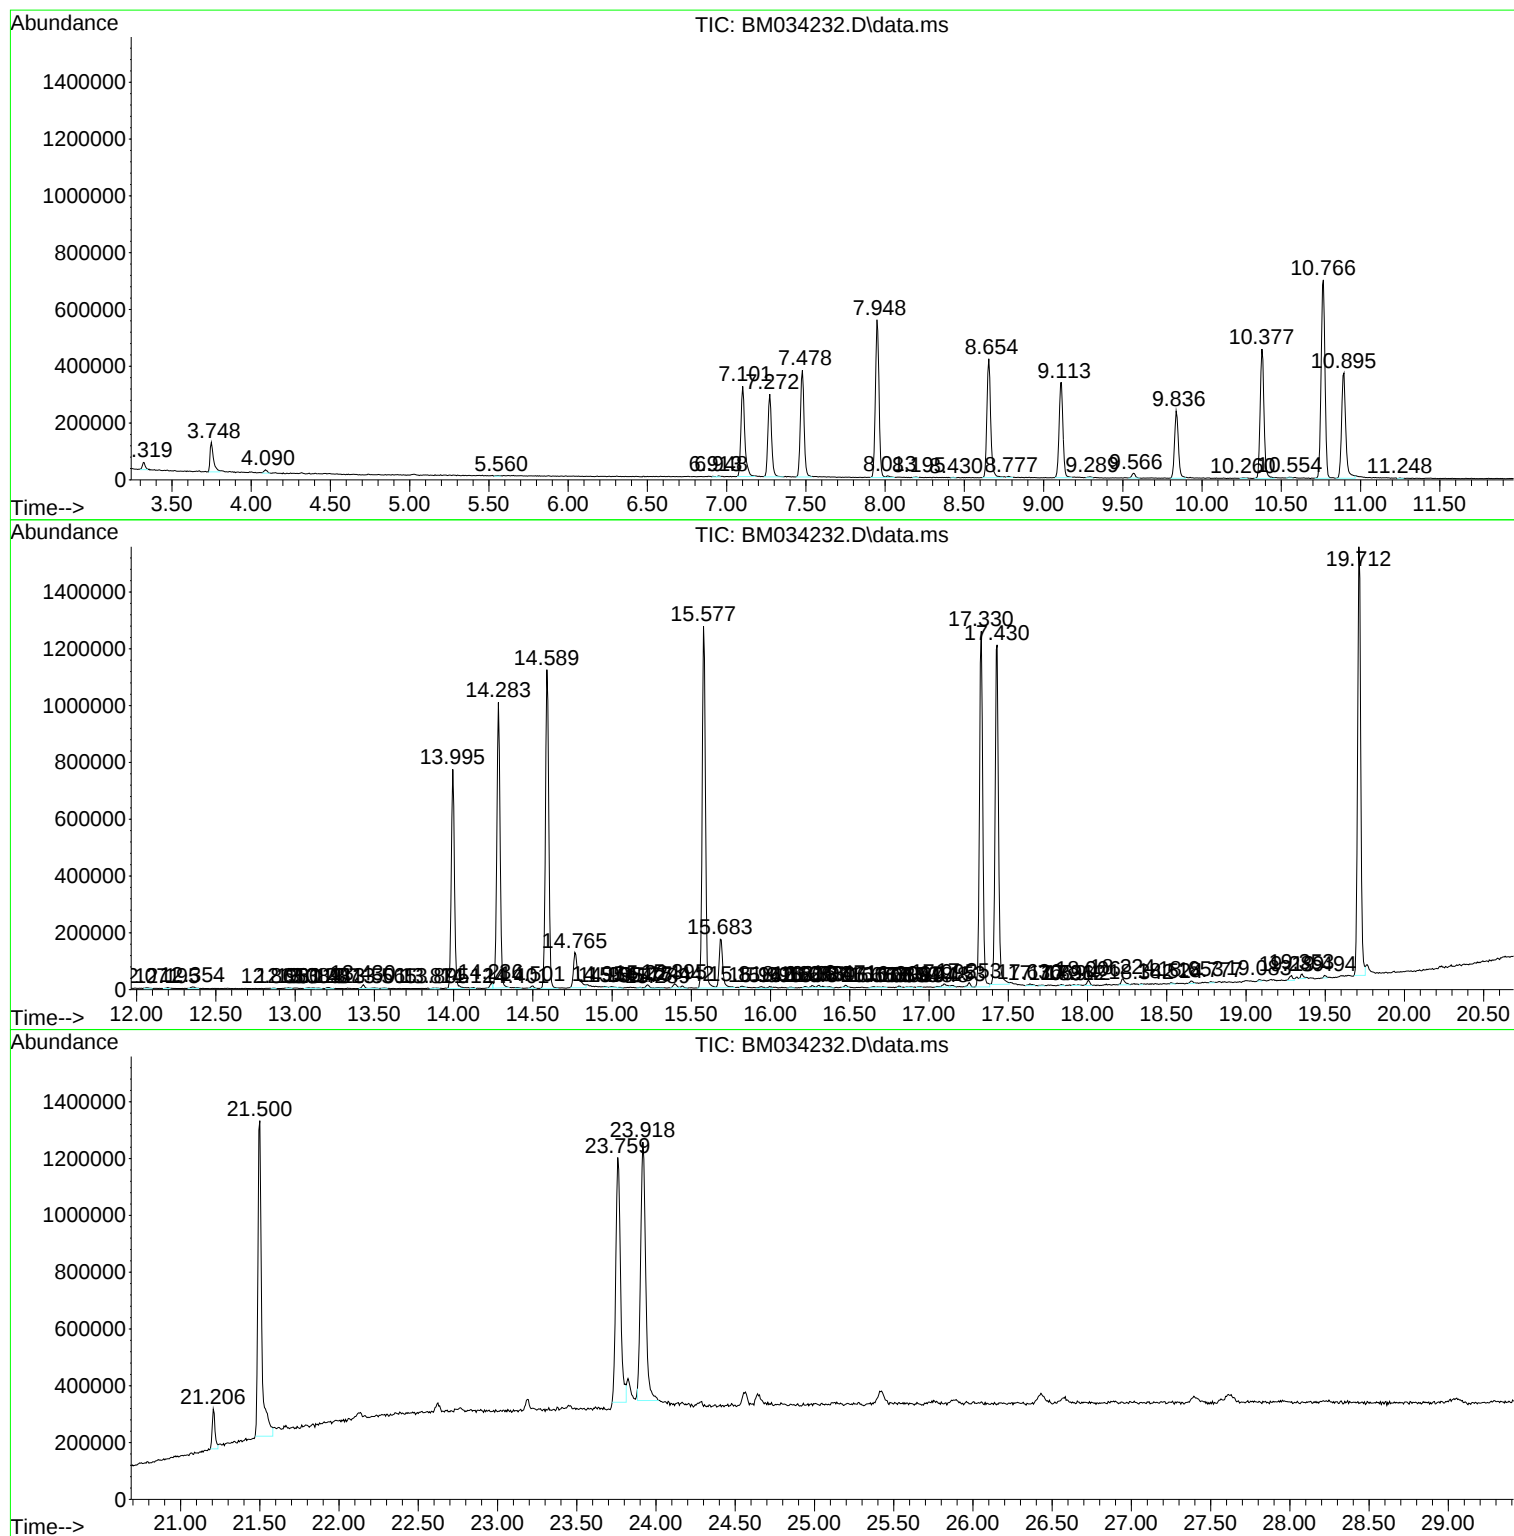

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034232.D
Acq On : 11 Mar 2022 21:37
Operator : CG/JU
Sample : N1816-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------