

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034235.D
 Acq On : 11 Mar 2022 23:26
 Operator : CG/JU
 Sample : N1816-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	19	rVB	39350	44616	1.45%	0.134%
2	3.749	84	87	100	rBV	114265	170687	5.54%	0.512%
3	4.090	142	145	149	rVB2	10367	12799	0.42%	0.038%
4	6.948	627	631	637	rBV7	3321	6144	0.20%	0.018%
5	7.101	651	657	667	rBV	497444	803697	26.09%	2.412%
6	7.272	680	686	696	rVB	445963	693722	22.52%	2.082%
7	7.478	714	721	730	rBV	569405	924624	30.02%	2.775%
8	7.948	794	801	808	rBV	545030	856029	27.79%	2.569%
9	8.019	811	813	819	rVB4	6039	7862	0.26%	0.024%
10	8.654	914	921	935	rBV	671946	1089071	35.36%	3.268%
11	9.107	991	998	1011	rBV	539819	883616	28.69%	2.652%
12	9.278	1025	1027	1033	rVB4	5495	8832	0.29%	0.027%
13	9.566	1070	1076	1083	rVB	37610	60214	1.95%	0.181%
14	9.837	1115	1122	1138	rBV	383564	660611	21.45%	1.982%
15	10.378	1206	1214	1226	rBV	728949	1210910	39.31%	3.634%
16	10.760	1272	1279	1288	rVB	693946	1186062	38.51%	3.559%
17	10.889	1294	1301	1326	rBV	562415	1069857	34.73%	3.211%
18	11.795	1452	1455	1460	rVB5	3758	4835	0.16%	0.015%
19	12.195	1518	1523	1531	rBV2	13611	22976	0.75%	0.069%
20	12.354	1543	1550	1555	rBV4	9020	18564	0.60%	0.056%
21	12.560	1581	1585	1592	rBV5	1756	3892	0.13%	0.012%
22	12.830	1628	1631	1634	rBV4	3434	3698	0.12%	0.011%
23	12.866	1634	1637	1644	rVB5	2973	4899	0.16%	0.015%
24	12.936	1644	1649	1652	rBV6	2845	5891	0.19%	0.018%
25	13.001	1657	1660	1668	rVB8	6069	9407	0.31%	0.028%
26	13.095	1671	1676	1681	rVV6	3879	6962	0.23%	0.021%
27	13.148	1681	1685	1688	rVB4	4339	6344	0.21%	0.019%
28	13.207	1691	1695	1699	rBV4	3010	4992	0.16%	0.015%
29	13.430	1728	1733	1740	rVB	25200	35651	1.16%	0.107%
30	13.566	1752	1756	1761	rVB4	2749	3839	0.12%	0.012%
31	13.995	1823	1829	1841	rBV	1130730	1572651	51.06%	4.719%
32	14.283	1871	1878	1891	rVV	1492734	2195128	71.26%	6.587%
33	14.389	1894	1896	1901	rVB5	2917	4372	0.14%	0.013%
34	14.495	1910	1914	1920	rVB4	6687	9038	0.29%	0.027%
35	14.589	1923	1930	1945	rVV	1091524	1608696	52.23%	4.827%
36	14.766	1955	1960	1976	rBV	234574	428777	13.92%	1.287%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
 Data File : BM034235.D
 Acq On : 11 Mar 2022 23:26
 Operator : CG/JU
 Sample : N1816-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBSD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
 Title : SVOA CALIBRATION

37	15.001	1996	2000	2005	rVB6	3994	6604	0.21%	0.020%
38	15.219	2033	2037	2044	rVB6	5312	10050	0.33%	0.030%
39	15.395	2062	2067	2072	rBV5	5200	10383	0.34%	0.031%
40	15.442	2072	2075	2078	rVB4	4073	4675	0.15%	0.014%
41	15.577	2092	2098	2111	rBV	1878267	2708091	87.92%	8.127%
42	15.683	2111	2116	2130	rVV	248547	385609	12.52%	1.157%
43	15.818	2135	2139	2145	rVB4	8766	12852	0.42%	0.039%
44	16.260	2211	2214	2219	rVB7	3025	4176	0.14%	0.013%
45	16.301	2219	2221	2224	rBV4	4214	3873	0.13%	0.012%
46	16.477	2246	2251	2253	rVB3	2942	3413	0.11%	0.010%
47	16.813	2303	2308	2311	rBV6	2705	3745	0.12%	0.011%
48	17.007	2337	2341	2345	rVB6	3300	4887	0.16%	0.015%
49	17.095	2352	2356	2358	rBV5	3128	4805	0.16%	0.014%
50	17.142	2363	2364	2368	rVB4	4659	4481	0.15%	0.013%
51	17.254	2380	2383	2387	rVB6	5511	6746	0.22%	0.020%
52	17.330	2389	2396	2406	rBV	1214297	1754965	56.97%	5.266%
53	17.430	2406	2413	2426	rBV	1845141	2683434	87.12%	8.053%
54	18.007	2508	2511	2515	rVB4	8683	11079	0.36%	0.033%
55	18.059	2515	2520	2521	rBV5	2281	3136	0.10%	0.009%
56	18.224	2544	2548	2557	rBV6	27247	46990	1.53%	0.141%
57	19.148	2702	2705	2707	rBV3	7268	8075	0.26%	0.024%
58	19.283	2723	2728	2732	rBV3	24574	35786	1.16%	0.107%
59	19.354	2736	2740	2749	rVV2	23047	47672	1.55%	0.143%
60	19.495	2762	2764	2770	rBV7	8486	14215	0.46%	0.043%
61	19.712	2795	2801	2808	rBV	2254248	3080244	100.00%	9.243%
62	21.206	3051	3055	3061	rBV2	200429	265701	8.63%	0.797%
63	21.495	3100	3104	3117	rBV	1034900	1699955	55.19%	5.101%
64	23.759	3482	3489	3499	rBV2	1304302	2850746	92.55%	8.555%
65	23.918	3509	3516	3535	rVB2	891753	2007290	65.17%	6.024%




Sum of corrected areas: 33323643

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034235.D
Acq On : 11 Mar 2022 23:26
Operator : CG/JU
Sample : N1816-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

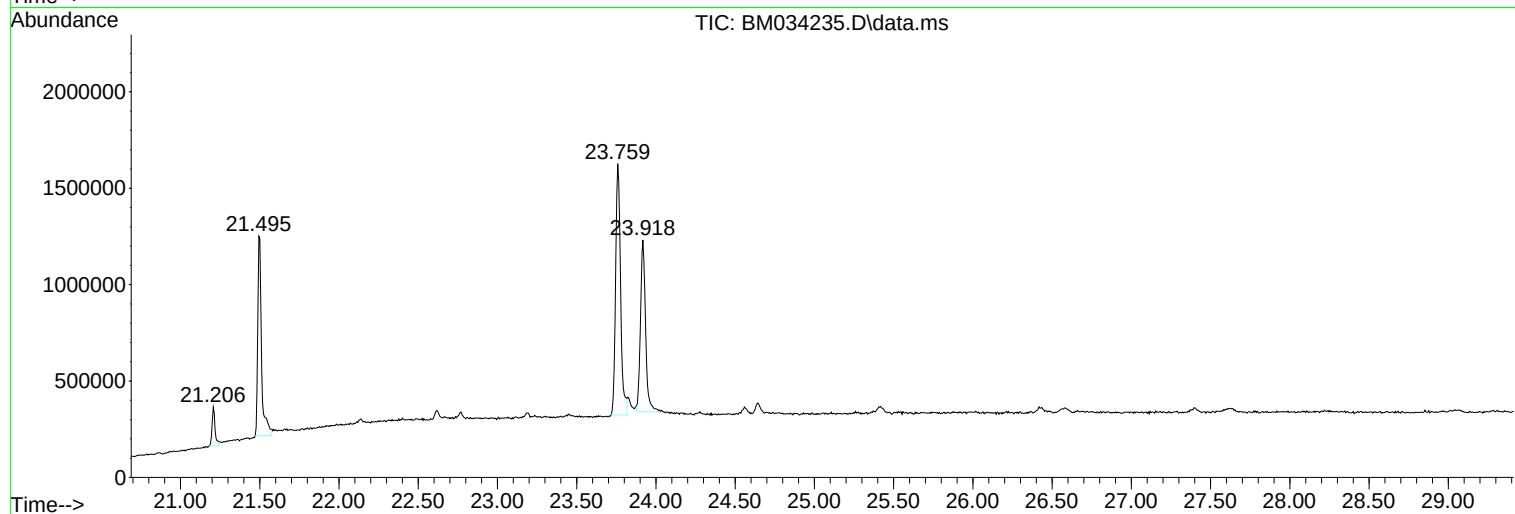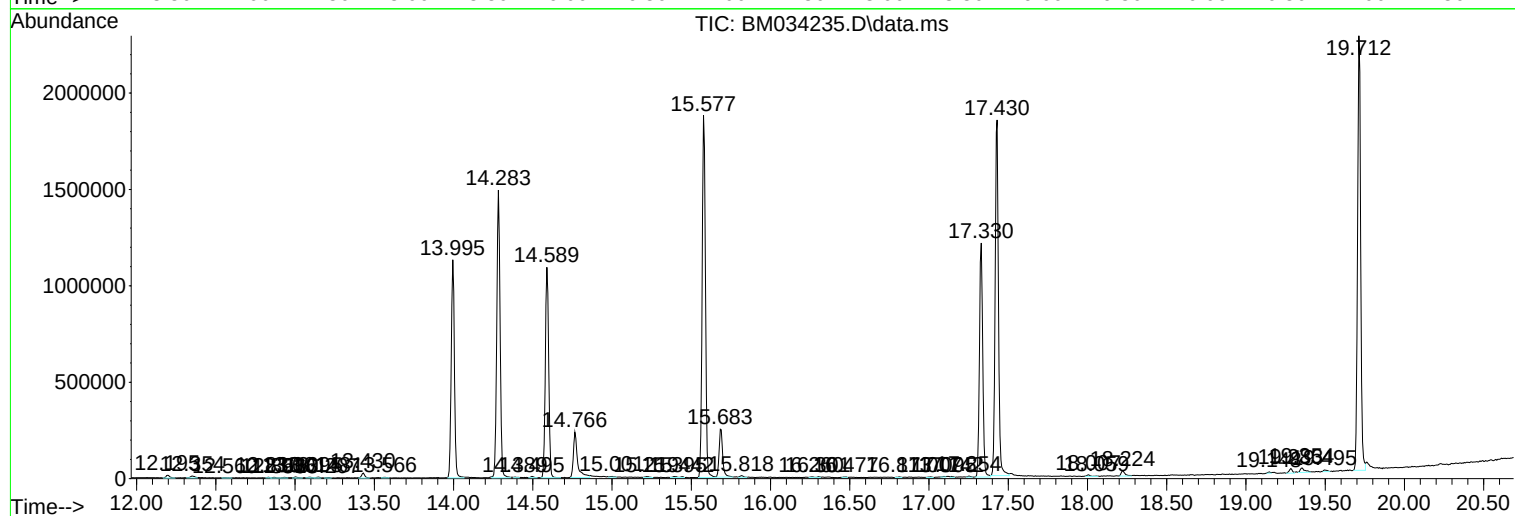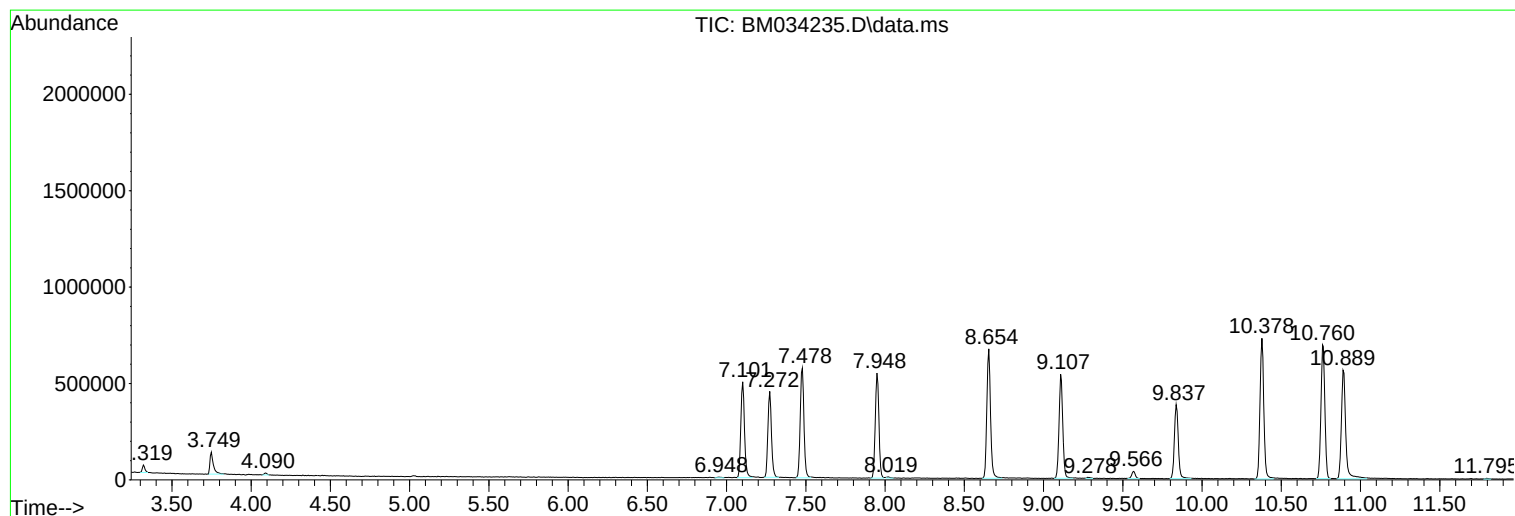

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034235.D
Acq On : 11 Mar 2022 23:26
Operator : CG/JU
Sample : N1816-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.206	3.13 ng/ul	265701	Chrysene-d12	21.500

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-		280	C20H40	074685-30-6	99
2	E-15-Heptadecenal		252	C17H32O	1000130-97-9	98
3	1-Hexacosene		364	C26H52	018835-33-1	95
4	1-Heneicosanol		312	C21H44O	015594-90-8	94
5	1-Nonadecene		266	C19H38	018435-45-5	94

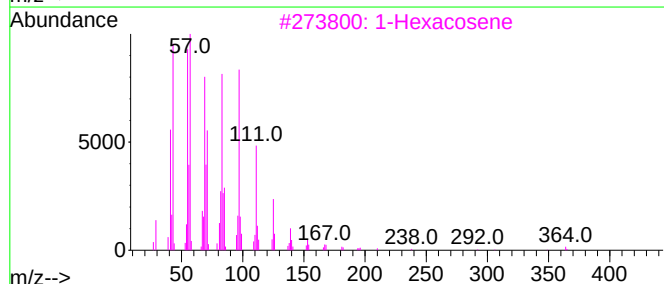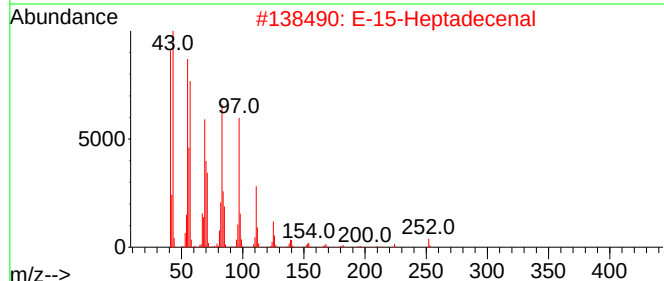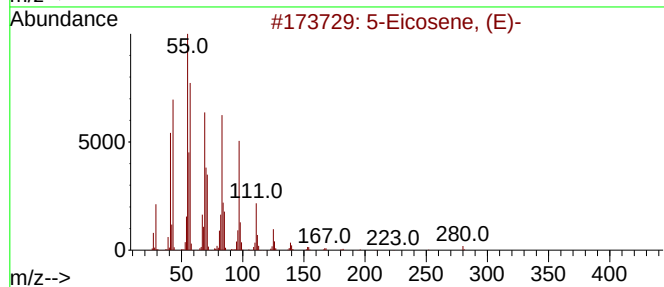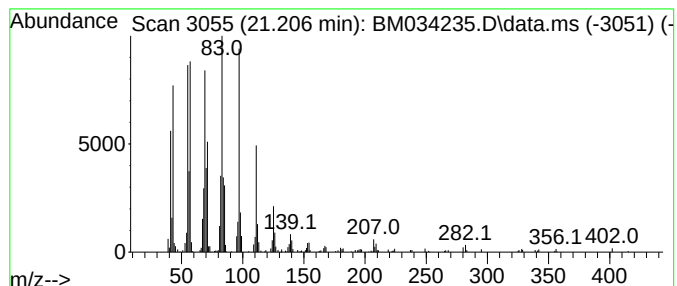

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031122\
Data File : BM034235.D
Acq On : 11 Mar 2022 23:26
Operator : CG/JU
Sample : N1816-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBSD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM031022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.206	3.1	ng/u1	265701	5	21.500	1699960	20.0