


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031215\
 Data File : BM000696.D
 Acq On : 12 Mar 2015 13:19
 Operator : TP/IZ
 Sample : DFTPP36
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP36

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 13 09:01:44 2015

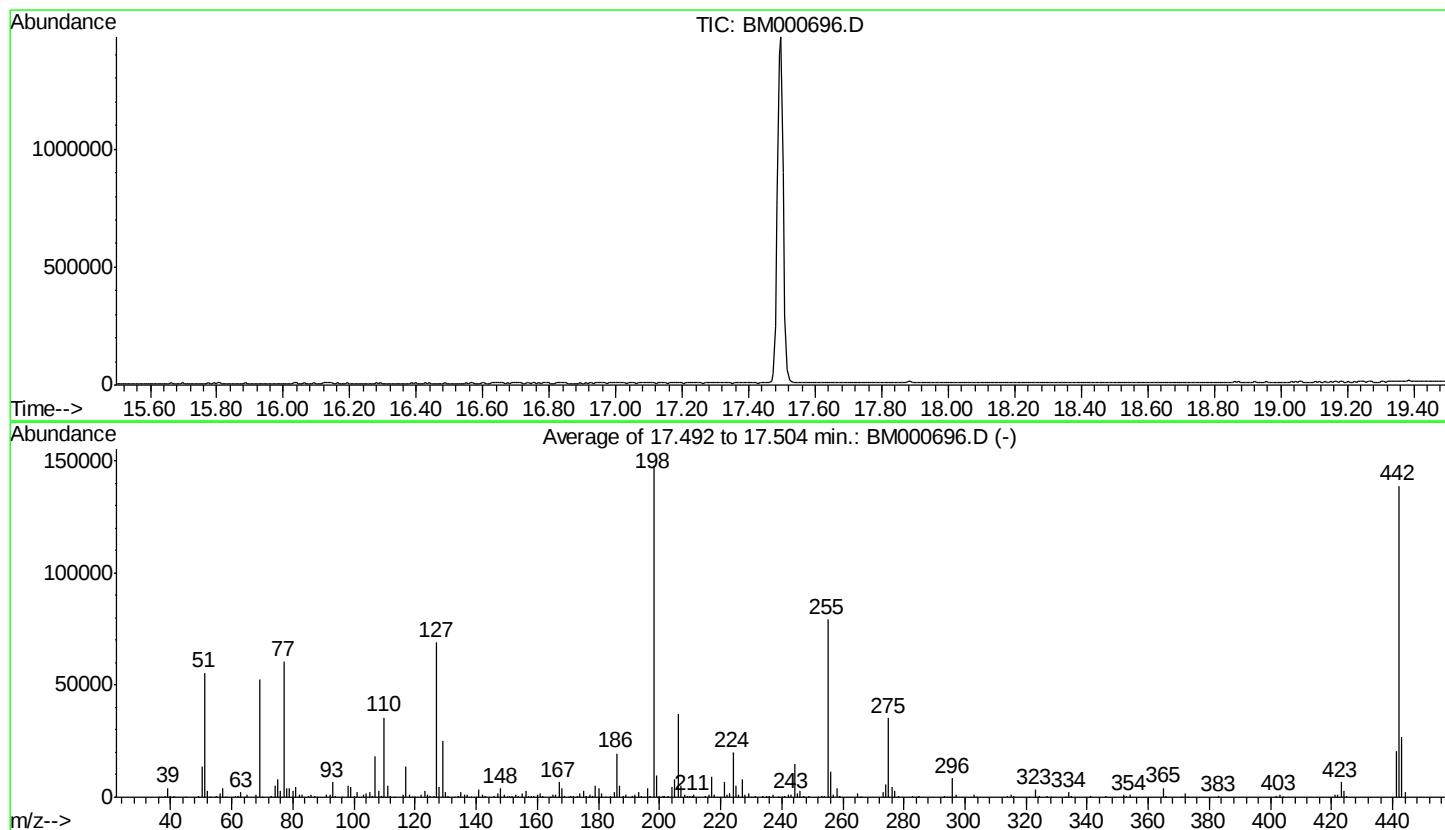

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	55589	PASS
68	69	0.00	2	1.7	889	PASS
69	198	0.00	100	35.5	52424	PASS
70	69	0.00	2	0.2	108	PASS
127	198	10	80	46.6	68778	PASS
197	198	0.00	2	0.4	523	PASS
198	198	100	100	100.0	147736	PASS
199	198	5	9	6.6	9792	PASS
275	198	10	60	23.9	35256	PASS
365	198	1	100	2.7	4014	PASS
441	443	0.01	100	76.3	20290	PASS
442	198	50	100	93.9	138760	PASS
443	442	15	24	19.2	26600	PASS