


Data Path : Z:\HPCHEM1\BNA_M\Data\BM031215\
 Data File : BM000696.D
 Acq On : 12 Mar 2015 13:19
 Operator : TP/IZ
 Sample : DFTPP36
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP36

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 13 09:01:44 2015

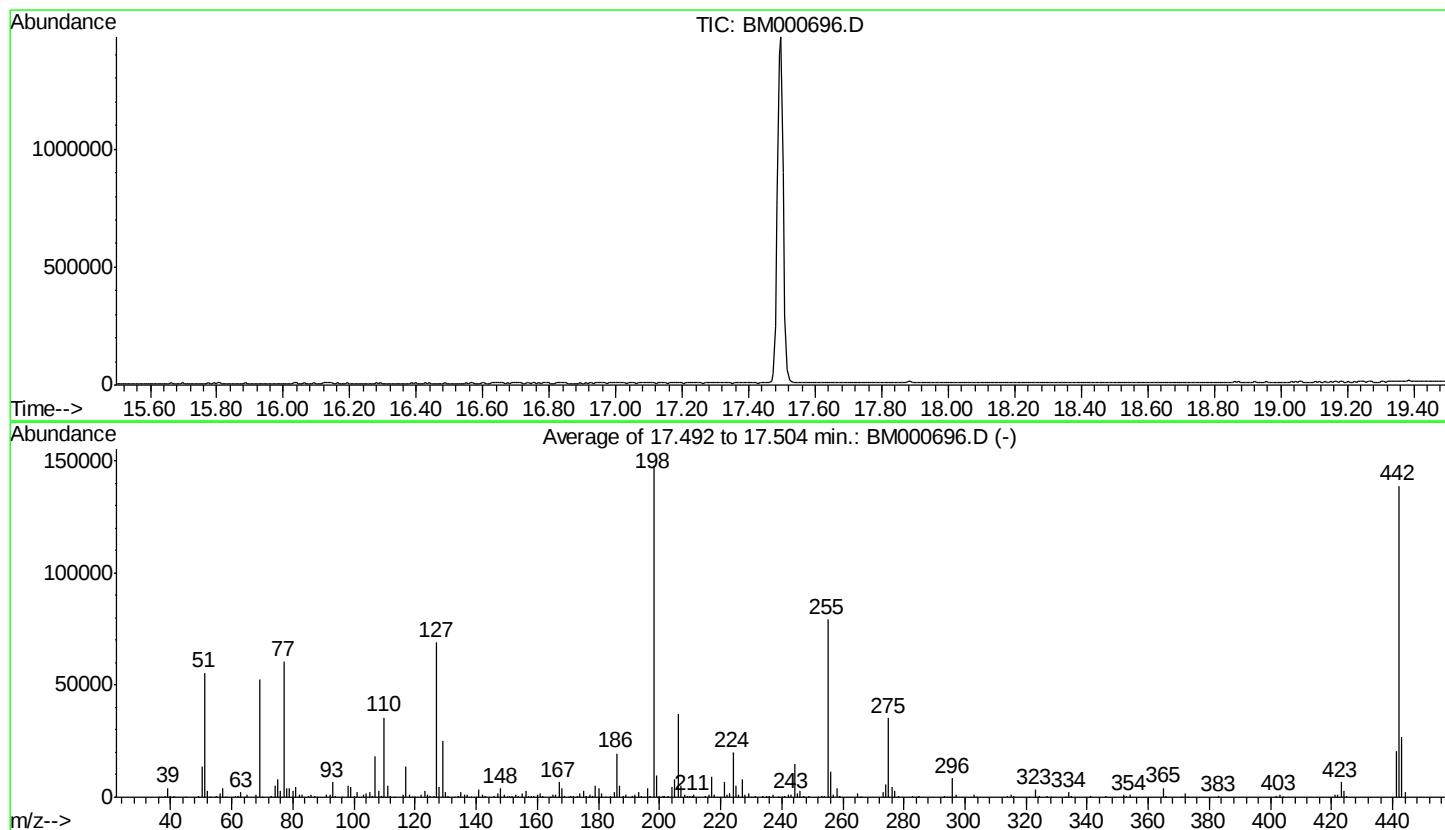

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	55589	PASS
68	69	0.00	2	1.7	889	PASS
69	198	0.00	100	35.5	52424	PASS
70	69	0.00	2	0.2	108	PASS
127	198	10	80	46.6	68778	PASS
197	198	0.00	2	0.4	523	PASS
198	198	100	100	100.0	147736	PASS
199	198	5	9	6.6	9792	PASS
275	198	10	60	23.9	35256	PASS
365	198	1	100	2.7	4014	PASS
441	443	0.01	100	76.3	20290	PASS
442	198	50	100	93.9	138760	PASS
443	442	15	24	19.2	26600	PASS

m/z	Abundance
35.90	315.0
37.10	559.0
38.00	793.0
39.10	5744.0
40.00	4231.0
41.00	658.0
44.00	3592.0
45.00	338.0
48.90	572.0
50.10	17096.0
51.10	71536.0
52.10	3615.0
53.00	311.0
55.10	468.0
56.00	1850.0
57.10	5299.0
58.00	387.0
61.00	719.0
62.10	1126.0
63.00	2482.0
64.00	484.0
65.00	1158.0
67.90	1049.0
69.00	66112.0
69.90	325.0
73.10	831.0
74.00	6594.0
75.00	10429.0
76.00	3078.0
77.10	75648.0
78.00	5119.0
79.00	5070.0
80.00	3635.0
81.00	5257.0
81.90	1090.0
83.00	1174.0
84.90	995.0
86.00	1389.0
87.10	539.0
87.90	350.0
91.00	1188.0
92.00	1423.0
93.00	8286.0
93.90	548.0
96.20	376.0
98.00	5573.0
99.00	5990.0
100.10	590.0
101.00	2914.0
103.00	1215.0
104.00	1927.0
105.00	2249.0
106.00	875.0
107.00	21376.0
108.00	3626.0
109.00	647.0
110.00	41928.0
111.00	6407.0
112.00	741.0
116.00	1317.0
117.00	15957.0
118.10	1254.0
118.90	379.0
119.80	339.0
122.00	1146.0
123.00	3779.0
124.00	1166.0
125.10	939.0
126.10	390.0
127.00	81784.0
128.00	5957.0
129.00	30480.0
130.00	2614.0
130.90	494.0
133.90	710.0
135.00	2601.0
136.00	1199.0
137.00	1532.0
138.10	343.0
140.10	354.0
141.00	4579.0
142.00	1462.0
143.10	749.0
145.90	643.0
147.00	1983.0
148.00	4216.0
149.00	1189.0
150.10	364.0
151.00	440.0
151.60	439.0
153.00	1138.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

154.00	1175.0
155.00	1988.0
156.10	3183.0
156.90	630.0
158.00	725.0
159.00	713.0
160.00	1296.0
161.00	1942.0
161.90	707.0
164.10	331.0
165.00	1418.0
166.10	1181.0
167.00	8184.0
168.00	5366.0
169.00	687.0
170.10	375.0
170.90	344.0
172.00	700.0
173.00	793.0
174.00	1980.0
175.10	2874.0
176.00	913.0
177.10	1398.0
178.00	433.0
179.00	5520.0
180.00	4591.0
181.00	2094.0
182.10	309.0
183.90	497.0
185.00	2290.0
186.10	21168.0
187.00	6168.0
187.90	614.0
188.90	1335.0
190.90	665.0
192.00	1378.0
193.00	2230.0
193.90	565.0
196.00	4467.0
196.90	1057.0
198.00	167488.0
199.00	10739.0
200.00	839.0
201.60	1016.0
202.90	845.0
204.10	5000.0
205.10	8743.0
206.00	42040.0
207.10	6750.0
208.10	1767.0
208.90	654.0
210.00	546.0
211.10	1770.0
215.10	439.0
216.10	872.0
217.00	10095.0
217.90	1503.0
221.10	7518.0
222.00	1855.0
223.00	2134.0
224.10	21952.0
225.10	5603.0
226.00	1296.0
227.00	8715.0
228.00	1017.0
229.00	1786.0
230.00	395.0
231.10	827.0
234.00	378.0
235.10	571.0
236.00	322.0
237.00	1239.0
238.80	359.0
241.00	441.0
242.00	1555.0
243.10	1337.0
244.10	15105.0
245.10	1866.0
246.00	2515.0
246.90	489.0
249.00	550.0
252.90	573.0
254.00	720.0
255.00	84200.0
256.00	13086.0
257.10	1193.0
258.00	4498.0
259.00	895.0
265.00	1844.0
273.00	2226.0
274.00	5818.0
275.00	36152.0
276.00	5076.0
277.00	3042.0
278.10	798.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

284.10	452.0
285.00	535.0
292.90	686.0
294.00	331.0
295.00	329.0
296.00	8840.0
296.90	1151.0
303.00	1329.0
304.00	415.0
314.10	430.0
315.00	1117.0
316.00	481.0
321.10	313.0
323.00	3051.0
324.10	732.0
326.90	514.0
332.80	327.0
334.10	2136.0
335.00	451.0
340.90	480.0
346.00	513.0
352.00	876.0
353.00	447.0
354.10	921.0
365.00	3676.0
365.90	719.0
372.00	1597.0
373.10	389.0
383.00	398.0
401.90	482.0
403.00	834.0
404.10	348.0
421.00	1016.0
421.90	624.0
423.10	5663.0
424.10	2610.0
425.00	466.0
441.00	17048.0
442.00	122848.0
443.00	23624.0
444.00	2152.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
38.10	791.0
39.10	4436.0
40.00	3639.0
41.10	829.0
44.00	4162.0
45.00	337.0
49.10	539.0
50.10	15943.0
51.10	63928.0
52.10	3267.0
55.00	509.0
56.00	2068.0
57.00	5588.0
61.10	655.0
62.00	1122.0
63.00	2390.0
65.10	1083.0
68.00	965.0
69.00	60312.0
73.00	963.0
74.00	5989.0
75.10	9223.0
76.10	3327.0
77.10	68472.0
78.10	4961.0
79.00	4804.0
80.00	3507.0
81.00	5072.0
82.00	1346.0
83.10	1336.0
84.90	789.0
86.00	1395.0
87.00	588.0
91.00	1245.0
92.00	1244.0
93.00	7517.0
93.90	632.0
96.10	397.0
98.00	6386.0
99.00	4946.0
100.10	370.0
101.00	3078.0
103.00	984.0
104.10	1685.0
105.00	2423.0
106.00	524.0
107.00	20776.0
108.00	3018.0
109.20	656.0
110.00	40616.0
111.00	5395.0
112.00	948.0
113.00	324.0
115.90	1105.0
117.00	16341.0
118.00	1224.0
120.00	377.0
121.90	1835.0
123.00	3558.0
124.00	1129.0
125.00	928.0
126.10	346.0
127.00	80816.0
128.00	5529.0
129.00	28992.0
130.00	2456.0
131.00	493.0
133.00	347.0
134.00	751.0
135.10	2568.0
136.00	1034.0
136.90	1383.0
138.10	325.0
140.10	444.0
141.00	3706.0
142.00	1208.0
143.00	1034.0
145.90	940.0
147.00	2355.0
148.00	4458.0
149.10	971.0
149.90	379.0
151.00	505.0
151.50	525.0
153.00	1319.0
153.90	647.0
155.10	2111.0
156.10	3366.0
157.00	712.0
157.90	686.0
158.80	661.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

160.00	1233.0
161.00	1640.0
161.90	431.0
164.10	314.0
165.00	1305.0
166.00	1209.0
167.00	7716.0
168.00	4139.0
169.10	642.0
170.90	466.0
172.00	890.0
173.10	991.0
173.90	1822.0
175.00	3117.0
175.90	1043.0
177.00	1565.0
177.80	319.0
179.00	6486.0
180.00	5143.0
181.00	2003.0
183.90	545.0
185.10	3165.0
186.00	23760.0
187.00	6292.0
188.00	878.0
188.90	1319.0
190.90	739.0
192.00	1810.0
193.00	2594.0
194.20	411.0
195.00	312.0
196.00	5066.0
198.00	174912.0
199.00	11898.0
200.00	721.0
201.20	839.0
202.90	854.0
204.10	5376.0
205.10	8857.0
206.10	42992.0
207.10	6823.0
208.00	1370.0
209.10	767.0
210.10	783.0
211.00	1455.0
215.00	537.0
216.00	1222.0
217.00	10784.0
218.00	1554.0
221.10	8332.0
221.90	1572.0
223.00	2159.0
224.10	23192.0
225.00	6246.0
226.10	980.0
227.00	9312.0
228.00	1228.0
229.00	1991.0
229.80	343.0
231.10	1003.0
234.00	669.0
235.10	733.0
236.10	457.0
237.00	1423.0
239.00	478.0
240.00	370.0
241.00	655.0
242.00	1170.0
243.00	1290.0
244.10	18208.0
245.00	2244.0
246.00	3165.0
247.10	675.0
249.00	910.0
252.00	350.0
252.90	379.0
254.10	1125.0
255.00	92416.0
256.10	13720.0
257.10	1151.0
258.00	4172.0
259.10	701.0
265.00	2158.0
266.20	379.0
273.10	2784.0
274.10	6987.0
275.00	42224.0
276.00	5338.0
277.00	3194.0
278.00	420.0
283.00	491.0
285.00	578.0
293.10	1092.0
296.00	9998.0
297.00	1812.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

303.00	1140.0
303.80	347.0
313.90	664.0
315.00	1029.0
316.10	615.0
323.00	4043.0
324.10	766.0
326.90	681.0
328.00	312.0
333.00	374.0
334.10	2398.0
334.90	802.0
340.90	716.0
345.90	883.0
352.10	1169.0
353.00	867.0
354.00	1279.0
365.00	4830.0
366.00	865.0
370.90	342.0
372.10	2014.0
372.90	509.0
383.00	639.0
402.00	930.0
403.00	1127.0
404.10	444.0
421.00	1180.0
422.00	1300.0
423.00	7726.0
424.00	2926.0
425.10	634.0
441.00	23792.0
442.00	165696.0
443.10	32472.0
444.00	2855.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
38.00	309.0
39.00	2564.0
40.00	4485.0
41.00	743.0
44.00	3896.0
48.90	365.0
50.10	8819.0
51.10	31304.0
52.00	1825.0
56.00	1100.0
57.00	3481.0
61.00	484.0
63.00	1266.0
65.10	807.0
68.10	654.0
69.00	30848.0
73.00	698.0
74.10	3178.0
75.00	5200.0
76.00	1843.0
77.10	36744.0
78.10	2582.0
79.00	2548.0
80.00	1875.0
81.00	2719.0
82.00	354.0
83.00	677.0
85.00	440.0
86.00	886.0
86.90	314.0
90.90	529.0
92.00	1070.0
93.00	4449.0
98.00	2689.0
99.00	2692.0
101.00	1286.0
102.90	576.0
104.00	1191.0
105.10	1557.0
107.00	12298.0
108.00	1495.0
108.90	438.0
110.00	23960.0
111.00	3174.0
111.90	524.0
115.90	552.0
117.00	8829.0
118.00	506.0
122.00	778.0
123.10	2979.0
123.90	738.0
124.90	351.0
126.10	342.0
127.00	43736.0
128.10	3084.0
129.00	16584.0
130.00	1389.0
130.80	324.0
133.90	466.0
135.10	1222.0
136.10	710.0
136.90	795.0
141.00	2233.0
141.90	771.0
143.00	456.0
146.00	481.0
147.00	1130.0
148.00	2652.0
148.90	622.0
151.40	309.0
153.00	692.0
154.00	547.0
155.10	1450.0
156.10	2138.0
157.00	352.0
157.90	366.0
159.90	861.0
161.00	1039.0
164.90	779.0
166.20	495.0
167.10	4152.0
167.90	3106.0
169.00	485.0
170.90	306.0
171.90	509.0
173.00	586.0
173.80	1009.0
175.00	1826.0
175.90	562.0
176.80	694.0
178.00	367.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

179.00	3629.0
180.00	2487.0
181.10	1295.0
185.10	1804.0
186.00	13495.0
187.00	3385.0
187.90	575.0
189.00	545.0
190.80	427.0
191.90	825.0
193.00	1327.0
193.90	446.0
196.10	2415.0
197.00	514.0
198.00	100808.0
199.00	6741.0
199.90	501.0
201.20	415.0
201.70	648.0
202.90	664.0
204.00	3356.0
205.00	6013.0
206.10	25952.0
207.10	4196.0
208.00	898.0
208.90	463.0
210.80	1019.0
216.10	608.0
217.00	6364.0
218.10	801.0
221.00	5464.0
222.10	842.0
223.00	1548.0
224.10	14241.0
225.00	3625.0
226.10	550.0
227.00	5603.0
228.00	810.0
228.90	1187.0
231.00	503.0
234.00	551.0
235.00	688.0
235.90	375.0
237.10	860.0
241.10	351.0
242.00	797.0
243.20	972.0
244.10	12035.0
245.00	1751.0
246.10	2467.0
247.00	518.0
249.00	619.0
254.10	422.0
255.00	60960.0
256.10	7693.0
257.00	819.0
258.10	3123.0
258.80	434.0
265.00	1080.0
265.80	337.0
273.00	1843.0
274.00	4224.0
275.00	27392.0
276.10	3583.0
277.00	2346.0
278.00	344.0
282.90	422.0
293.10	541.0
296.00	6624.0
297.10	939.0
303.10	924.0
315.00	833.0
315.90	447.0
323.00	2564.0
326.90	401.0
334.10	1635.0
341.00	310.0
345.90	600.0
352.00	718.0
353.00	636.0
354.00	758.0
365.00	3536.0
366.00	628.0
372.00	1456.0
383.00	540.0
402.00	788.0
403.10	1100.0
403.80	383.0
421.00	940.0
422.00	990.0
423.00	6831.0
424.00	2451.0
441.00	20032.0
442.00	127736.0
443.00	23704.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

443.90

2042.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

Scan 2510 (17.451 min): BM000696.D
DFTPP36

m/z	Abundance
40.00	3552.0
41.00	401.0
44.00	3963.0
57.00	515.0
123.00	754.0
207.00	813.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36