

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031218\
 Data File : BM014531.D
 Acq On : 12 Mar 2018 23:23
 Operator : SJ/JU
 Sample : J1813-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6F48

Quant Time: Mar 13 02:51:03 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	80587	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	348031	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.14	164	216612	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	524058	20.00	ng/ul	0.00
75) Chrysene-d12	21.13	240	586870	20.00	ng/ul	0.00
83) Perylene-d12	23.29	264	543992	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.05	96	5059	2.69	ng/uL	0.00
5) Phenol-d5	6.69	99	139087	20.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	88564	21.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	118598	22.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	106699	17.90	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	60563	23.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	68772	25.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	113026	20.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	125054	23.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.56	166	482404	26.97	ng/ul	0.00
46) Acenaphthylene-d8	13.83	160	577460	26.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	17349	7.02	ng/ul	-0.02
57) Fluorene-d10	15.14	176	396295	24.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	61683	19.62	ng/ul	0.00
70) Anthracene-d10	17.00	188	635511	25.13	ng/ul	0.00
76) Pyrene-d10	19.32	212	749992	24.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.16	264	689453	26.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.62	163	76644	4.35	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031218\
Data File : BM014531.D
Acq On : 12 Mar 2018 23:23
Operator : SJ/JU
Sample : J1813-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6F48

Quant Time: Mar 13 02:51:03 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 13 02:49:59 2018
Response via : Initial Calibration

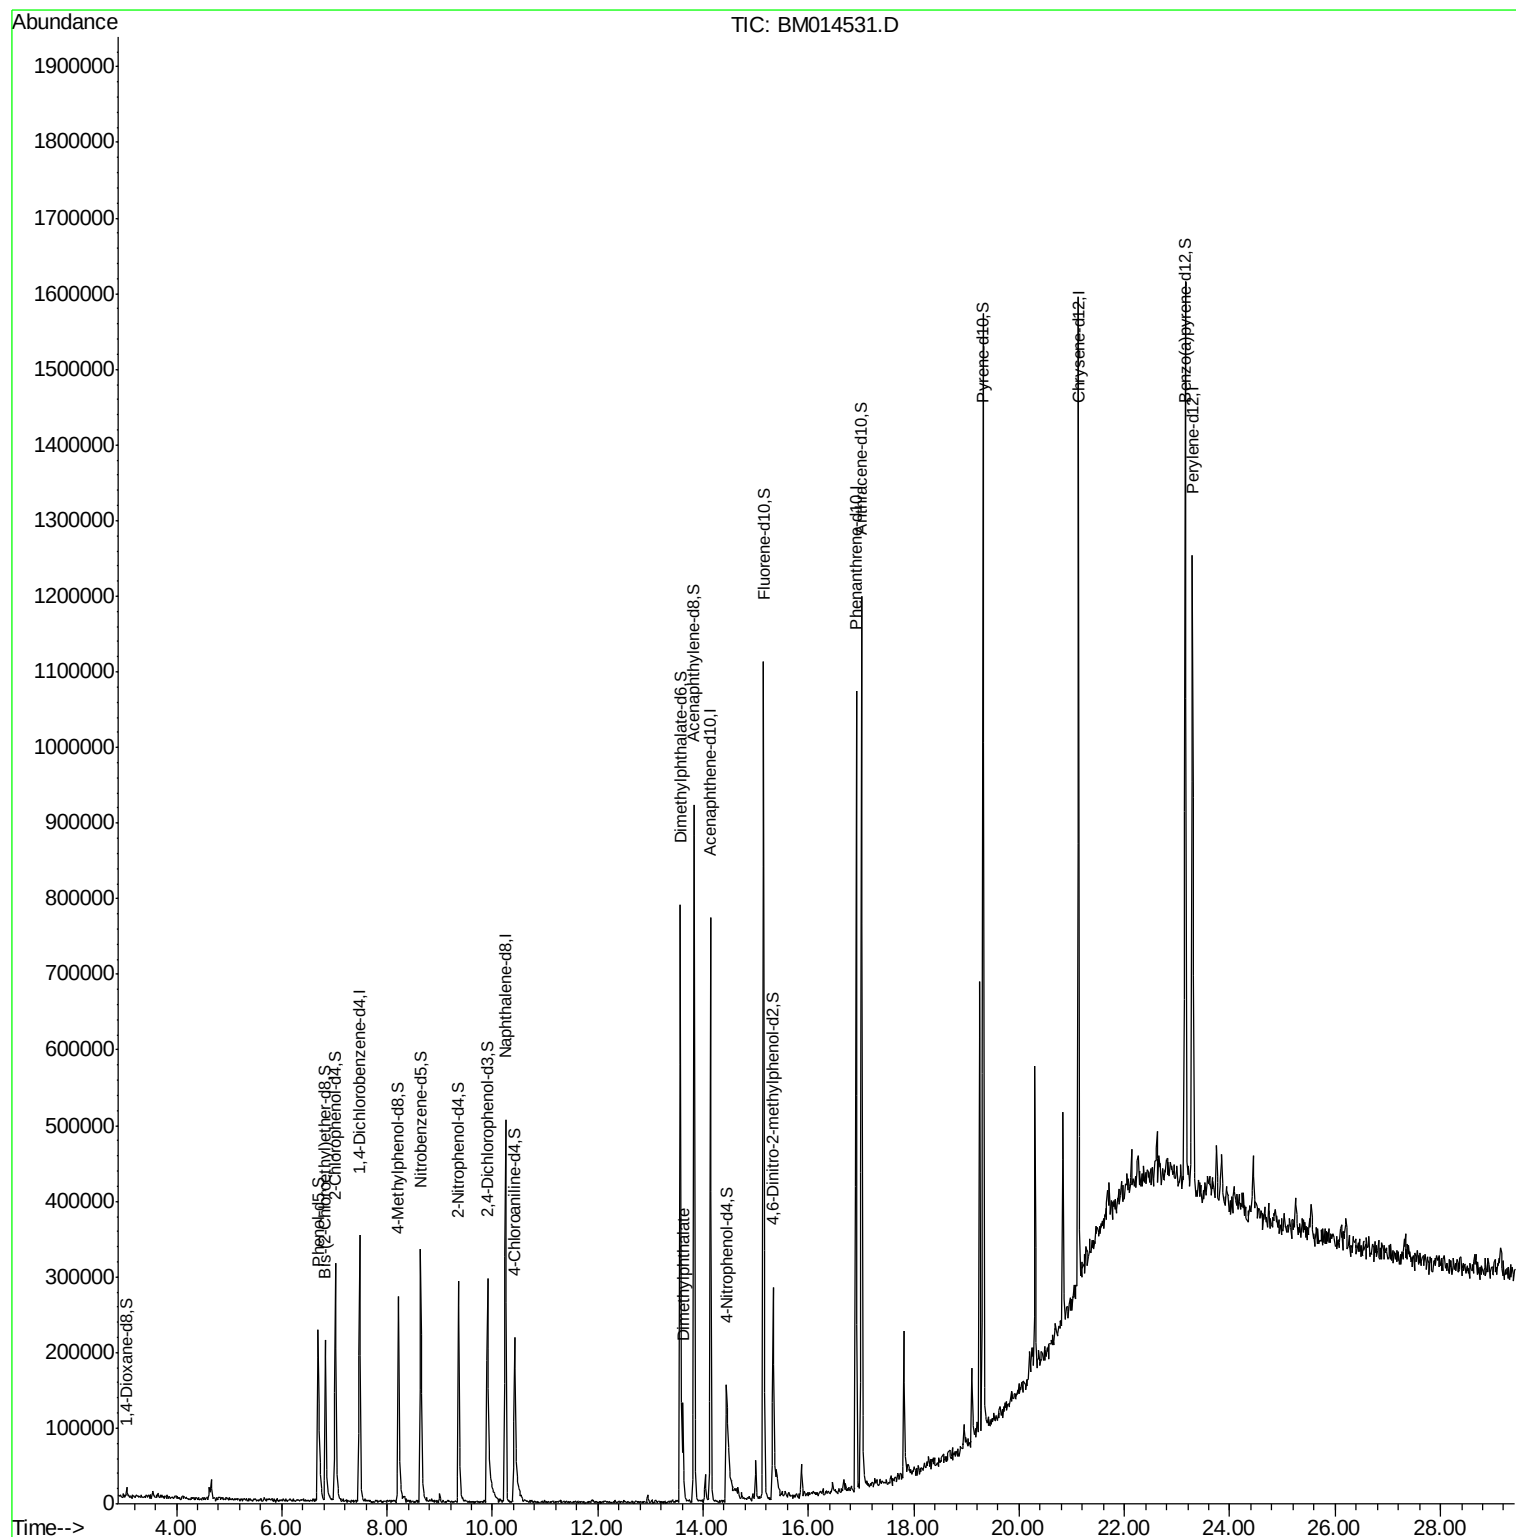

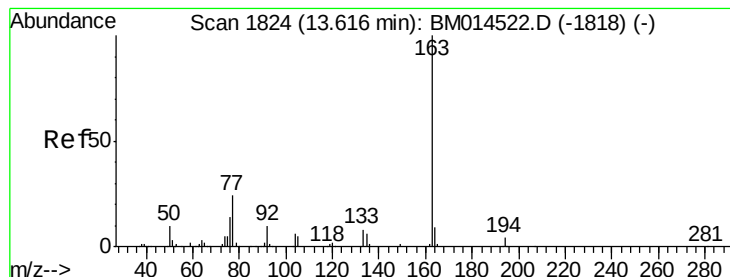

#44

Dimethylphthalate

Concen: 4.35 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM014531.D

Acq: 12 Mar 2018 23:23

Instrument :

BNA_M

ClientSampleId :

F6F48



Tgt Ion:163 Resp: 76644

Ion Ratio Lower Upper

163 100

194 3.5 3.5 5.3#

164 9.1 8.2 12.4

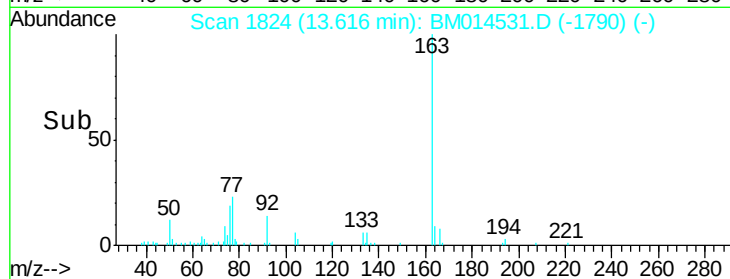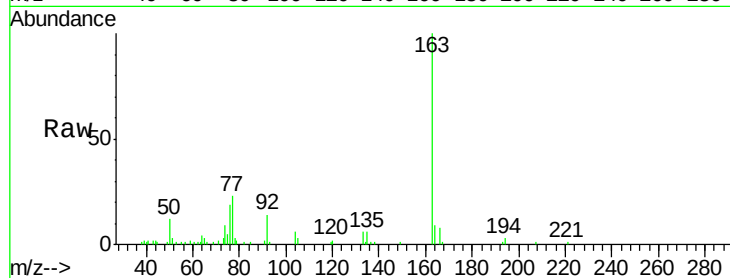

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

