


Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA M\Data\BM031218\
 Data File : BM014532.D
 Acq On : 12 Mar 2018 23:59
 Operator : SJ/JU
 Sample : J1813-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1


Quant Time: Mar 13 05:03:27 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

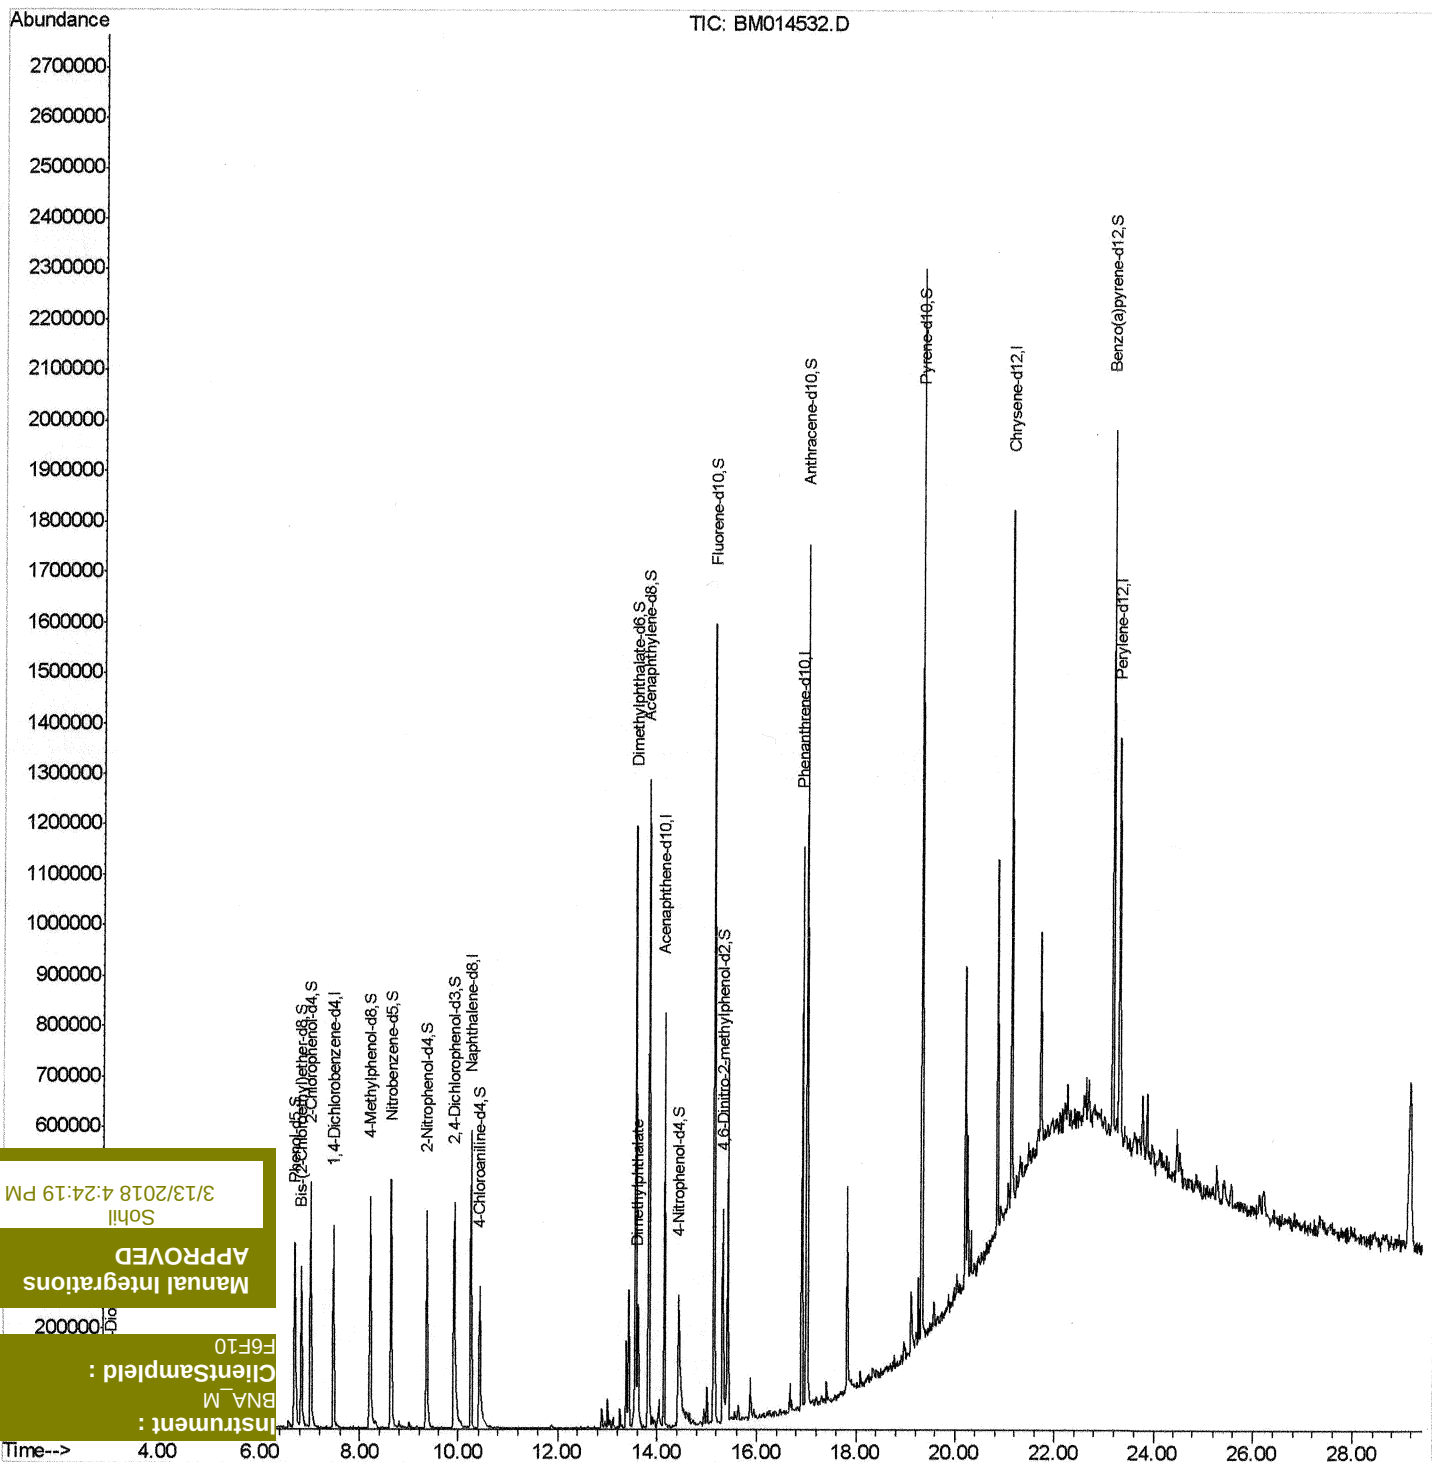

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA M\Data\BM031218\
 Data File : BM014532.D
 Acq On : 12 Mar 2018 23:59
 Operator : SJ/JU
 Sample : J1813-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 13 02:51:11 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

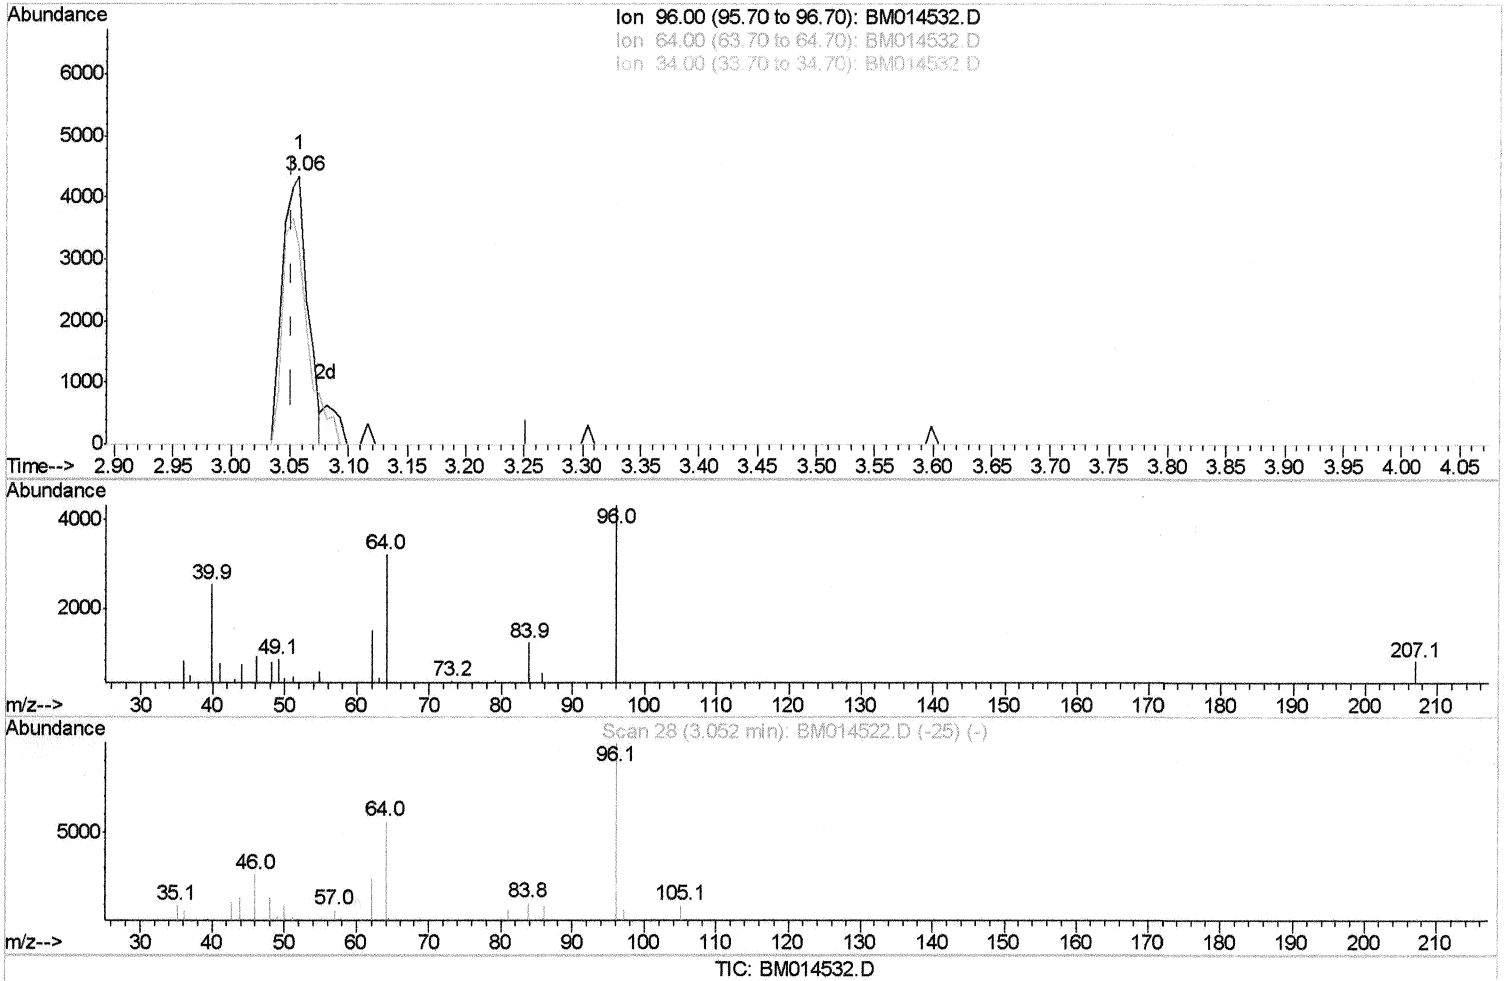

(3) 1,4-Dioxane-d8 (S)

3.057min (+0.006) 3.00ng/uL

response 6413

3/13/2018 4:24:19 PM

Sohil

APPROVED

Manual Integrations

34.00 00.00 00.00

FF10 00

ClientSampled :


BNA_M

Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA M\Data\BM031218\
 Data File : BM014532.D
 Acq On : 12 Mar 2018 23:59
 Operator : SJ/JU
 Sample : J1813-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 13 02:51:11 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

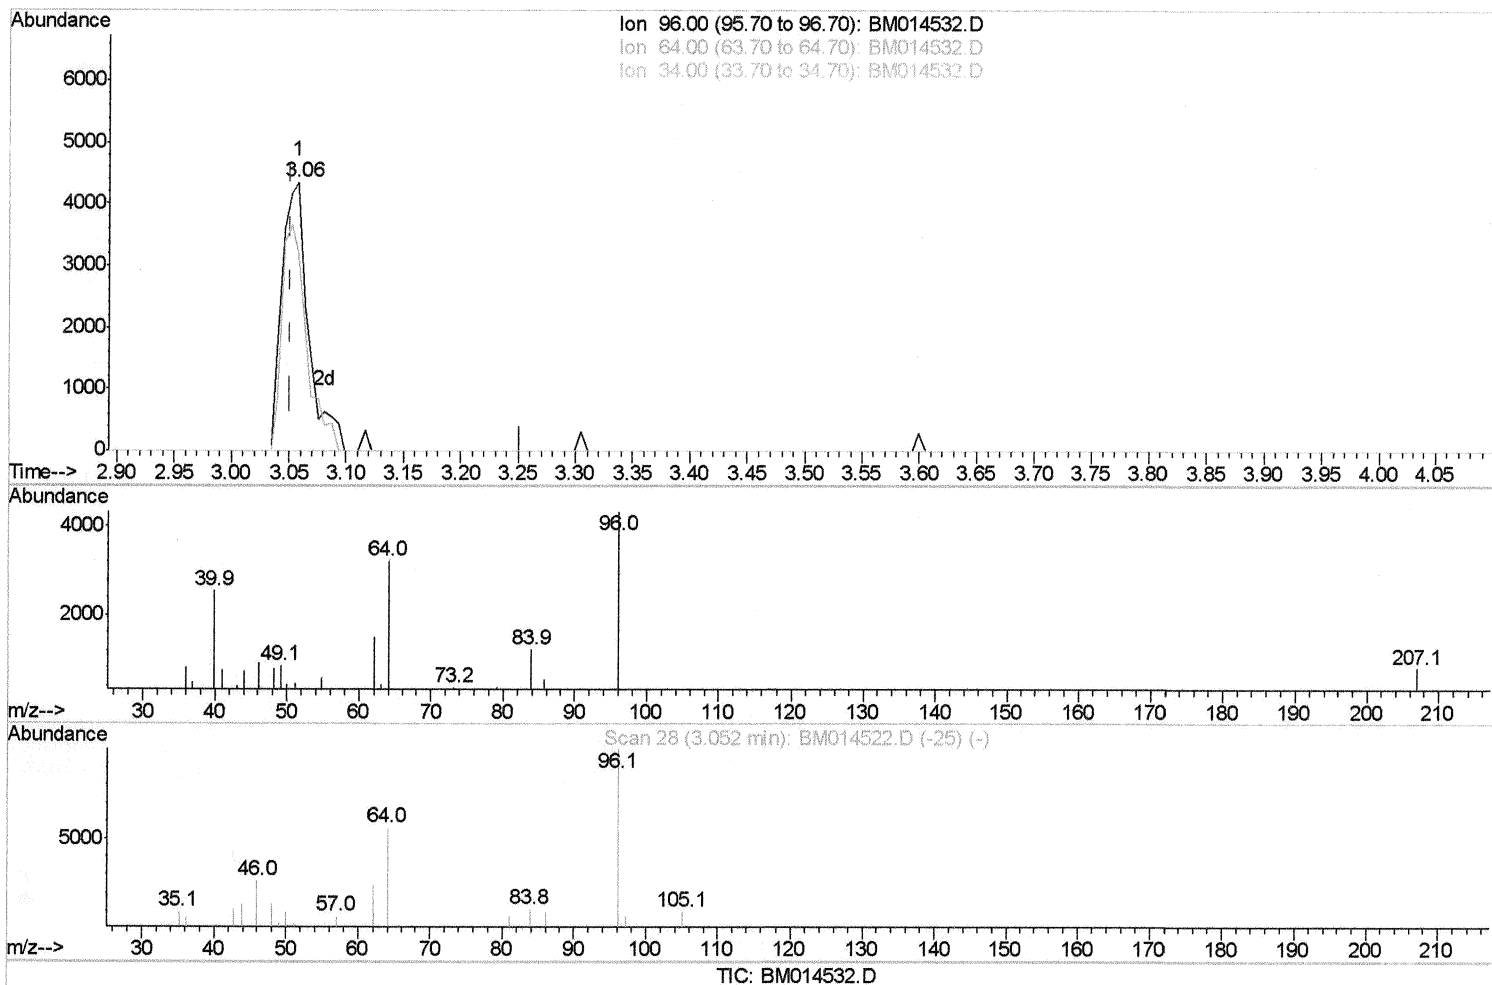

(3) 1,4-Dioxane-d8 (S)

3.057min (+0.006) 3.27ng/uL m

response 6987

JU 3/16/18

3/13/2018 4:24:19 PM

Sohil

APPROVED

Manual Integrations

34.00 00.00 00.00

FF10

ClientSampled :

BNA_M

Instrument :

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA M\Data\BM031218\
 Data File : BM014532.D
 Acq On : 12 Mar 2018 23:59
 Operator : SJ/JU
 Sample : J1813-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 13 05:03:27 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	91507	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	389498	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.14	164	230891	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	559683	20.00	ng/ul	0.00
75) Chrysene-d12	21.13	240	589668	20.00	ng/ul	0.00
83) Perylene-d12	23.29	264	496169	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	6987m	3.27	ng/uL	0.00
5) Phenol-d5	6.68	99	211033	27.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	130879	27.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	171488	28.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	167793	24.79	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	90877	31.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	104109	34.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	176332	28.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	169539	27.89	ng/ul	0.00
43) Dimethylphthalate-d6	13.56	166	666402	34.95	ng/ul	0.00
46) Acenaphthylene-d8	13.83	160	820801	34.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	78321	29.75	ng/ul	-0.03
57) Fluorene-d10	15.14	176	563650	33.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.32	200	87371	26.02	ng/ul	0.00
70) Anthracene-d10	17.00	188	863653	31.98	ng/ul	0.00
76) Pyrene-d10	19.32	212	997408	32.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.16	264	815000	33.75	ng/ul	0.00

JU 3/16/18

Target Compounds

				Ovalue
44) Dimethylphthalate	13.62	163	142440	7.576 ng/ul# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

3/13/2018 4:24:19 PM

Sohil

APPROVED
Manual IntegrationsInstrument :
BNA_M
Client Sampled :
F6F10