

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031218\
 Data File : BM014525.D
 Acq On : 12 Mar 2018 19:46
 Operator : SJ/JU
 Sample : J1813-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6F17

Manual Integrations
 APPROVED

Sohil
 3/13/2018 4:24:00 PM

Quant Time: Mar 13 04:15:57 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 02:49:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	48564	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	218502	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.14	164	145880	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.91	188	372149	20.00	ng/ul	0.00
75) Chrysene-d12	21.13	240	484246	20.00	ng/ul	0.00
83) Perylene-d12	23.30	264	468574	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	3481	3.07	ng/uL	0.00
5) Phenol-d5	6.69	99	111191	27.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	67778	27.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	86819	27.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	96432	26.85	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	46268	28.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	53936	32.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	97390m	28.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	123176m	36.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	420369	34.89	ng/ul	0.00
46) Acenaphthylene-d8	13.83	160	471180	31.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	44971	27.04	ng/ul	-0.01
57) Fluorene-d10	15.14	176	335473	31.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	55481	24.85	ng/ul	0.00
70) Anthracene-d10	17.01	188	588902	32.80	ng/ul	0.00
76) Pyrene-d10	19.32	212	707961	28.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.16	264	762116	33.42	ng/ul	0.00

Target Compounds				Ovalue	
44) Dimethylphthalate	13.62	163	54626	4.598	ng/ul# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM031218\
Data File : BM014525.D
Acq On : 12 Mar 2018 19:46
Operator : SJ/JU
Sample : J1813-02
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F6F17

Quant Time: Mar 13 04:15:57 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 13 02:49:59 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/13/2018 4:24:00 PM

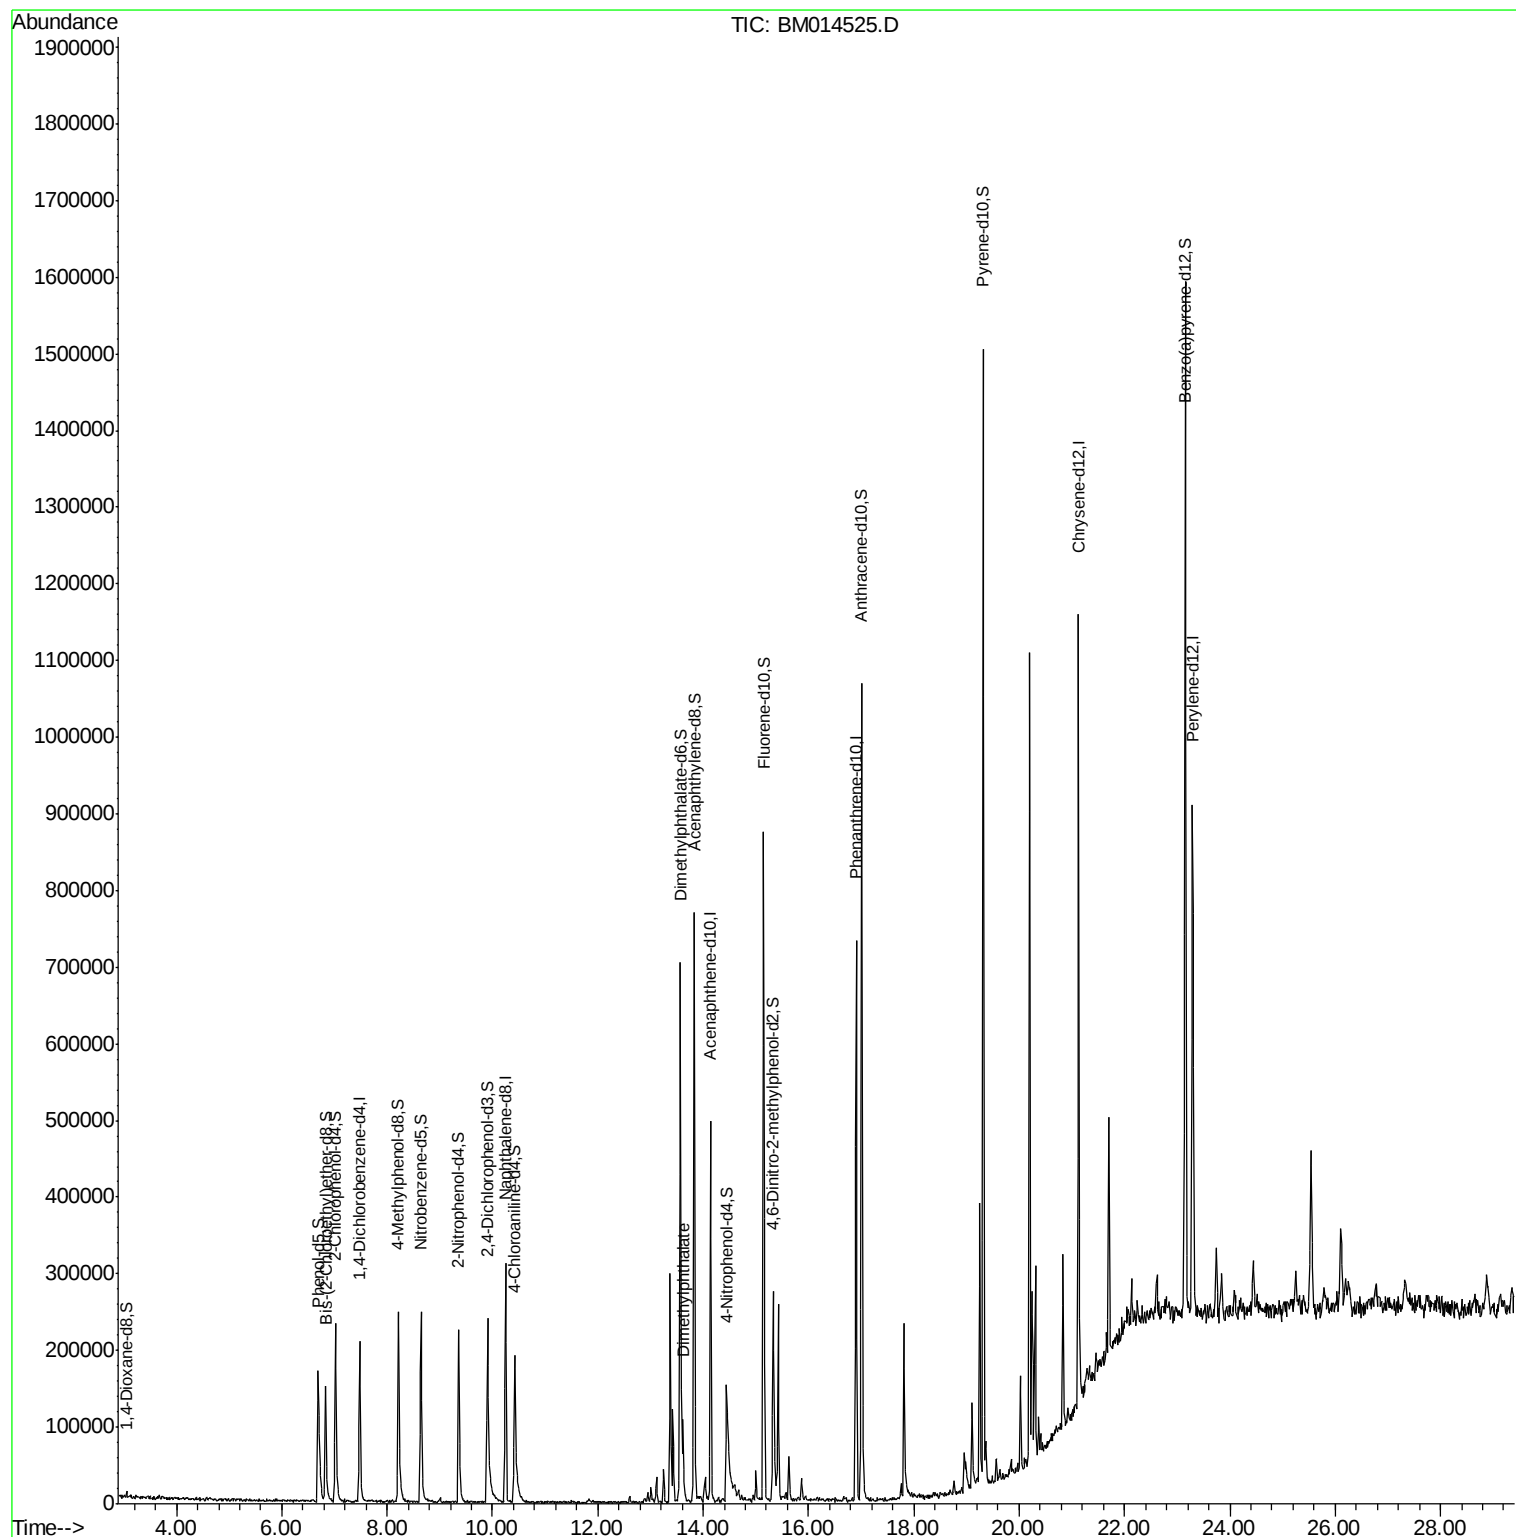

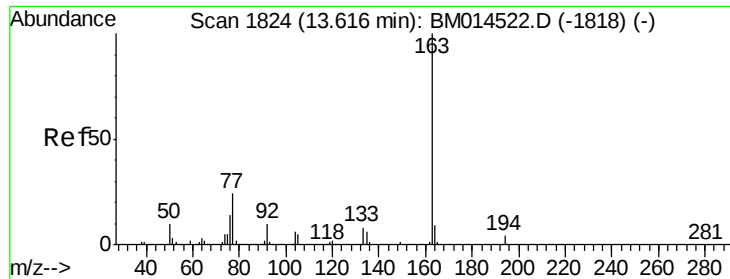

#44
 Dimethylphthalate
 Concen: 4.598 ng/ul
 RT: 13.62 min Scan# 1824
 Delta R.T. -0.00 min
 Lab File: BM014525.D
 Acq: 12 Mar 2018 19:46

Instrument :
 BNA_M
 ClientSampleId :
 F6F17

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.8	3.5	5.3
164	6.9	8.2	12.4

Manual Integrations
 APPROVED

Sohil
 3/13/2018 4:24:00 PM

