

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
 Data File : BM019132.D
 Acq On : 13 Mar 2019 04:51
 Operator : JU/SJ
 Sample : K1849-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C135-CON

Quant Time: Mar 13 06:01:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	206536	20.00	ng	0.00
21) Naphthalene-d8	10.45	136	841450	20.00	ng	0.00
39) Acenaphthene-d10	14.32	164	562133	20.00	ng	0.00
64) Phenanthrene-d10	17.07	188	1391481	20.00	ng	0.00
76) Chrysene-d12	21.27	240	1426684	20.00	ng	0.00
87) Perylene-d12	23.50	264	1281671	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	1584589	124.25	ng	0.00
7) Phenol-d6	6.85	99	2004566	107.46	ng	0.00
23) Nitrobenzene-d5	8.83	82	1662994	93.42	ng	0.00
42) 2,4,6-Tribromophenol	15.82	330	1339500	161.39	ng	0.00
45) 2-Fluorobiphenyl	12.93	172	3640598	84.24	ng	0.00
79) Terphenyl-d14	19.71	244	7123360	99.12	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
Data File : BM019132.D
Acq On : 13 Mar 2019 04:51
Operator : JU/SJ
Sample : K1849-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C135-CON

Quant Time: Mar 13 06:01:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

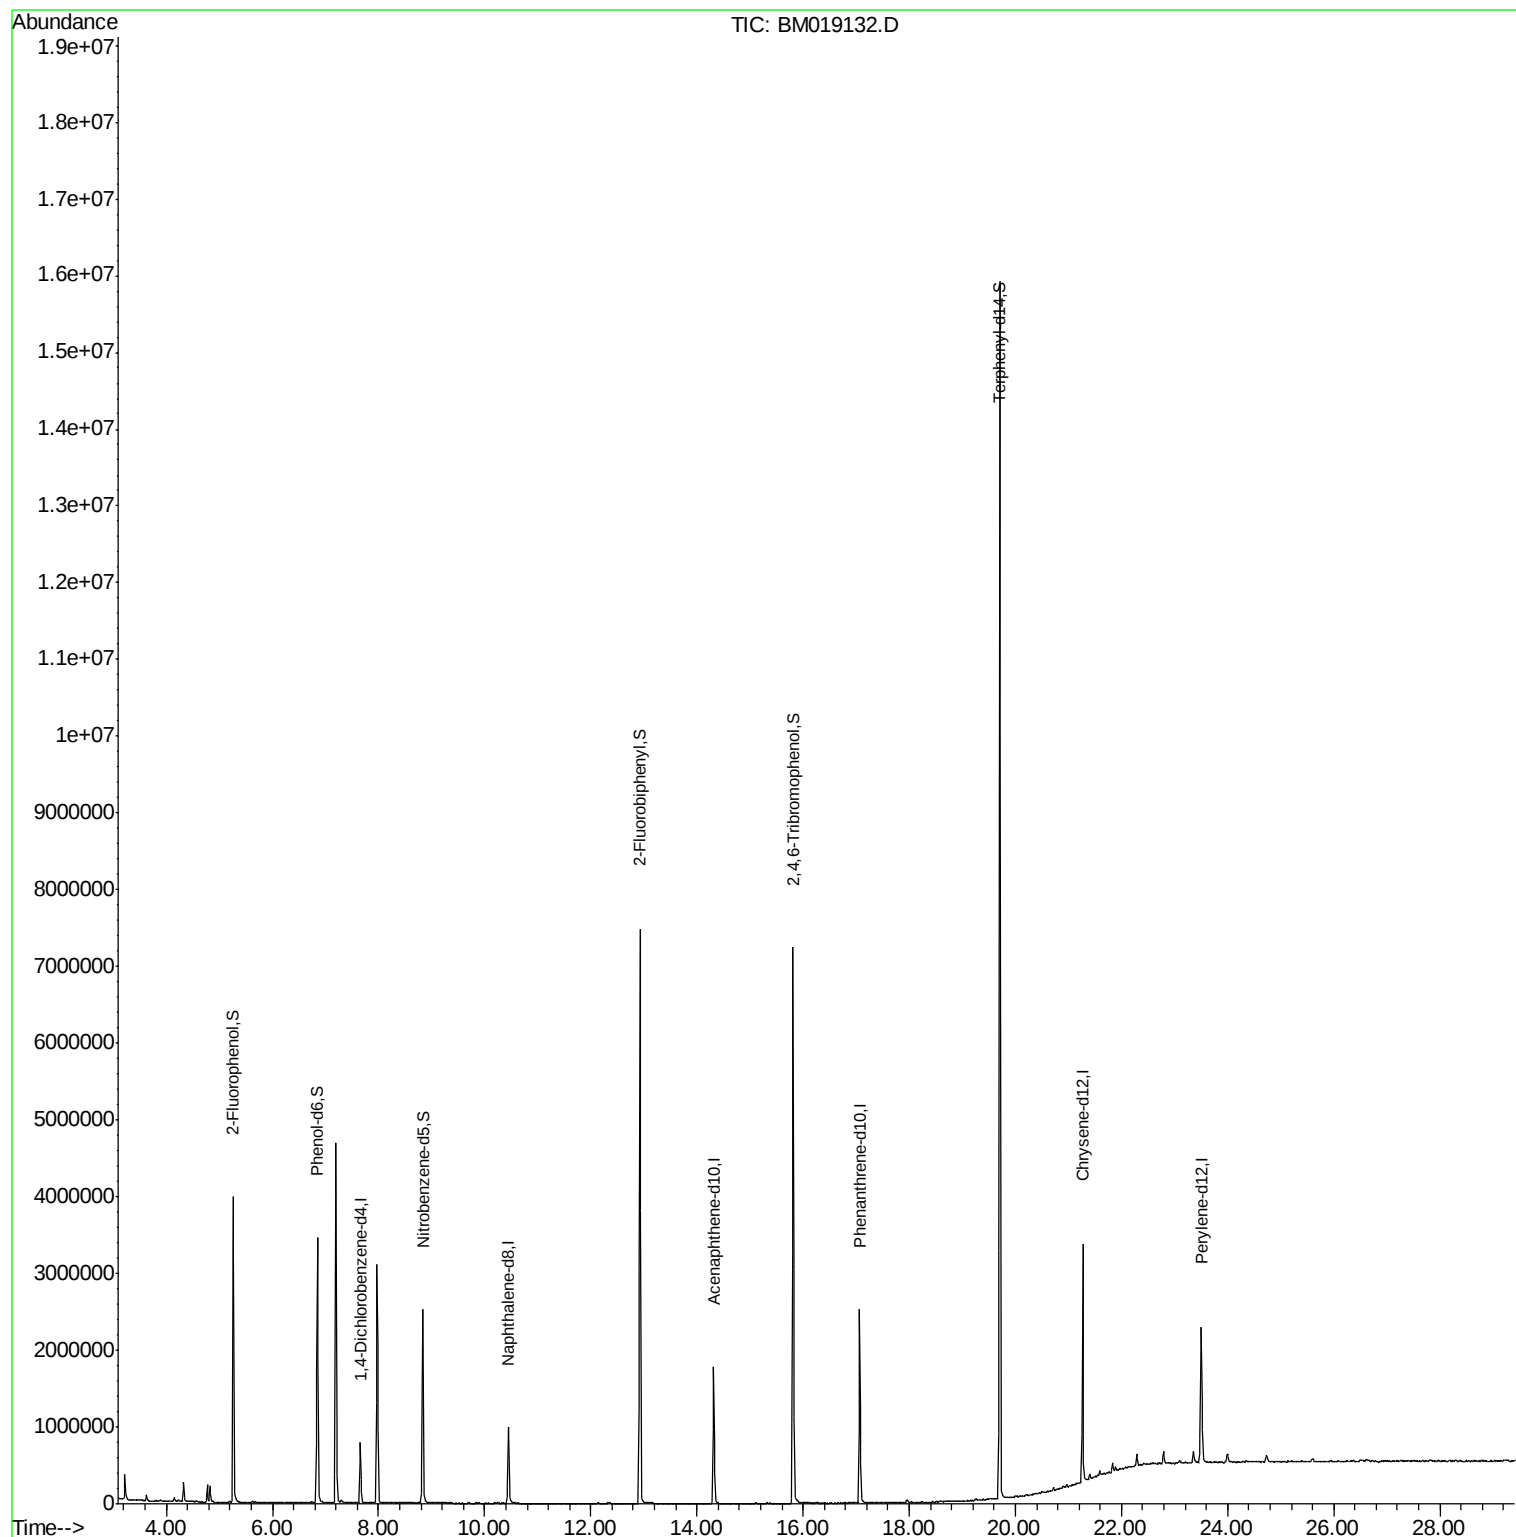




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.66 min Scan# 778
Delta R.T. 0.00 min
Lab File: BM019132.D
Acq: 13 Mar 2019 04:51

Instrument :
BNA_M
ClientSampleId :
C135-CON

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.4	125.3	187.9
115	59.3	49.4	74.0



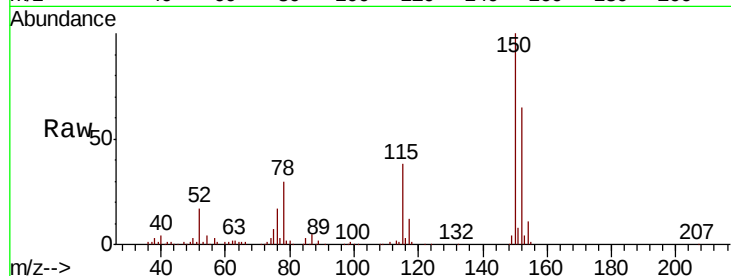


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

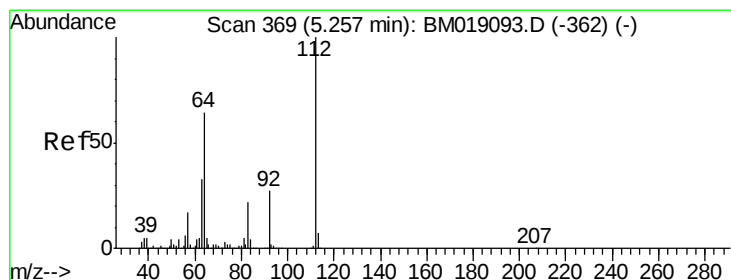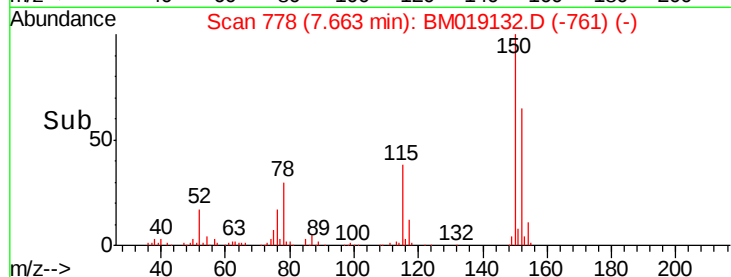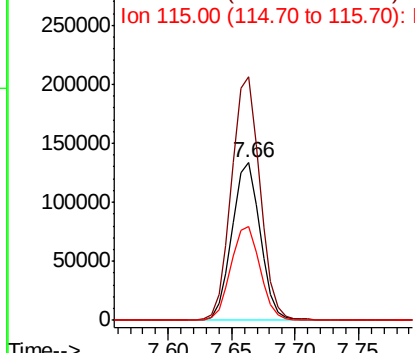

#5

2-Fluorophenol
Concen: 124.250 ng
RT: 5.26 min Scan# 370
Delta R.T. 0.01 min
Lab File: BM019132.D
Acq: 13 Mar 2019 04:51

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.1	51.4	77.0
63	31.3	26.6	40.0


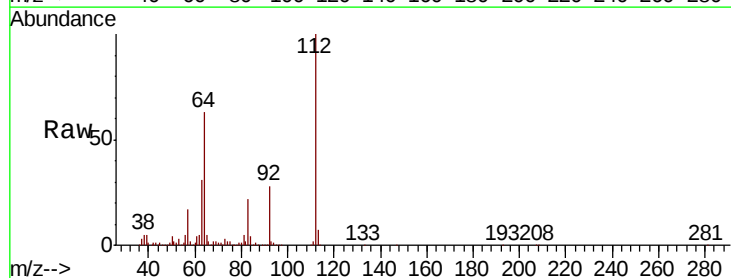



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

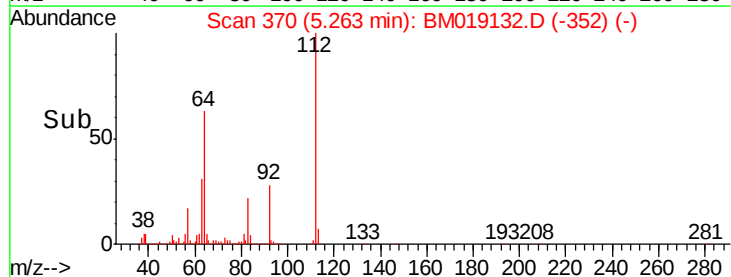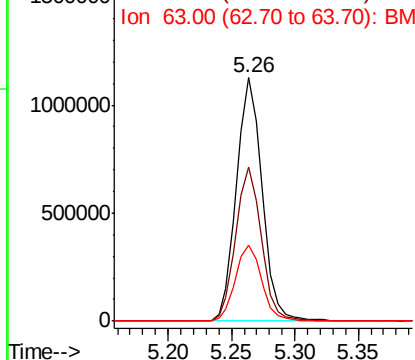

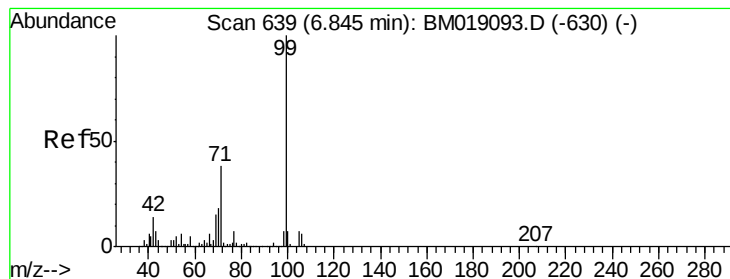

#7

Phenol-d6

Concen: 107.459 ng

RT: 6.85 min Scan# 639

Delta R.T. 0.00 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51

Instrument :


BNA_M

ClientSampleId :

C135-CON

Tot Ion: 99 Resp: 2004566

Ion	Ratio	Lower	Upper
99	100		
42	13.9	10.9	16.3
71	37.7	30.3	45.5



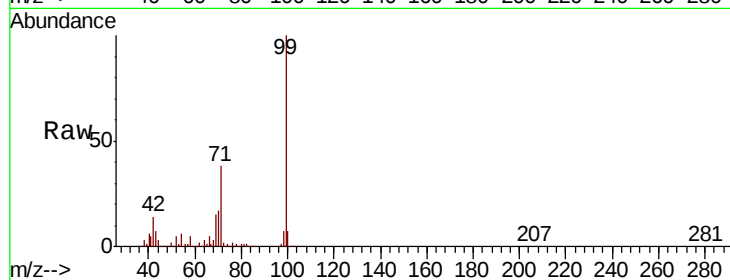


Abundance

Ion 99.00 (98.70 to 99.70): BM019093.D (-630) (-)

Ion 42.00 (41.70 to 42.70): BM019093.D (-630) (-)

Ion 71.00 (70.70 to 71.70): BM019093.D (-630) (-)

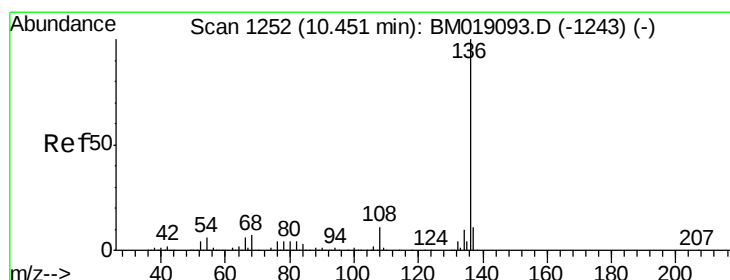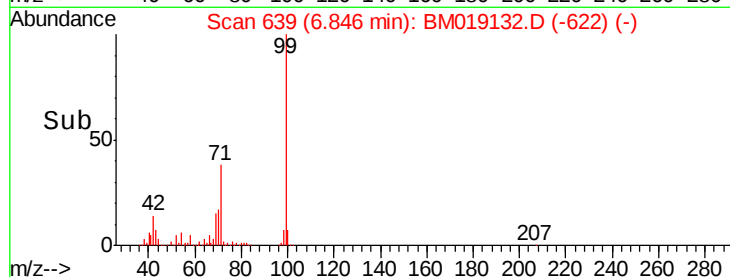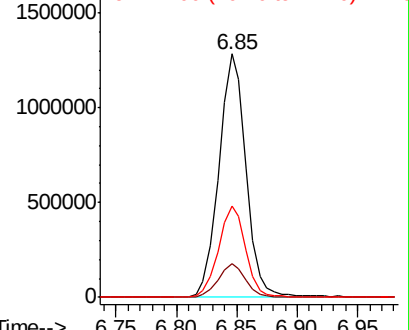

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.45 min Scan# 1251


Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51

Tgt Ion: 136 Resp: 841450

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	13.0
54	6.7	5.2	7.8
68	7.4	5.8	8.8

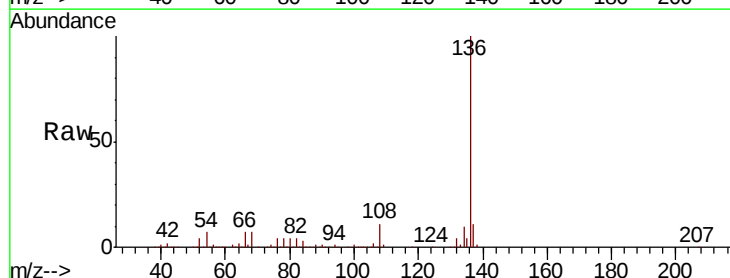



Abundance

Ion 136.00 (135.70 to 136.70): BM019093.D (-1243) (-)

Ion 137.00 (136.70 to 137.70): BM019093.D (-1243) (-)

Ion 54.00 (53.70 to 54.70): BM019093.D (-1243) (-)

Ion 68.00 (67.70 to 68.70): BM019093.D (-1243) (-)



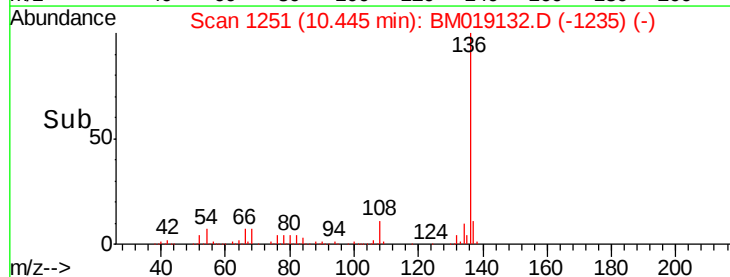
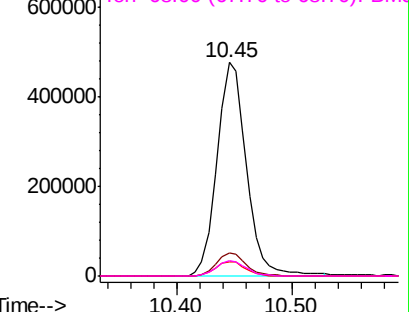




#23
Nitrobenzene-d5
Concen: 93.422 ng
RT: 8.83 min Scan# 977
Delta R.T. 0.00 min
Lab File: BM019132.D
Acq: 13 Mar 2019 04:51




Instrument :
BNA_M
ClientSampleId :
C135-CON


Tot Ion: 82 Resp: 1662994
Ion Ratio Lower Upper
82 100
128 37.5 29.4 44.2
54 36.3 29.9 44.9

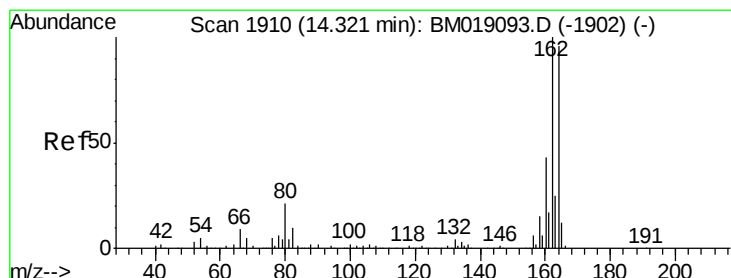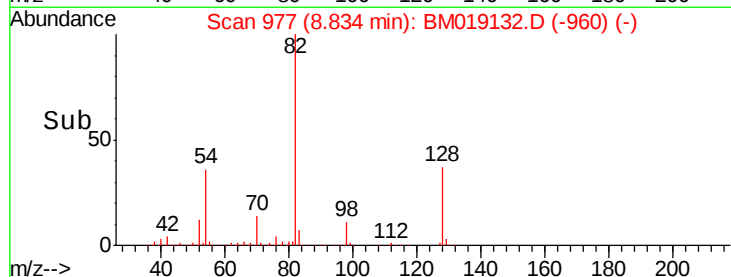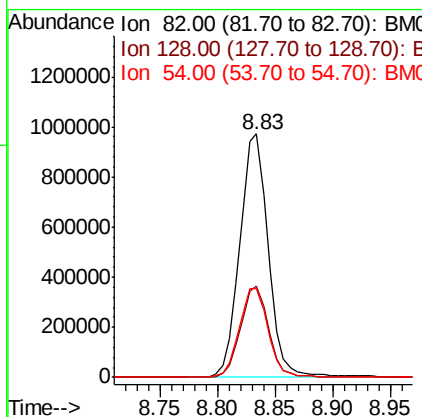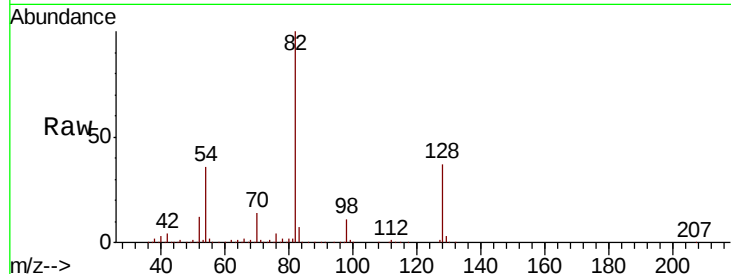

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.32 min Scan# 1909
Delta R.T. -0.01 min
Lab File: BM019132.D
Acq: 13 Mar 2019 04:51

Tgt Ion:164 Resp: 562133
Ion Ratio Lower Upper
164 100
162 105.3 83.5 125.3
160 47.0 36.3 54.5

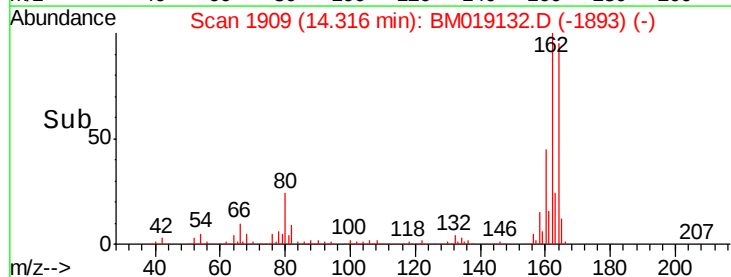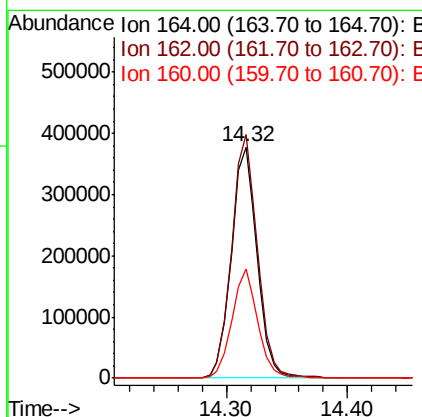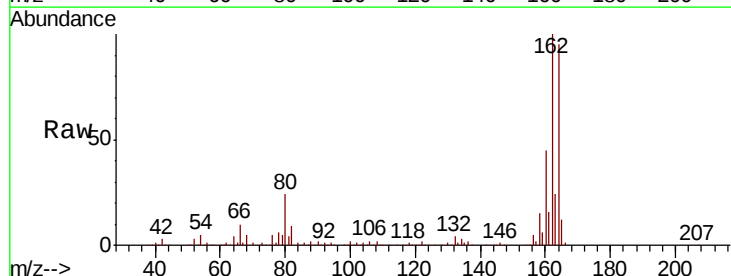

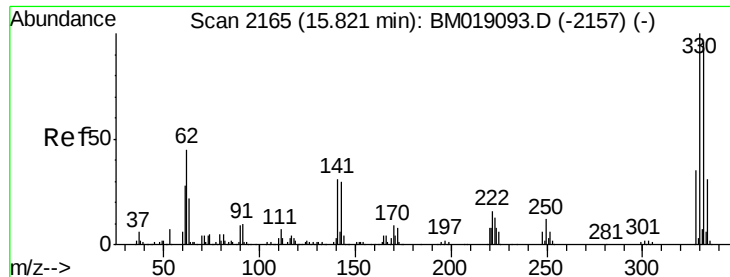

#42

2,4,6-Tribromophenol

Concen: 161.391 ng

RT: 15.82 min Scan# 2164

Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51

Instrument :

BNA_M

ClientSampleId :

C135-CON


Tot Ion:330 Resp: 1339500

Ion Ratio Lower Upper




330 100

332 96.7 76.8 115.2

141 32.8 27.0 40.4

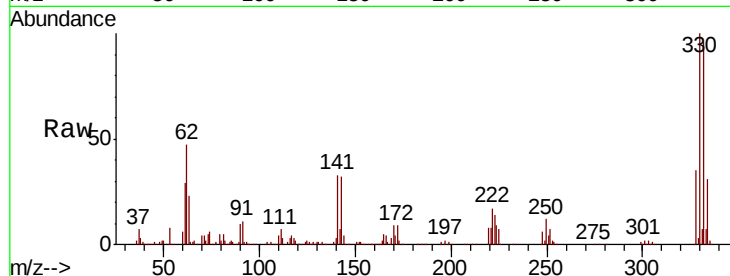

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

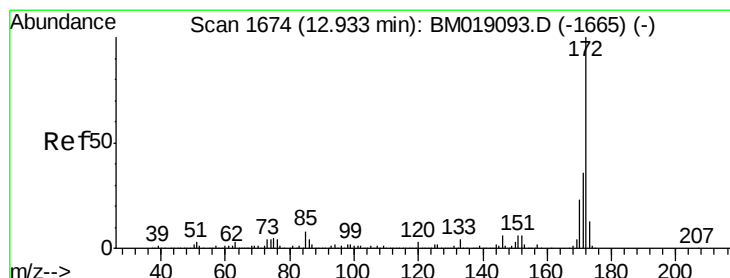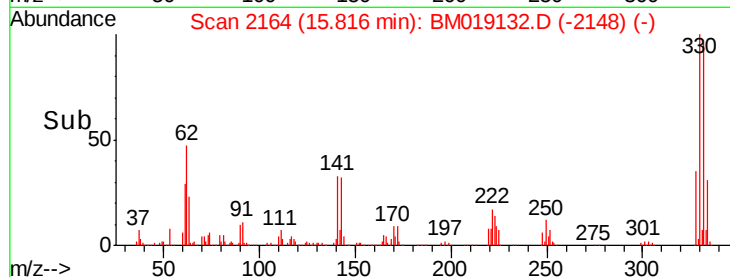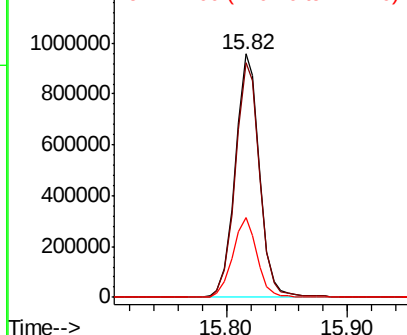

#45

2-Fluorobiphenyl

Concen: 84.242 ng

RT: 12.93 min Scan# 1673

Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51


Tgt Ion:172 Resp: 3640598

Ion Ratio Lower Upper



172 100


171 36.2 28.6 42.8

170 23.6 18.6 28.0

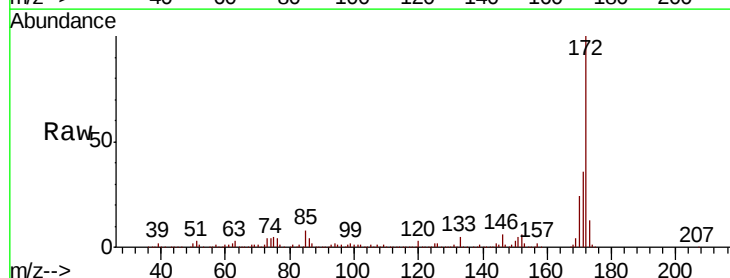

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

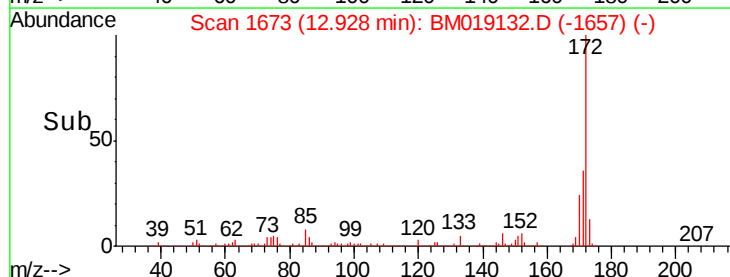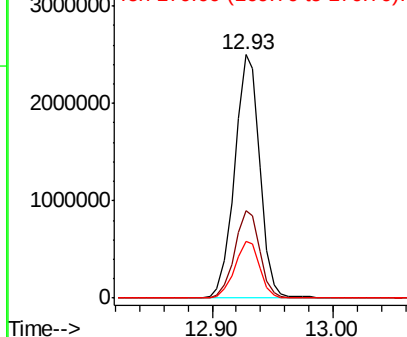

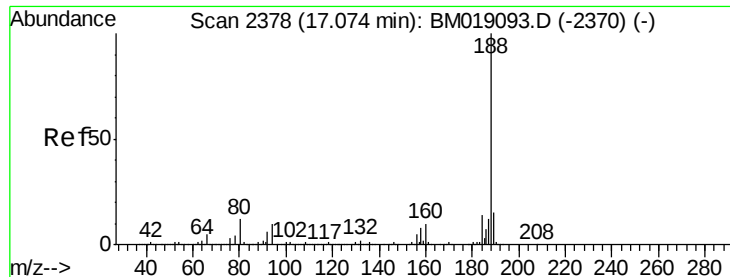

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.07 min Scan# 2377

Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51

Instrument :

BNA_M

ClientSampleId :

C135-CON


Tot Ion:188 Resp: 1391481

Ion Ratio Lower Upper

188 100

94 10.2 8.1 12.1




80 12.5 9.7 14.5

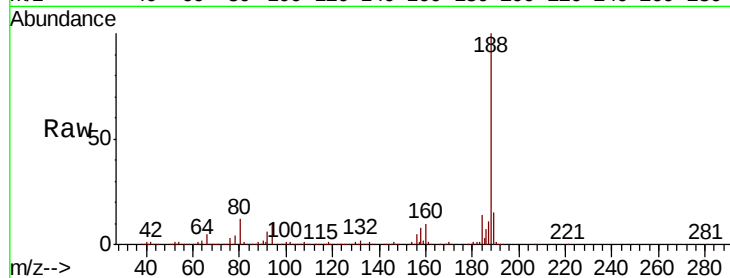

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

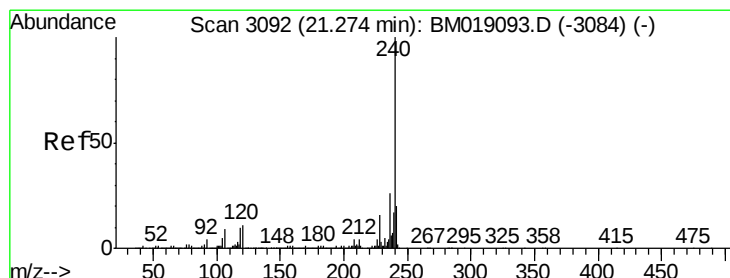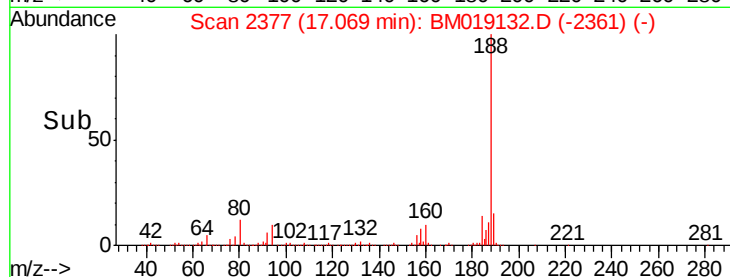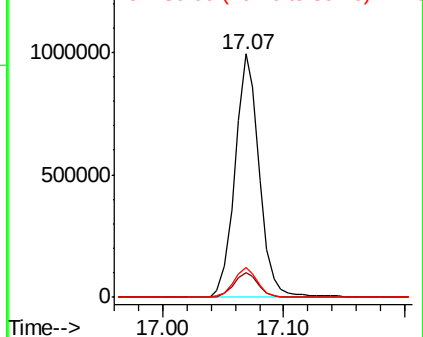

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.27 min Scan# 3091

Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51


Tgt Ion:240 Resp: 1426684

Ion Ratio Lower Upper

240 100

120 11.2 8.9 13.3



236 26.2 21.0 31.4

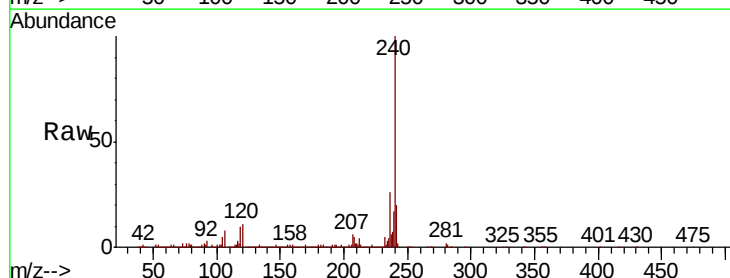


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

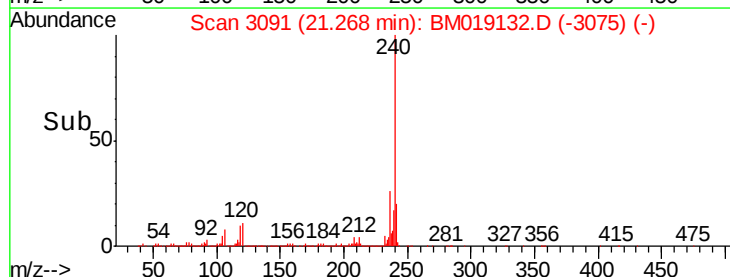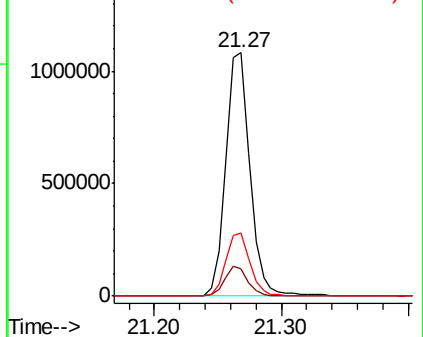

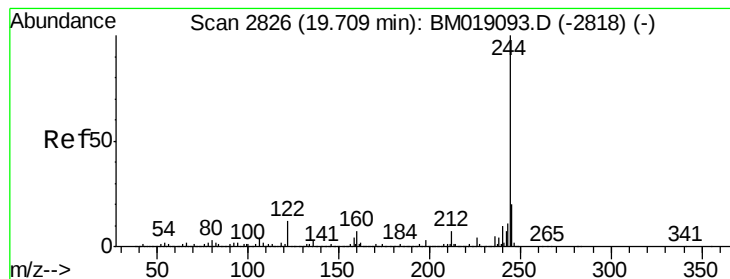

#79

Terphenyl-d14

Concen: 99.121 ng

RT: 19.71 min Scan# 2826

Delta R.T. 0.00 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51

Instrument :

BNA_M

ClientSampleId :

C135-CON


Tot Ion:244 Resp: 7123360

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.2




122 11.3 9.4 14.2

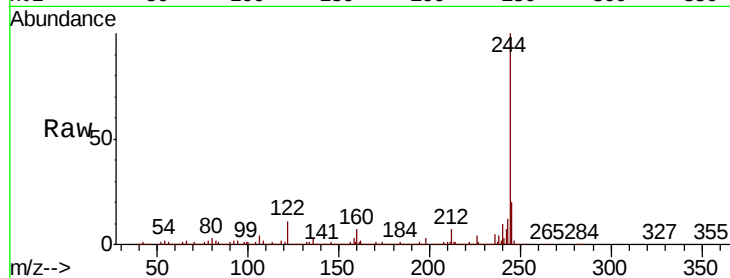

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

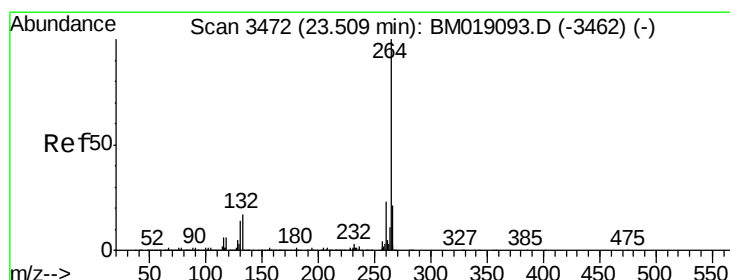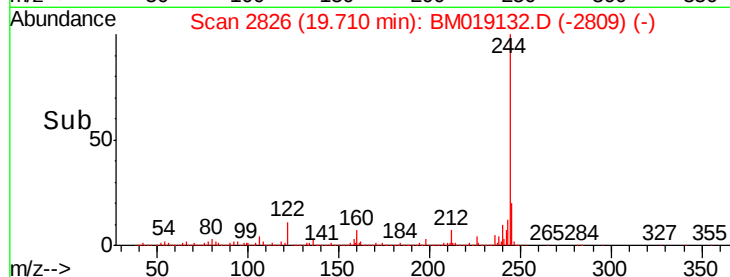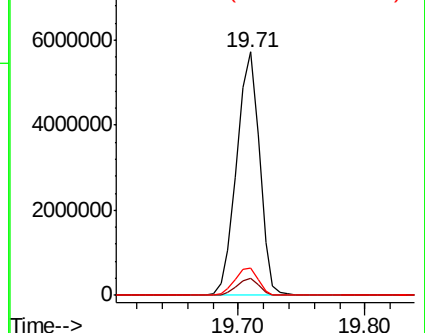

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.50 min Scan# 3471

Delta R.T. -0.01 min

Lab File: BM019132.D

Acq: 13 Mar 2019 04:51


Tgt Ion:264 Resp: 1281671

Ion Ratio Lower Upper

264 100

260 23.4 18.6 28.0

265 22.4 17.3 25.9

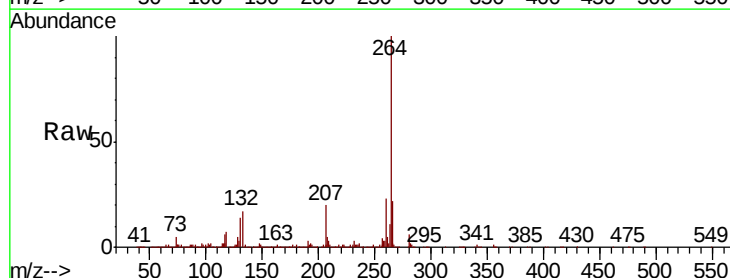

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

