

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
 Data File : BM019113.D
 Acq On : 12 Mar 2019 15:52
 Operator : JU/SJ
 Sample : K1817-17RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PST-028-SW012-1-030619RE

Integration Parameters: rteint.p

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	363	369	389	rBV	2153103	3274309	38.44%	5.594%
2	6.840	631	638	659	rBV	2460127	3995178	46.90%	6.826%
3	7.198	692	699	716	rBV	2385492	3814407	44.78%	6.517%
4	7.663	771	778	787	rBV	808916	1281506	15.04%	2.189%
5	7.981	825	832	844	rBV	1514856	2489188	29.22%	4.253%
6	8.834	969	977	997	rBV	1196296	2203820	25.87%	3.765%
7	10.451	1244	1252	1273	rBV	1046912	1932469	22.69%	3.302%
8	12.928	1666	1673	1698	rBV	3494021	5350723	62.81%	9.142%
9	13.786	1812	1819	1830	rBV	198379	332575	3.90%	0.568%
10	14.316	1902	1909	1928	rBV2	1867214	2885830	33.88%	4.930%
11	15.816	2157	2164	2181	rBV	3241132	4710938	55.30%	8.049%
12	17.068	2371	2377	2394	rBV	2398623	3635585	42.68%	6.211%
13	17.962	2523	2529	2551	rBV	405297	790829	9.28%	1.351%
14	19.251	2743	2748	2757	rBV	132513	231411	2.72%	0.395%
15	19.709	2820	2826	2841	rBV	6795694	8518382	100.00%	14.554%
16	20.968	3036	3040	3050	rBV	1250815	1520284	17.85%	2.597%
17	21.268	3086	3091	3100	rBV	3454982	4496482	52.79%	7.682%
18	21.403	3111	3114	3123	rBV4	97158	144464	1.70%	0.247%
19	21.833	3184	3187	3189	rBV	172951	215878	2.53%	0.369%
20	21.856	3189	3191	3201	rVB2	304002	450284	5.29%	0.769%
21	22.292	3262	3265	3269	rBV	165266	205472	2.41%	0.351%
22	22.797	3347	3351	3355	rBV	241305	308897	3.63%	0.528%
23	22.845	3356	3359	3368	rVB5	147095	263899	3.10%	0.451%
24	23.362	3443	3447	3452	rVB2	164221	251411	2.95%	0.430%
25	23.509	3465	3472	3489	rVB	2181421	4315019	50.66%	7.372%
26	24.003	3553	3556	3563	rVB	182025	301417	3.54%	0.515%
27	24.097	3567	3572	3585	rVB3	267468	609978	7.16%	1.042%


Sum of corrected areas: 58530635

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
Data File : BM019113.D
Acq On : 12 Mar 2019 15:52
Operator : JU/SJ
Sample : K1817-17RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PST-028-SW012-1-030619RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

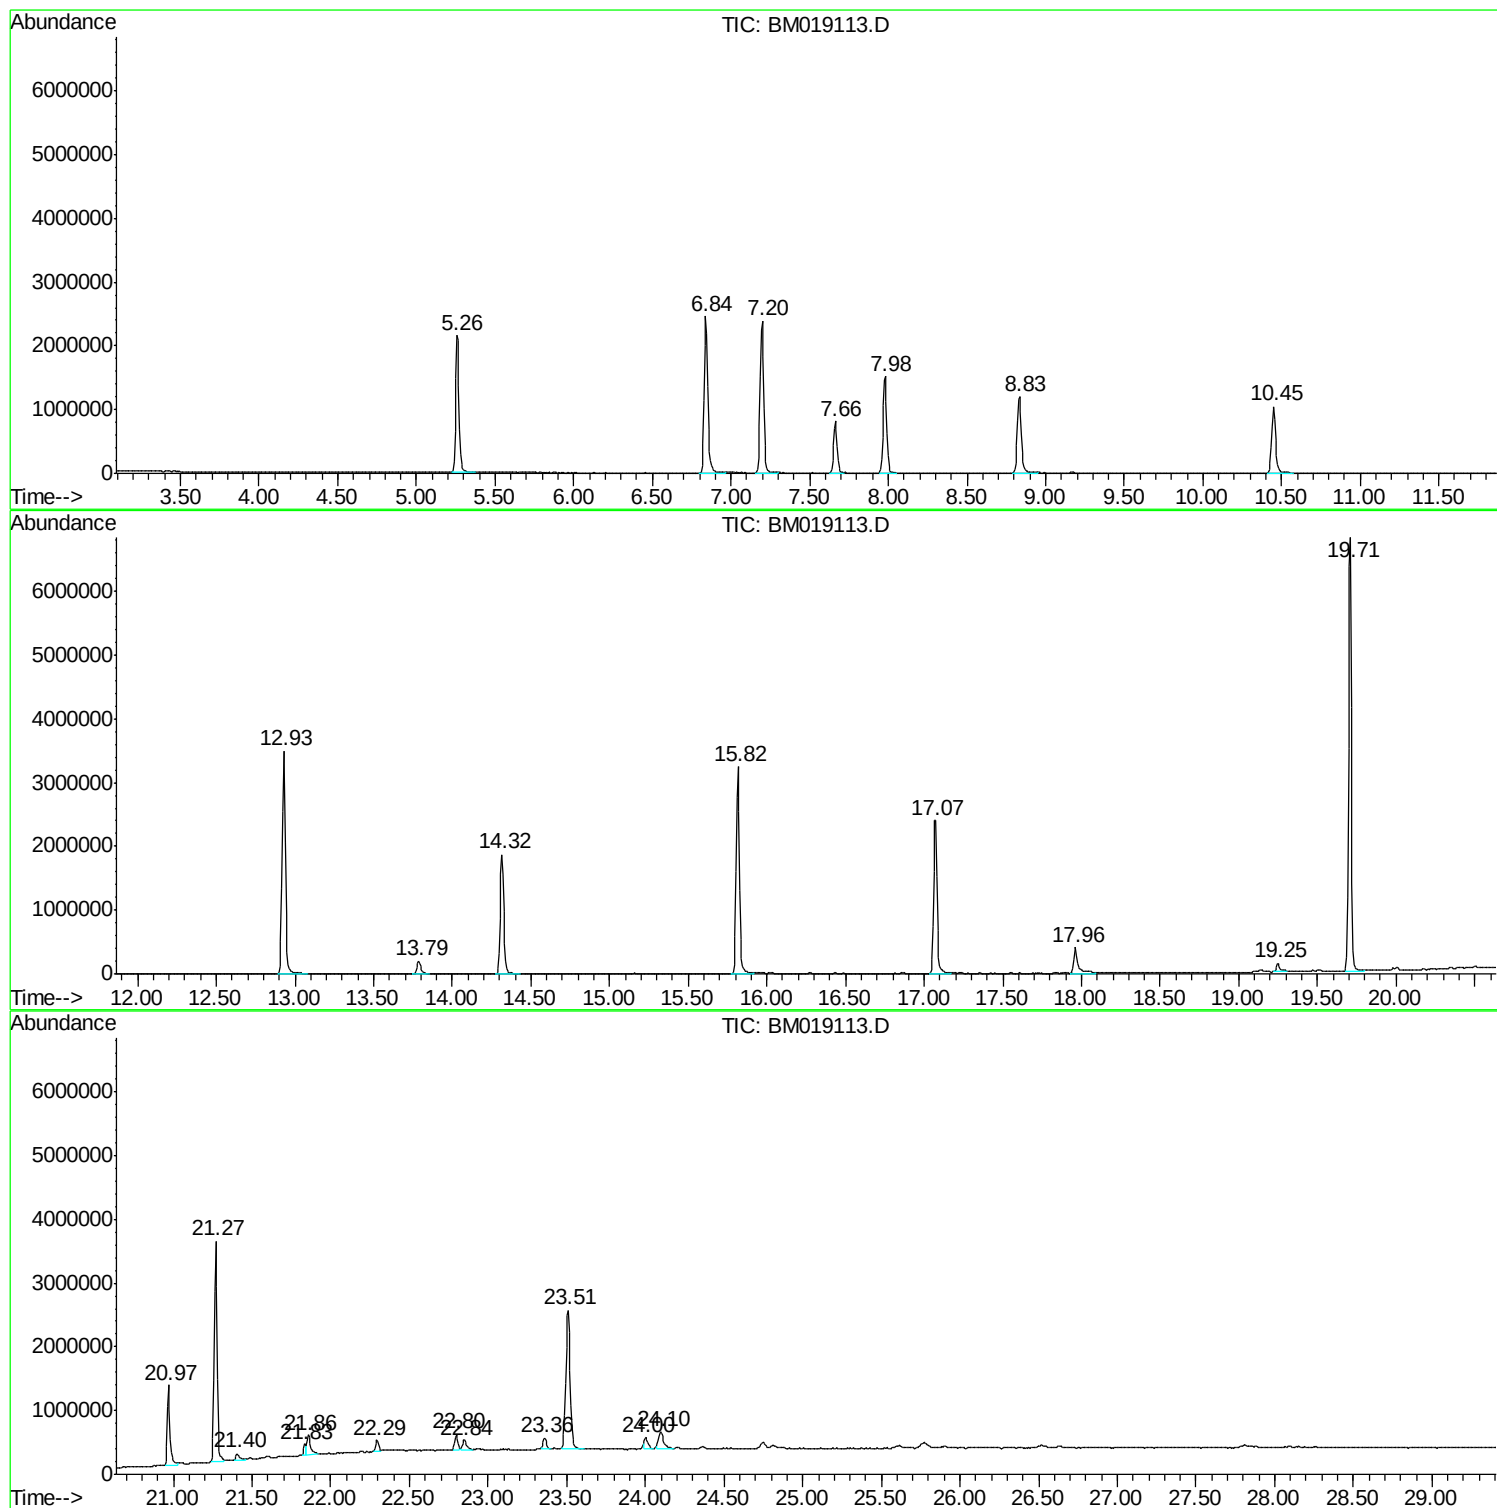

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031219\
Data_File : BM019113.D
Acq_On : 12-Mar-2019 15:522
Operator : JU/SJJ
Sample : K1817-17REE
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
PST-028-SW012-1-030619RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
