

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
 Data File : BM019123.D
 Acq On : 12 Mar 2019 21:57
 Operator : JU/SJ
 Sample : K1842-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB-030719

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	363	369	386	rBV	1993299	3028994	14.23%	3.636%
2	6.840	632	638	658	rBV	1279765	2076862	9.75%	2.493%
3	7.198	691	699	712	rBV	3949801	6365051	29.90%	7.641%
4	7.663	771	778	787	rBV	832502	1334281	6.27%	1.602%
5	7.975	824	831	847	rBV	3198520	5260298	24.71%	6.315%
6	8.834	968	977	993	rBV	2767082	4764124	22.38%	5.719%
7	10.445	1244	1251	1273	rBV	1029190	1904194	8.94%	2.286%
8	12.928	1666	1673	1692	rBV	8118680	12136648	57.01%	14.570%
9	14.316	1902	1909	1926	rBV2	1810281	2864508	13.45%	3.439%
10	15.816	2157	2164	2181	rBV	7687839	10583043	49.71%	12.705%
11	17.068	2371	2377	2394	rBV	2477729	3588535	16.86%	4.308%
12	19.709	2820	2826	2840	rBV	18755031	21290382	100.00%	25.559%
13	21.268	3086	3091	3104	rBV	3276361	4299060	20.19%	5.161%
14	23.509	3465	3472	3484	rVB	1977149	3803285	17.86%	4.566%


Sum of corrected areas: 83299265

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
Data File : BM019123.D
Acq On : 12 Mar 2019 21:57
Operator : JU/SJ
Sample : K1842-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-030719

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

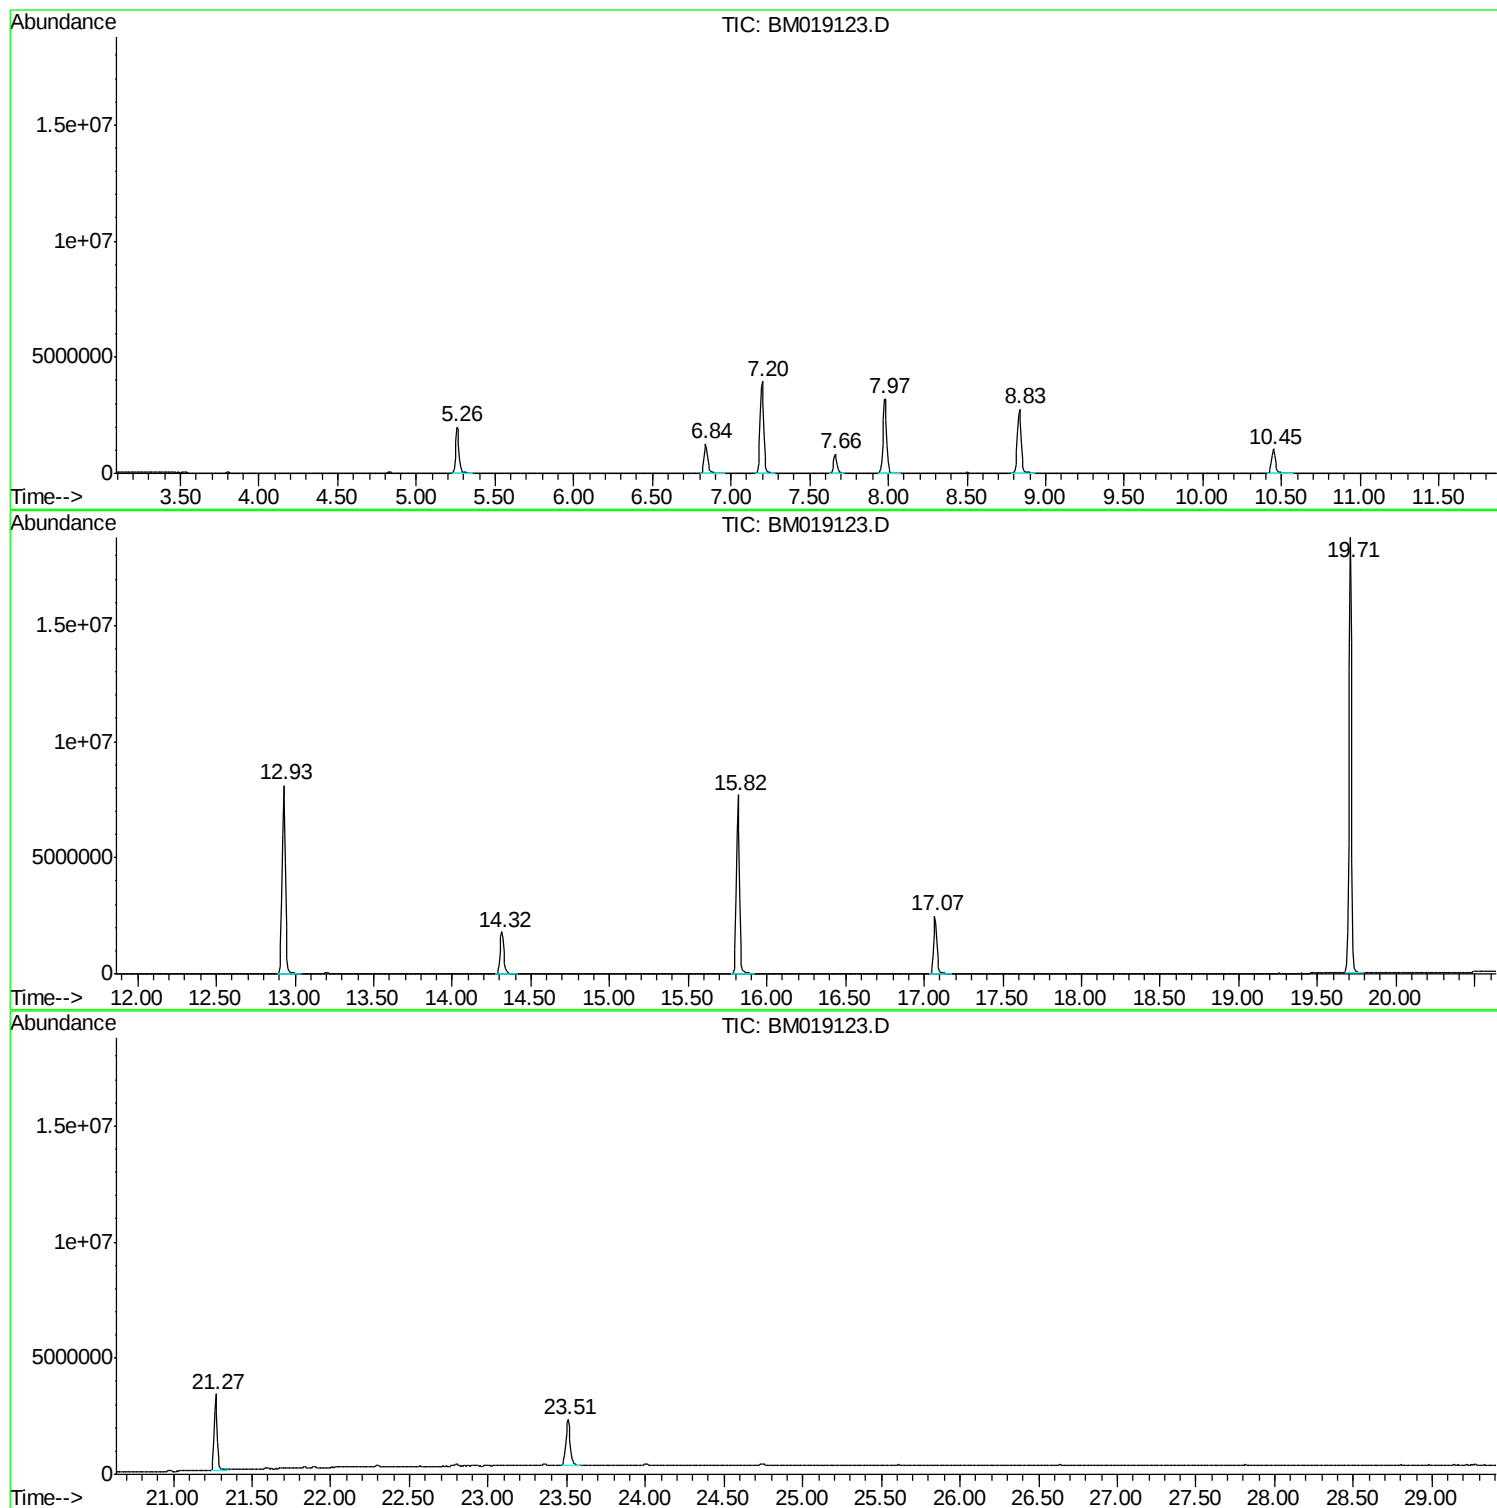

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
Data File : BM019123.D
Acq On : 12 Mar 2019 21:57
Operator : JU/SJ
Sample : K1842-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-030719










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.20 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.20	95.41 ng	6365050	1,4-Dichlorobenzene-d4	7.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	22
3			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4			(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
5			Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

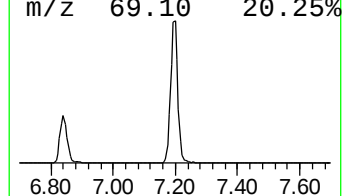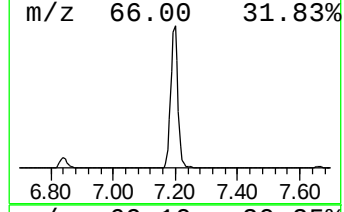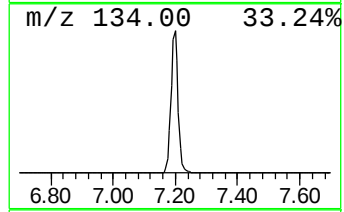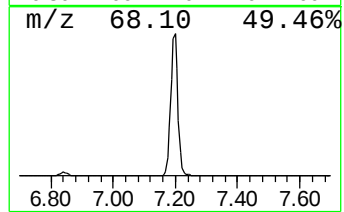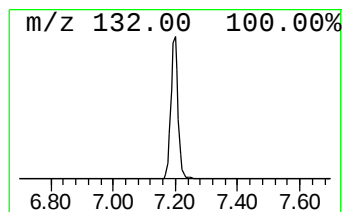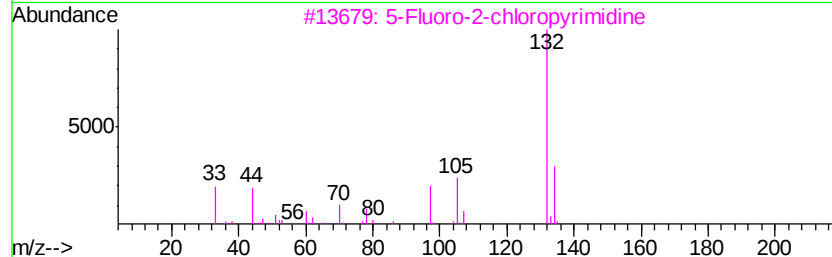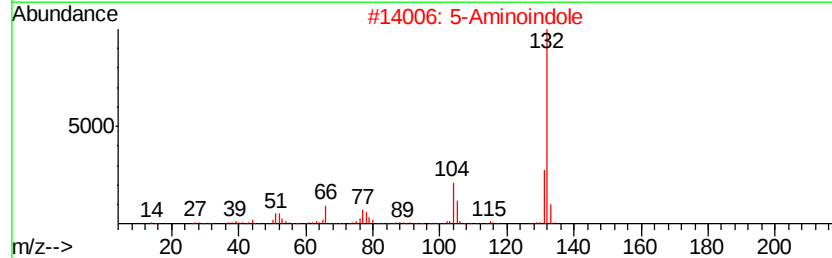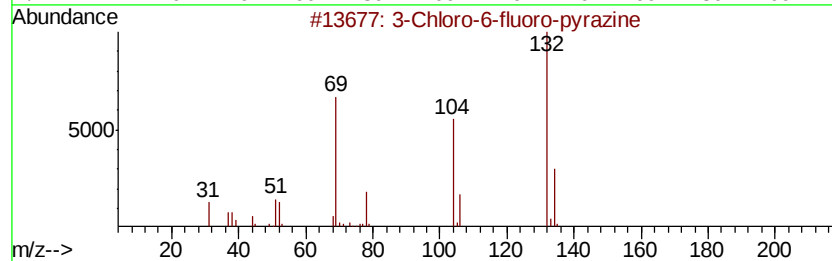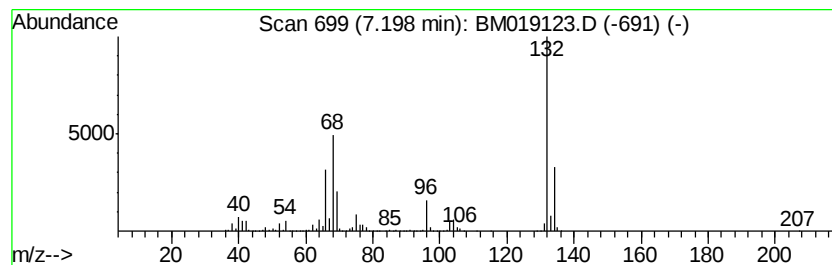

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM031219\
Data File : BM019123.D
Acq On : 12 Mar 2019 21:57
Operator : JU/SJ
Sample : K1842-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-030719

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.20	7.20	95.4	ng	6365050	1	7.66	1334280	20.0