


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
 Data File : BM019106.D
 Acq On : 12 Mar 2019 11:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

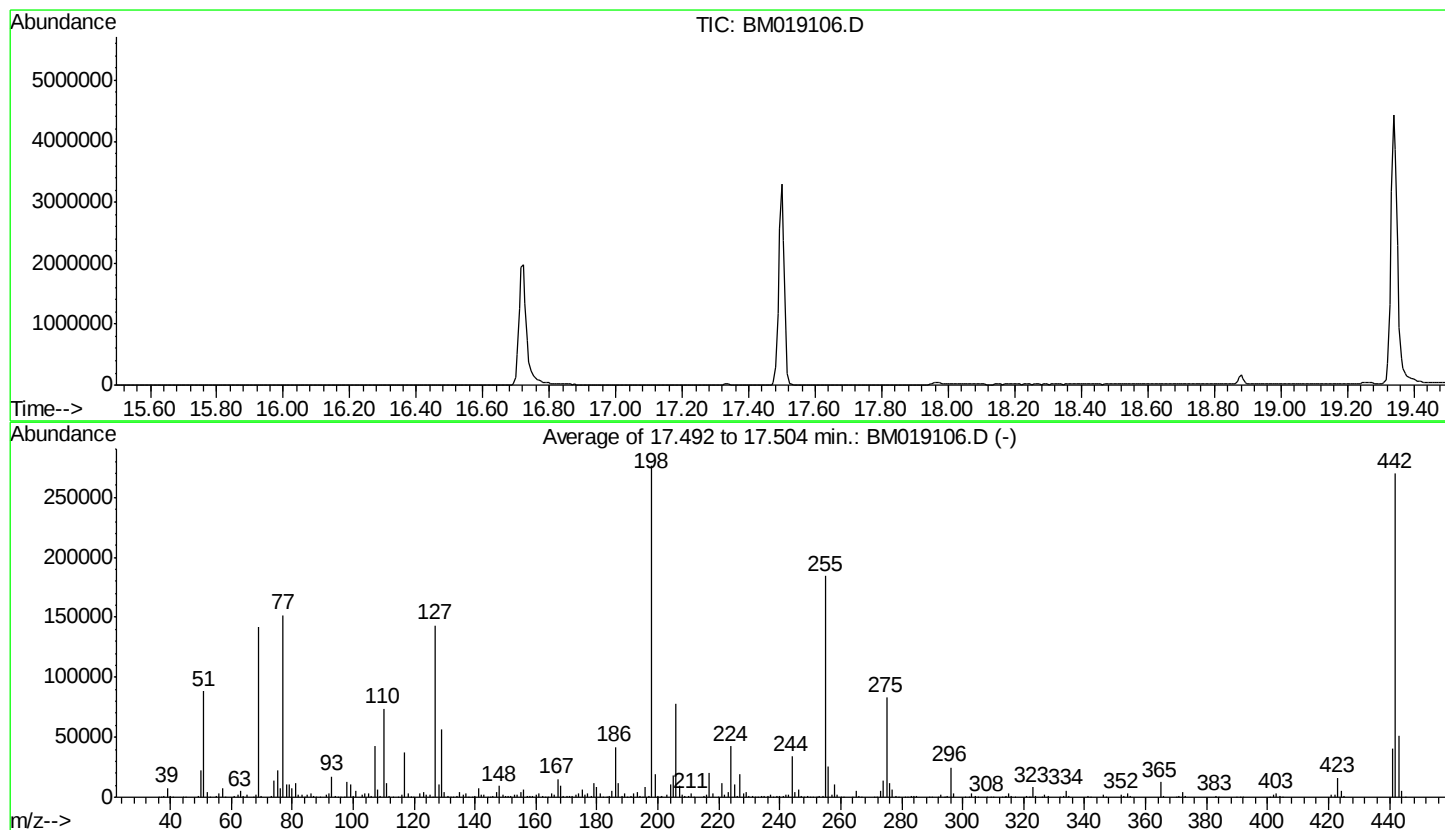

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	88408	PASS
68	69	0.00	2	1.8	2526	PASS
69	198	0.00	100	51.4	142085	PASS
70	69	0.00	2	0.5	753	PASS
127	198	10	80	51.7	143085	PASS
197	198	0.00	2	0.6	1602	PASS
198	198	100	100	100.0	276501	PASS
199	198	5	9	6.8	18811	PASS
275	198	10	60	30.0	82904	PASS
365	198	1	100	4.5	12538	PASS
441	198	0.01	100	14.8	40829	PASS
442	198	50	100	97.8	270485	PASS
443	442	15	24	19.1	51730	PASS