


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031219\
 Data File : BM019125.D
 Acq On : 13 Mar 2019 00:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

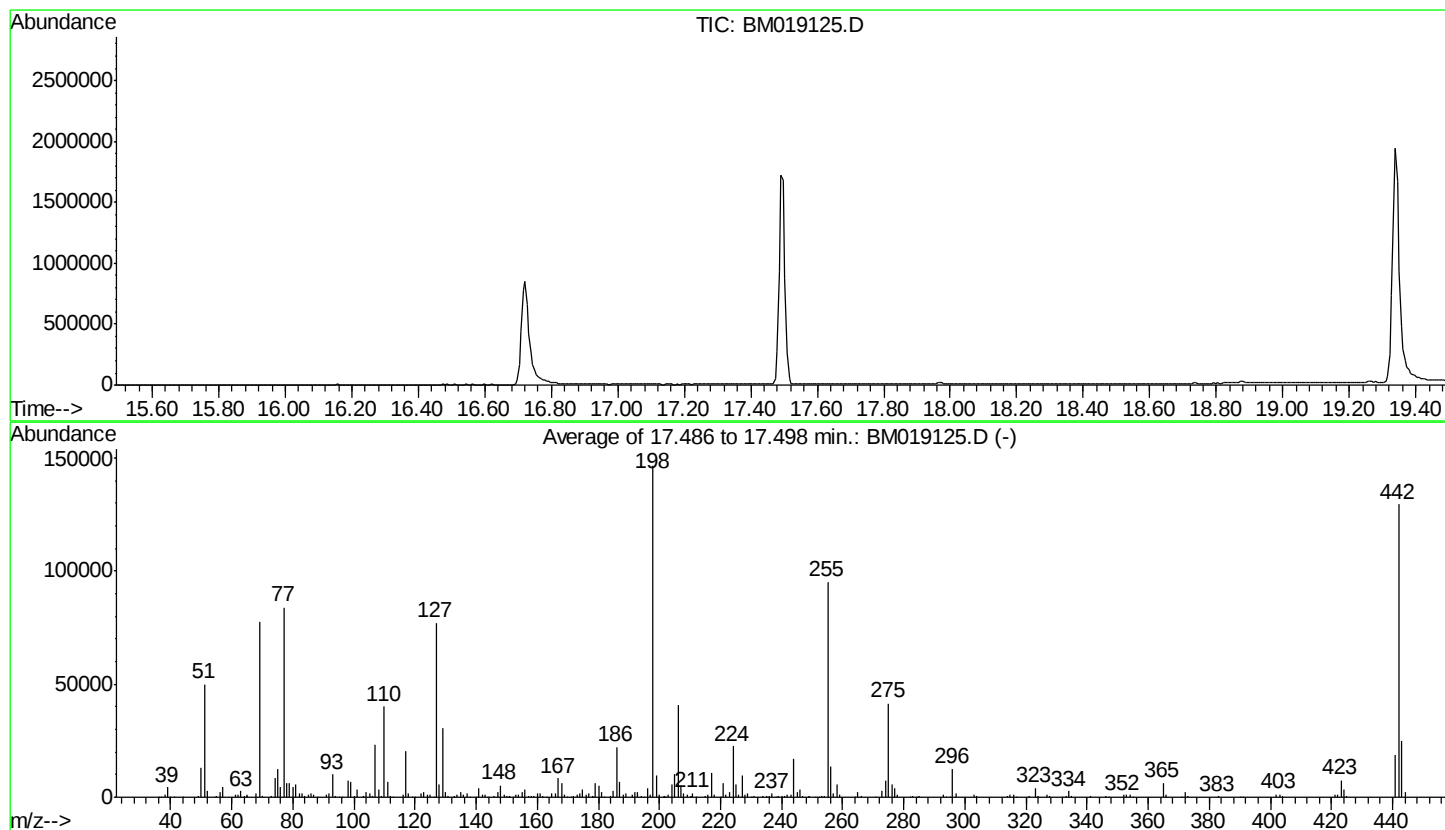

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	50013	PASS
68	69	0.00	2	2.0	1571	PASS
69	198	0.00	100	53.0	77709	PASS
70	69	0.00	2	0.5	370	PASS
127	198	10	80	52.6	77136	PASS
197	198	0.00	2	0.8	1146	PASS
198	198	100	100	100.0	146544	PASS
199	198	5	9	6.6	9710	PASS
275	198	10	60	28.3	41445	PASS
365	198	1	100	4.4	6441	PASS
441	198	0.01	100	12.9	18937	PASS
442	198	50	100	88.4	129538	PASS
443	442	15	24	19.4	25087	PASS