


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025527.D
Acq On : 12 Mar 2020 18:00
Operator : CG/JU
Sample : PB127292BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 13 05:10:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
3/16/2020 1:50:17 PM

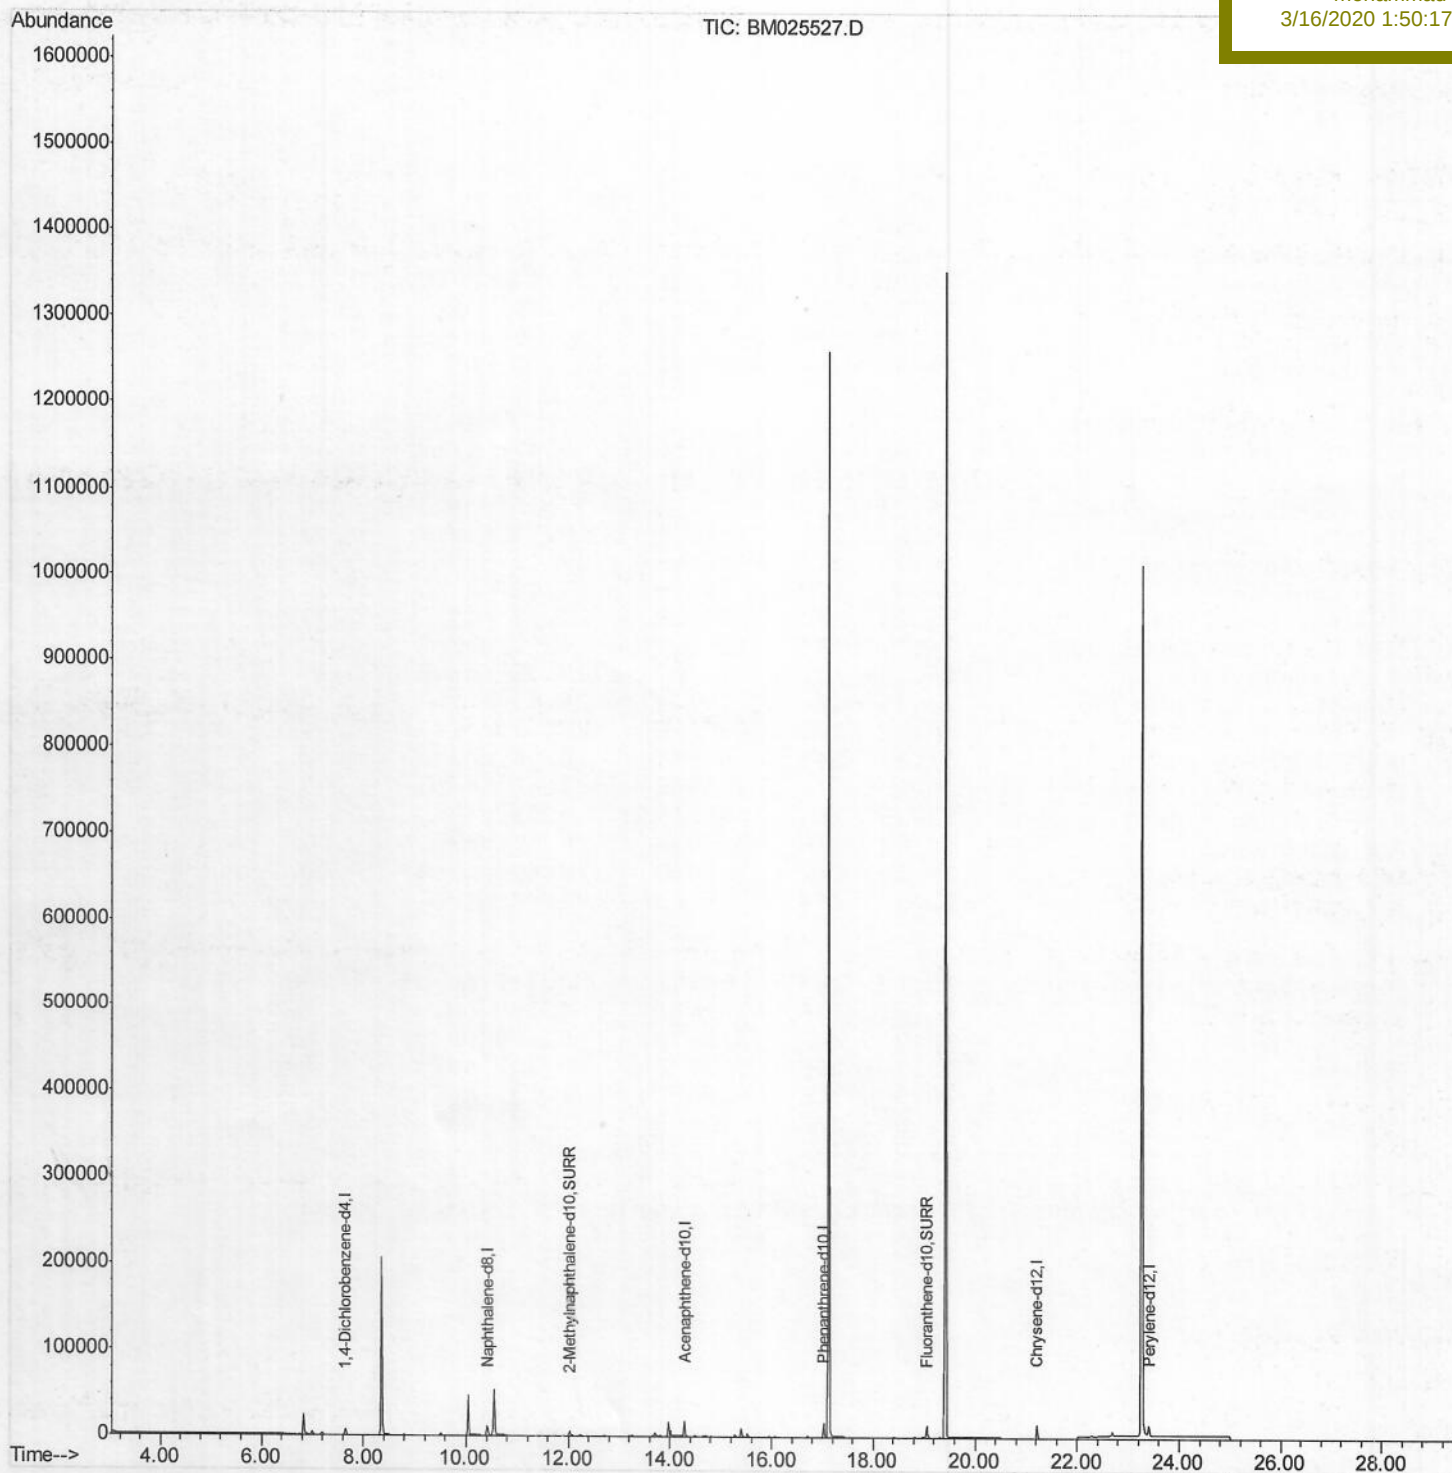


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025527.D
Acq On : 12 Mar 2020 18:00
Operator : CG/JU
Sample : PB127292BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 13 05:09:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
3/16/2020 1:50:17 PM

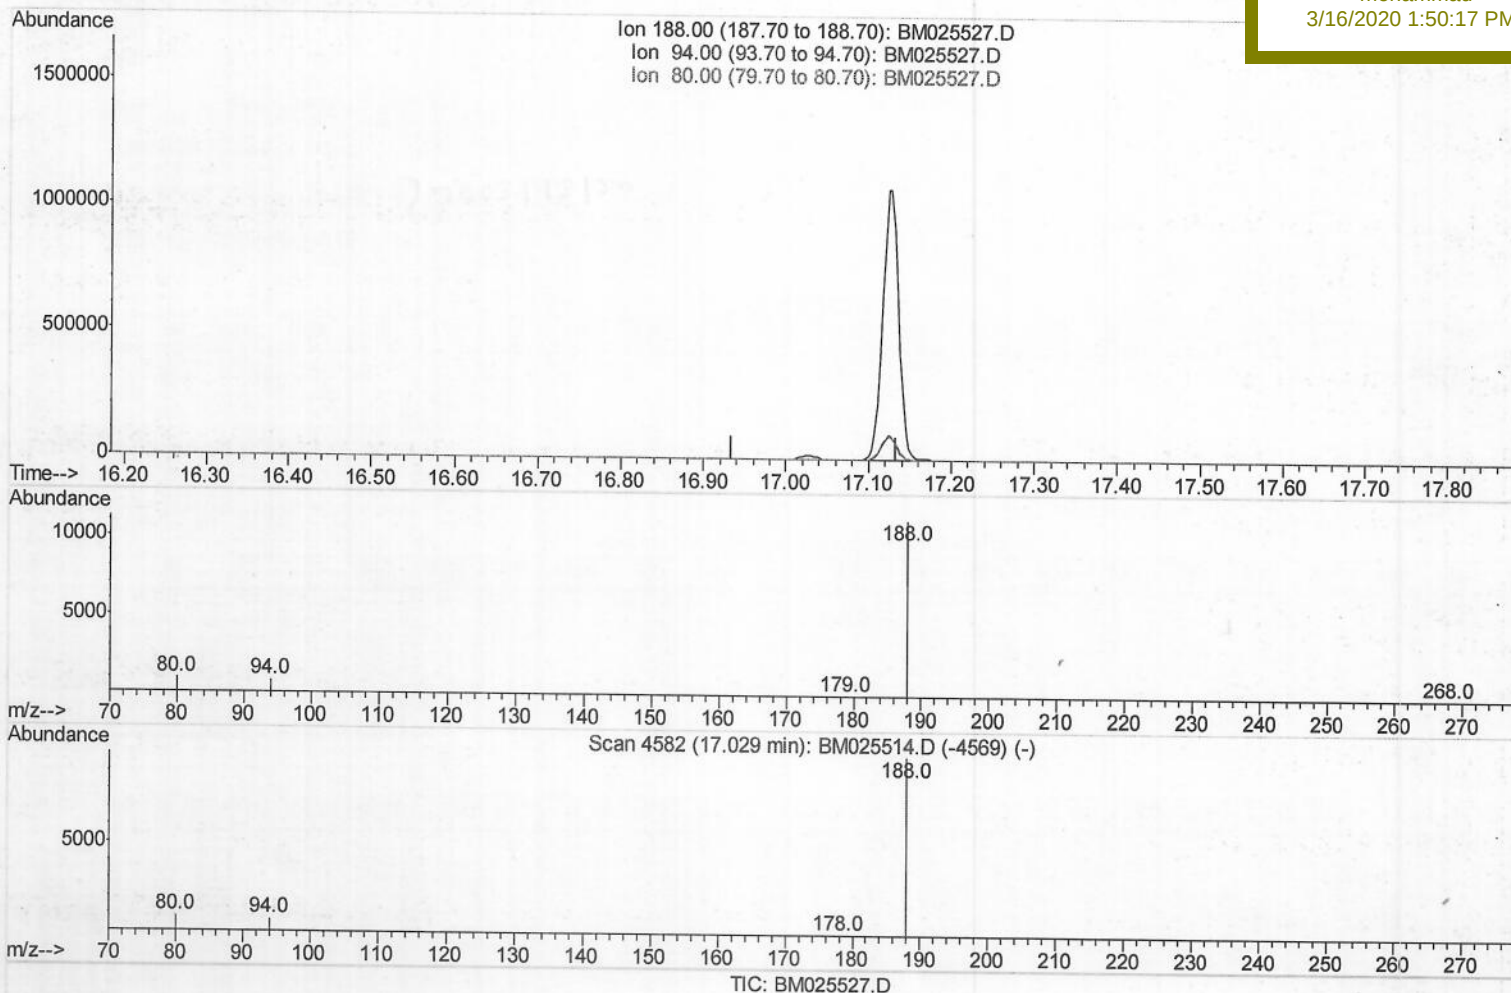

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\

Data File : BM025527.D

Acq On : 12 Mar 2020 18:00

Operator : CG/JU

Sample : PB127292BL

Misc :

ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 13 05:09:47 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


SBLK92

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:17 PM

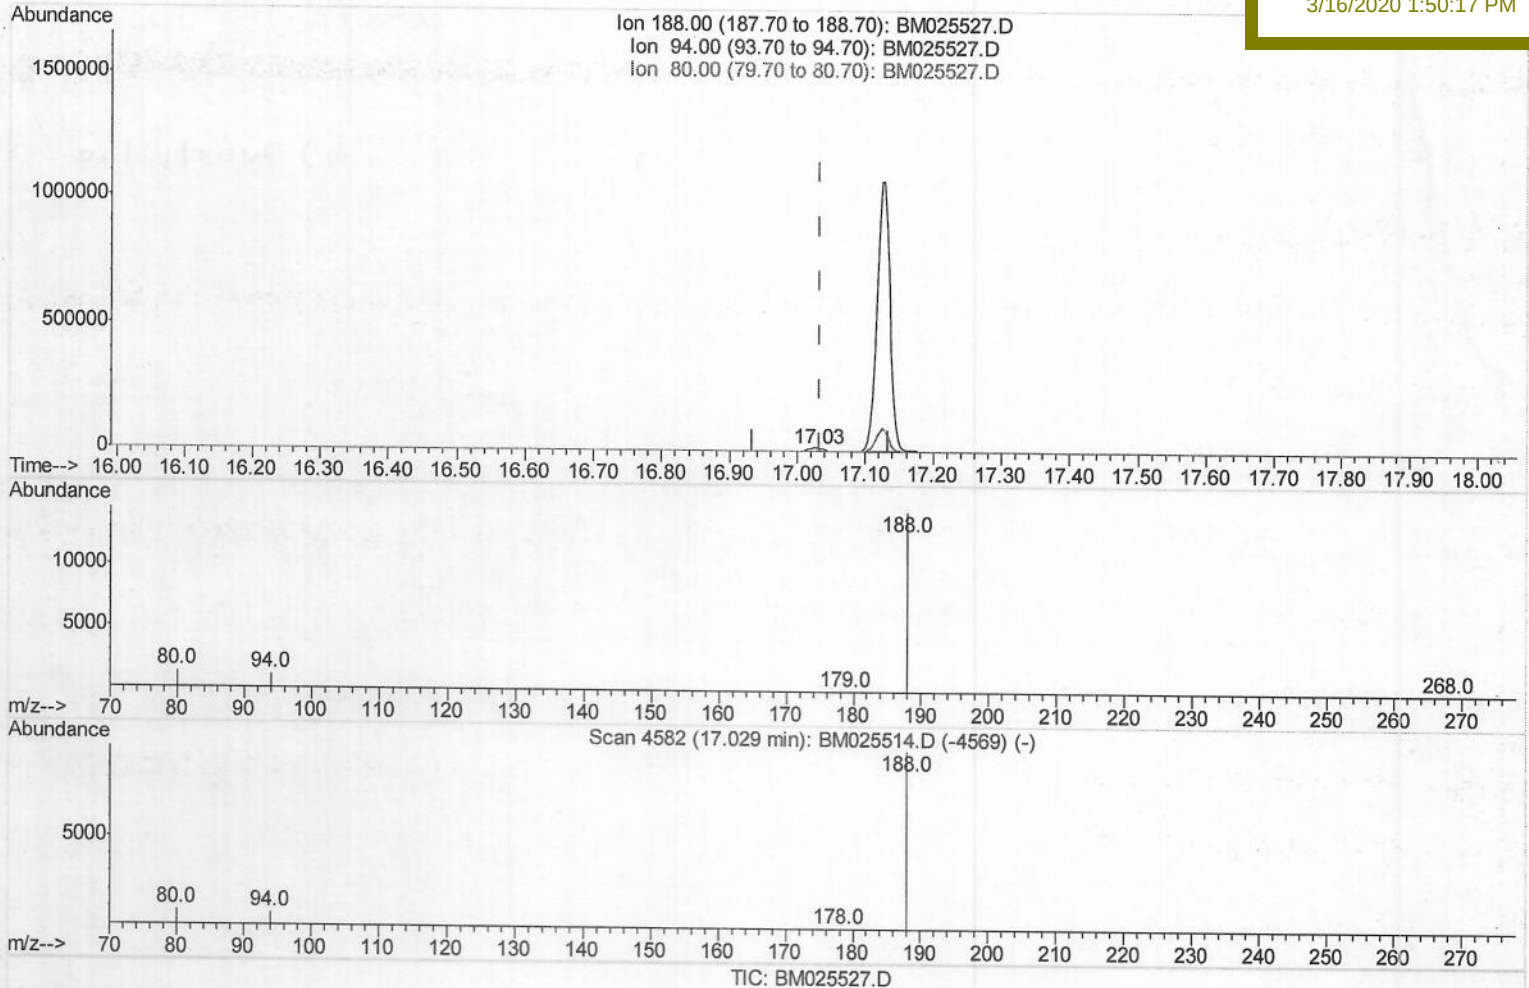

(10) Phenanthrene-d10 (I)

17.027min (-0.007) 0.40ng/ul m>50 03/16/20

response 20179

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.89
80.00	8.70	9.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
 Data File : BM025527.D
 Acq On : 12 Mar 2020 18:00
 Operator : CG/JU
 Sample : PB127292BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 13 05:10:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK92

Manual Integrations
 APPROVED

mohammad
 3/16/2020 1:50:17 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3364	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	9998	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	20179m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	13673	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	15082	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	7135	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	14852	0.27	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 03/16/20