

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025528.D
Acq On : 12 Mar 2020 18:37
Operator : CG/JU
Sample : PB127294BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 13 05:12:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :


SBLK94

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:20 PM

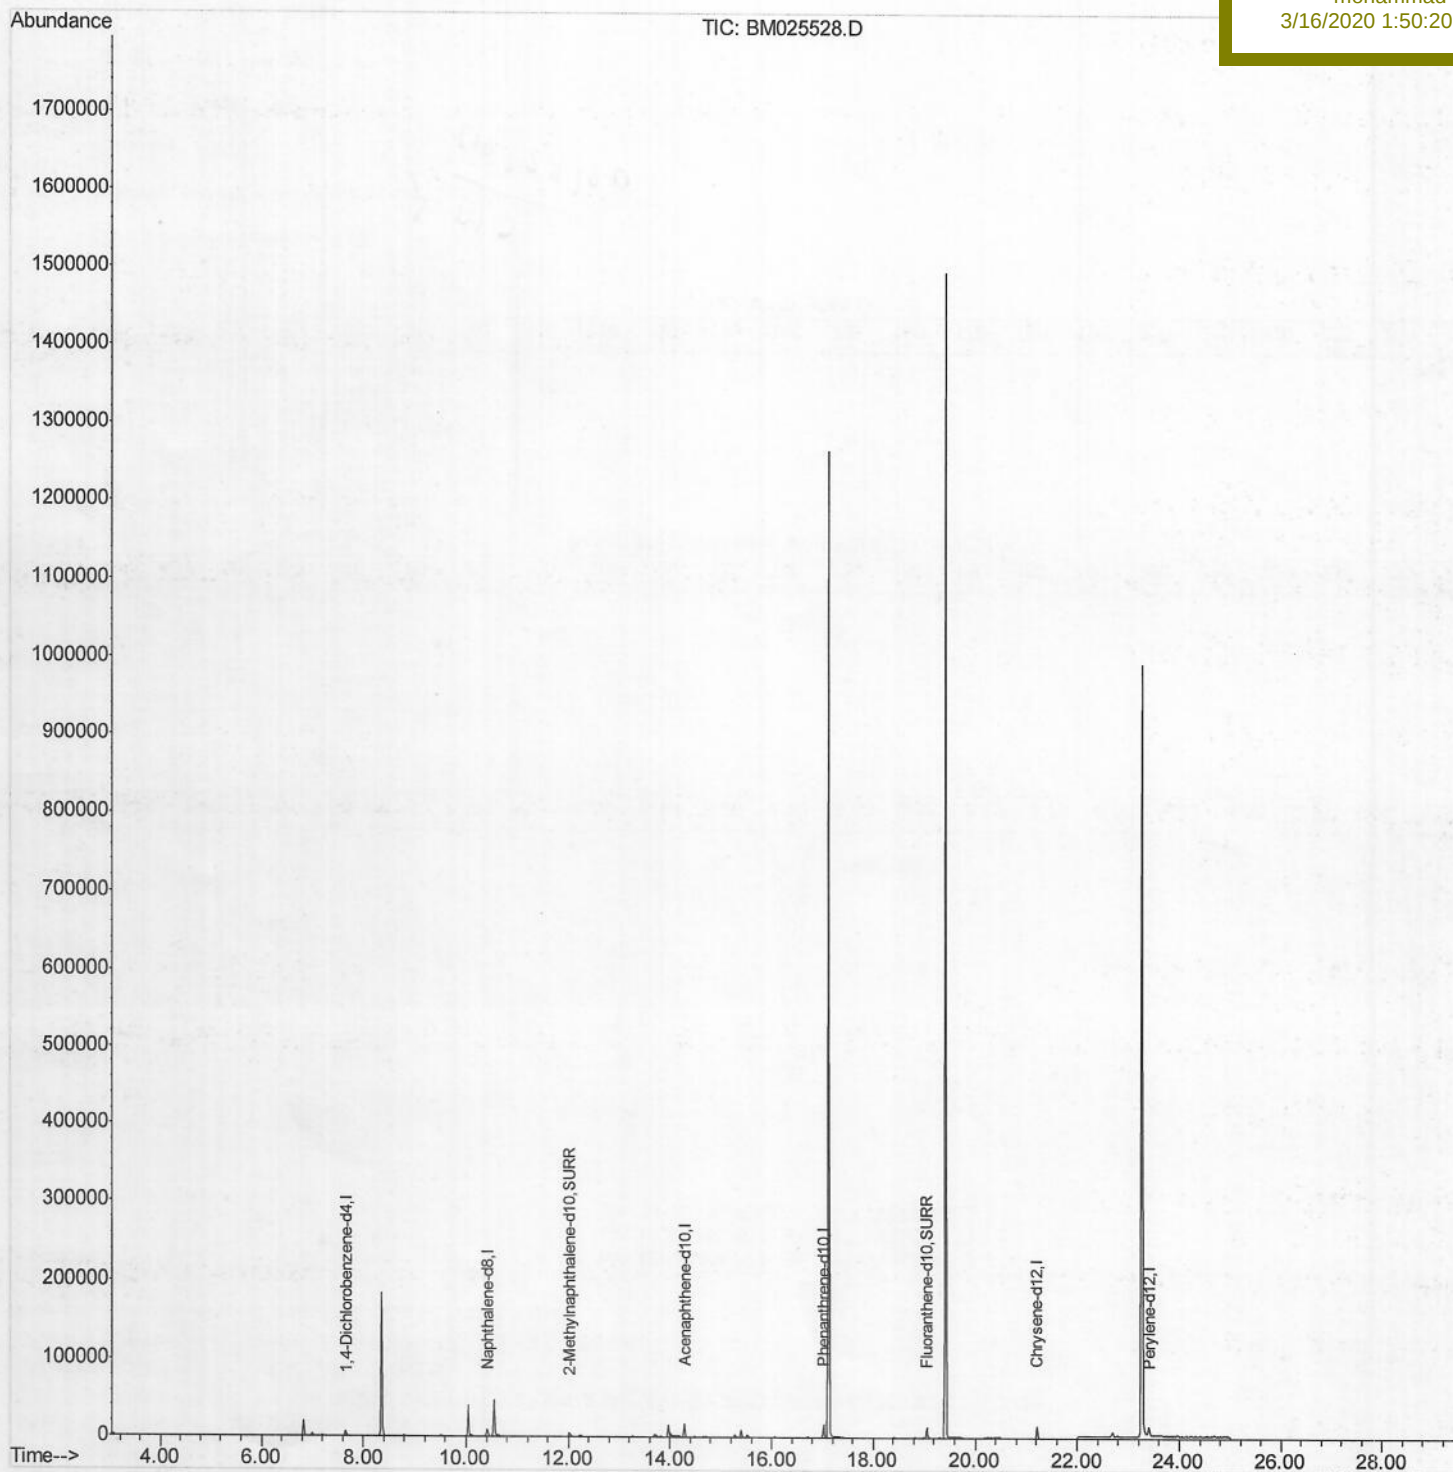

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025528.D
Acq On : 12 Mar 2020 18:37
Operator : CG/JU
Sample : PB127294BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 13 05:11:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK94

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:20 PM

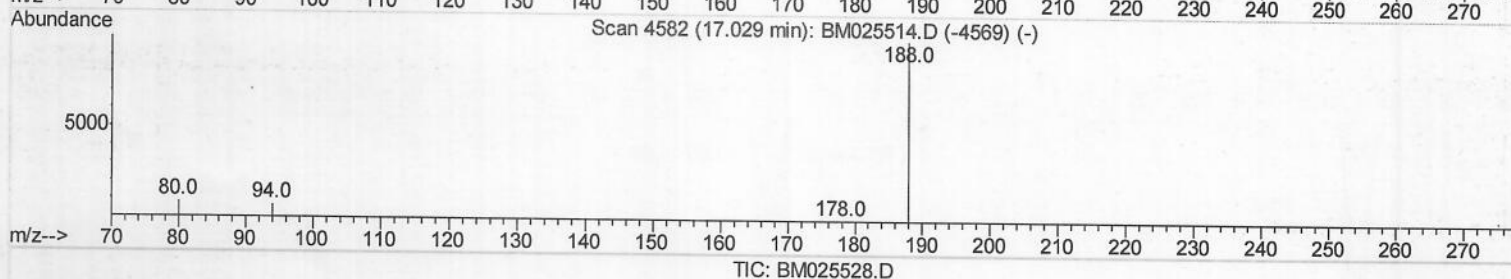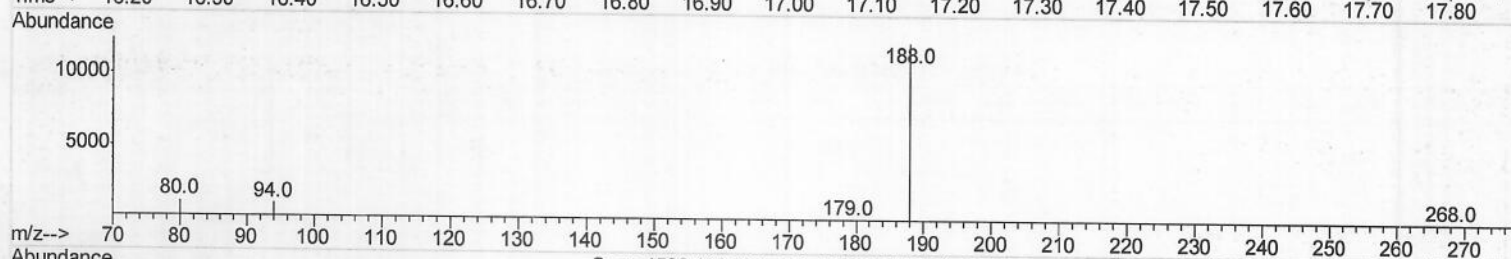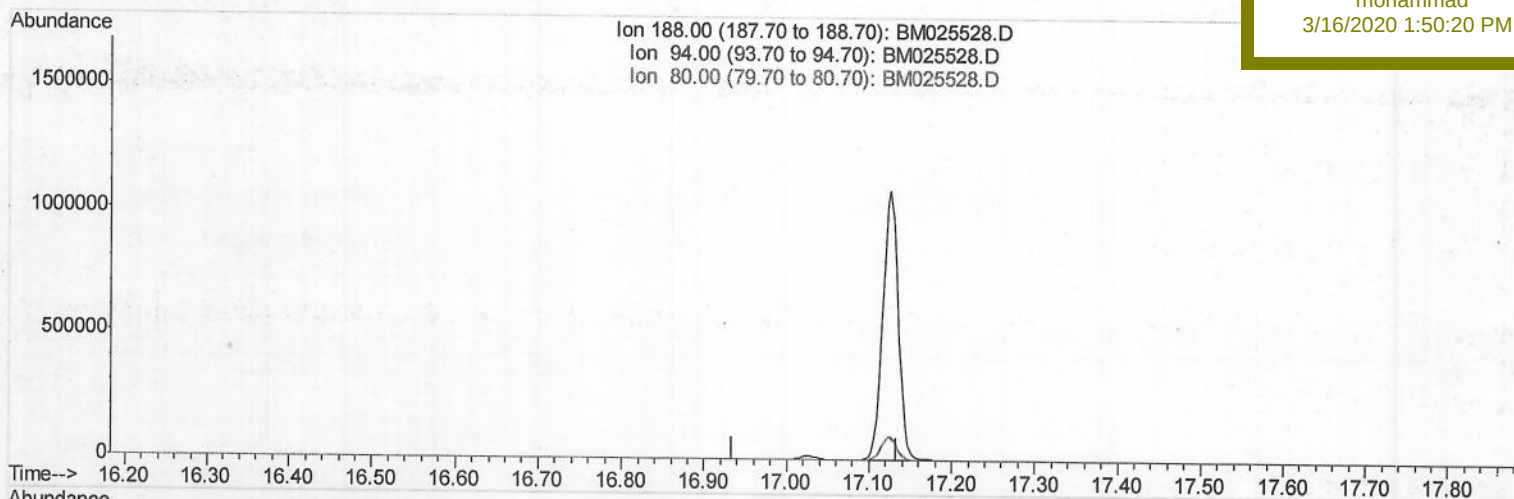

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\

Data File : BM025528.D

Acq On : 12 Mar 2020 18:37

Operator : CG/JU

Sample : PB127294BL

Misc :

ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 13 05:11:39 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

Client Sample ID :




SBLK94

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:20 PM

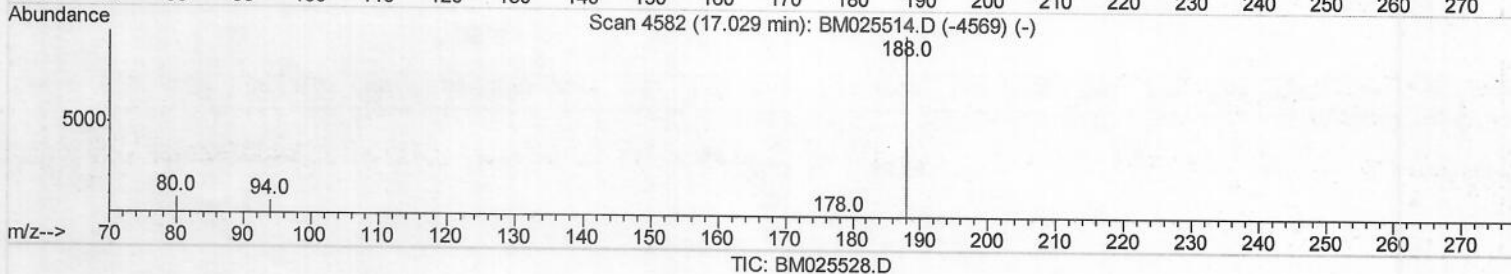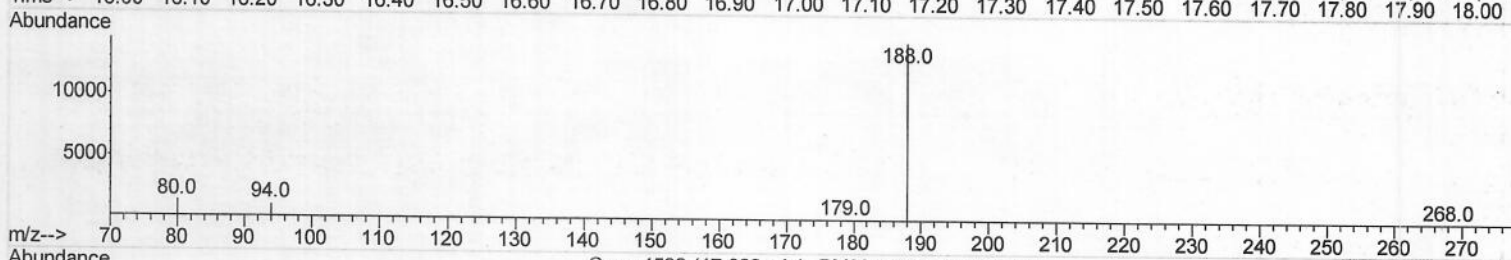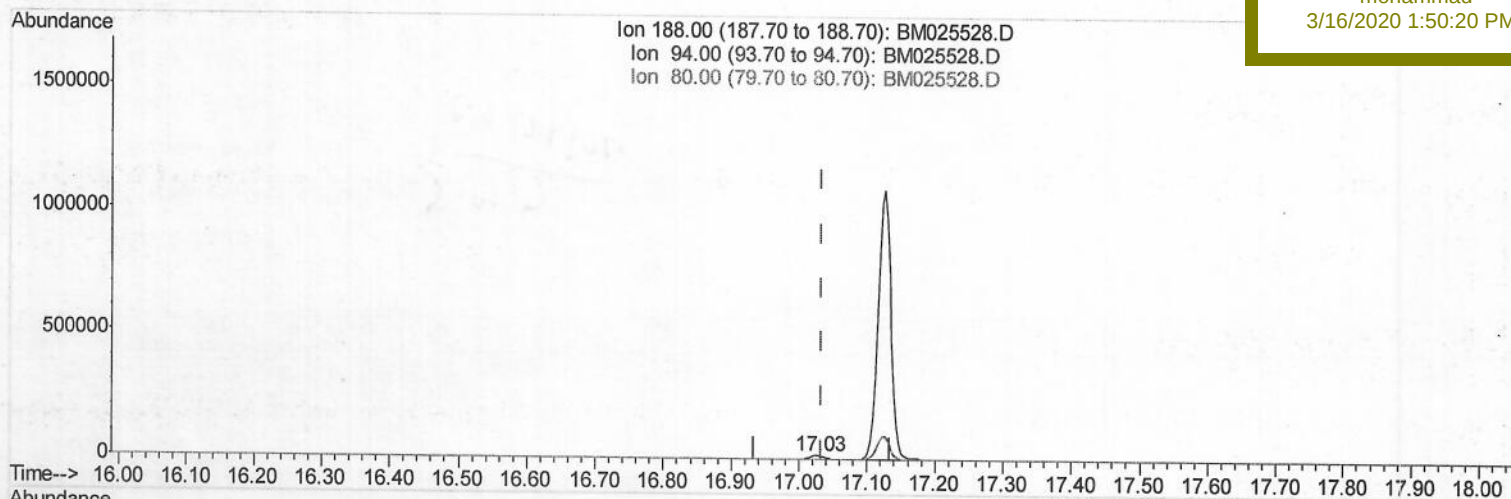

(10) Phenanthrene-d10 (I)

17.029min (-0.005) 0.40ng/ul m>ju 03/16/20

response 19861

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.43
80.00	8.70	8.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025528.D
Acq On : 12 Mar 2020 18:37
Operator : CG/JU
Sample : PB127294BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Mar 13 05:12:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

mohammad
3/16/2020 1:50:20 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	2945	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	12328	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	8892	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	19861m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	14792	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	14579	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	6183	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	16017	0.29	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 03/16/20