


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025534.D
Acq On : 12 Mar 2020 22:13
Operator : CG/JU
Sample : L1782-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 13 05:23:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

mohammad
3/16/2020 1:50:41 PM

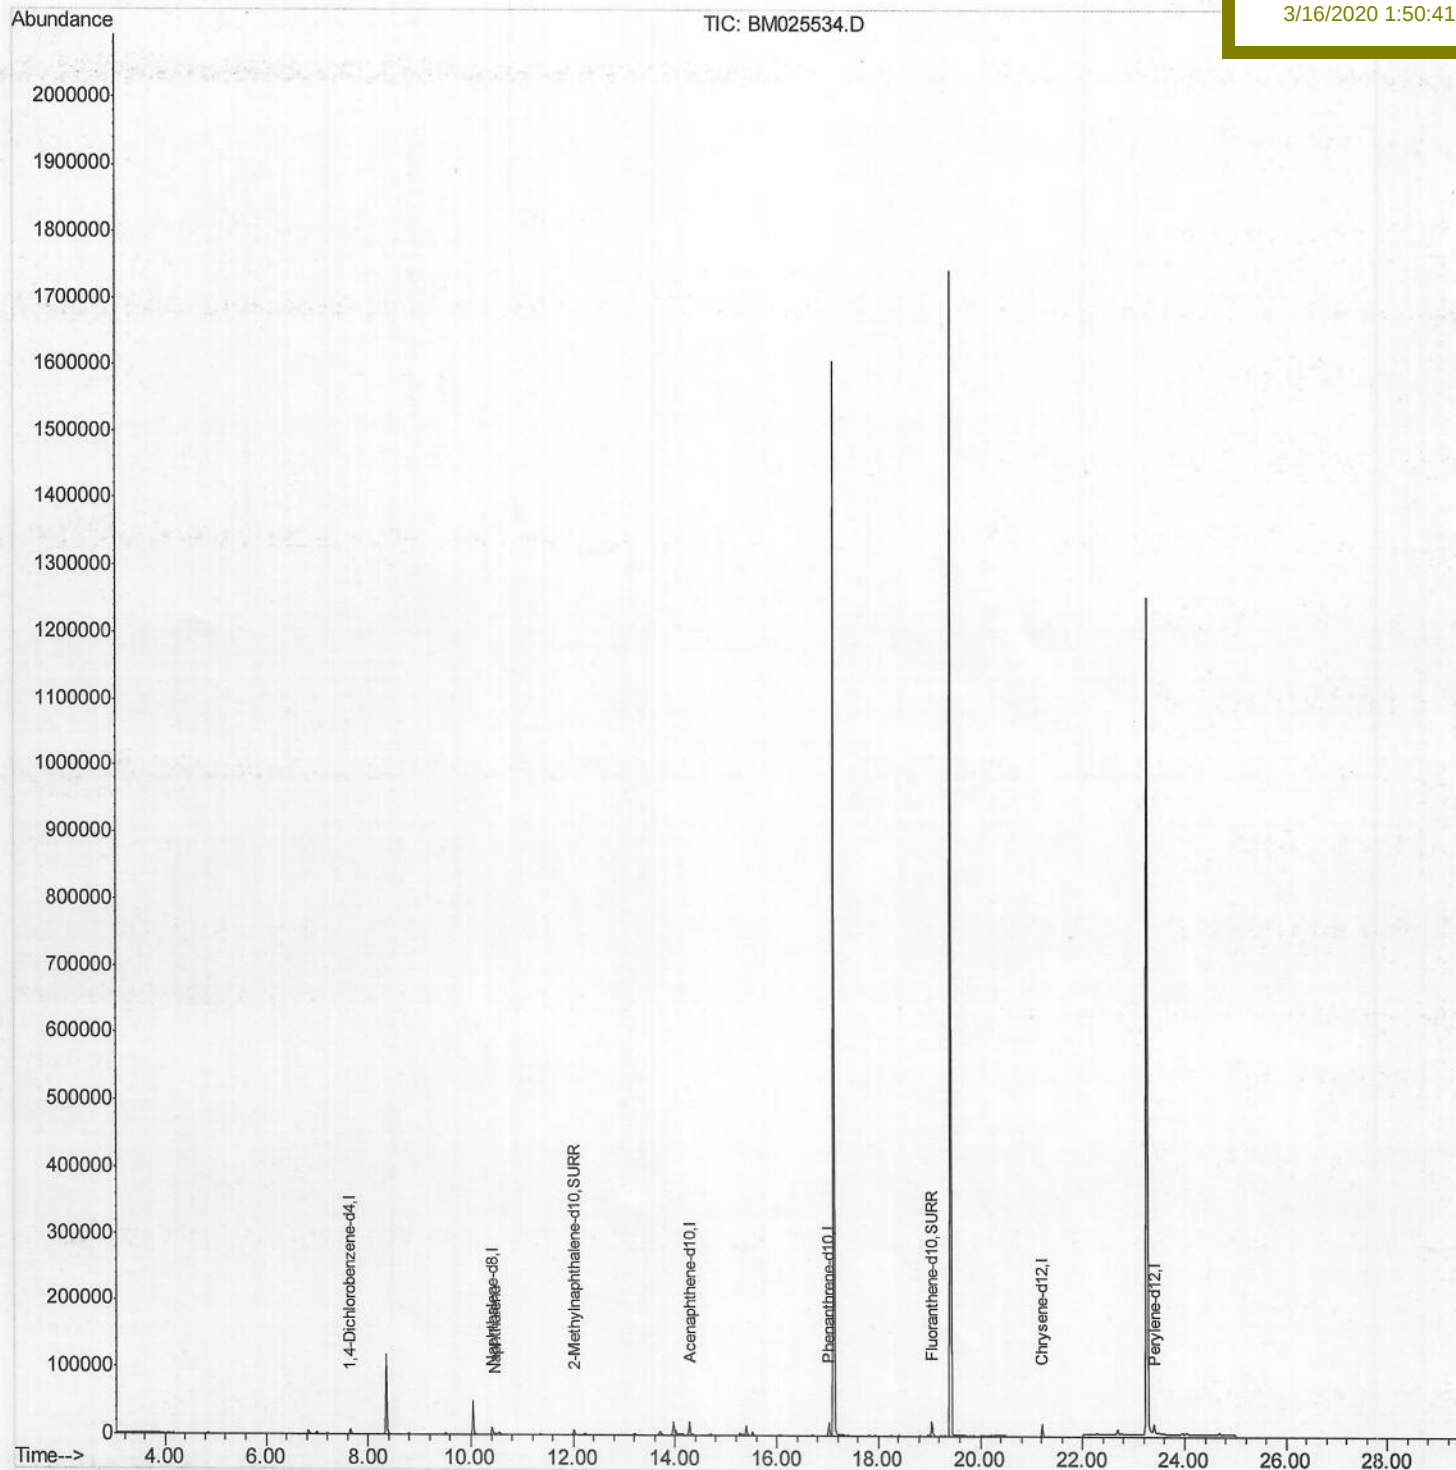

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\

Data File : BM025534.D

Acq On : 12 Mar 2020 22:13

Operator : CG/JU

Sample : L1782-06

Misc :

ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 13 05:22:52 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


C0AB0

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:41 PM

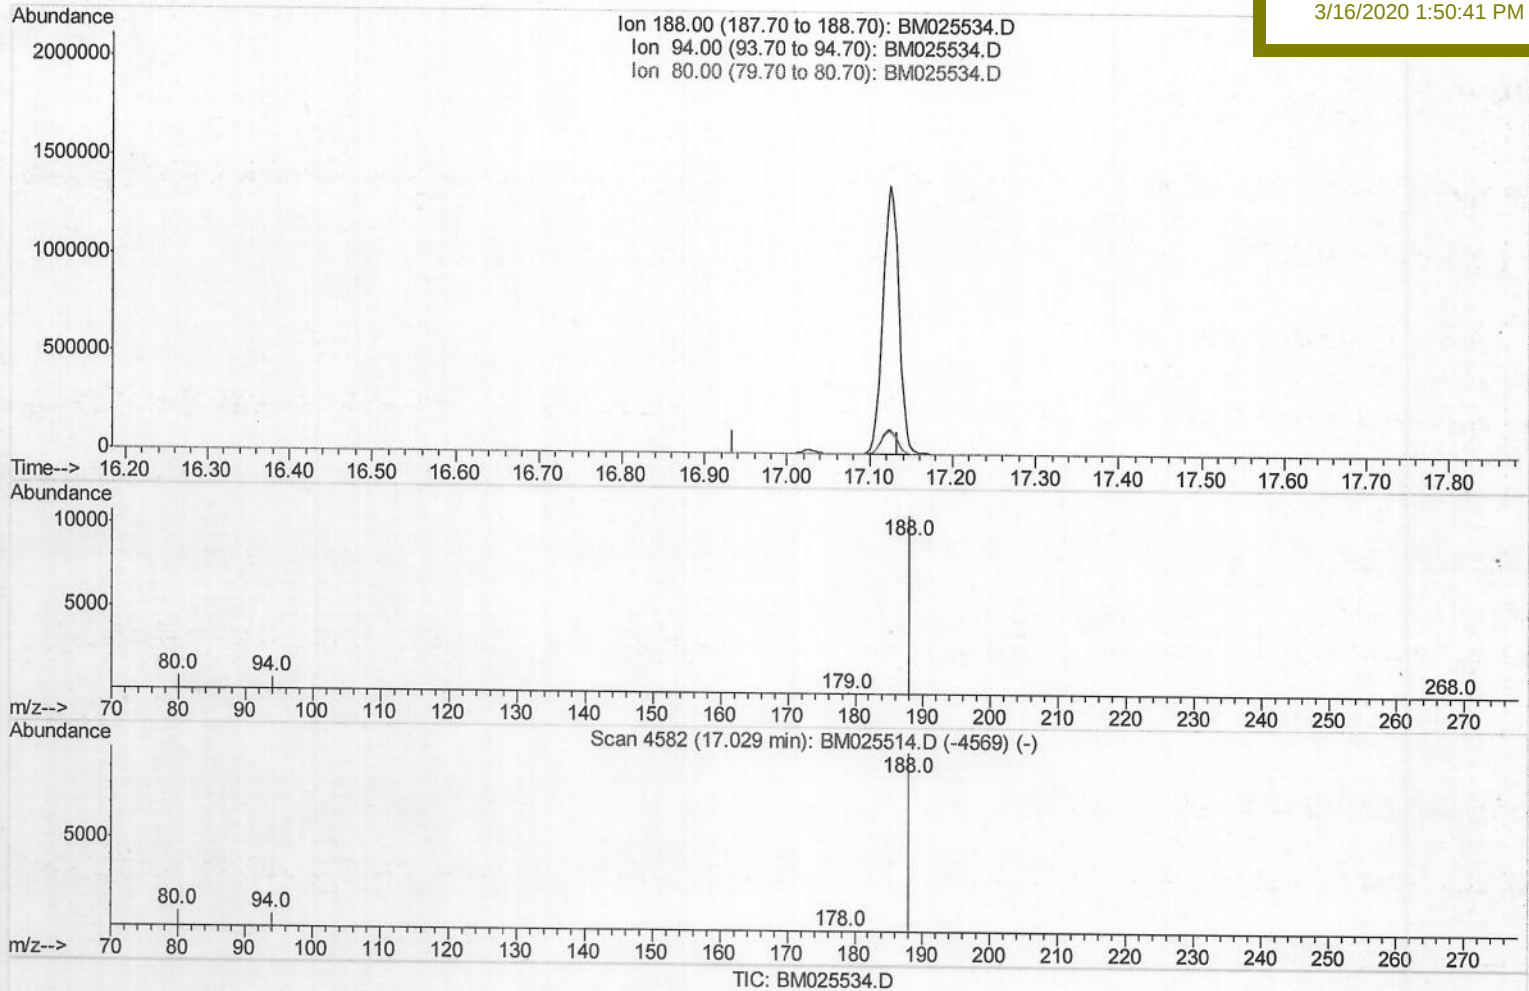

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
 Data File : BM025534.D
 Acq On : 12 Mar 2020 22:13
 Operator : CG/JU
 Sample : L1782-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 13 05:22:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 C0AB0

Manual Integrations
APPROVED

mohammad
 3/16/2020 1:50:41 PM

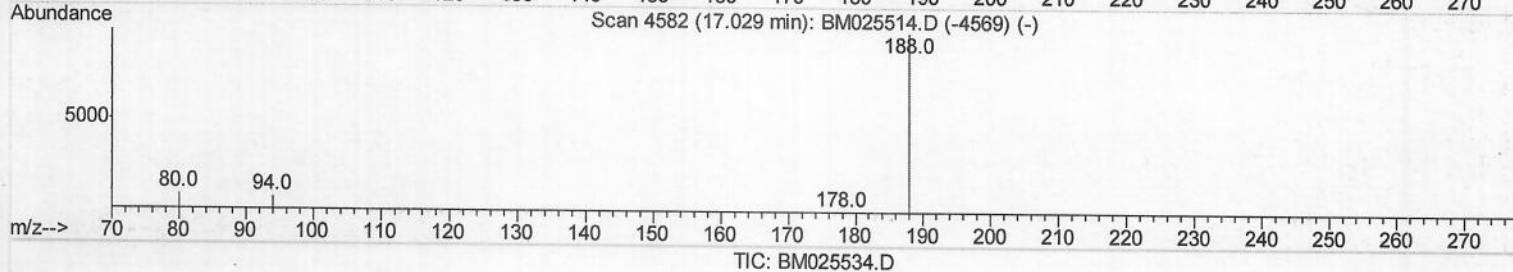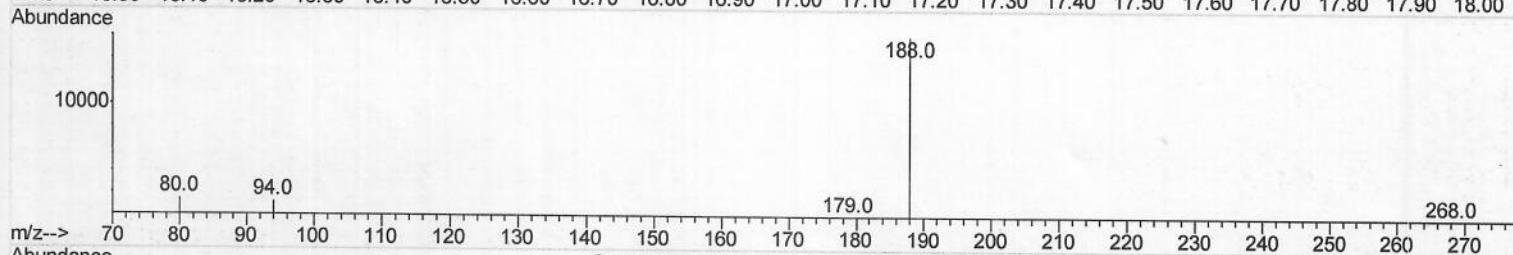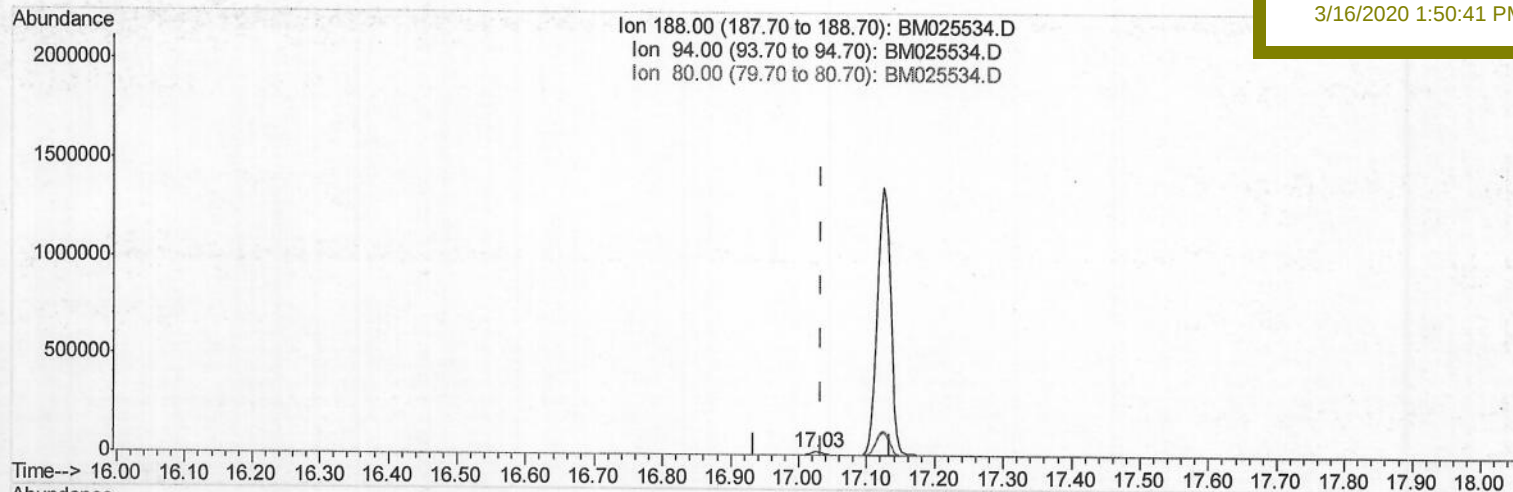

TIC: BM025534.D

(10) Phenanthrene-d10 (I)

17.027min (-0.007) 0.40ng/ul m>ju 03/16/20

response 21750

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.19
80.00	8.70	9.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
 Data File : BM025534.D
 Acq On : 12 Mar 2020 22:13
 Operator : CG/JU
 Sample : L1782-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB0

Quant Time: Mar 13 05:23:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/16/2020 1:50:41 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3349	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14515	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	10473	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	21750m	0.40	ng/ul	0.00
16) Chrysene-d12	21.21	240	15511	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	16778	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9734	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	24211	0.40	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.47	128	1192	0.028	ng/ul#	Ovalue 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed