


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
Data File : BM025538.D
Acq On : 13 Mar 2020 00:38
Operator : CG/JU
Sample : L1782-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Mar 13 05:32:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C0AB1

Manual Integrations
APPROVED

mohammad
3/16/2020 1:50:54 PM

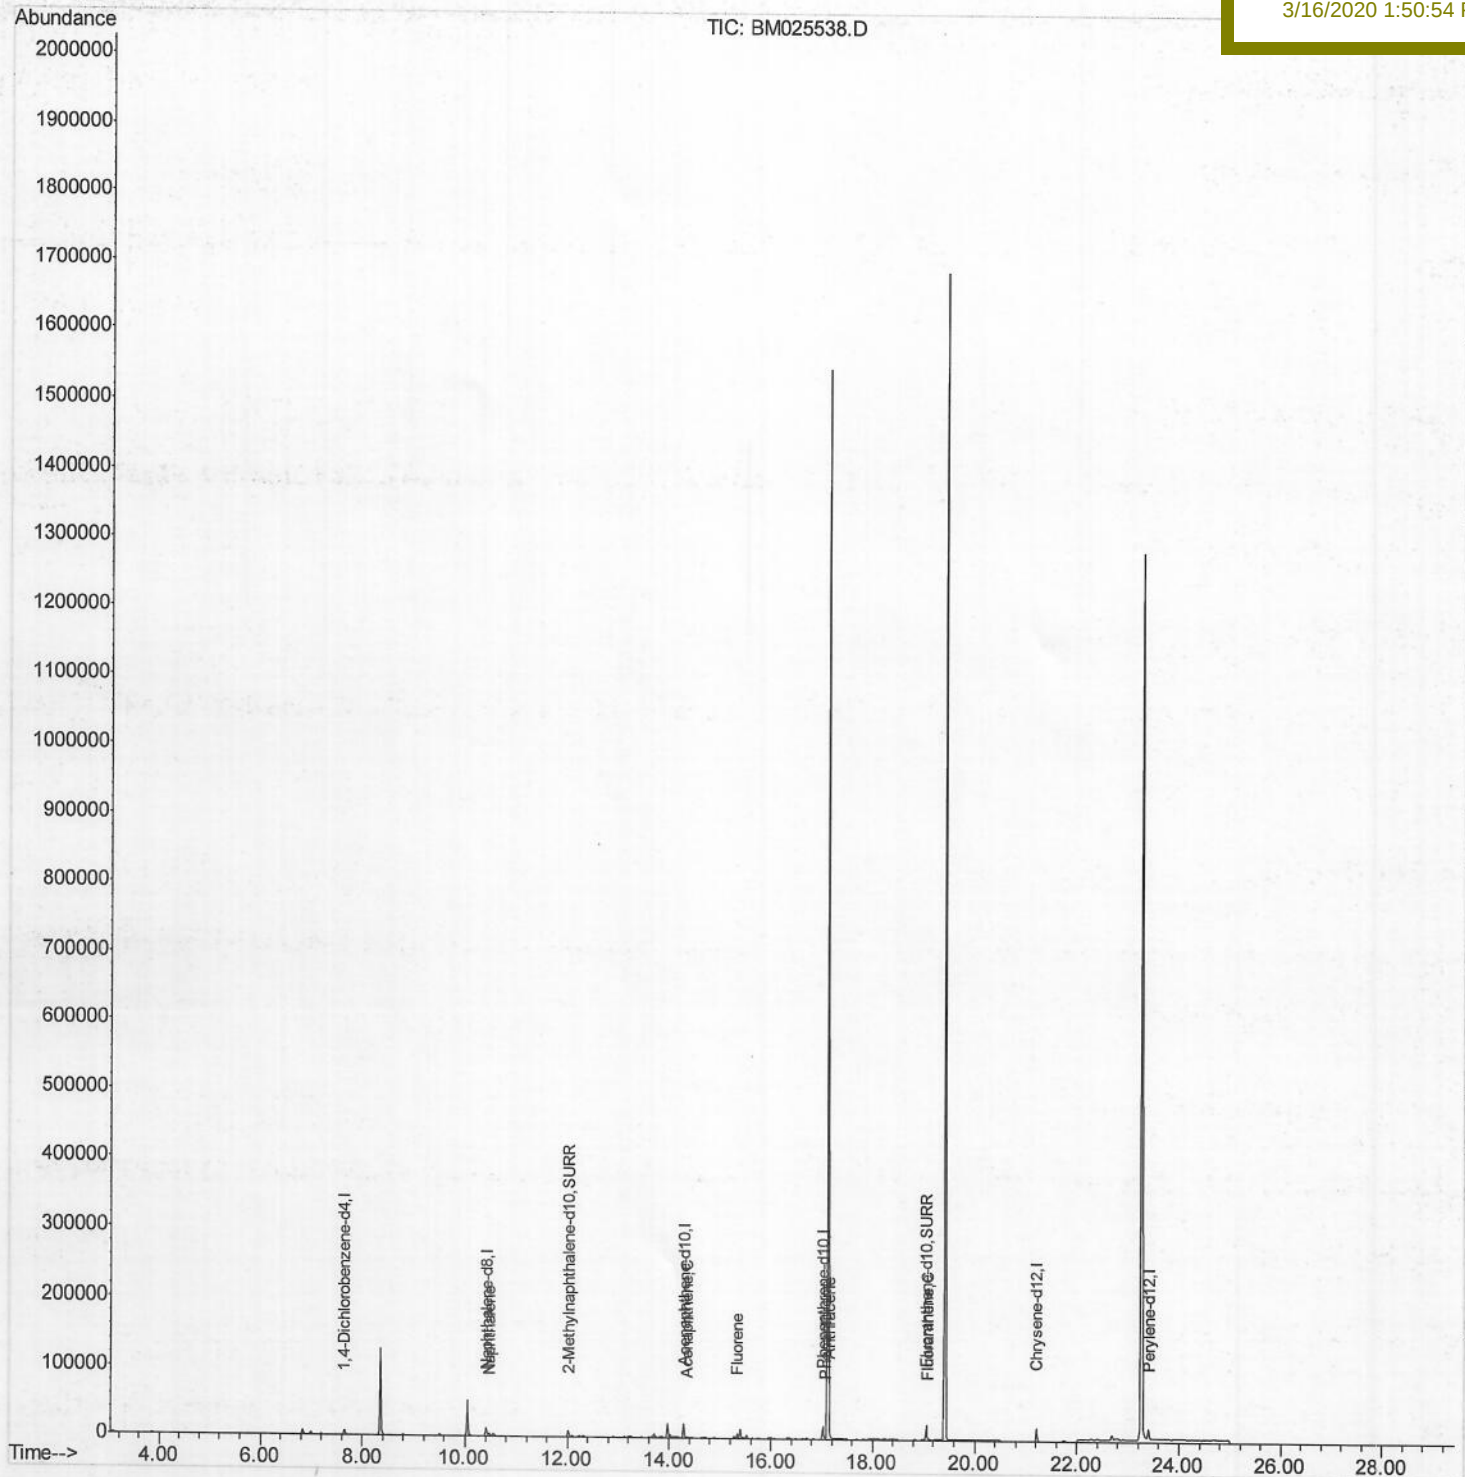

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\

Data File : BM025538.D

Acq On : 13 Mar 2020 00:38

Operator : CG/JU

Sample : L1782-07

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Mar 13 05:31:23 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0AB1

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:54 PM

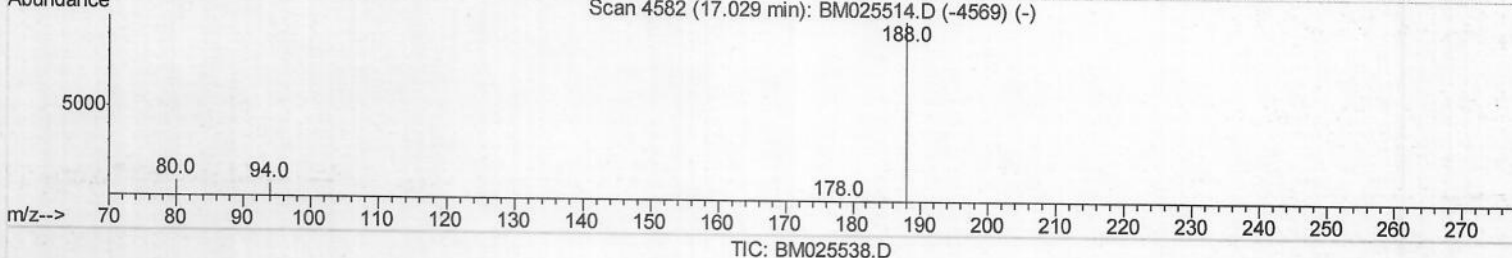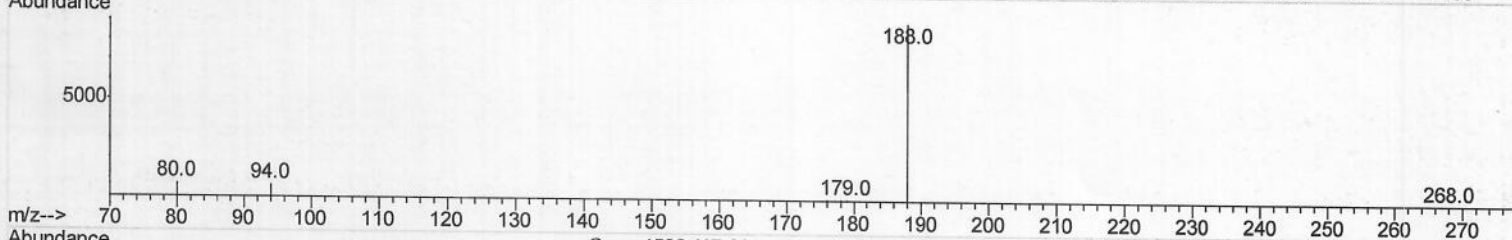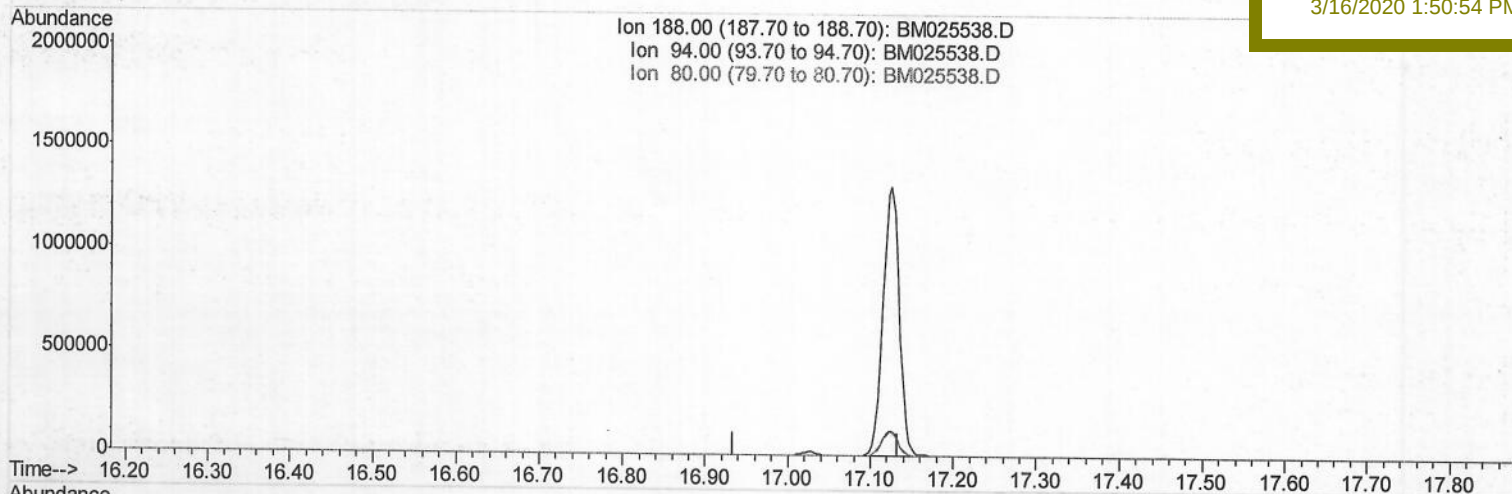

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\

Data File : BM025538.D

Acq On : 13 Mar 2020 00:38

Operator : CG/JU

Sample : L1782-07

Misc :

ALS Vial : 25 Sample Multiplier: 1

Quant Time: Mar 13 05:31:23 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




C0AB1

Manual Integrations

APPROVED

mohammad

3/16/2020 1:50:54 PM

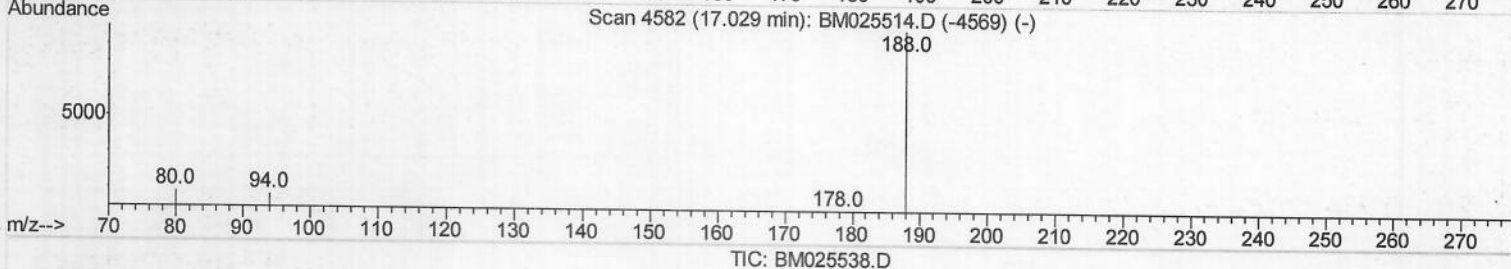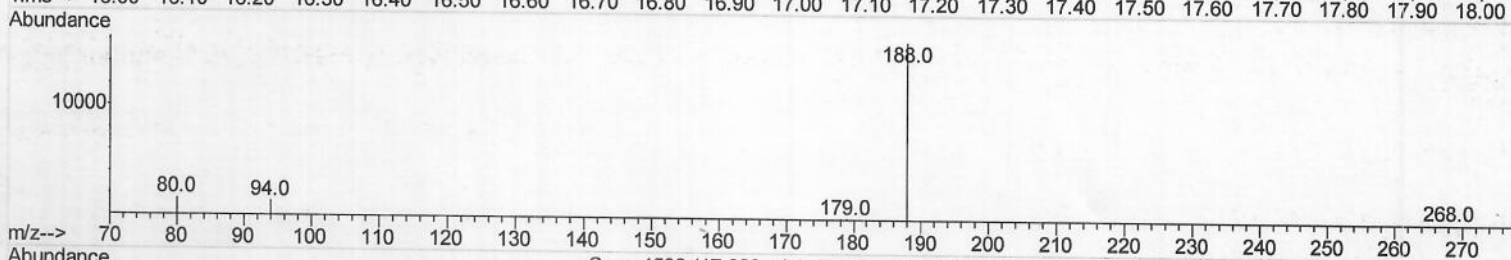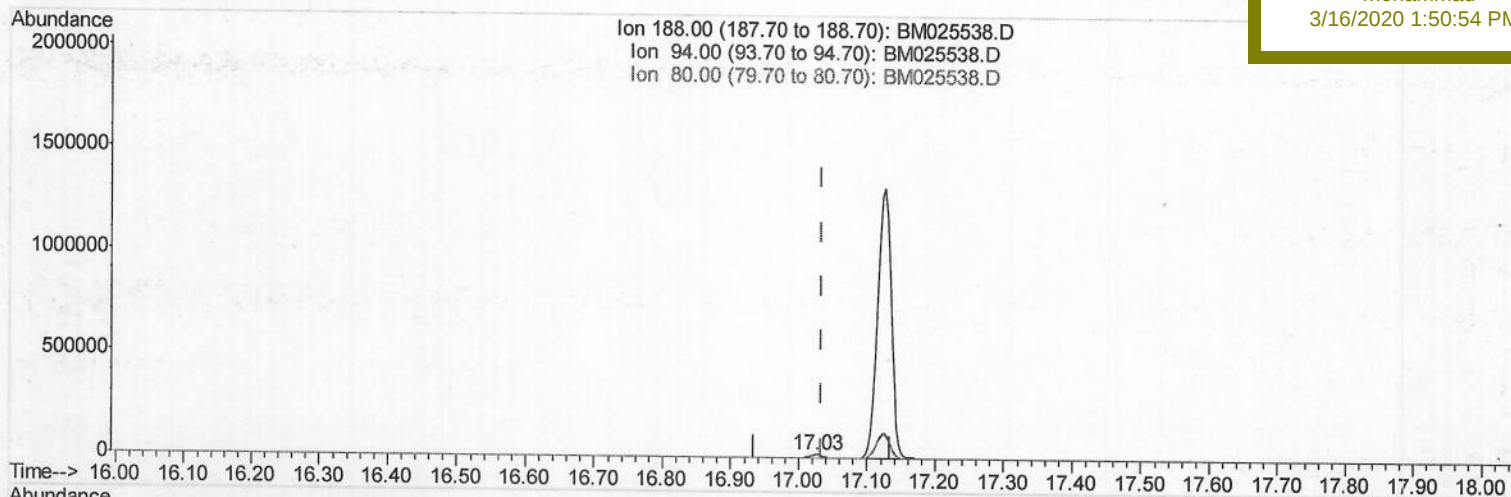

(10) Phenanthrene-d10 (I)

17.025min (-0.009) 0.40ng/ul m > 50 03/16/20

response 22028

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.44
80.00	8.70	9.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031220\
 Data File : BM025538.D
 Acq On : 13 Mar 2020 00:38
 Operator : CG/JU
 Sample : L1782-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB1

Quant Time: Mar 13 05:32:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/16/2020 1:50:54 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3488	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	14960	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	10698	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	22028m	0.40	ng/ul	0.00
16) Chrysene-d12	21.21	240	16575	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	17722	0.40	ng/ul	-0.01

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	10115	0.38	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	24237	0.40	ng/ul	0.00

Target Compounds				Ovalue		
3) Naphthalene	10.47	128	4700	0.106	ng/ul	98
8) Acenaphthene	14.34	153	864	0.023	ng/ul	94
9) Fluorene	15.33	166	4062	0.087	ng/ul	99
12) Phenanthrene	17.07	178	2736	0.039	ng/ul#	89
13) Anthracene	17.16	178	1977	0.033	ng/ul#	87
15) Fluoranthene	19.08	202	2532	0.033	ng/ul	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed