

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
 Data File : BM029107.D
 Acq On : 12 Mar 2021 12:28
 Operator : CG/JU
 Sample : PB135107BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135107BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.199	371	376	393	rBB	213987	296503	61.67%	12.513%
2	6.822	646	652	671	rBB	193648	296890	61.75%	12.529%
3	7.622	783	788	795	rBB	35453	51143	10.64%	2.158%
4	8.798	982	988	1000	rBV	120056	189029	39.32%	7.977%
5	10.410	1256	1262	1271	rBB	43376	67521	14.04%	2.849%
6	12.904	1680	1686	1694	rBB	276320	383461	79.75%	16.183%
7	14.292	1917	1922	1928	rBB	58024	79546	16.54%	3.357%
8	15.798	2172	2178	2185	rBB	190528	260550	54.19%	10.996%
9	17.045	2385	2390	2396	rBB	64476	84070	17.49%	3.548%
10	19.674	2832	2837	2842	rVB	424366	480800	100.00%	20.291%
11	21.221	3096	3100	3106	rBV	76436	88520	18.41%	3.736%
12	23.362	3459	3464	3470	rVB2	53770	91541	19.04%	3.863%




Sum of corrected areas: 2369574

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029107.D
Acq On : 12 Mar 2021 12:28
Operator : CG/JU
Sample : PB135107BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135107BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

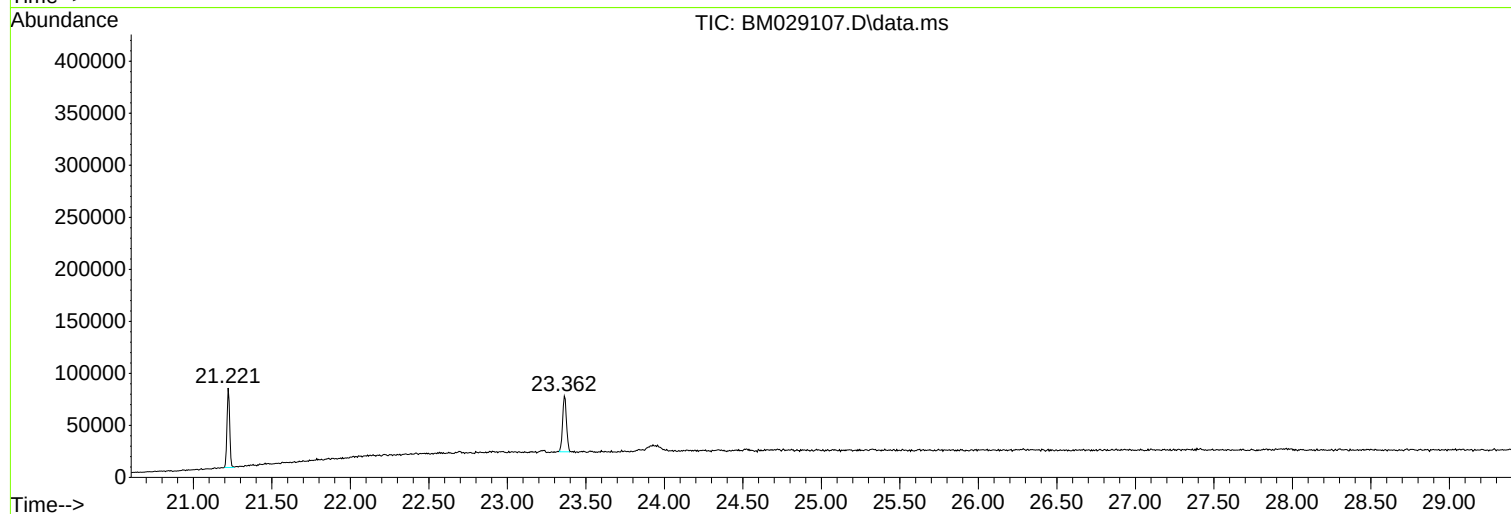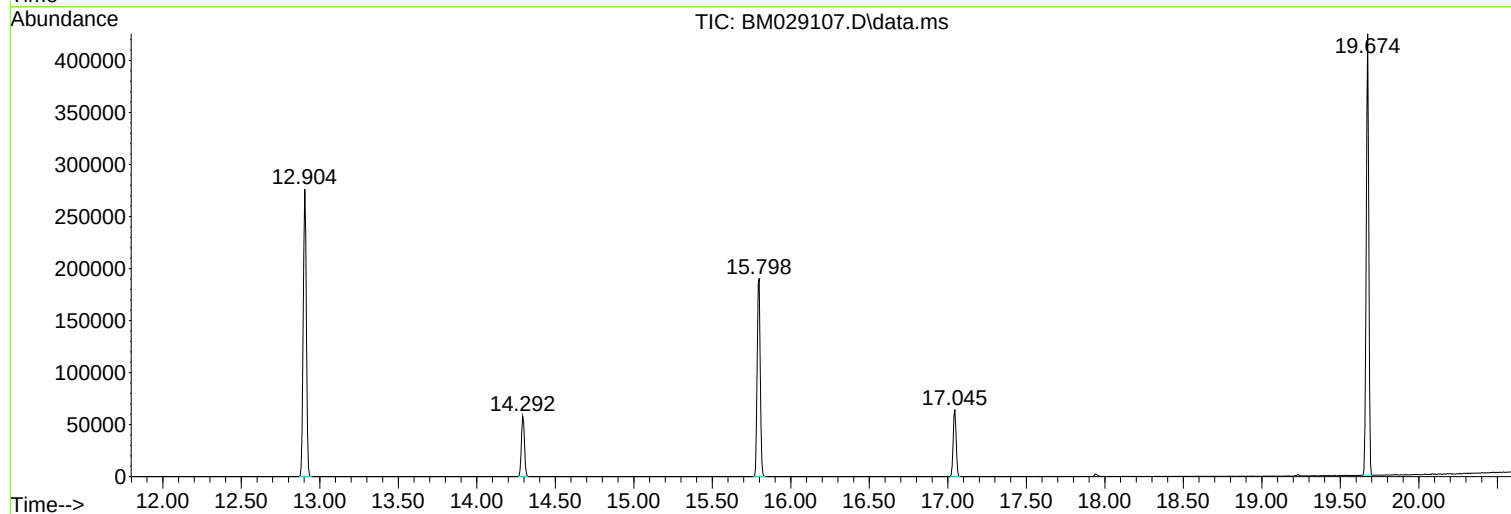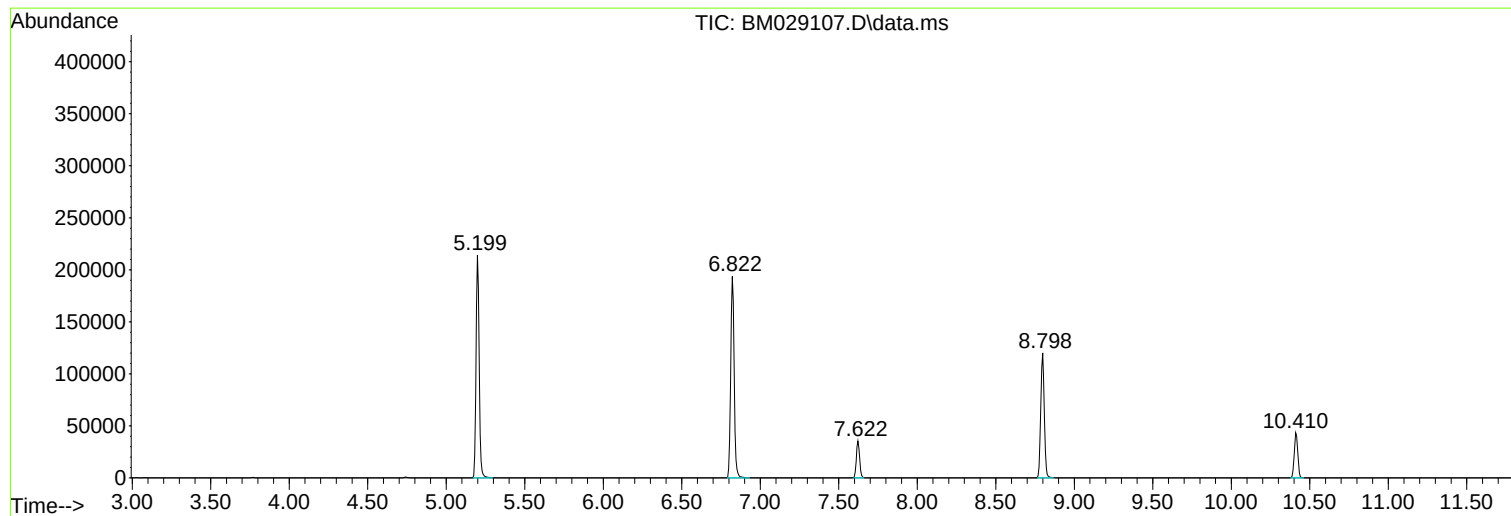

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029107.D
Acq On : 12 Mar 2021 12:28
Operator : CG/JU
Sample : PB135107BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135107BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029107.D
Acq On : 12 Mar 2021 12:28
Operator : CG/JU
Sample : PB135107BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135107BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------