

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
 Data File : BM029112.D
 Acq On : 12 Mar 2021 15:35
 Operator : CG/JU
 Sample : PB135109BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135109BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.199	371	376	386	rBV	202781	278884	61.28%	12.534%
2	6.822	646	652	666	rBV	182856	277343	60.94%	12.464%
3	7.622	783	788	797	rBB	32590	48433	10.64%	2.177%
4	8.798	981	988	999	rBV	109568	178524	39.23%	8.023%
5	10.410	1256	1262	1271	rBB	40065	63199	13.89%	2.840%
6	12.904	1680	1686	1694	rBB	262911	361007	79.33%	16.225%
7	14.292	1917	1922	1928	rBB	53618	73577	16.17%	3.307%
8	15.792	2172	2177	2186	rBB	179088	241636	53.10%	10.860%
9	17.045	2384	2390	2397	rBB	56657	76748	16.86%	3.449%
10	19.674	2831	2837	2841	rBV	379124	455090	100.00%	20.453%
11	21.221	3096	3100	3106	rVB2	72057	81722	17.96%	3.673%
12	23.362	3458	3464	3472	rVB2	49362	88902	19.54%	3.995%




Sum of corrected areas: 2225065

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029112.D
Acq On : 12 Mar 2021 15:35
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

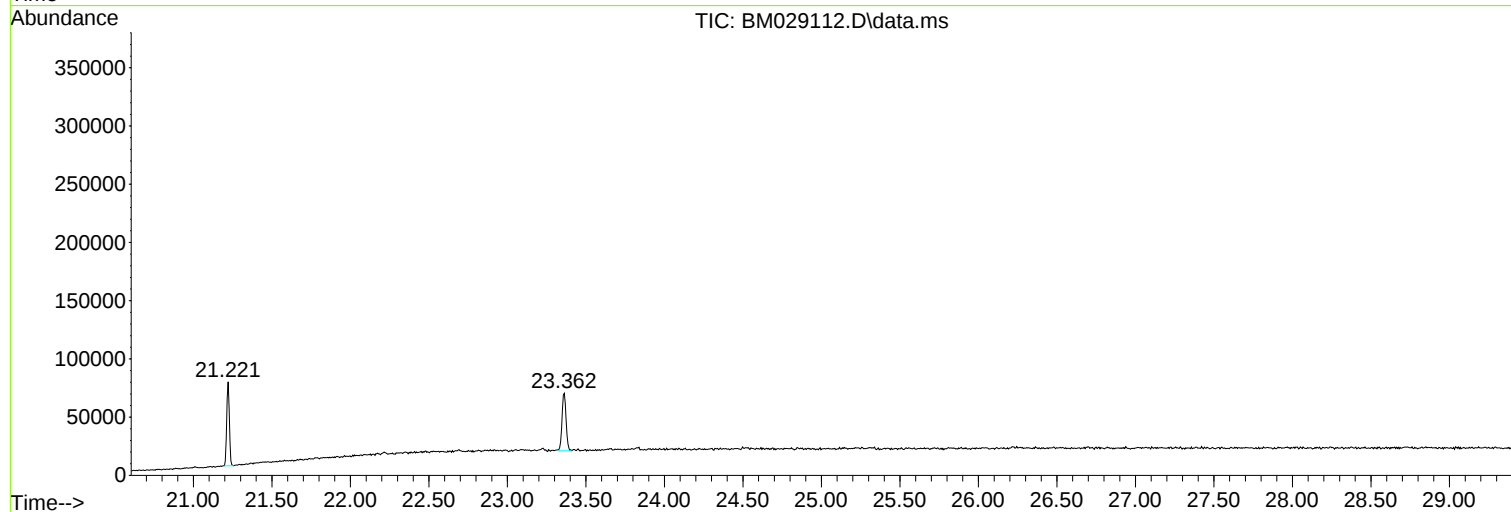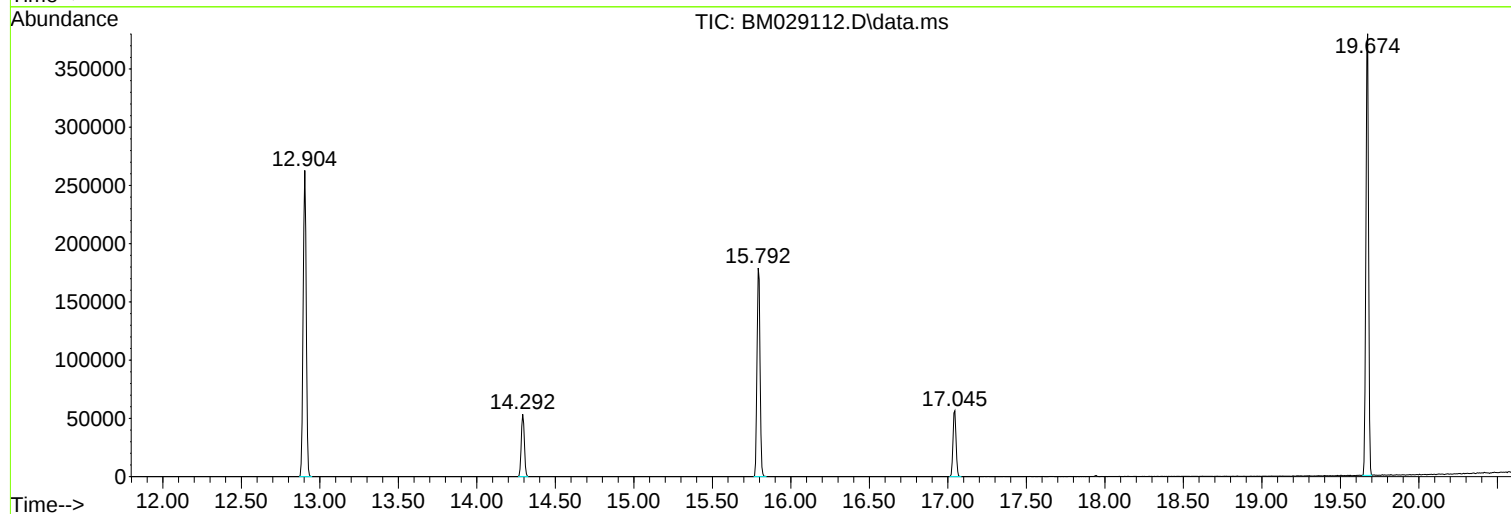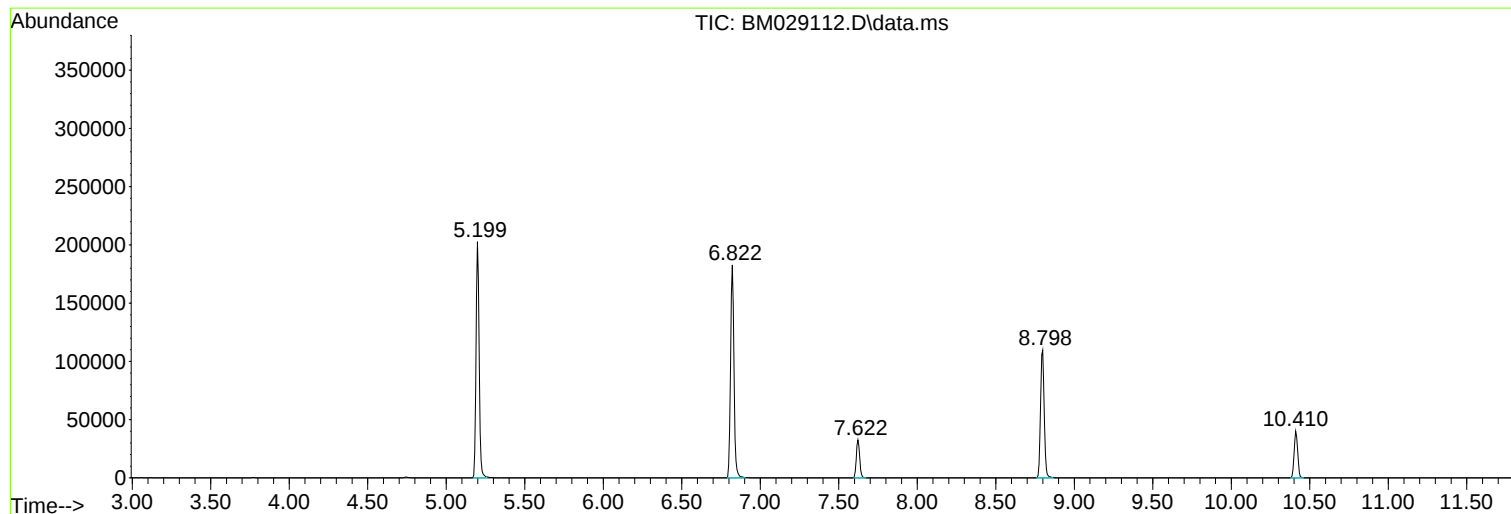

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029112.D
Acq On : 12 Mar 2021 15:35
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029112.D
Acq On : 12 Mar 2021 15:35
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------