
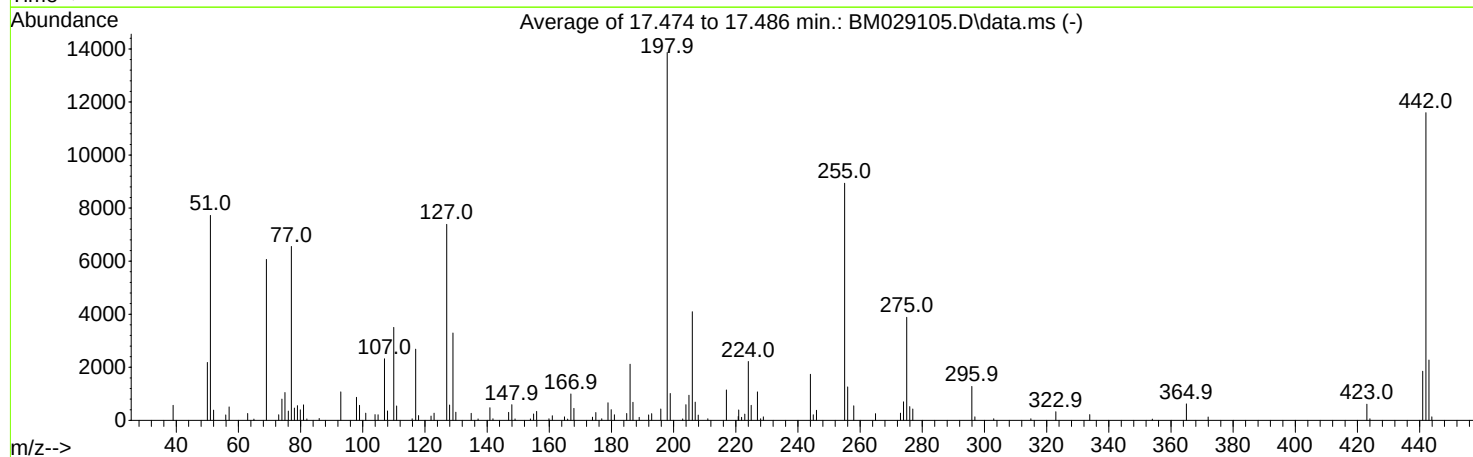


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
 Data File : BM029105.D
 Acq On : 12 Mar 2021 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 12 12:30:15 2021

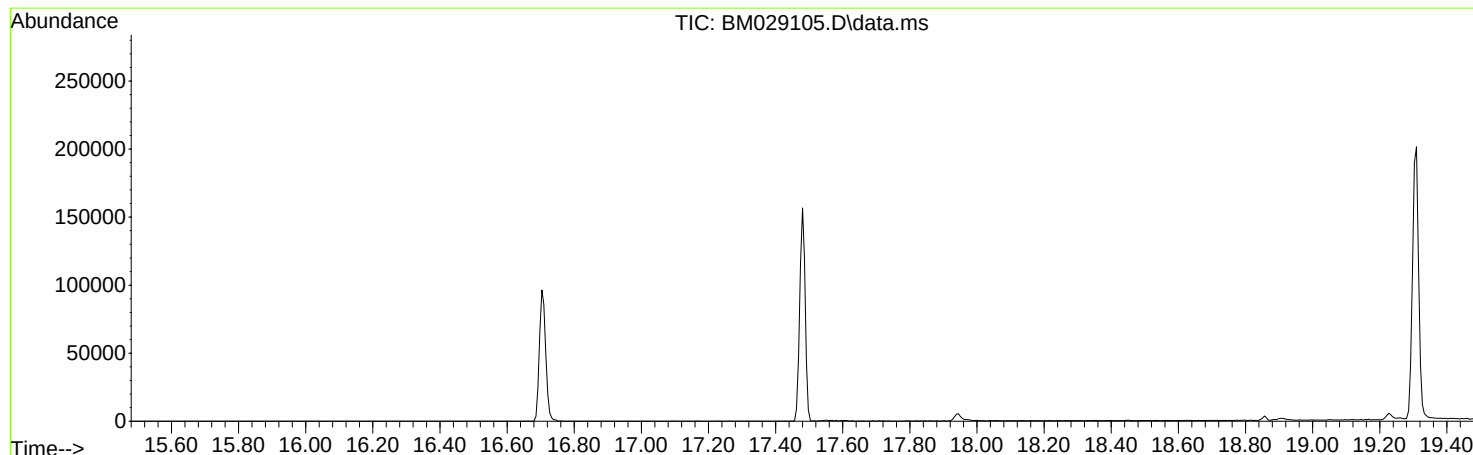

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457




Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.7	7726	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	6070	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	7390	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13865	PASS
199	198	5	9	7.3	1016	PASS
275	198	10	60	28.0	3884	PASS
365	198	1	100	4.5	623	PASS
441	198	0.01	100	13.3	1849	PASS
442	442	50	100	100.0	11600	PASS
443	442	15	24	19.6	2272	PASS

	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
3/12/2021	BNA_M	<u>BM029105.D</u>
Compound Name	Response	Retention Time
DDT	53855	20.52
DDD	517	20.09
DDE	0	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
517	54372	0.95

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029105.D
Acq On : 12 Mar 2021 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 12 11:58:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

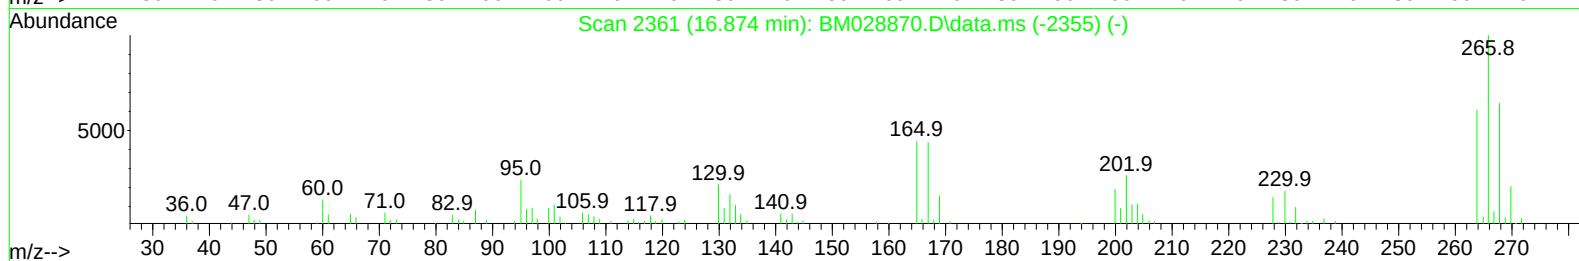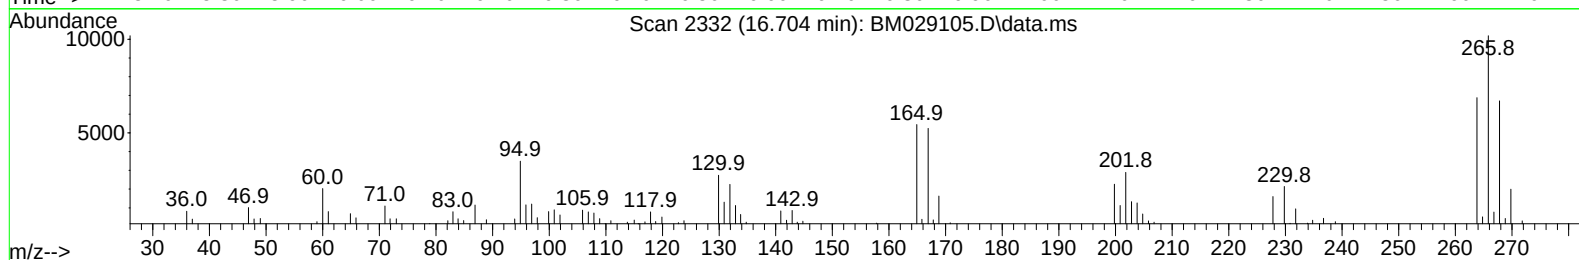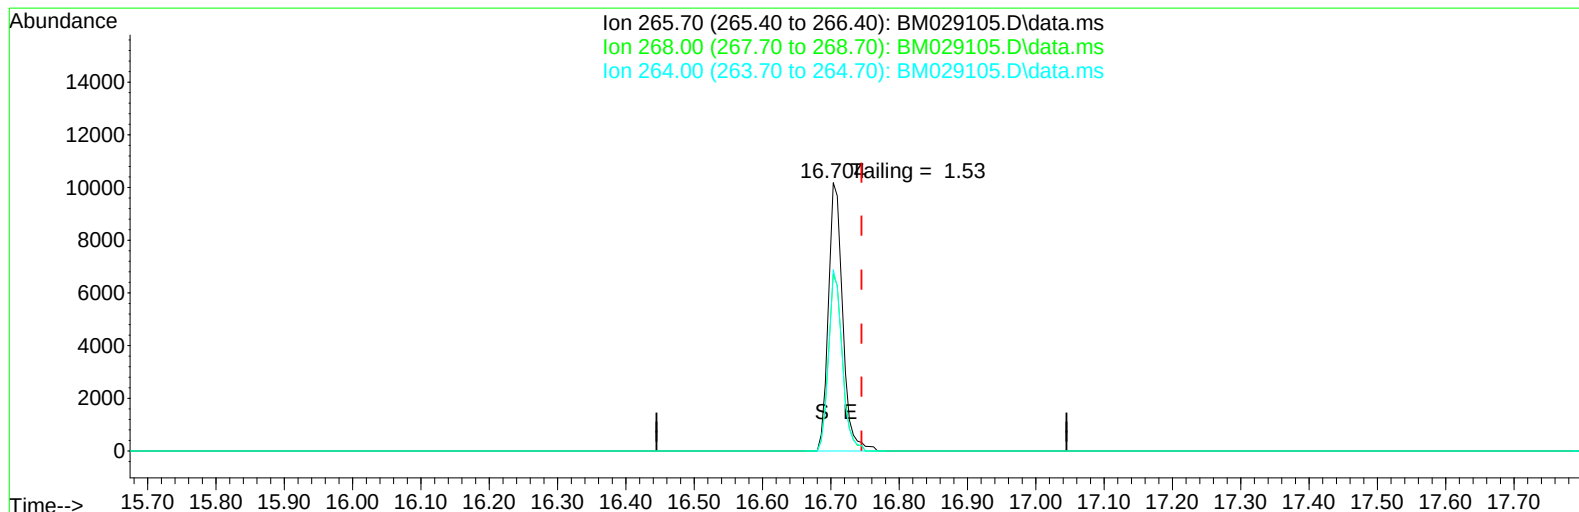

TIC: BM029105.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.041) 0.00 ng




response 14732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.84
264.00	63.30	67.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031221\
Data File : BM029105.D
Acq On : 12 Mar 2021 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 12 11:58:05 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

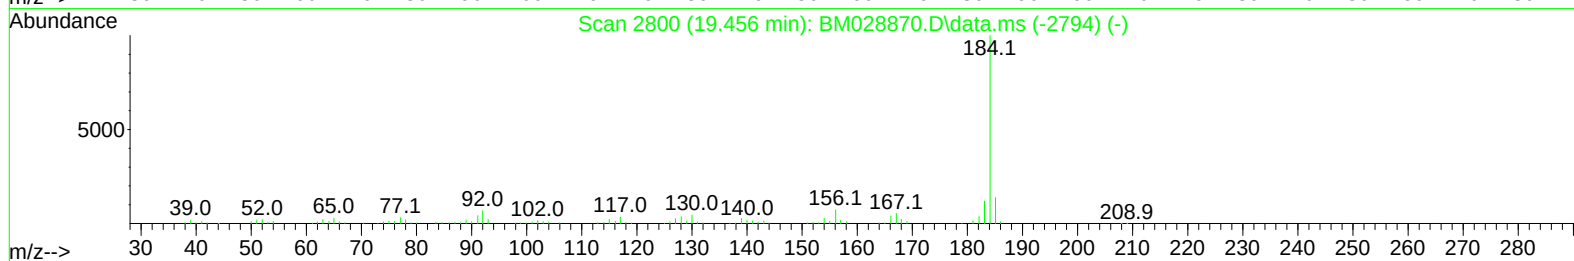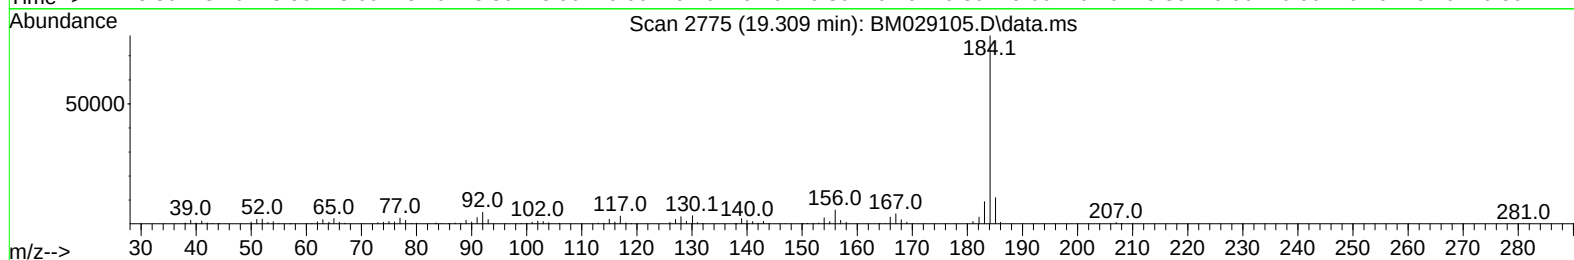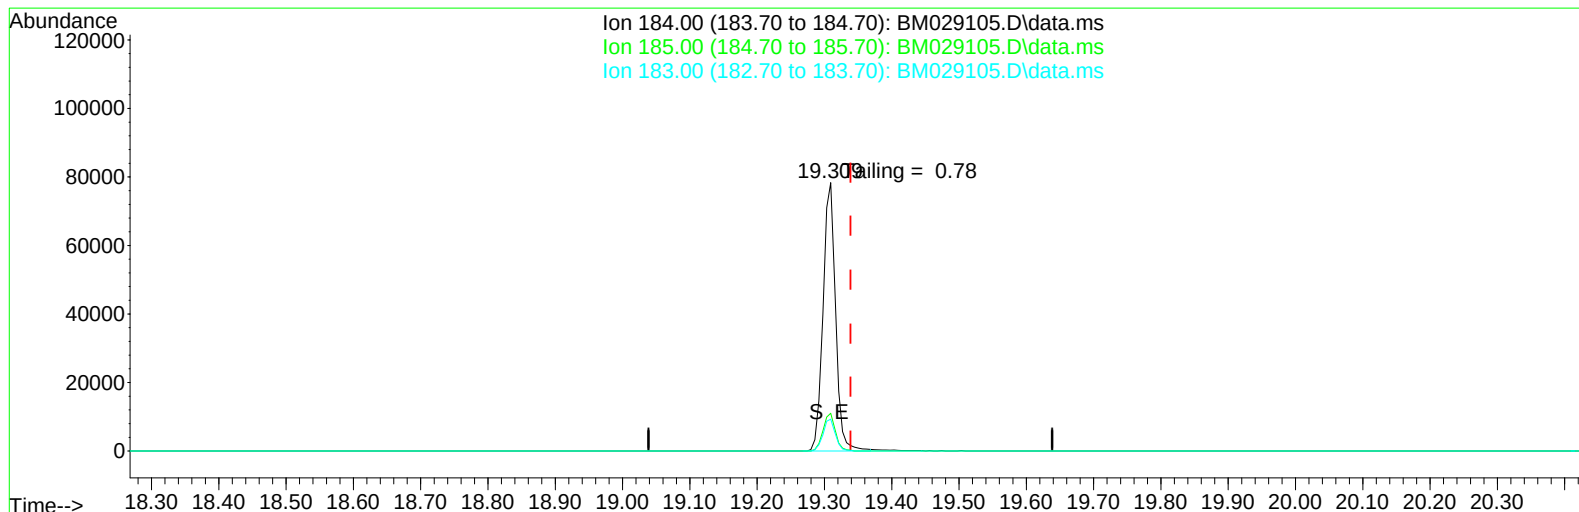

TIC: BM029105.D\data.ms

(77) Benzidine

19.309min (-0.030) 0.00 ng

response 102126

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.09
183.00	12.10	11.88
0.00	0.00	0.00