

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031224\
 Data File : BM044590.D
 Acq On : 12 Mar 2024 14:18
 Operator : MA/JU
 Sample : P1703-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/13/2024
 Supervised By :mohammad ahmed 03/14/2024

Quant Time: Mar 12 15:02:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 14:02:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.719	152	6368	0.400	ng/ul	0.00
4) Naphthalene-d8	10.501	136	22540	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.362	164	12296	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.115	188	27732m	0.400	ng/ul	0.00
17) Chrysene-d12	21.319	240	19347m	0.400	ng/ul	0.00
23) Perylene-d12	23.566	264	15160m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	38610	4.625	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.101	152	11665	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.150	212	24808	0.365	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.310	88	4956	0.581	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031224\  
Data File : BM044590.D  
Acq On    : 12 Mar 2024   14:18  
Operator  : MA/JU  
Sample    : P1703-01  
Misc      :  
ALS Vial  : 8    Sample Multiplier: 1
```


Instrument :
BNA_M
ClientSampleId :
BH7G7

Manual Integrations

Reviewed By :Jagrut Upadhyay 03/13/2024
Supervised By :mohammad ahmed 03/14/2024


Quant Time: Mar 12 15:02:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM031124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Mon Mar 11 14:02:17 2024
Response via : Initial Calibration

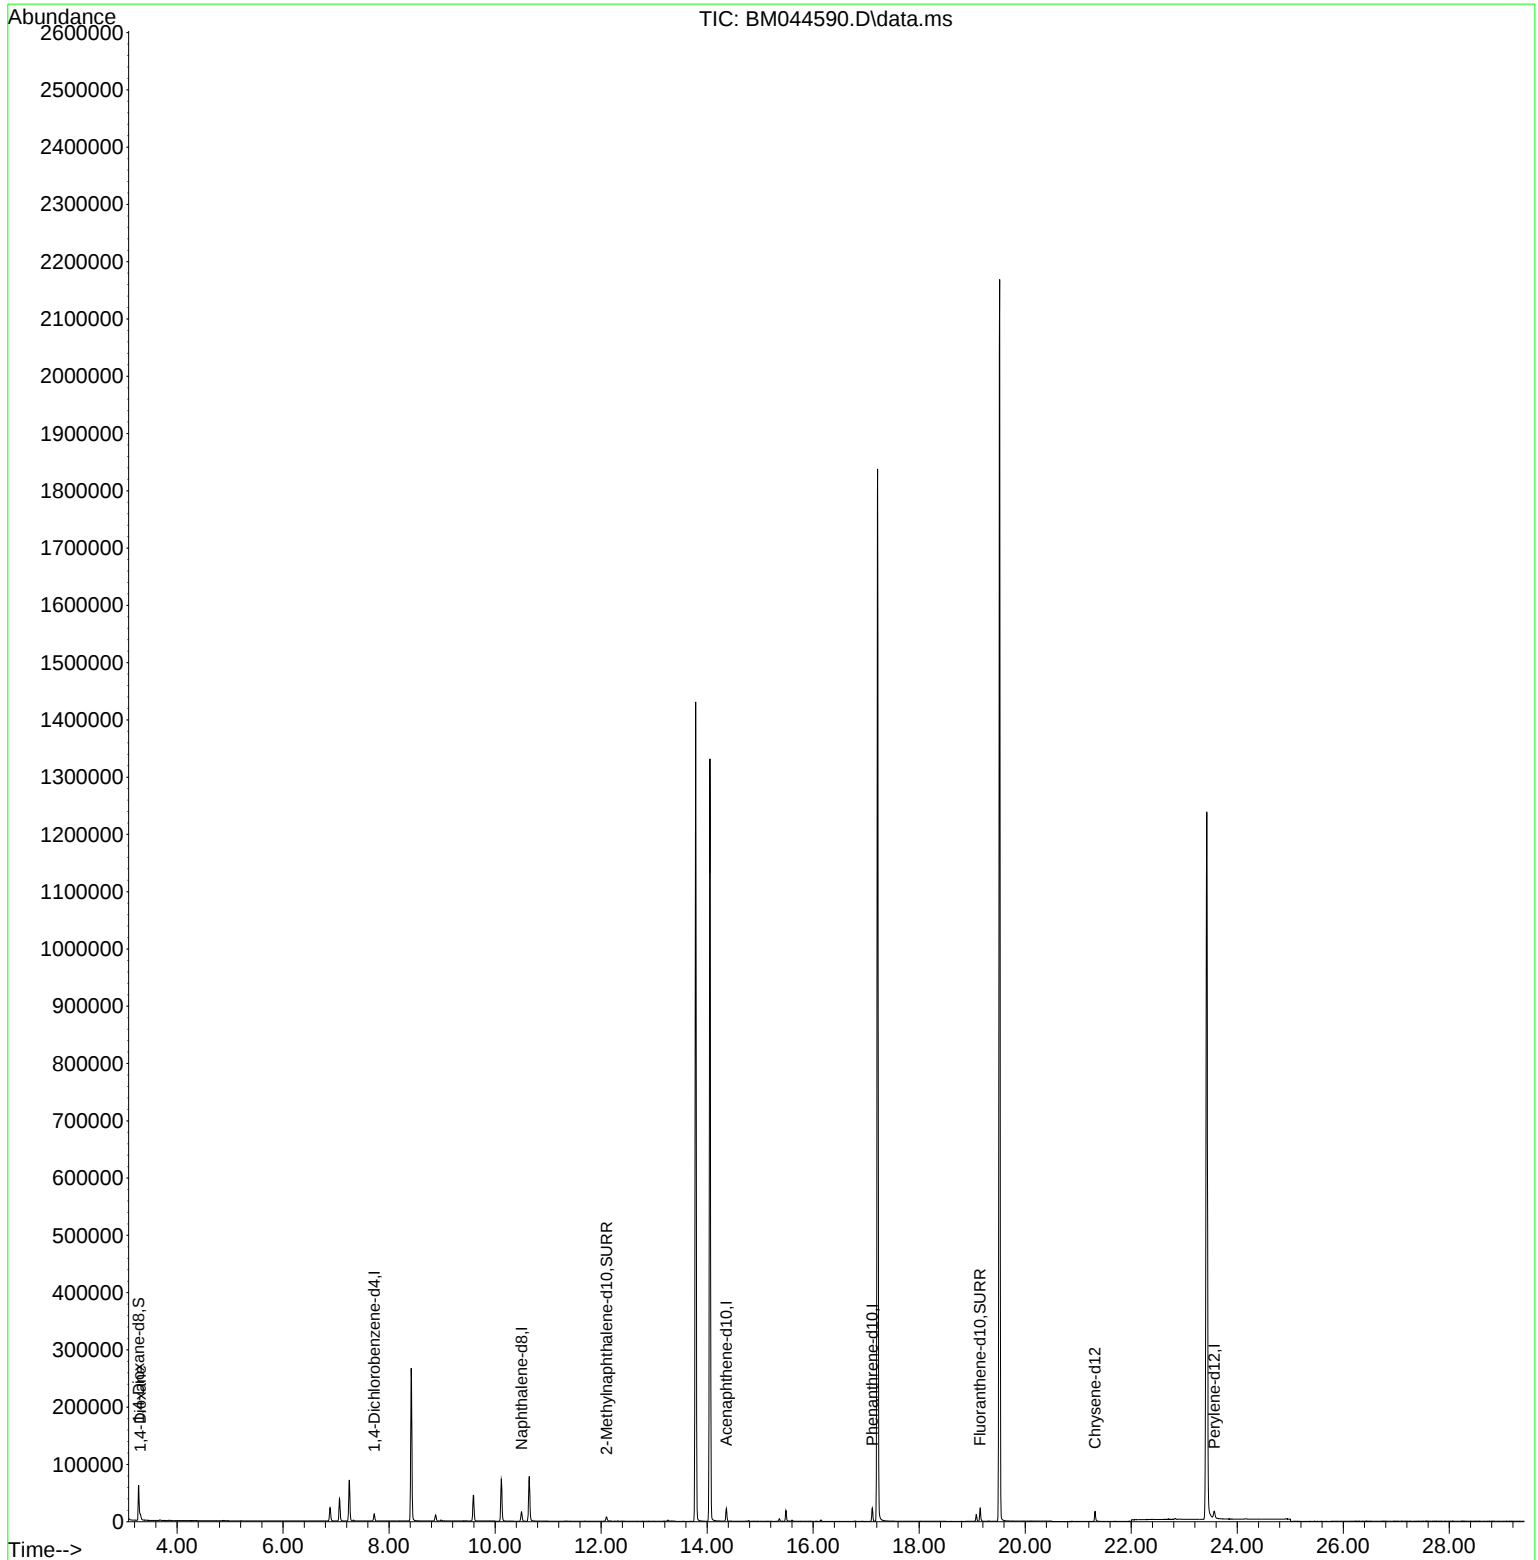

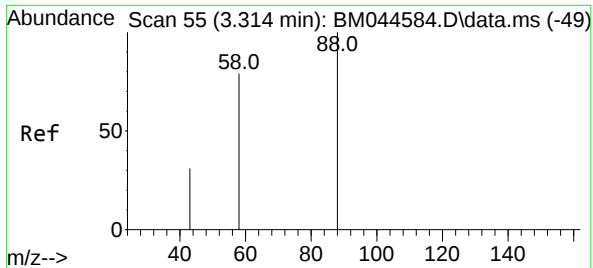

#2
 1,4-Dioxane
 Concen: 0.581 ng/ul
 RT: 3.310 min Scan# 54
 Delta R.T. -0.005 min
 Lab File: BM044590.D
 Acq: 12 Mar 2024 14:18

Instrument :
 BNA_M
 ClientSampleId :
 BH7G7

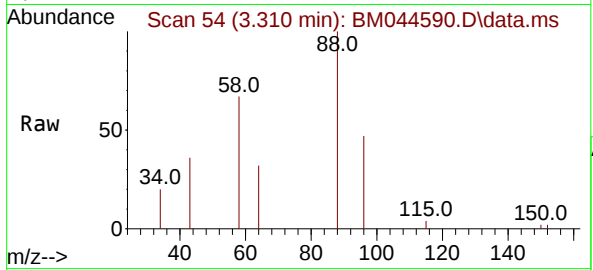

Tgt Ion: 88 Resp: 4950

Ion	Ratio	Lower	Upper
88	100		
43	35.7	21.4	32.0
58	66.9	35.6	53.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/13/2024
 Supervised By :mohammad ahmed 03/14/2024

