
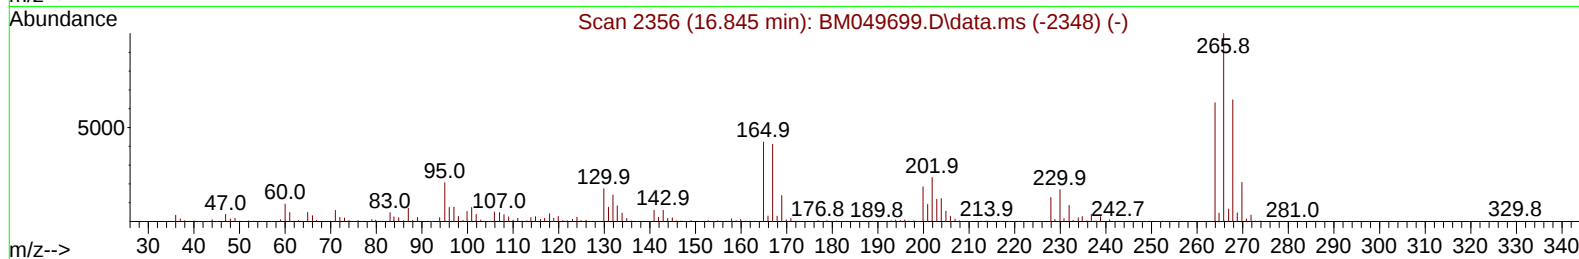
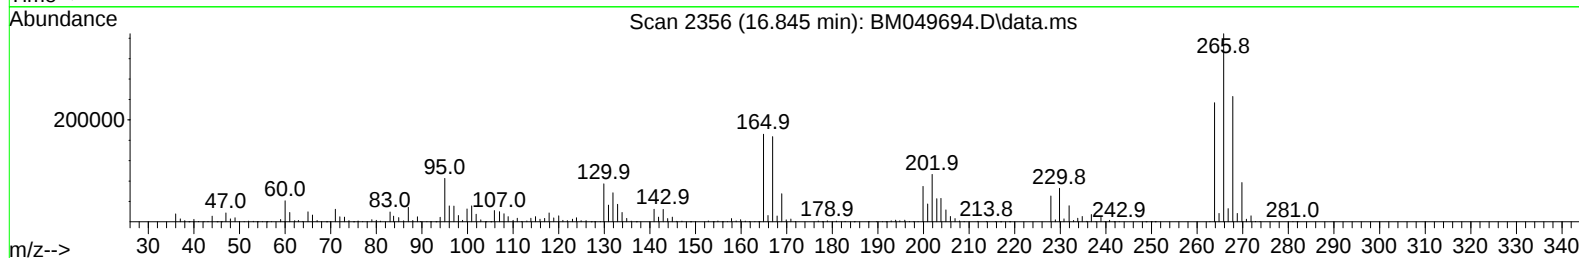


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031225\
Data File : BM049694.D
Acq On : 12 Mar 2025 15:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 02:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 01:48:09 2025
Response via : Initial Calibration

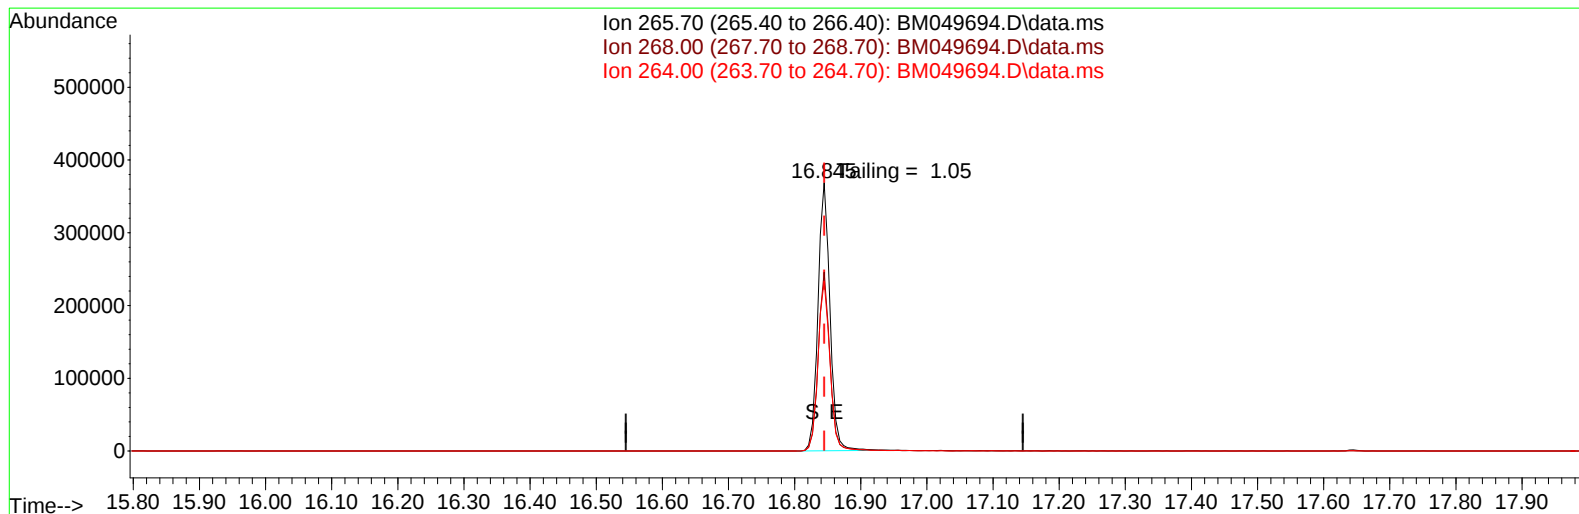

TIC: BM049694.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.000) 0.00 ng

response 472442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.62
264.00	63.20	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031225\
Data File : BM049694.D
Acq On : 12 Mar 2025 15:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 13 02:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 01:48:09 2025
Response via : Initial Calibration

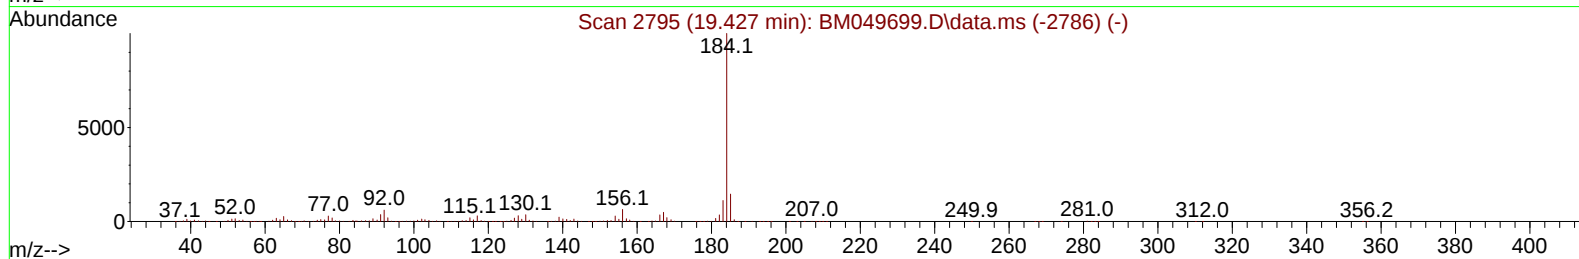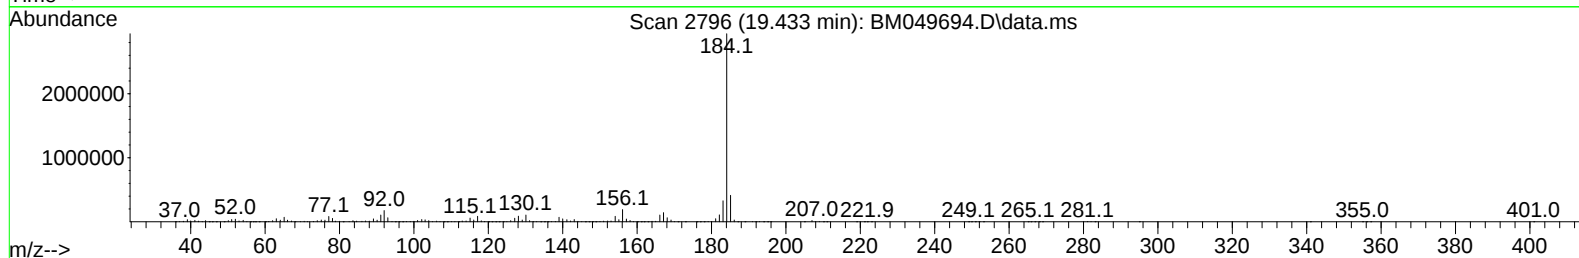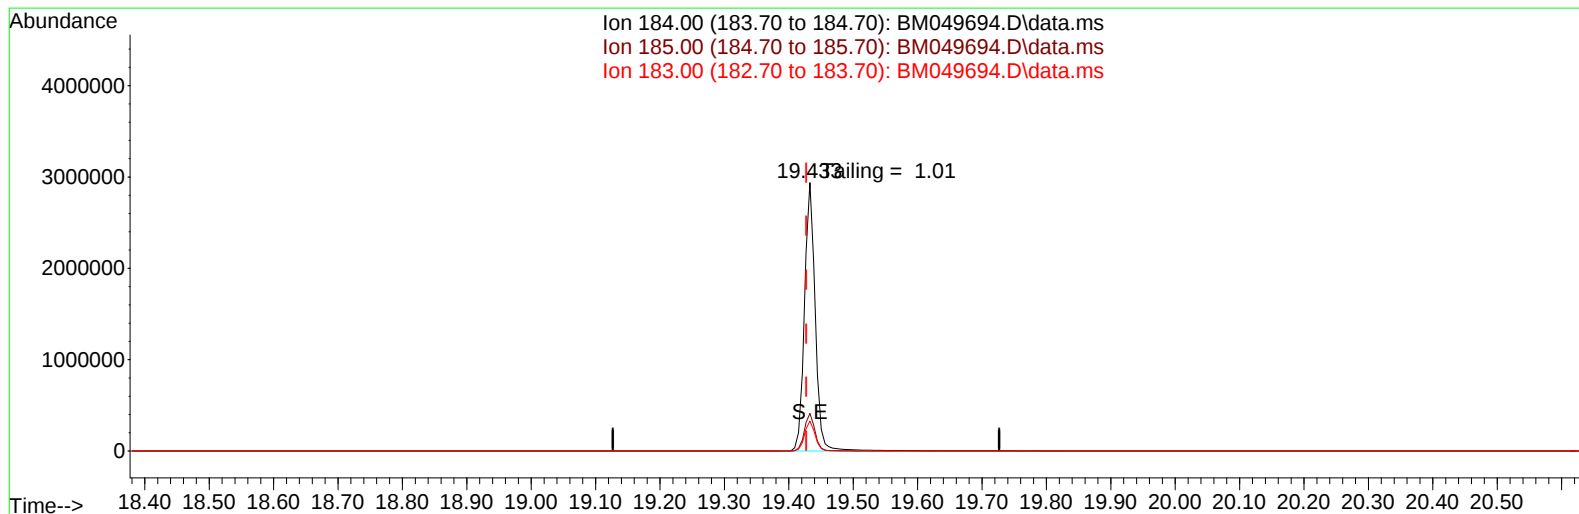

TIC: BM049694.D\data.ms

(77) Benzidine

19.433min (+ 0.006) 0.00 ng

response 3444869

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.02
183.00	11.20	11.20
0.00	0.00	0.00