
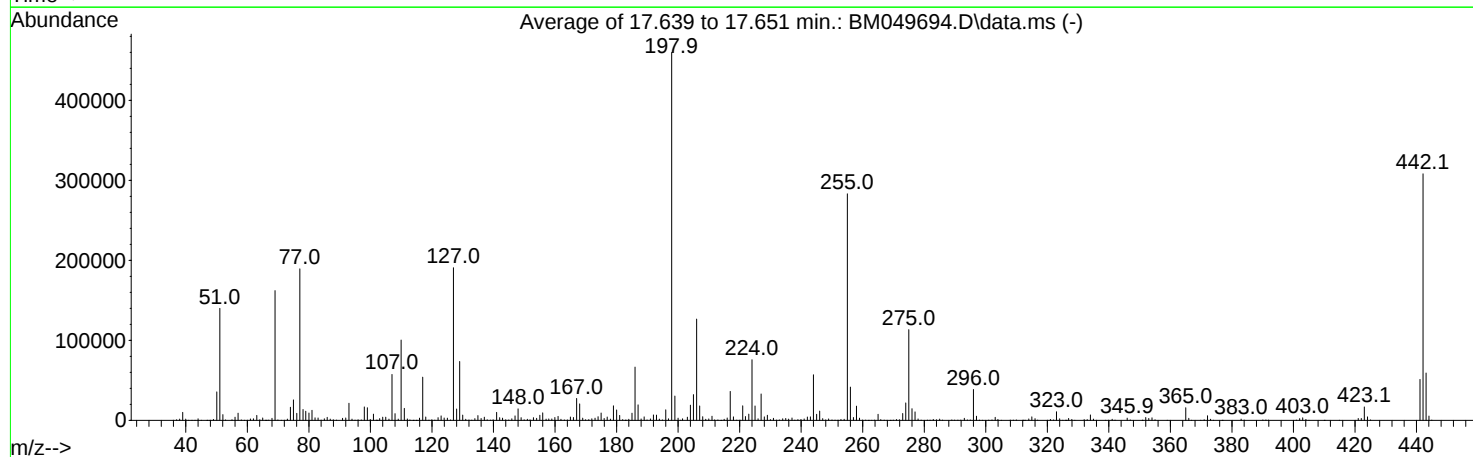


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031225\
Data File : BM049694.D
Acq On : 12 Mar 2025 15:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 01:48:09 2025

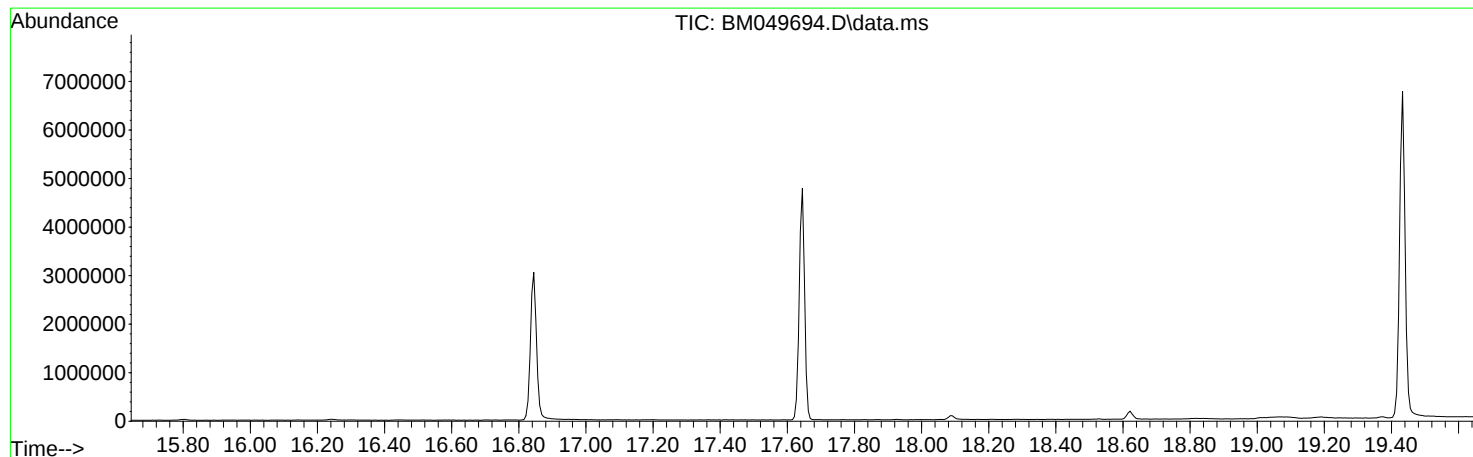

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	140010	PASS
68	69	0.00	2	1.6	2655	PASS
69	198	0.00	100	35.3	162326	PASS
70	69	0.00	2	0.4	677	PASS
127	198	10	80	41.5	190749	PASS
197	198	0.00	2	0.4	1956	PASS
198	198	100	100	100.0	459883	PASS
199	198	5	9	6.6	30328	PASS
275	198	10	60	24.7	113515	PASS
365	198	1	100	3.5	15888	PASS
441	198	0.01	100	11.1	51165	PASS
442	442	50	100	100.0	308181	PASS
443	442	15	24	19.2	59176	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/12/2025	BNA_M	<u>BM049694.D</u>
Compound Name	Response	Retention Time
DDT	1542656	20.674
DDD	9167	20.286
DDE	257	19.056
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9424	1552080	0.61

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031225\
Data File : BM049694.D
Acq On : 12 Mar 2025 15:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 13 02:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 01:48:09 2025
Response via : Initial Calibration

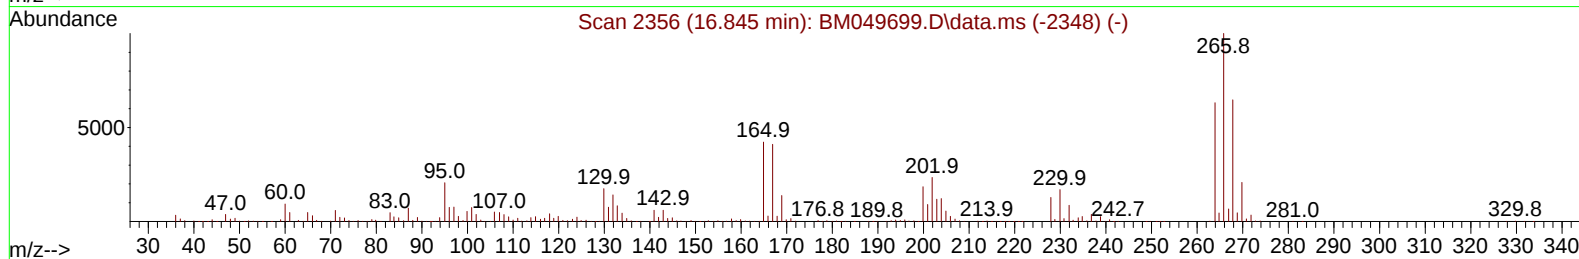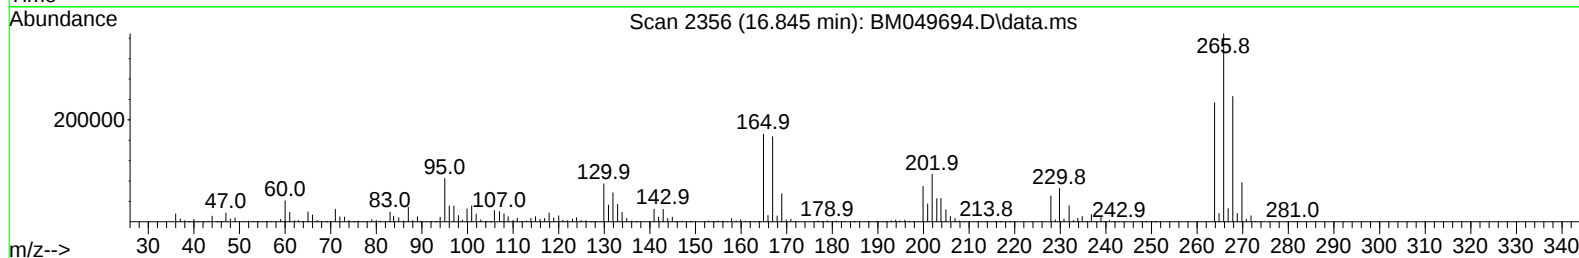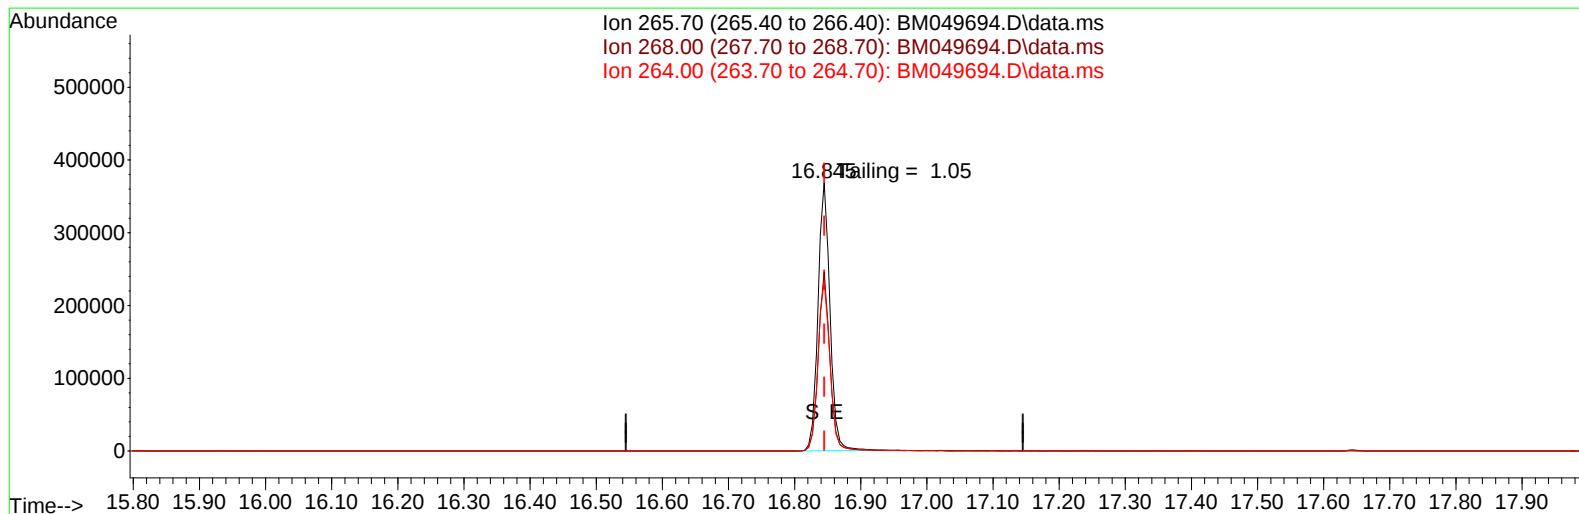

TIC: BM049694.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.000) 0.00 ng




response 472442

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.62
264.00	63.20	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031225\
Data File : BM049694.D
Acq On : 12 Mar 2025 15:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 13 02:01:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 01:48:09 2025
Response via : Initial Calibration

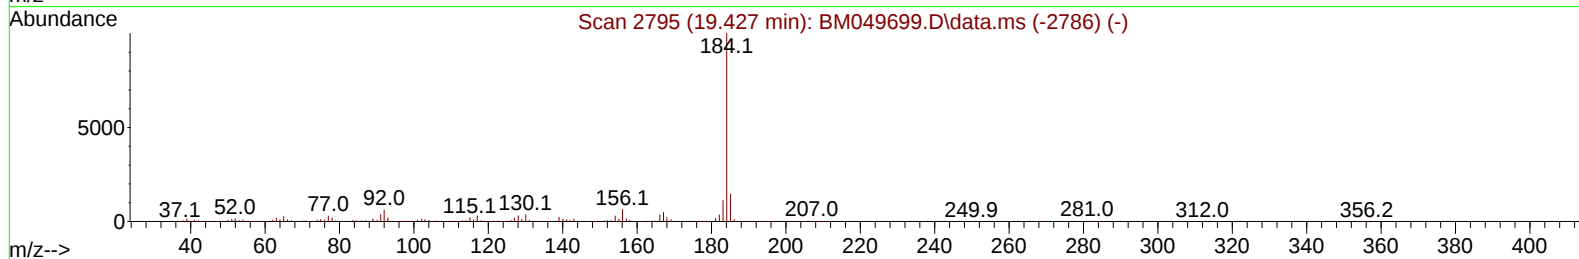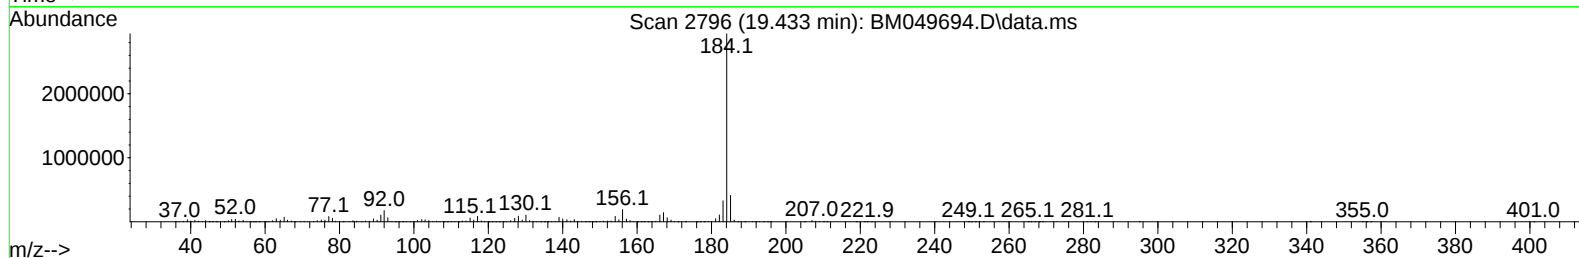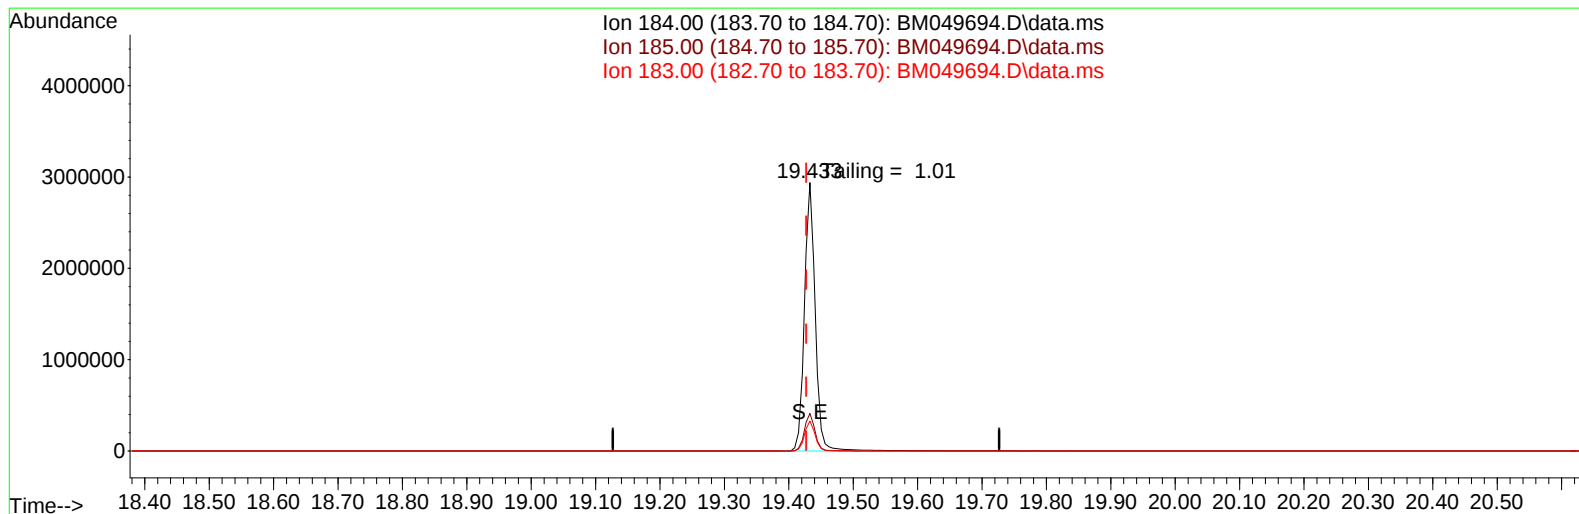

TIC: BM049694.D\data.ms

(77) Benzidine

19.433min (+ 0.006) 0.00 ng

response 3444869

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.02
183.00	11.20	11.20
0.00	0.00	0.00