
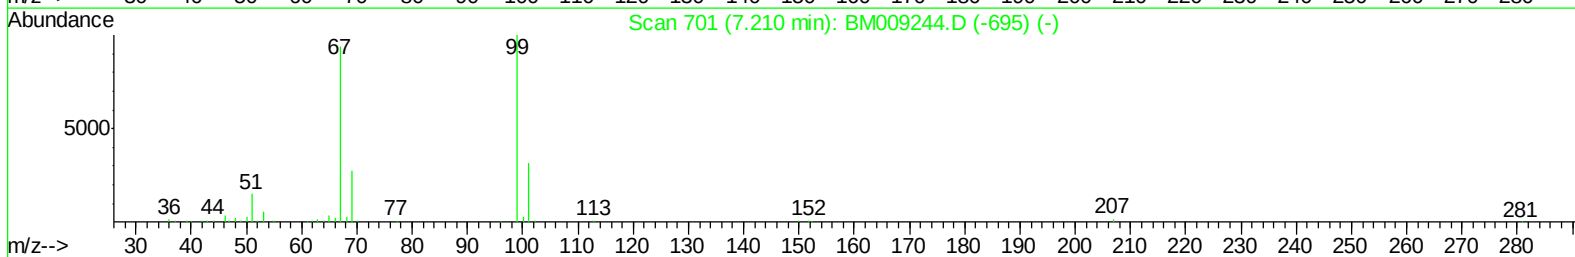
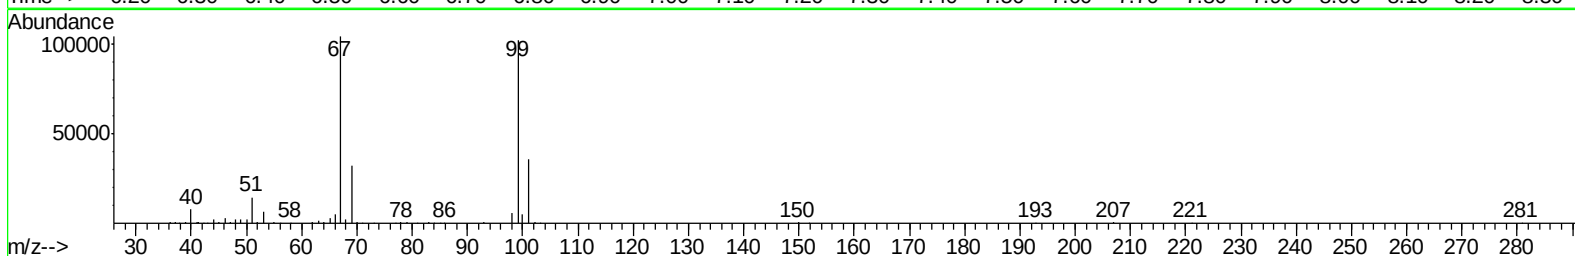


Data Path : Z:\HPCHEM1\BNA M\DATA\BM031317\
Data File : BM009251.D
Acq On : 14 Mar 2017 12:22
Operator : SJ/MA
Sample : I2235-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 15 02:02:14 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-2016\SOM-EPA-BM031317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 15 01:51:24 2017
Response via : Initial Calibration

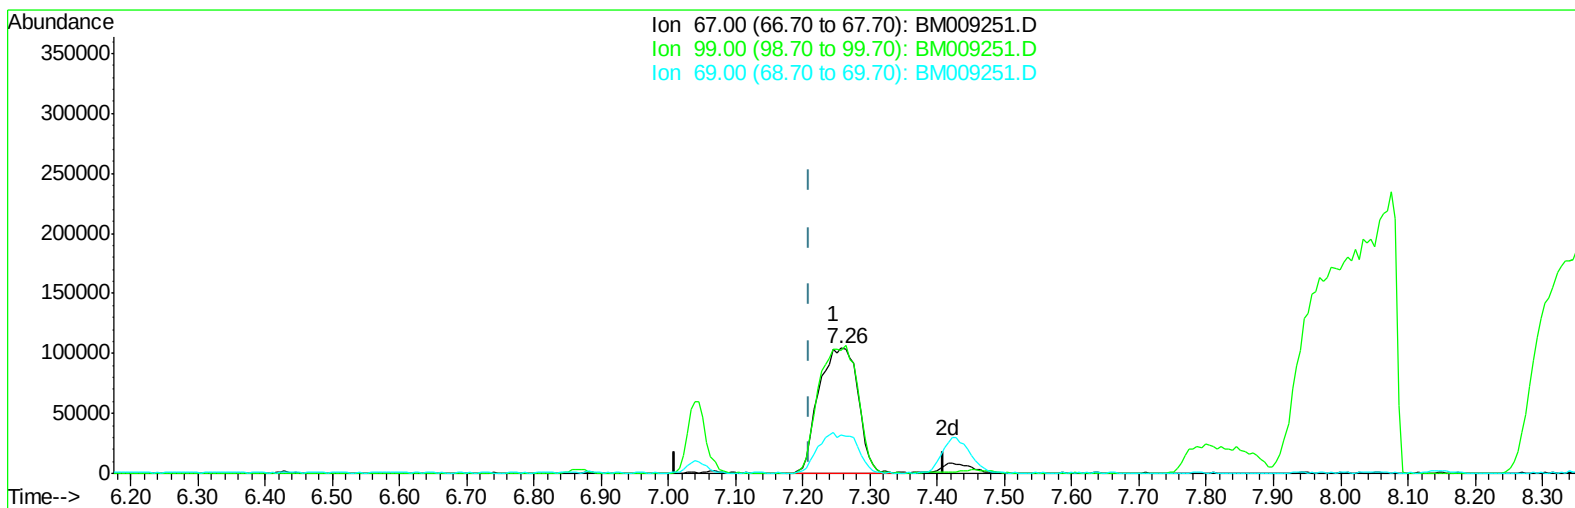

TIC: BM009251.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

7.257min (+0.047) 21.51ng/ul m

response 423878

Ion	Exp%	Act%
67.00	100	100
99.00	135.60	97.63#
69.00	32.50	30.71
0.00	0.00	0.00