

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031318\
 Data File : BM014546.D
 Acq On : 13 Mar 2018 14:27
 Operator : SJ/JU
 Sample : J1813-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F6F35

Quant Time: Mar 13 16:13:15 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 13 16:10:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	62067	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	281251	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.14	164	177031	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	432113	20.00	ng/ul	0.00
75) Chrysene-d12	21.12	240	524179	20.00	ng/ul	0.00
83) Perylene-d12	23.29	264	519986	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.05	96	4245	2.93	ng/uL	0.00
5) Phenol-d5	6.69	99	123993	23.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	80786	25.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	99934	24.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	93607	20.39	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	53922	25.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	62712	29.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	112941	25.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	108298	24.67	ng/ul	0.00
43) Dimethylphthalate-d6	13.56	166	422890	28.93	ng/ul	0.00
46) Acenaphthylene-d8	13.83	160	500421	27.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	32097	15.90	ng/ul	-0.02
57) Fluorene-d10	15.15	176	349857	26.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.33	200	51473	19.86	ng/ul	0.00
70) Anthracene-d10	17.00	188	547134	26.24	ng/ul	0.00
76) Pyrene-d10	19.32	212	669845	24.78	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.15	264	685799	27.10	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.62	163	76105	5.279	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031318\
Data File : BM014546.D
Acq On : 13 Mar 2018 14:27
Operator : SJ/JU
Sample : J1813-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F6F35

Quant Time: Mar 13 16:13:15 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 13 16:10:56 2018
Response via : Initial Calibration

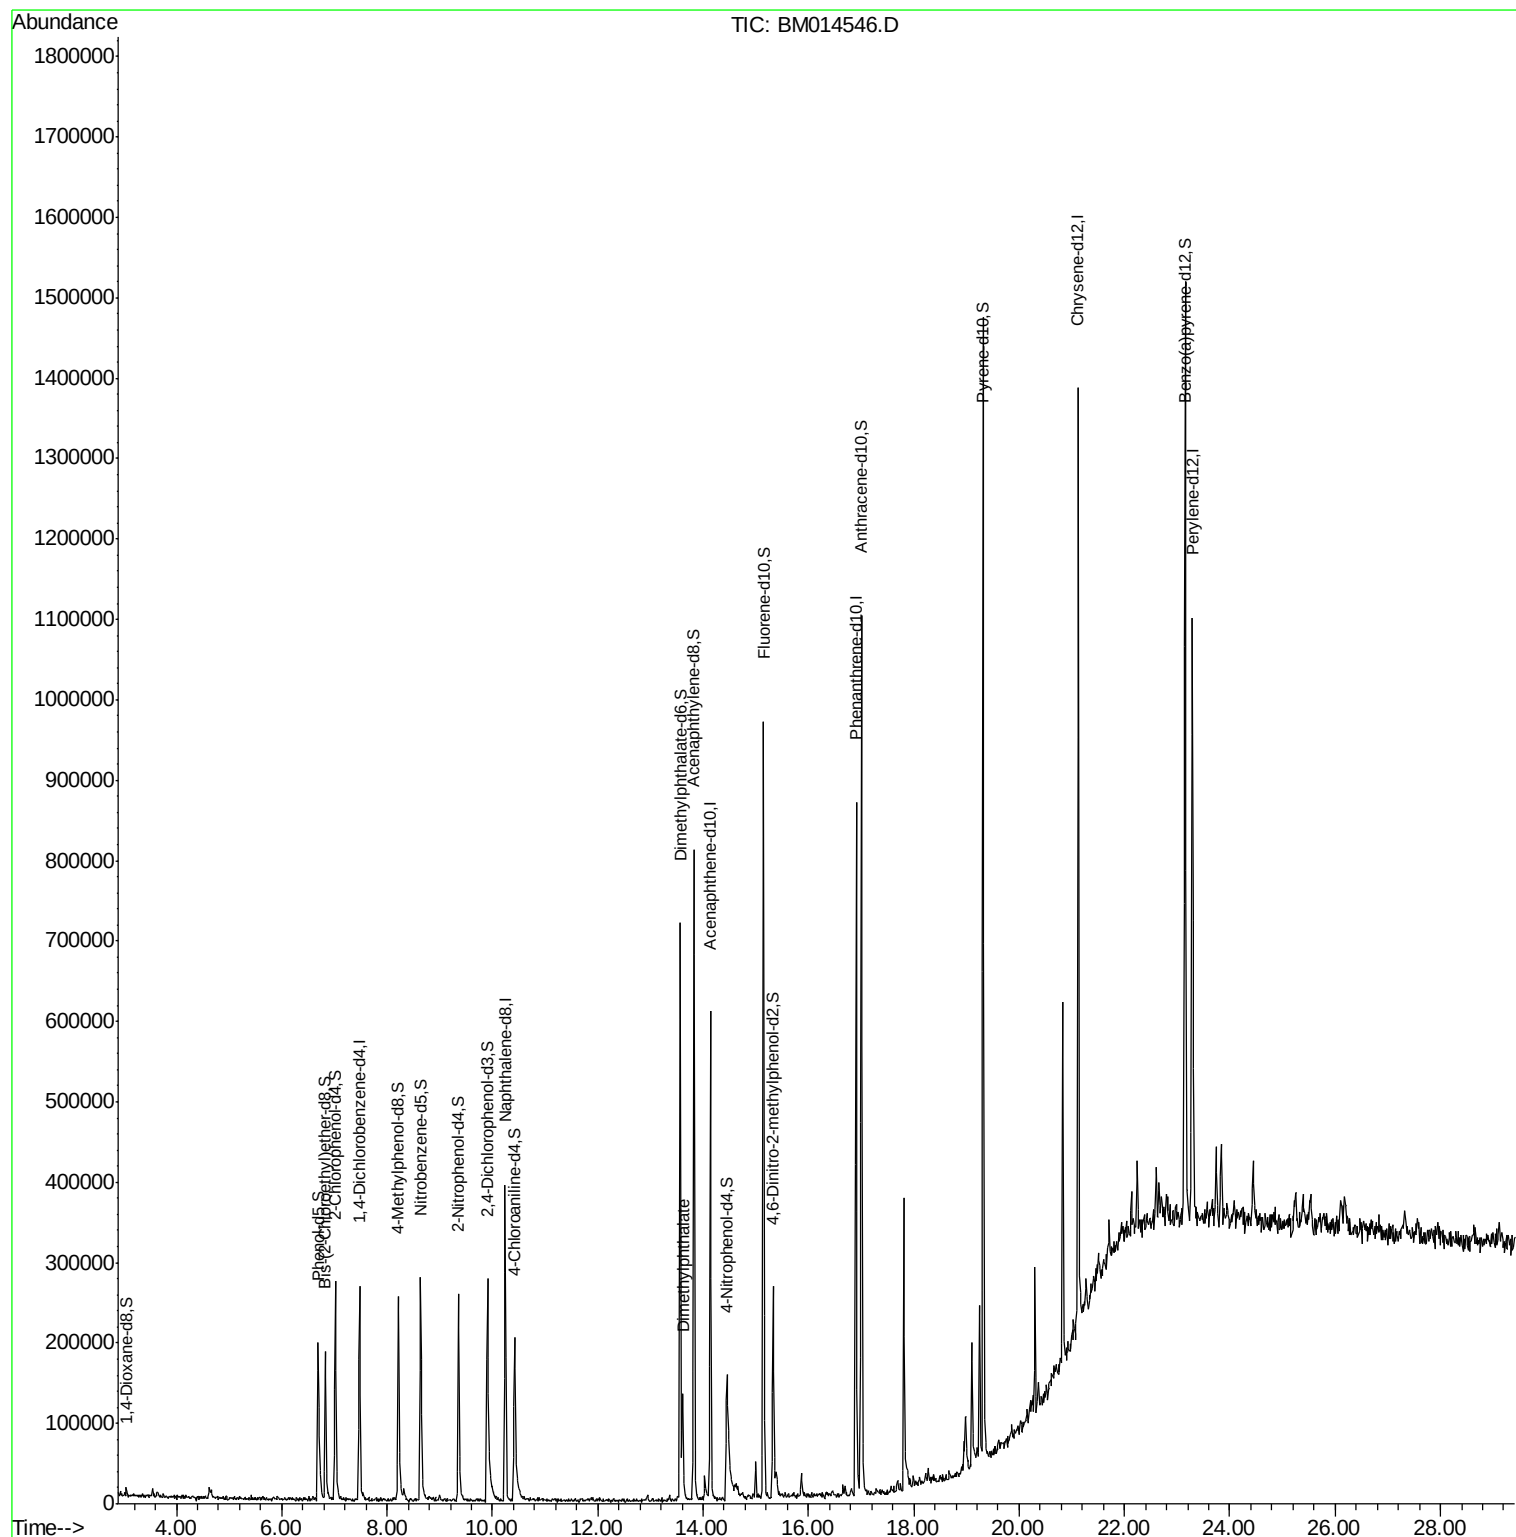


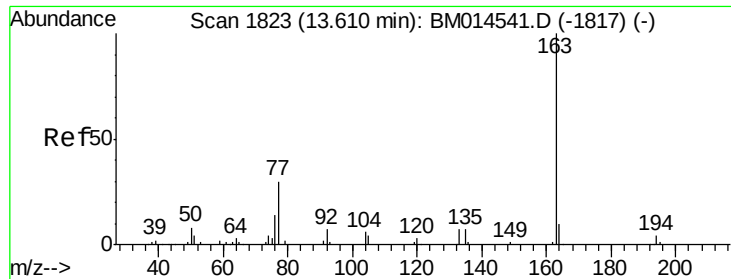

#44
 Dimethylphthalate
 Concen: 5.279 ng/ul
 RT: 13.62 min Scan# 1824
 Delta R.T. 0.00 min
 Lab File: BM014546.D
 Acq: 13 Mar 2018 14:27

Instrument :
 BNA_M
 ClientSampleId :
 F6F35

Tot Ion:163 Resp: 76105
 Ion Ratio Lower Upper
 163 100
 194 3.2 3.5 5.3#
 164 12.1 8.2 12.4

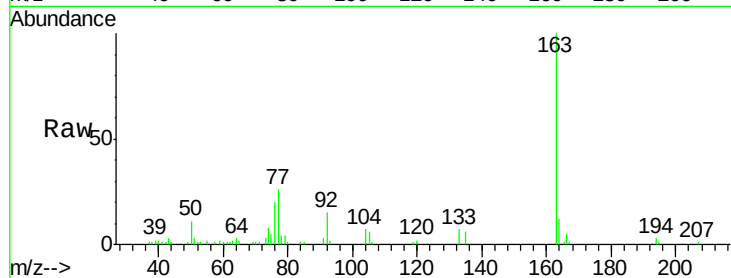

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

