
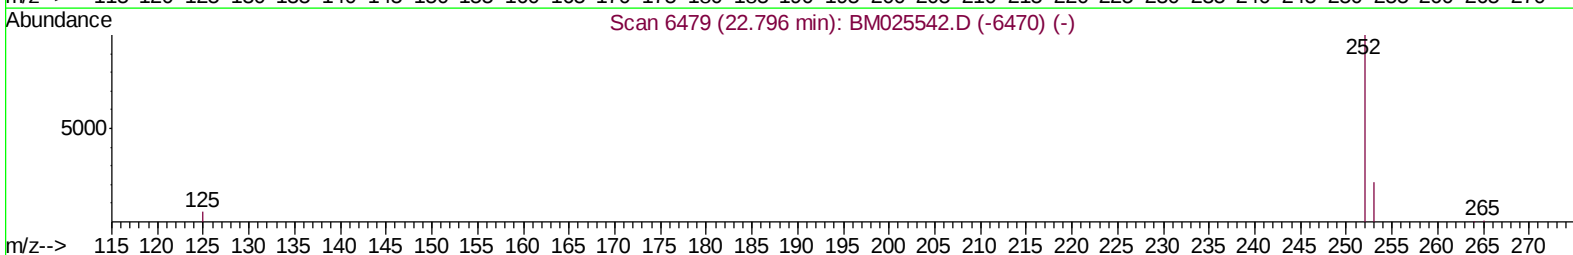
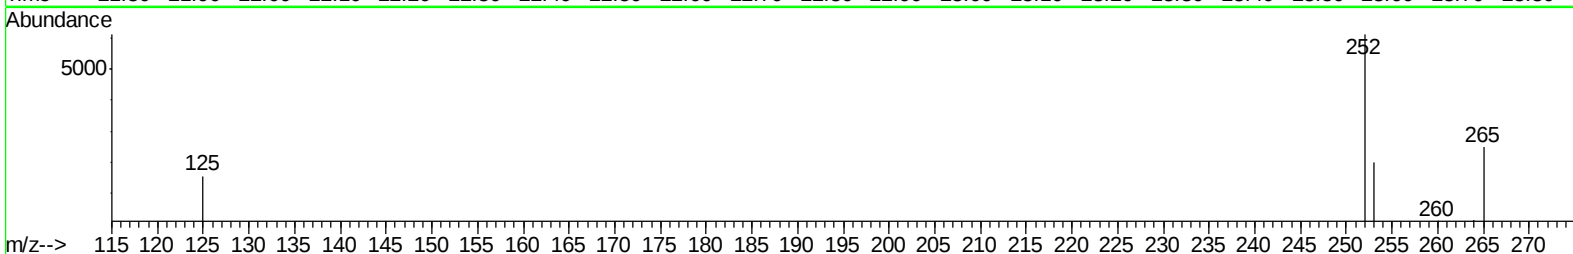


Data File : BM025545.D
Acq On : 13 Mar 2020 17:34
Operator : CG/JU
Sample : L1677-05DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 16 05:39:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 05:37:34 2020
Response via : Initial Calibration

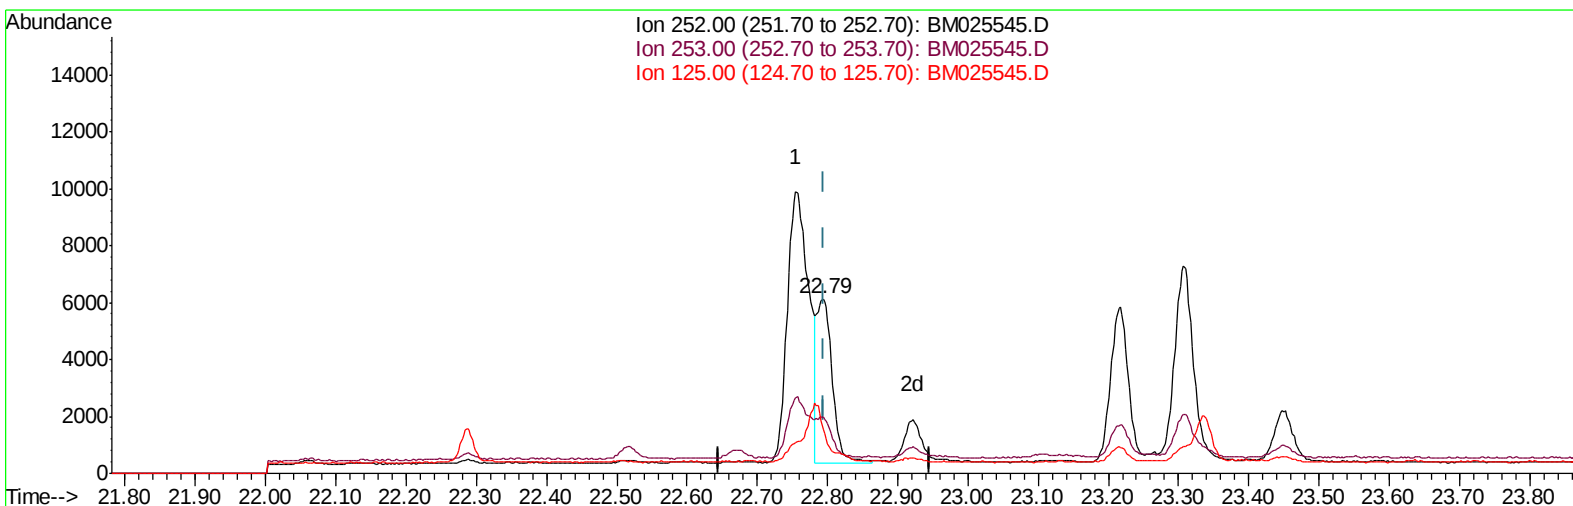

TIC: BM025545.D

(22) Benzo(k)fluoranthene

22.793min (-0.002) 0.17ng/ul m

response 9117

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	32.45#
125.00	8.90	25.17#
0.00	0.00	0.00