
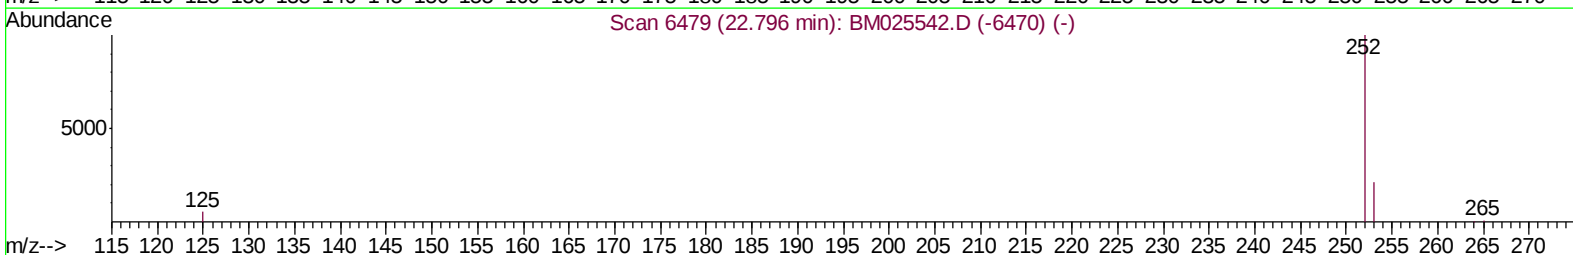
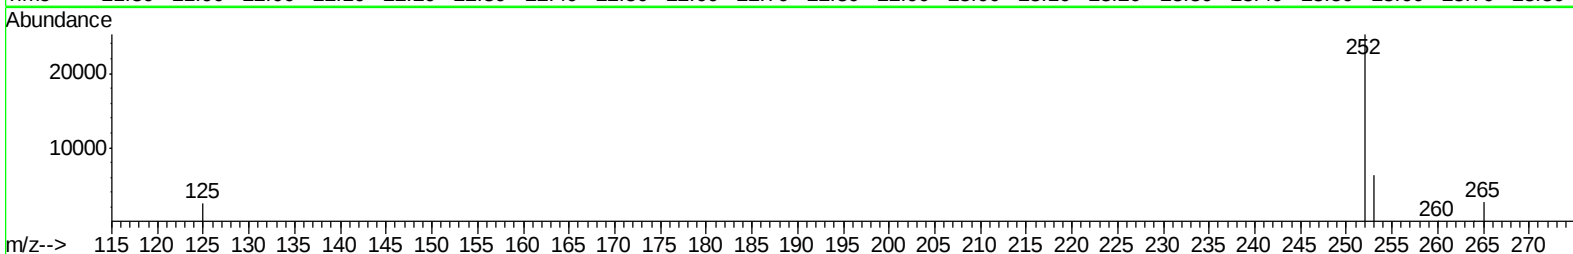


Data File : BM025551.D
Acq On : 13 Mar 2020 21:13
Operator : CG/JU
Sample : L1786-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Mar 16 05:40:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 05:37:34 2020
Response via : Initial Calibration

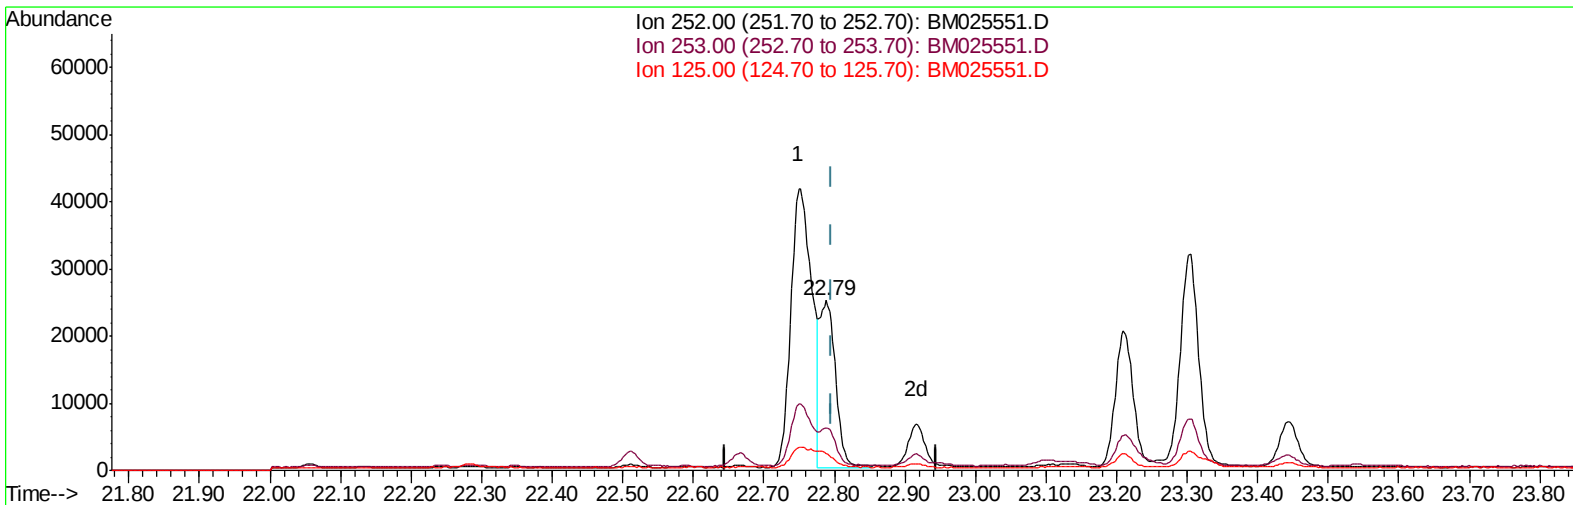

TIC: BM025551.D

(22) Benzo(k)fluoranthene

22.788min (-0.008) 0.51ng/ul m

response 38821

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	24.96
125.00	8.90	9.99
0.00	0.00	0.00