
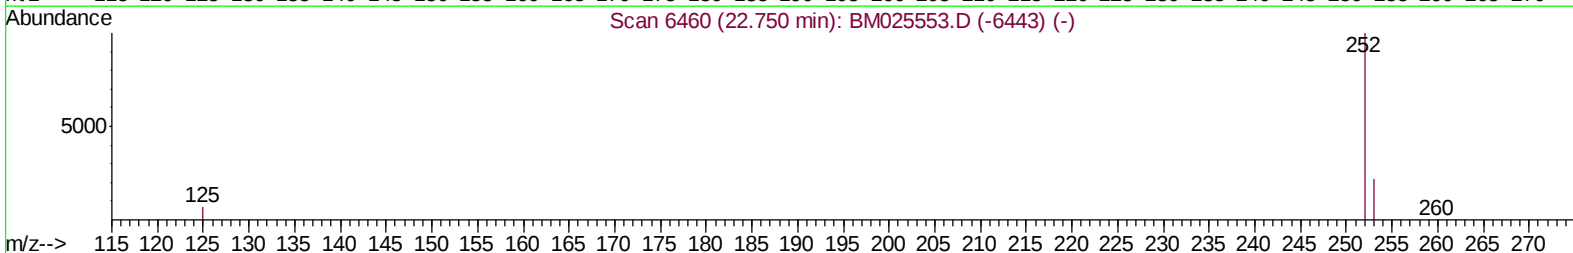
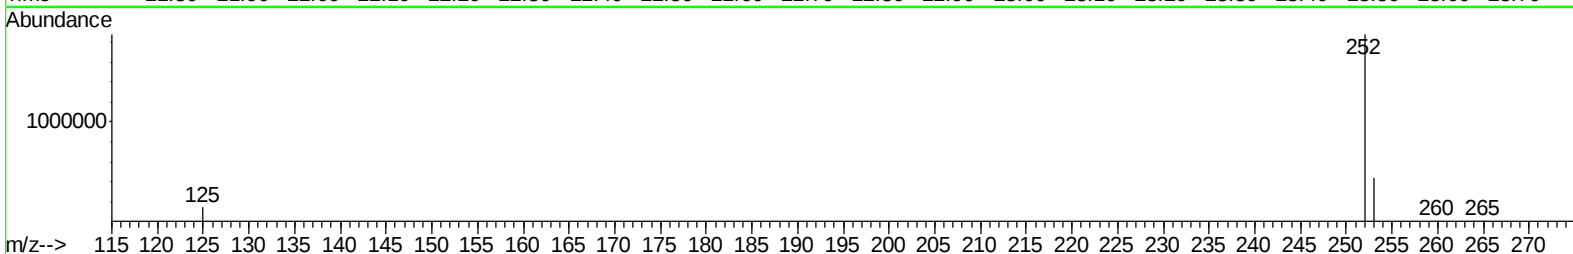


Data File : BM025555.D
Acq On : 14 Mar 2020 00:14
Operator : CG/JU
Sample : L1786-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 16 06:47:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

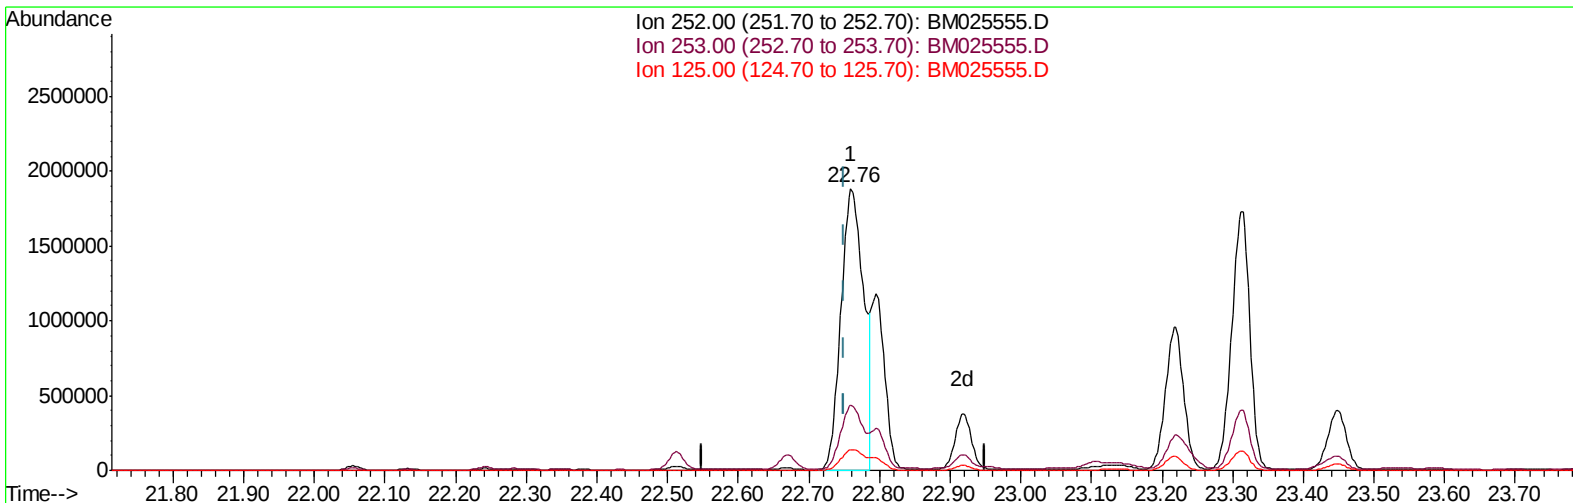

TIC: BM025555.D

(21) Benzo(b)fluoranthene

22.759min (+0.010) 42.18ng/ul m

response 4198299

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	23.26
125.00	8.80	7.43
0.00	0.00	0.00