
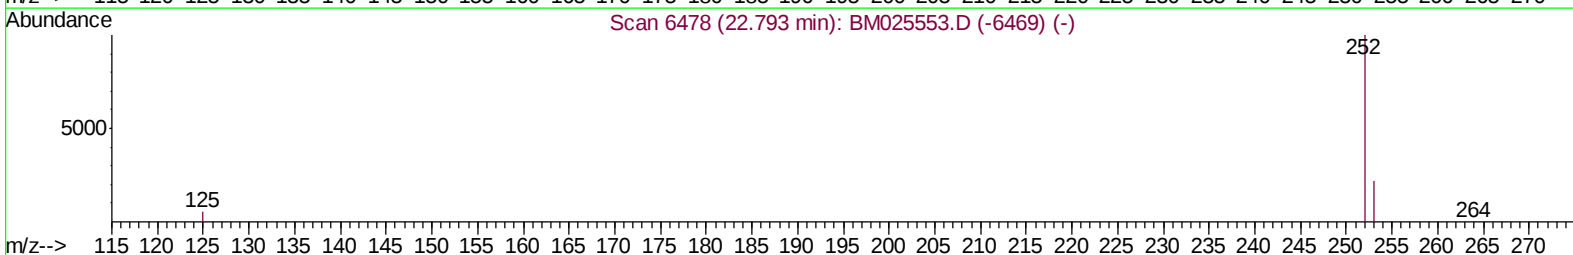
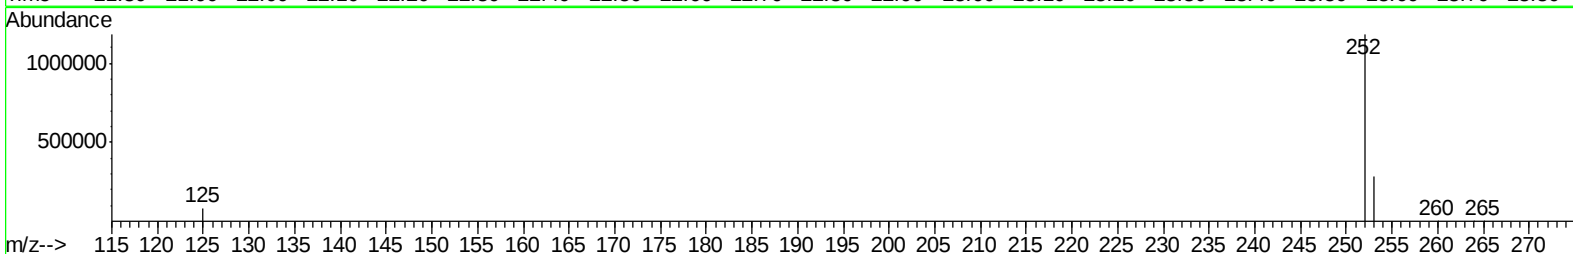


Data File : BM025555.D
Acq On : 14 Mar 2020 00:14
Operator : CG/JU
Sample : L1786-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 16 06:47:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

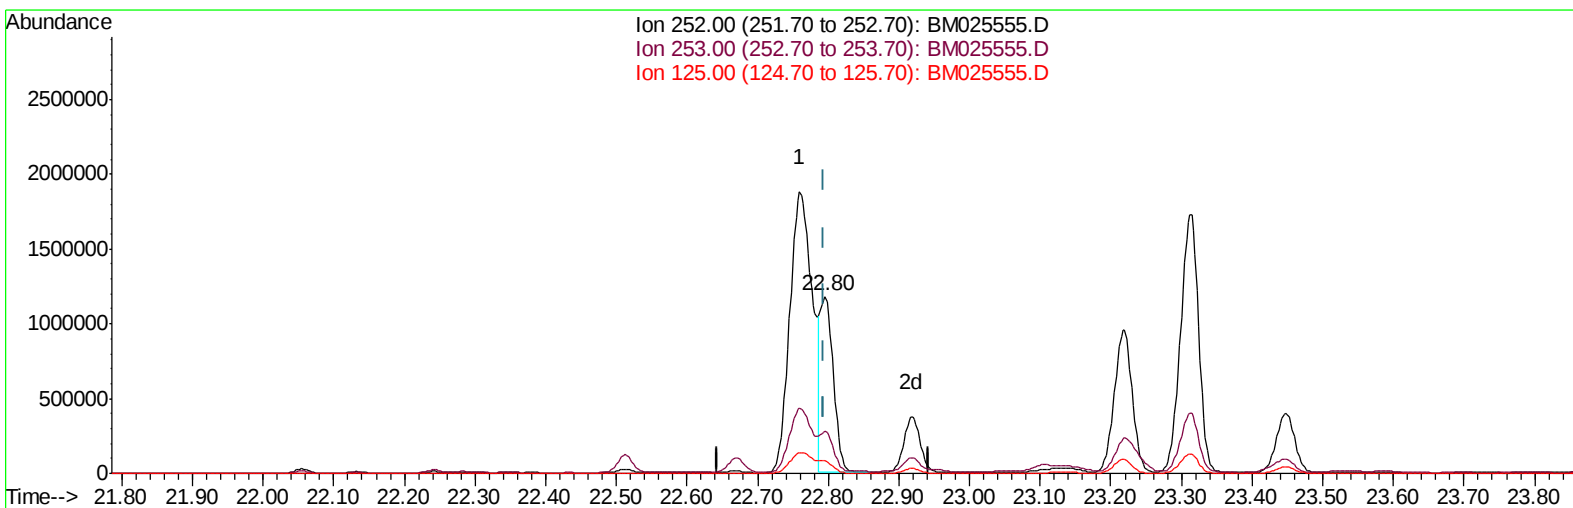

TIC: BM025555.D

(22) Benzo(k)fluoranthene

22.796min (+0.002) 14.73ng/ul m

response 1536100

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.71
125.00	8.90	7.07#
0.00	0.00	0.00