
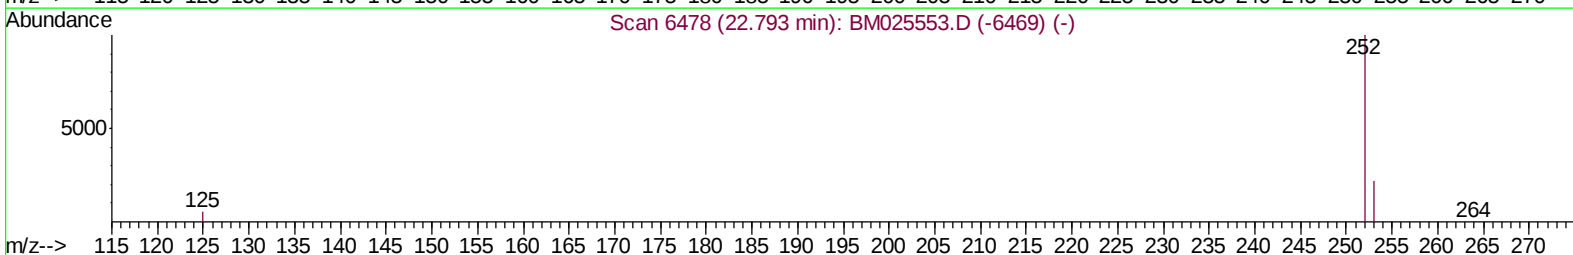
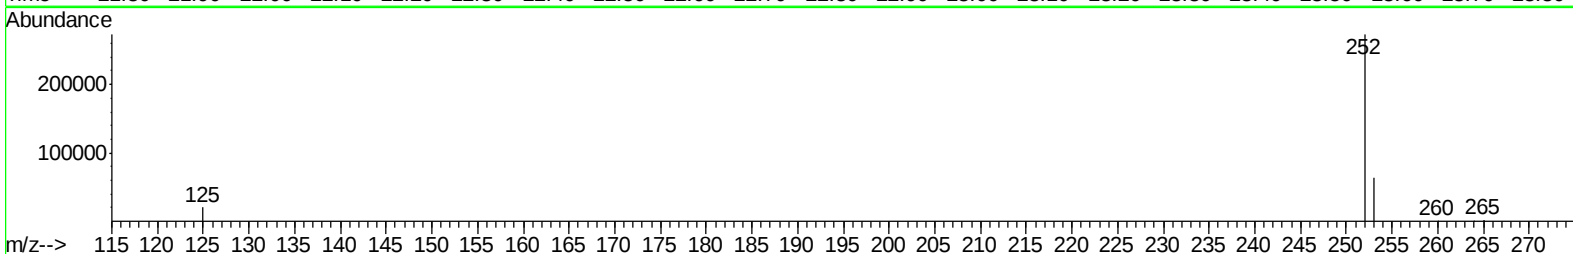


Data File : BM025557.D
Acq On : 14 Mar 2020 01:27
Operator : CG/JU
Sample : L1786-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 16 06:47:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

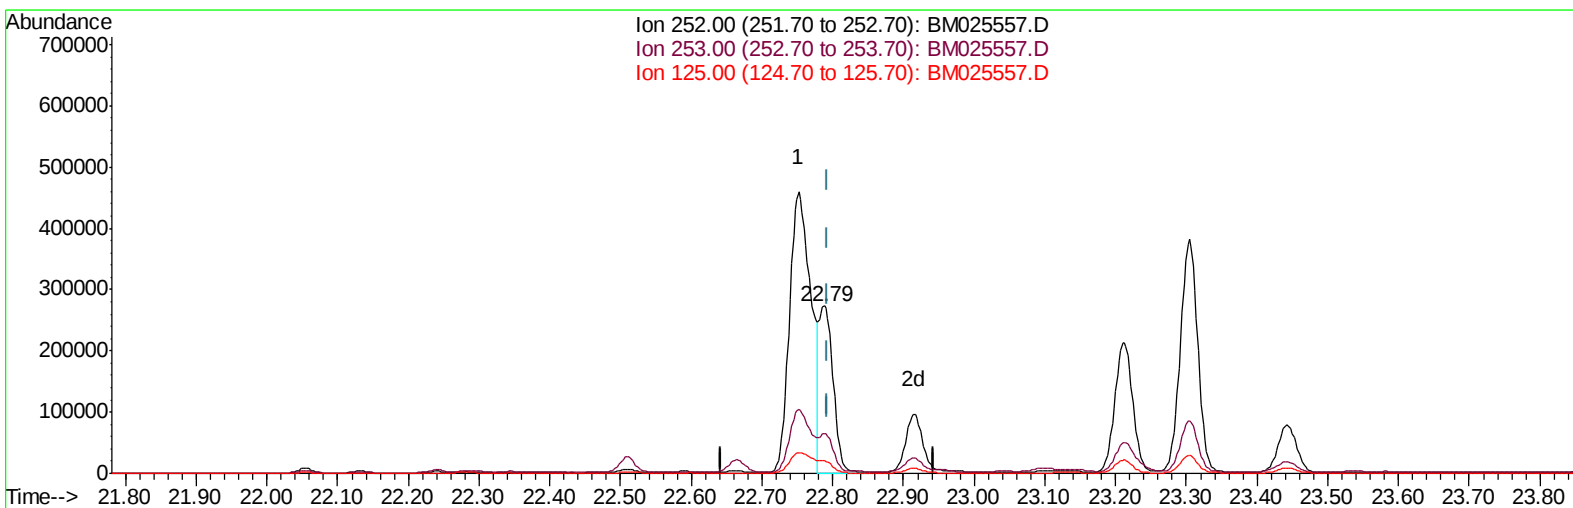

TIC: BM025557.D

(22) Benzo(k)fluoranthene

22.788min (-0.005) 4.49ng/ul m

response 371950

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.68
125.00	8.90	7.40
0.00	0.00	0.00