
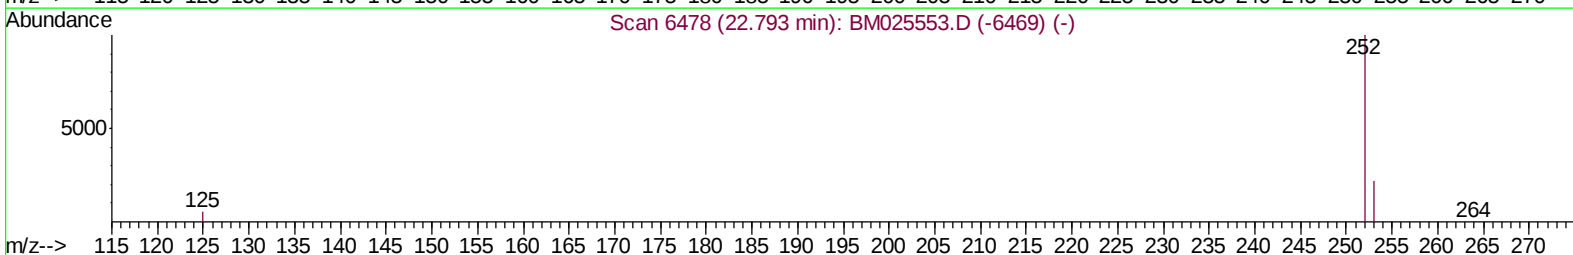
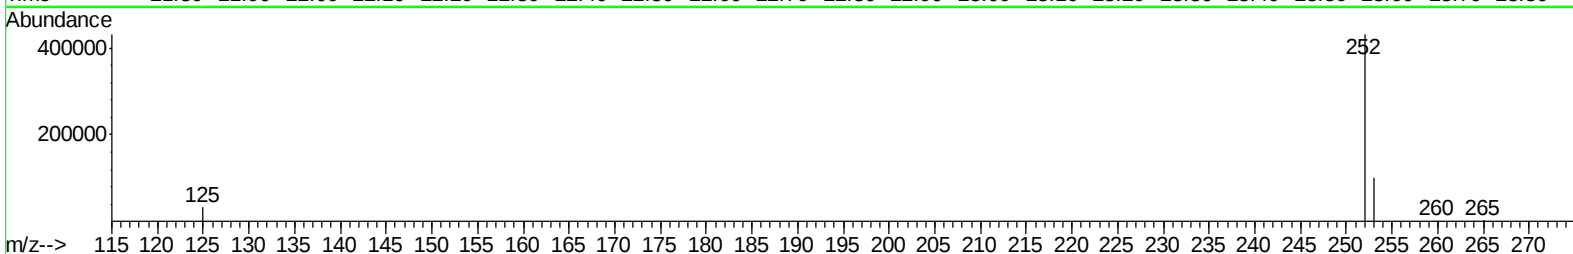


Data File : BM025558.D
Acq On : 14 Mar 2020 02:03
Operator : CG/JU
Sample : L1786-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Mar 16 06:47:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

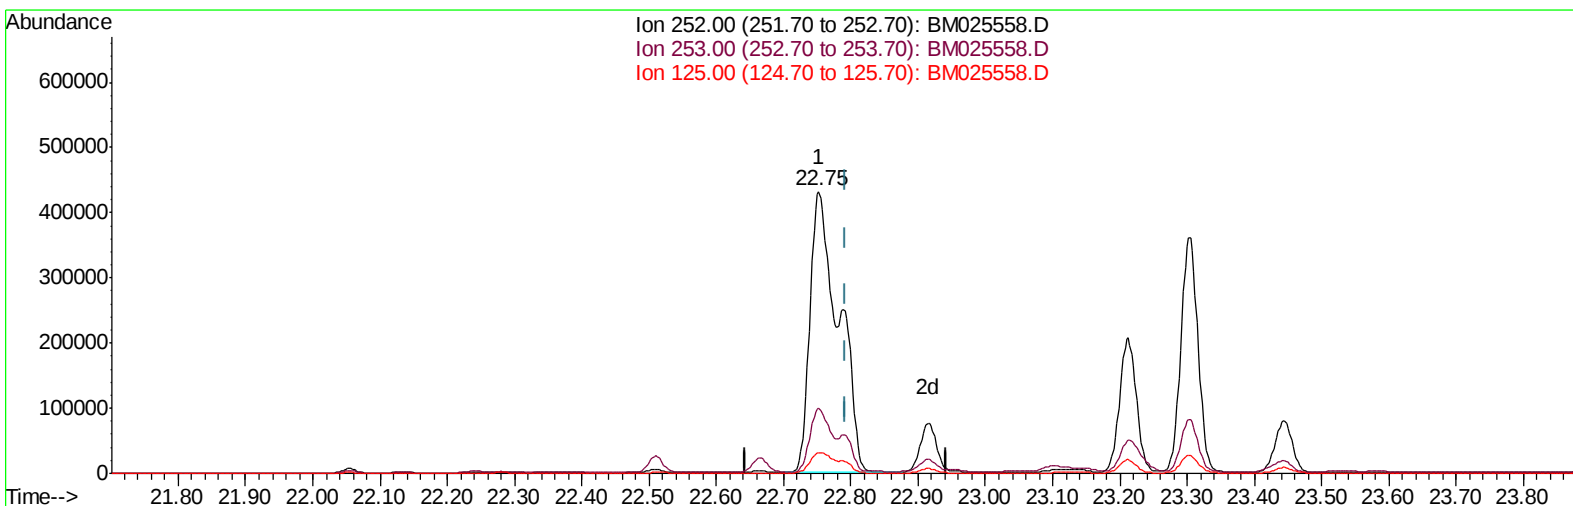

TIC: BM025558.D

(22) Benzo(k)fluoranthene

22.752min (-0.041) 18.07ng/ul

response 1275769

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	23.13
125.00	8.90	7.39
0.00	0.00	0.00