
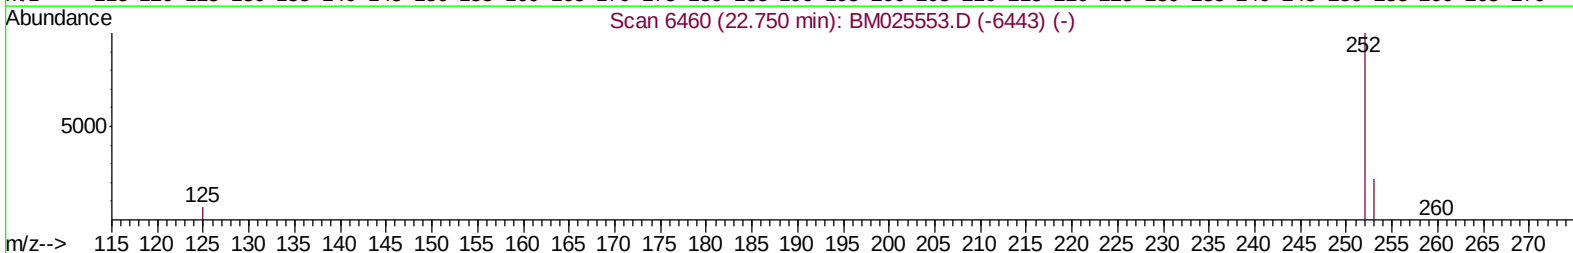
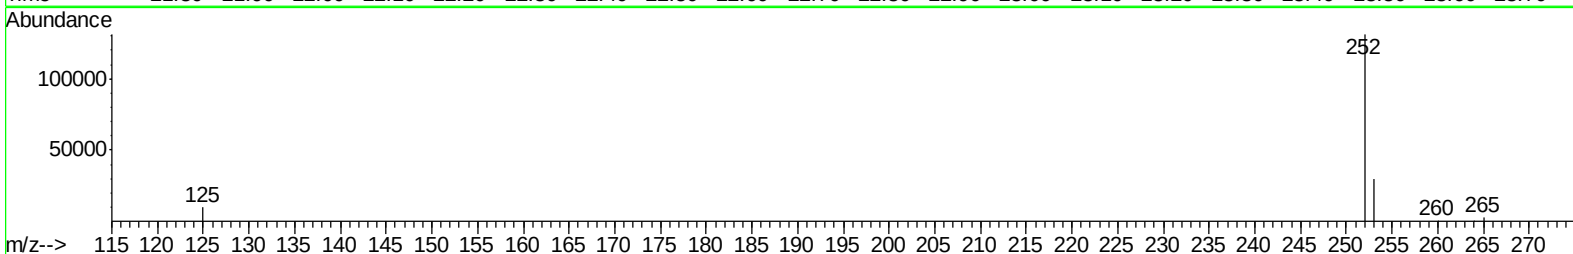


Data File : BM025559.D
Acq On : 14 Mar 2020 02:39
Operator : CG/JU
Sample : L1786-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Mar 16 06:48:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

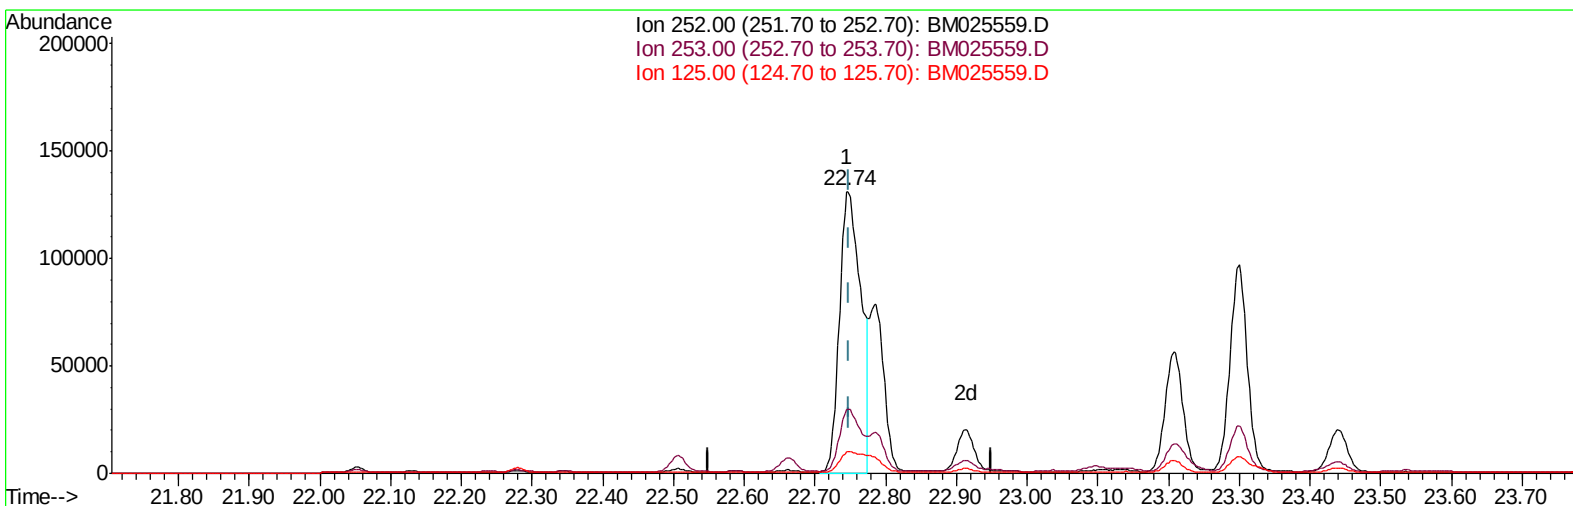

TIC: BM025559.D

(21) Benzo(b)fluoranthene

22.745min (-0.005) 4.84ng/ul m

response 274744

Ion	Exp%	Act%
252.00	100	100
253.00	25.10	22.90
125.00	8.80	7.60
0.00	0.00	0.00