
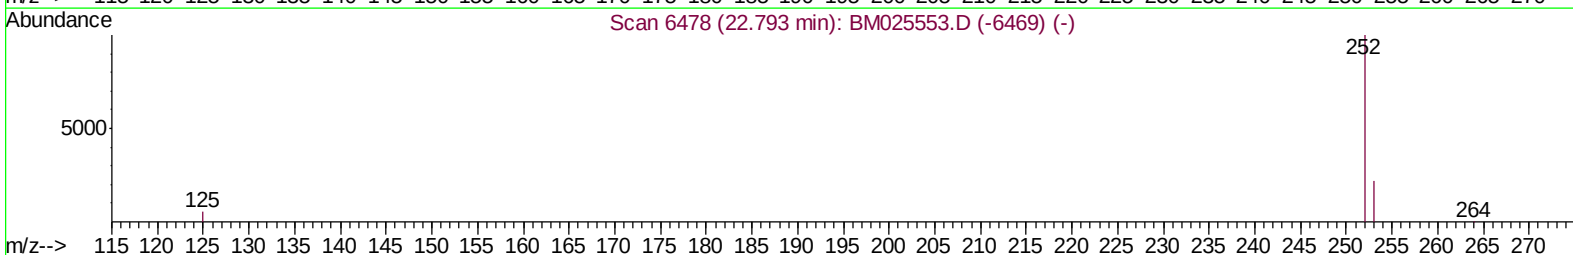
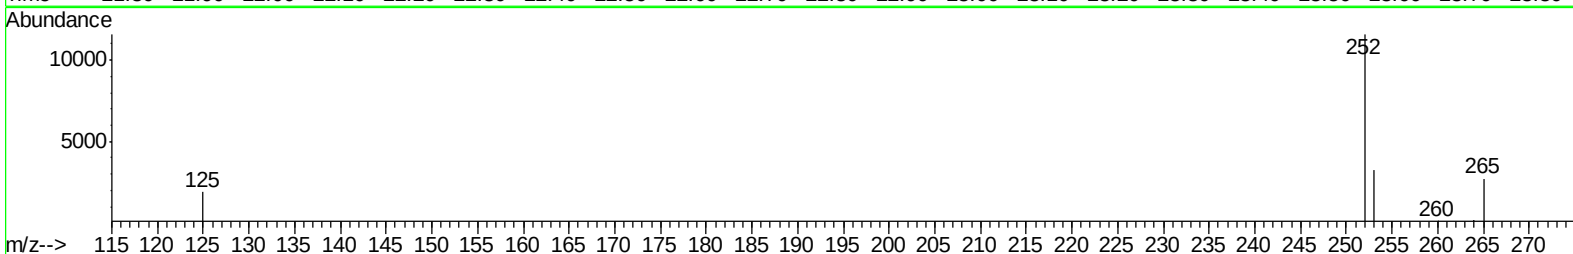


Data File : BM025560.D
Acq On : 14 Mar 2020 03:15
Operator : CG/JU
Sample : L1786-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 16 07:09:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

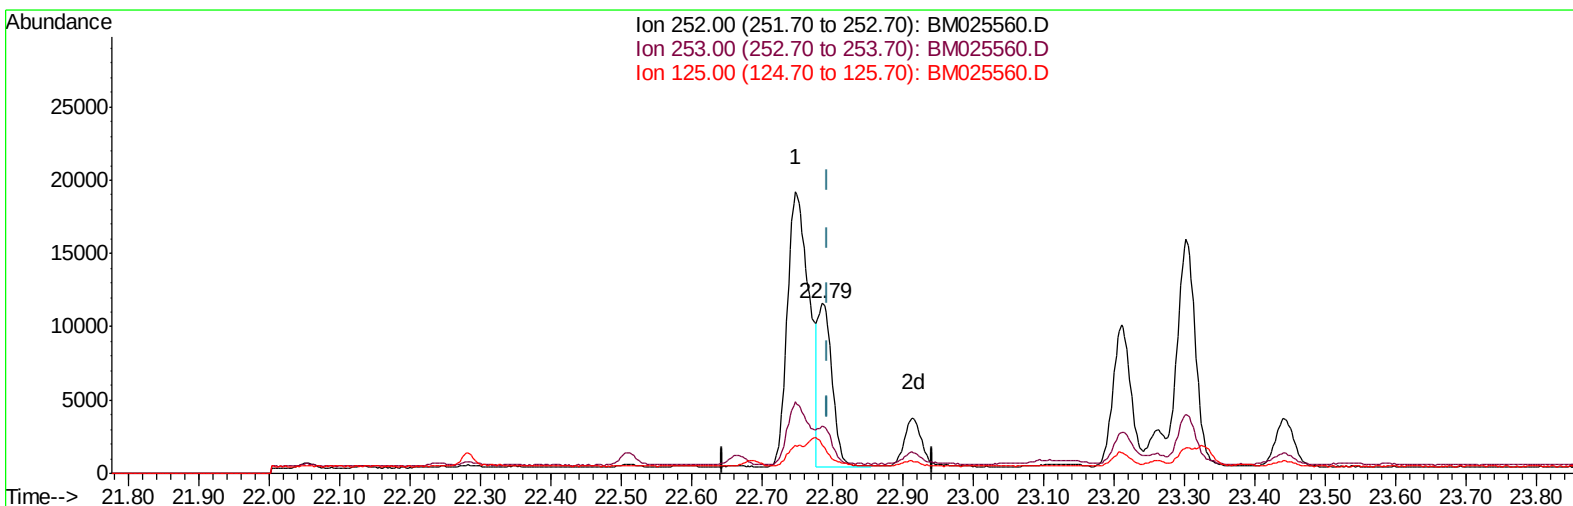

TIC: BM025560.D

(22) Benzo(k)fluoranthene

22.786min (-0.007) 0.21ng/ul m

response 15975

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	28.11
125.00	8.90	16.43#
0.00	0.00	0.00