
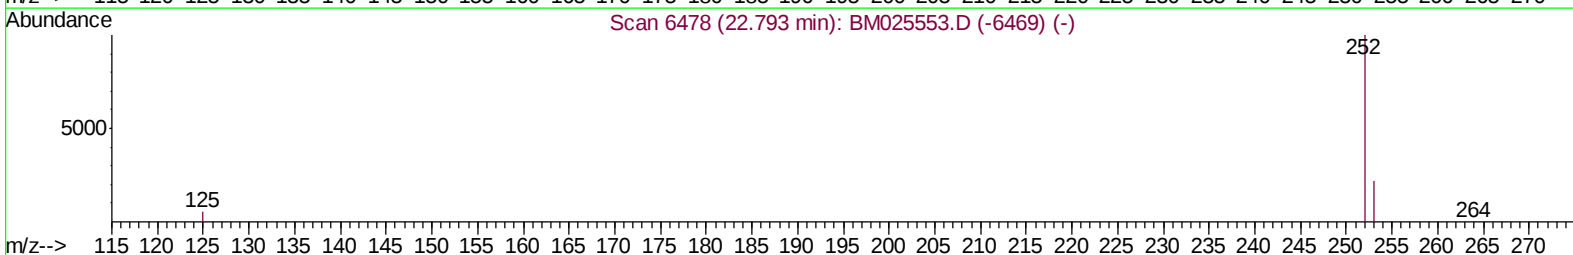
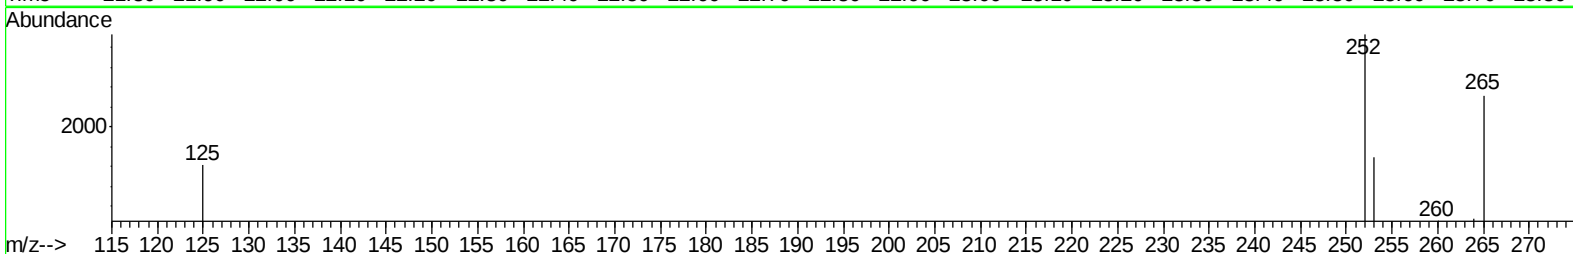


Data File : BM025563.D
Acq On : 14 Mar 2020 05:02
Operator : CG/JU
Sample : L1786-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 16 07:26:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 16 06:44:28 2020
Response via : Initial Calibration

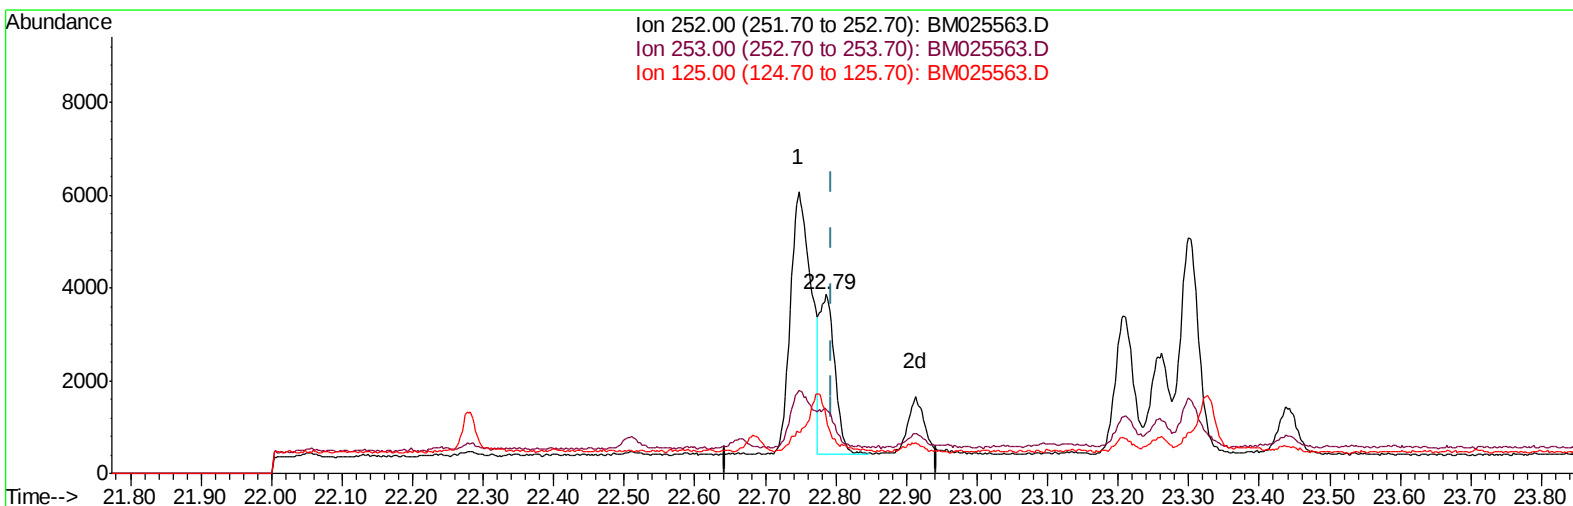

TIC: BM025563.D

(22) Benzo(k)fluoranthene

22.786min (-0.007) 0.07ng/ul m

response 5153

Ion	Exp%	Act%
252.00	100	100
253.00	24.80	36.05#
125.00	8.90	31.62#
0.00	0.00	0.00